

Data Path : S:\HPCHEM1\HPLC_L\Data\HL102512\
Data File : HL003652.D
Signal(s) : VWD1A.CH
Acq On : 25-Oct-2012, 12:16
Operator : HLM
Sample : 8330NG-CCV
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :

Integration File: events.e
Quant Time: Nov 16 03:20:42 2012
Quant Method : S:\HPCHEM1\HPLC_L\methods\HL102412.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Oct 25 10:56:40 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units


System Monitoring Compounds			
Target Compounds			
18) T PETN	17.759f	6904	0.746 ug/L


(f)=RT Delta > 1/2 Window

(m)=manual int.

Instrument :
HPLC_L
ClientSampleId :

```
Volume Inj. :
Signal Phase :
Signal Info :
```

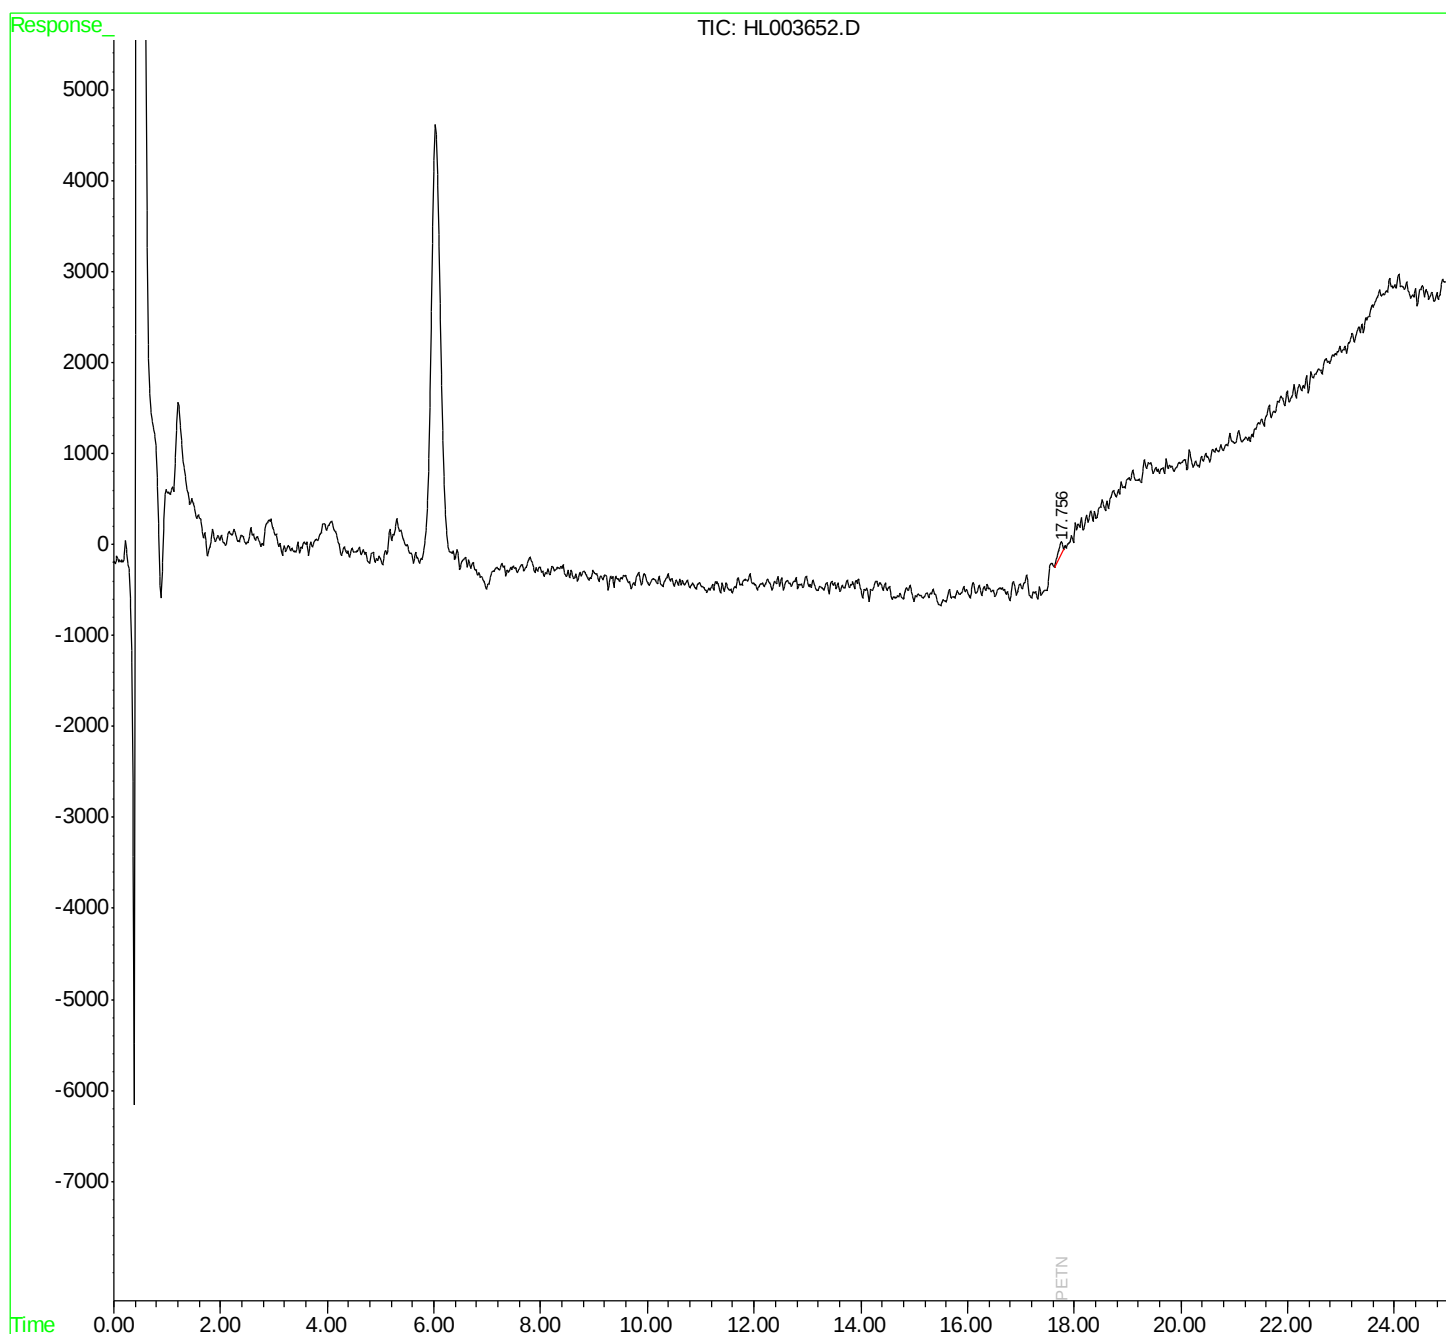


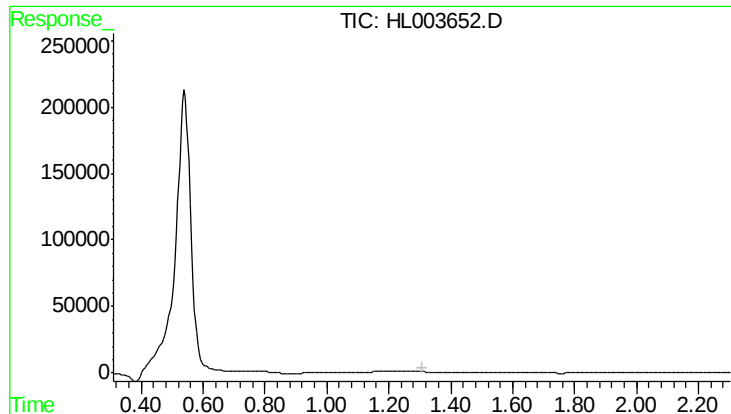

#1 4-Nitroaniline

R.T.: 0.000 min
 Exp R.T.: 1.307 min
 Response: 0
 Conc: N.D.

Instrument :
 HPLC_L
 ClientSampleId :

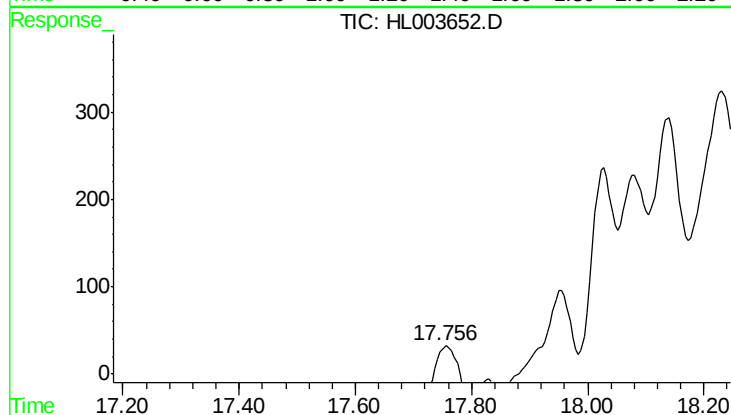

#18 PETN

R.T.: 17.759 min
 Delta R.T.: 0.131 min
 Response: 6904
 Conc: 0.75 ug/L