

Data Path : S:\HPCHEM1\HPLC_L\Data\HL102512\
Data File : HL003664.D
Signal(s) : VWD1A.CH
Acq On : 25-Oct-2012, 17:38
Operator : HLM
Sample : 8330-CCV
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
LabSampleId :
8330-CCV

Integration File: events.e
Quant Time: Nov 16 03:22:01 2012
Quant Method : S:\HPCHEM1\HPLC_L\methods\HL102412.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Oct 25 10:56:40 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
8) T	4-Amino-2,6-dinitroto...	6.870	5657391	783.995 ug/L
10) T	2,6-Dinitrotoluene	8.035	7854491	911.315 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_L\Data\HL102512\
Data File : HL003664.D
Signal(s) : VWD1A.CH
Acq On : 25-Oct-2012, 17:38
Operator : HLM
Sample : 8330-CCV
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
LabSampleId :
8330-CCV

Integration File: events.e
Quant Time: Nov 16 03:22:01 2012
Quant Method : S:\HPCHEM1\HPLC_L\methods\HL102412.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Oct 25 10:56:40 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

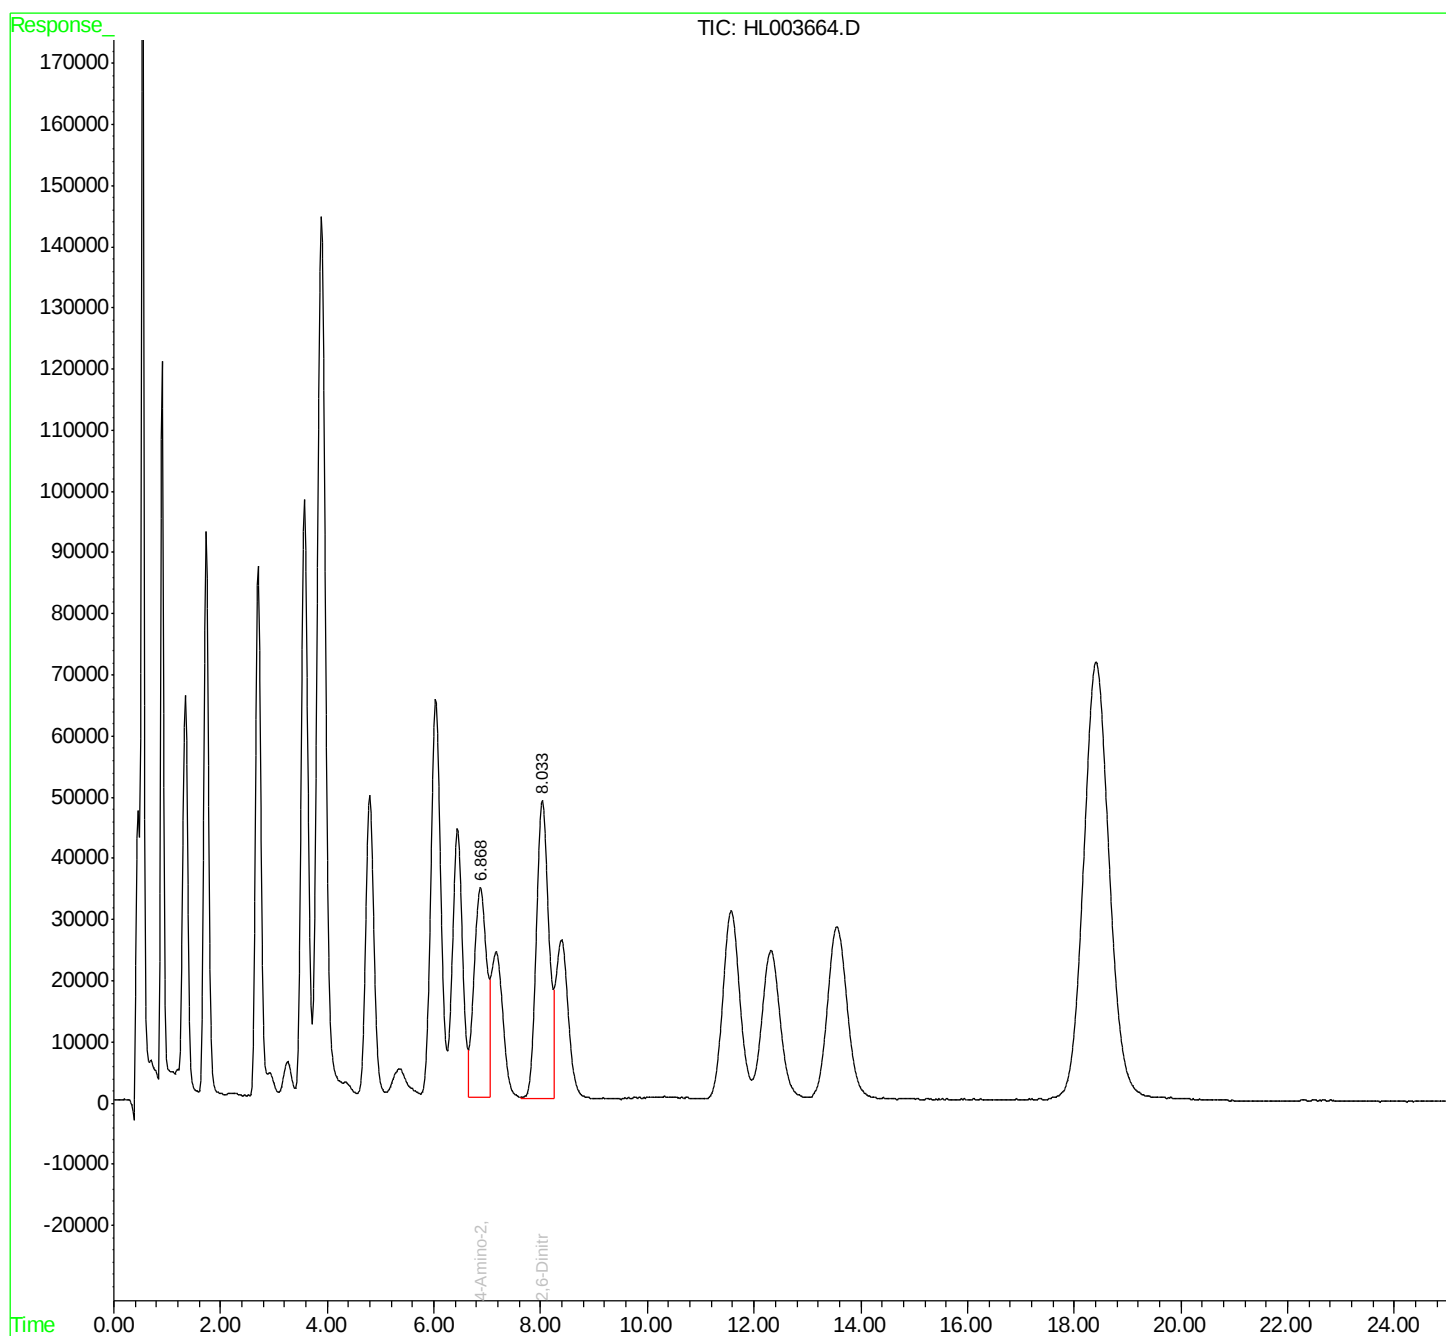


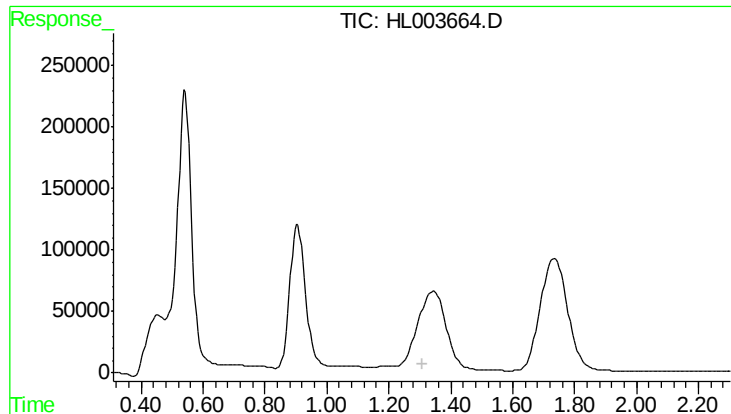

#1 4-Nitroaniline


R.T.: 0.000 min
Exp R.T.: 1.307 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
LabSampleId :
8330-CCV

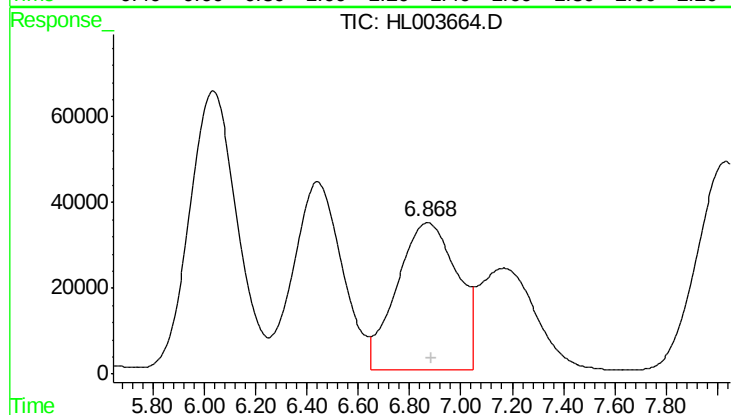

#8 4-Amino-2,6-dinitrotoluene

R.T.: 6.870 min
Delta R.T.: -0.016 min
Response: 5657391
Conc: 784.00 ug/L

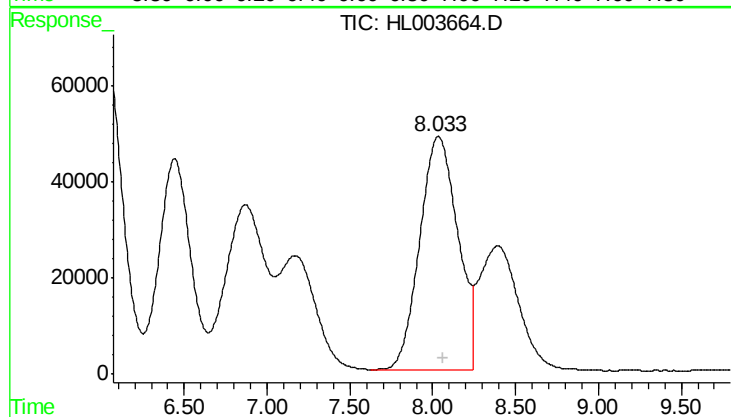

#10 2,6-Dinitrotoluene

R.T.: 8.035 min
Delta R.T.: -0.029 min
Response: 7854491
Conc: 911.32 ug/L