

Data Path : S:\HPCHEM1\HPLC\_L\Data\HL102512\  
Data File : HL003676.D  
Signal(s) : VWD1A.CH  
Acq On : 25-Oct-2012, 23:01  
Operator : HLM  
Sample : 8330-CCV  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
HPLC\_L  
LabSampleId :  
8330-CCV

Integration File: events.e  
Quant Time: Nov 16 03:23:24 2012  
Quant Method : S:\HPCHEM1\HPLC\_L\methods\HL102412.M  
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)  
QLast Update : Thu Oct 25 10:56:40 2012  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. :  
Signal Phase :  
Signal Info :

|                             | Compound                 | R.T.  | Response | Conc Units   |
|-----------------------------|--------------------------|-------|----------|--------------|
| -----                       |                          |       |          |              |
| System Monitoring Compounds |                          |       |          |              |
| Target Compounds            |                          |       |          |              |
| 8) T                        | 4-Amino-2,6-dinitroto... | 6.890 | 5655058  | 783.672 ug/L |
| 10) T                       | 2,6-Dinitrotoluene       | 8.058 | 7900642  | 916.670 ug/L |
| -----                       |                          |       |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC\_L\Data\HL102512\  
Data File : HL003676.D  
Signal(s) : VWD1A.CH  
Acq On : 25-Oct-2012, 23:01  
Operator : HLM  
Sample : 8330-CCV  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
HPLC\_L  
LabSampleId :  
8330-CCV

Integration File: events.e  
Quant Time: Nov 16 03:23:24 2012  
Quant Method : S:\HPCHEM1\HPLC\_L\methods\HL102412.M  
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)  
QLast Update : Thu Oct 25 10:56:40 2012  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. :  
Signal Phase :  
Signal Info :

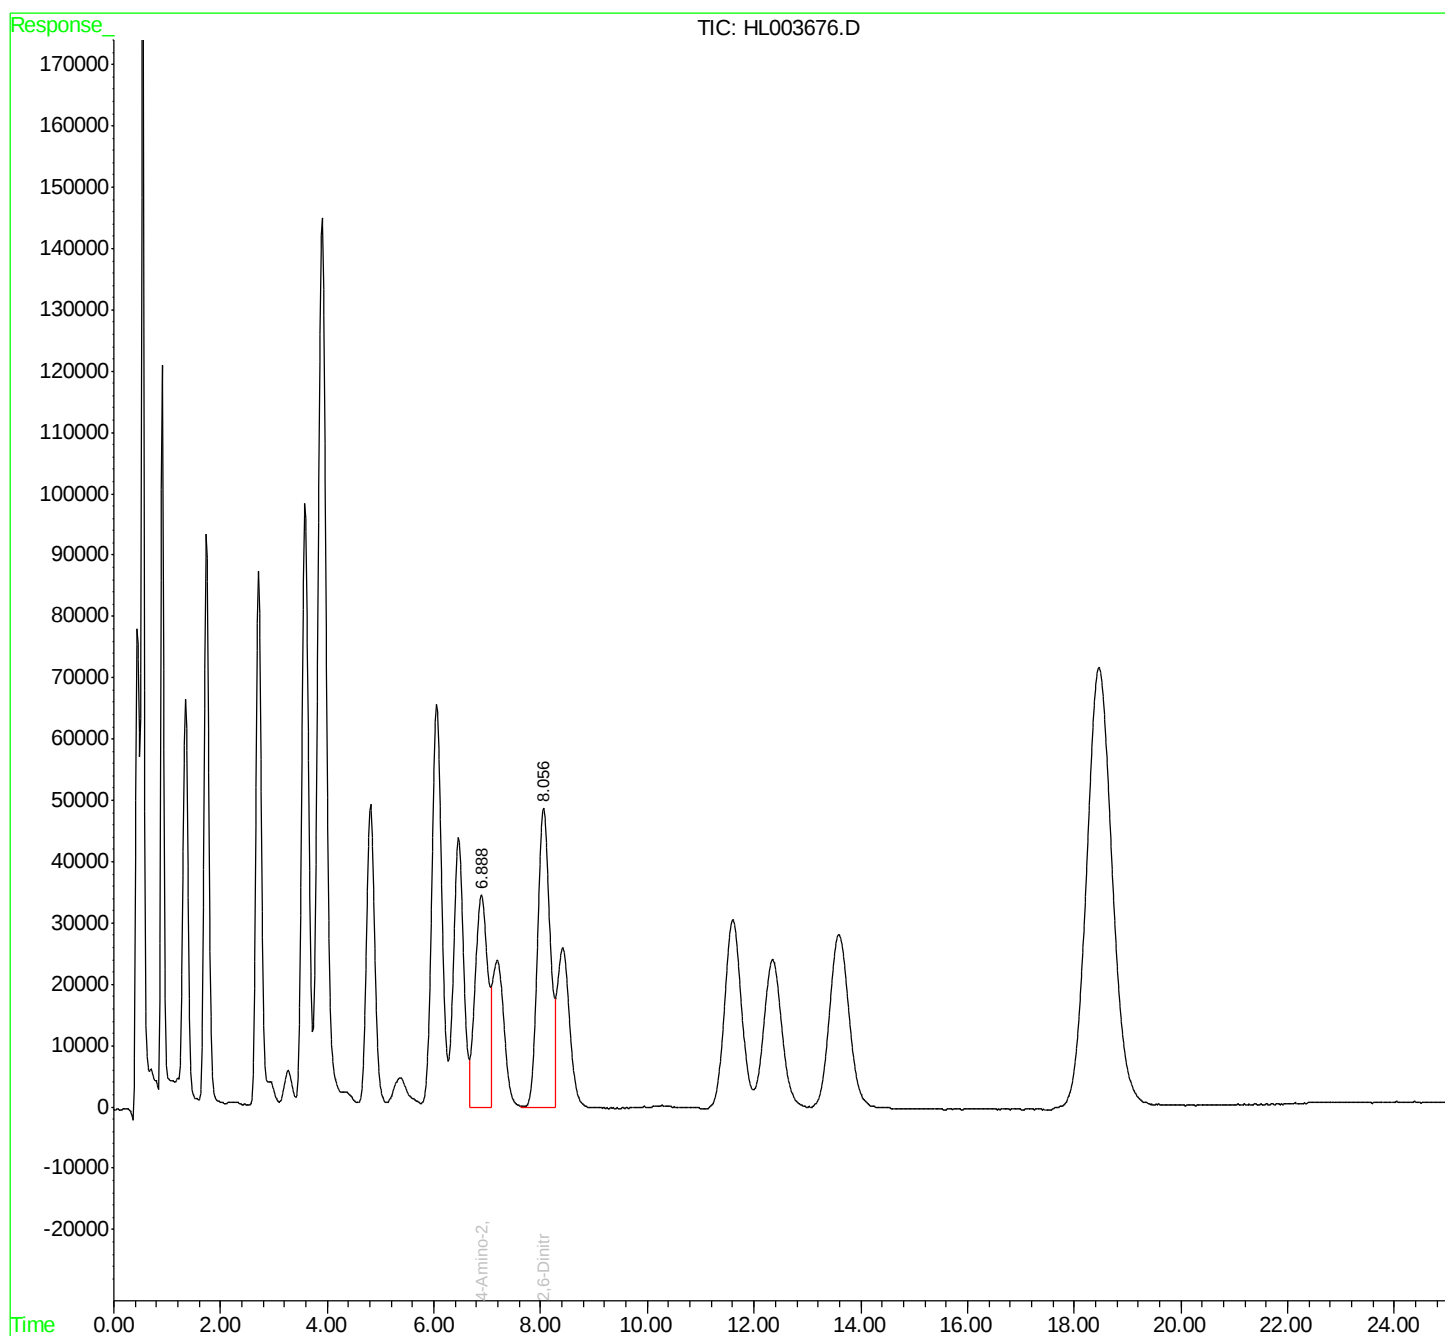


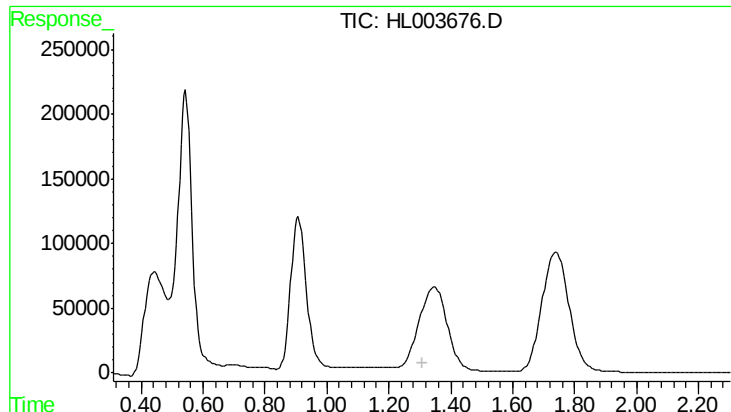

# #1 4-Nitroaniline


R.T.: 0.000 min  
Exp R.T.: 1.307 min  
Response: 0  
Conc: N.D.

Instrument :  
HPLC\_L  
LabSampleId :  
8330-CCV

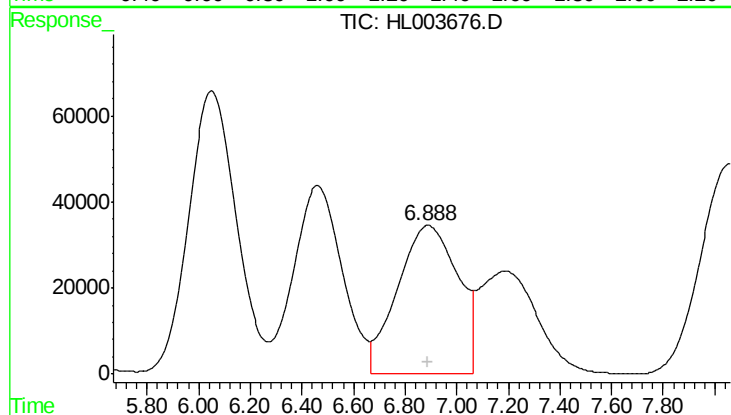

# #8 4-Amino-2,6-dinitrotoluene

R.T.: 6.890 min  
Delta R.T.: 0.003 min  
Response: 5655058  
Conc: 783.67 ug/L

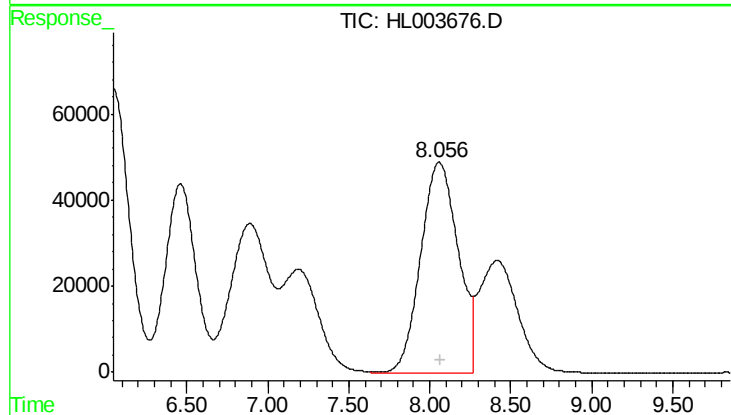

# #10 2,6-Dinitrotoluene

R.T.: 8.058 min  
Delta R.T.: -0.006 min  
Response: 7900642  
Conc: 916.67 ug/L