

Data Path : S:\HPCHEM1\HPLC_L\Data\HL102512\
 Data File : HL003676.D
 Signal(s) : VWD1A.CH
 Acq On : 25-Oct-2012, 23:01
 Operator : HLM
 Sample : 8330-CCV
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 HPLC_L
 LabSampleId :
 8330-CCV

Integration File: events.e
 Quant Time: Nov 16 03:09:46 2012
 Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL102412.M
 Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 QLast Update : Fri Oct 26 11:35:15 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.349	3912907	978.787 ug/L
Spiked Amount 300.000	Range 37 - 149	Recovery	= 326.26%#
Target Compounds			
2) T HMX	0.908	4177429	1031.337 ug/L
3) T RDX	1.741	5679424	1055.188 ug/L
4) T 1,3,5-Trinitrobenzene	2.714f	6000811	505.829 ug/L
5) T Tetryl	6.052f	8471572	994.833 ug/L
6) T 2,4,6-Trinitrotoluene	6.462f	5746861	504.343 ug/L
7) T 2-Amino-4,6-dinitroto...	6.890f	5655058	521.601 ug/L
8) T 4-Amino-2,6-dinitroto...	7.189f	3746812	519.229 ug/L
9) T 2,4-Dinitrotoluene	8.058f	7900642	494.778 ug/L
10) T 2,6-Dinitrotoluene	8.417f	4317693	500.959 ug/L
11) T 1,3-Dinitrobenzene	3.588f	8446468	510.497 ug/L
12) T Nitrobenzene	4.813f	5338044	498.781 ug/L
13) T 2-Nitrotoluene	11.604f	6766774	999.061 ug/L
14) T 3-Nitrotoluene	13.592f	7351109	1020.148 ug/L
15) T 4-Nitrotoluene	12.349f	5831552	1002.753 ug/L
16) T 3,5-Dinitroaniline	3.906	15970250	1017.142 ug/L
18) T PETN	18.469f	23835841	2573.859 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_L\Data\HL102512\
Data File : HL003676.D
Signal(s) : VWD1A.CH
Acq On : 25-Oct-2012, 23:01
Operator : HLM
Sample : 8330-CCV
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
LabSampleId :
8330-CCV

Integration File: events.e
Quant Time: Nov 16 03:09:46 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL102412.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Fri Oct 26 11:35:15 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

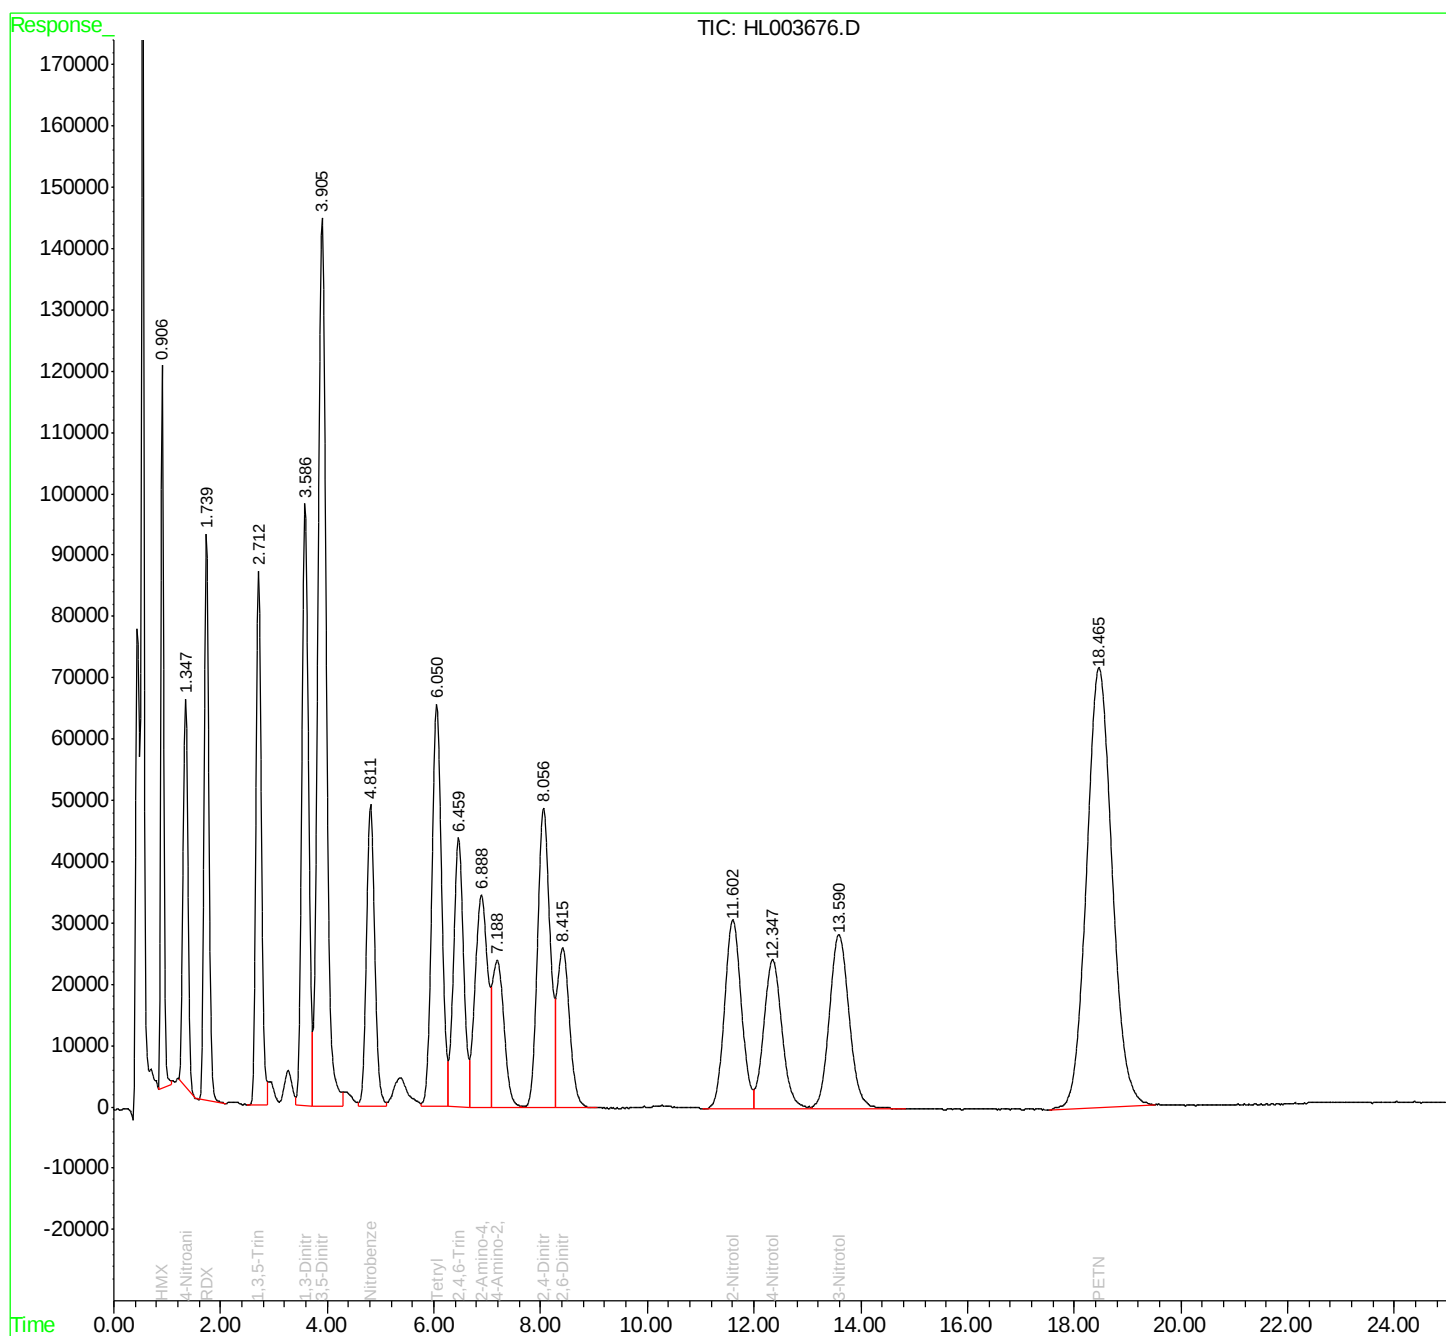


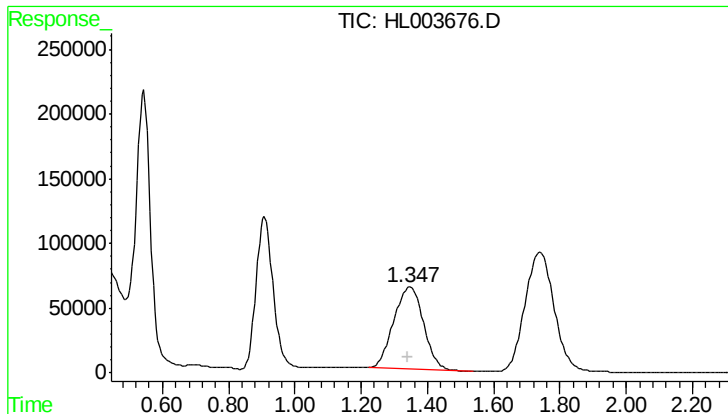

#1 4-Nitroaniline


R.T.: 1.349 min
Delta R.T.: 0.007 min
Response: 3912907
Conc: 978.79 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

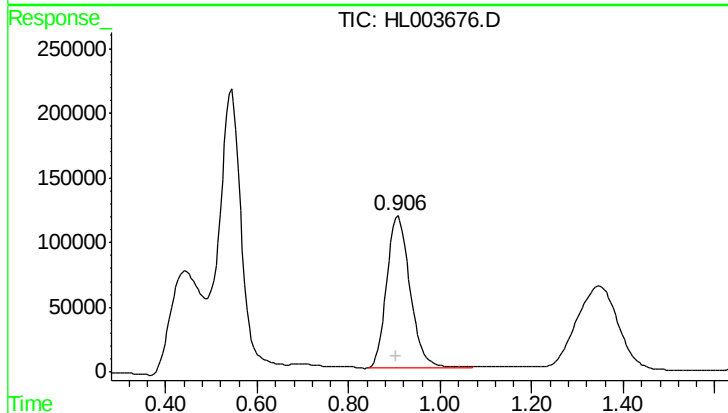


#2 HMX

R.T.: 0.908 min
Delta R.T.: 0.005 min
Response: 4177429
Conc: 1031.34 ug/L

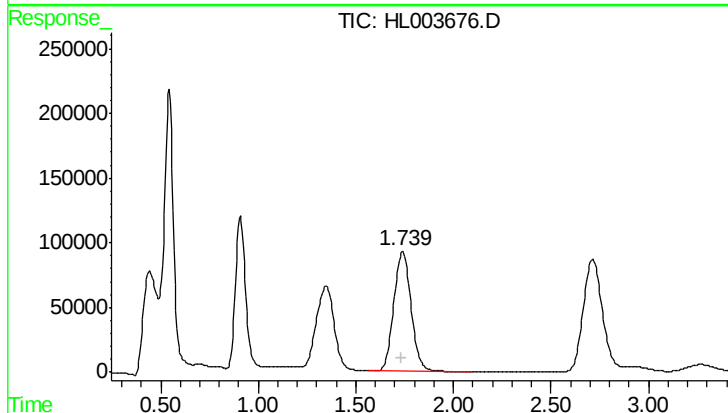


#3 RDX

R.T.: 1.741 min
Delta R.T.: 0.009 min
Response: 5679424
Conc: 1055.19 ug/L

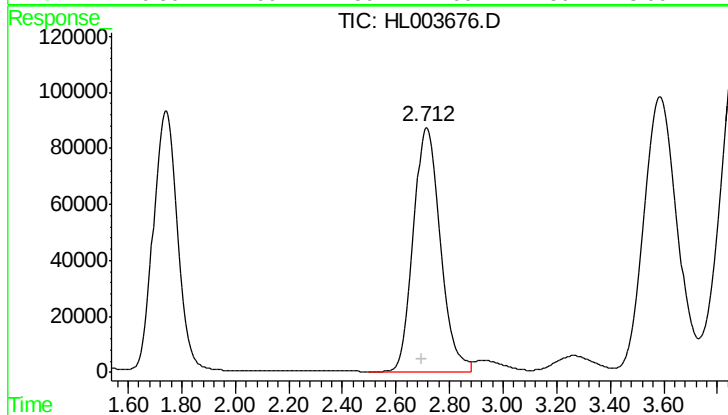

#4 1,3,5-Trinitrobenzene


R.T.: 2.714 min
Delta R.T.: 0.015 min
Response: 6000811
Conc: 505.83 ug/L

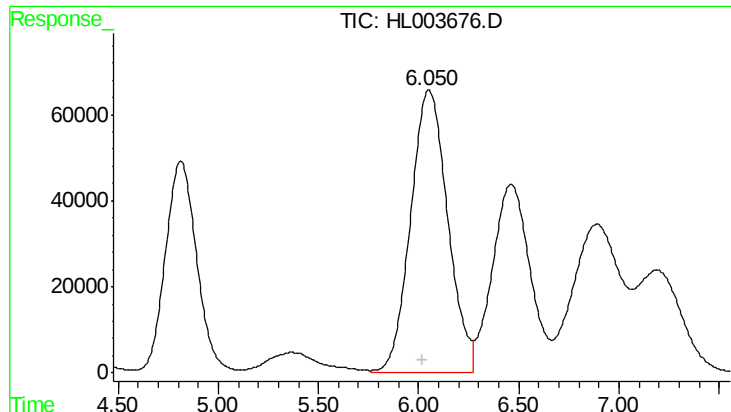

#5 Tetryl


R.T.: 6.052 min
Delta R.T.: 0.034 min
Response: 8471572
Conc: 994.83 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

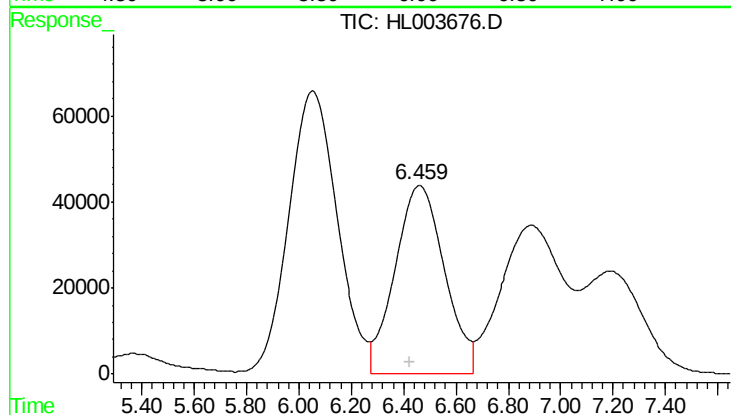


#6 2,4,6-Trinitrotoluene

R.T.: 6.462 min
Delta R.T.: 0.036 min
Response: 5746861
Conc: 504.34 ug/L

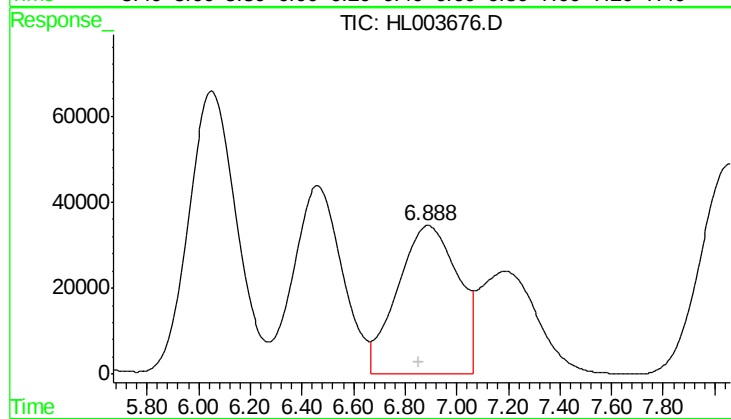


#7 2-Amino-4,6-dinitrotoluene

R.T.: 6.890 min
Delta R.T.: 0.037 min
Response: 5655058
Conc: 521.60 ug/L

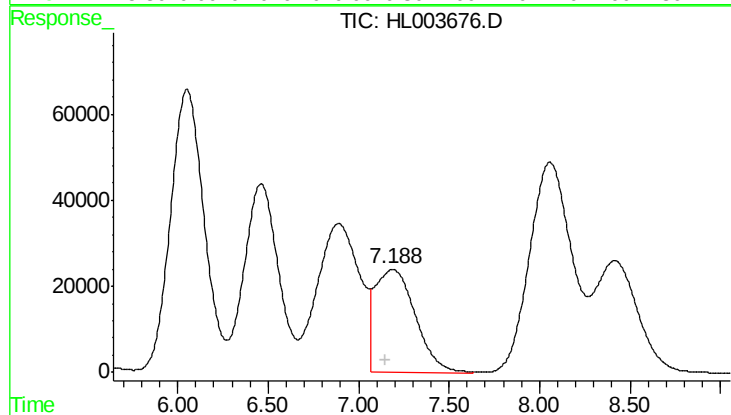

#8 4-Amino-2,6-dinitrotoluene


R.T.: 7.189 min
Delta R.T.: 0.040 min
Response: 3746812
Conc: 519.23 ug/L

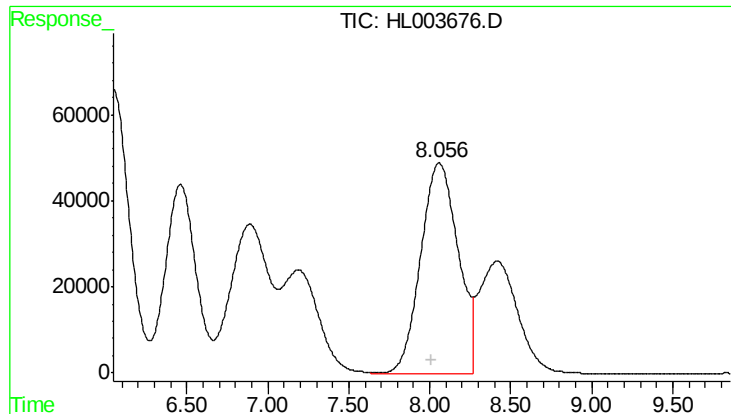

#9 2,4-Dinitrotoluene


R.T.: 8.058 min
Delta R.T.: 0.044 min
Response: 7900642
Conc: 494.78 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

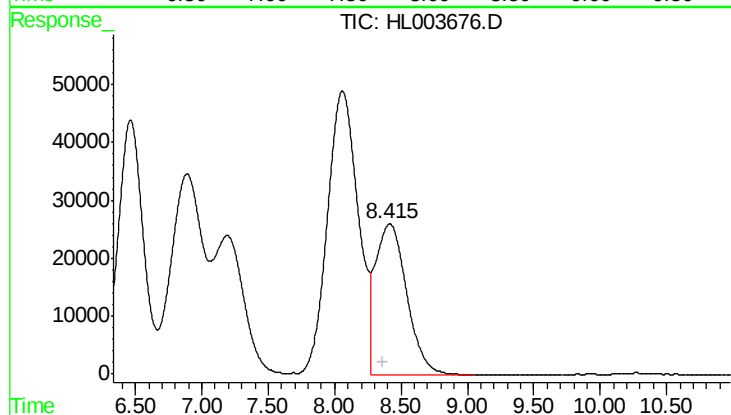


#10 2,6-Dinitrotoluene

R.T.: 8.417 min
Delta R.T.: 0.049 min
Response: 4317693
Conc: 500.96 ug/L

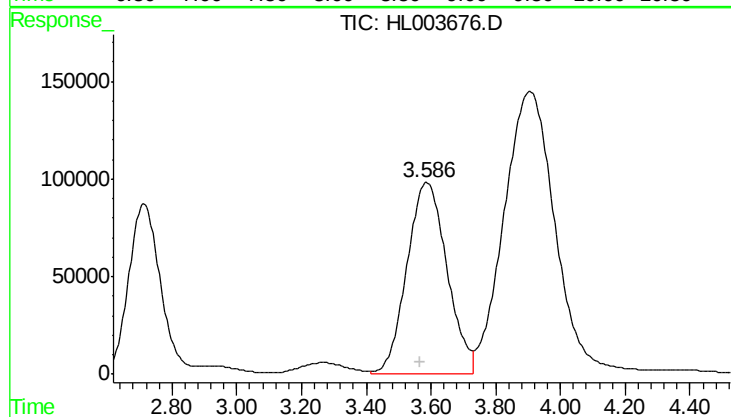


#11 1,3-Dinitrobenzene

R.T.: 3.588 min
Delta R.T.: 0.020 min
Response: 8446468
Conc: 510.50 ug/L

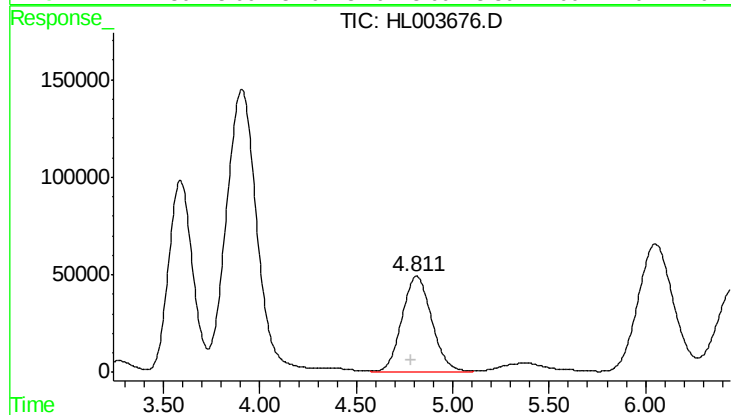

#12 Nitrobenzene


R.T.: 4.813 min
Delta R.T.: 0.027 min
Response: 5338044
Conc: 498.78 ug/L

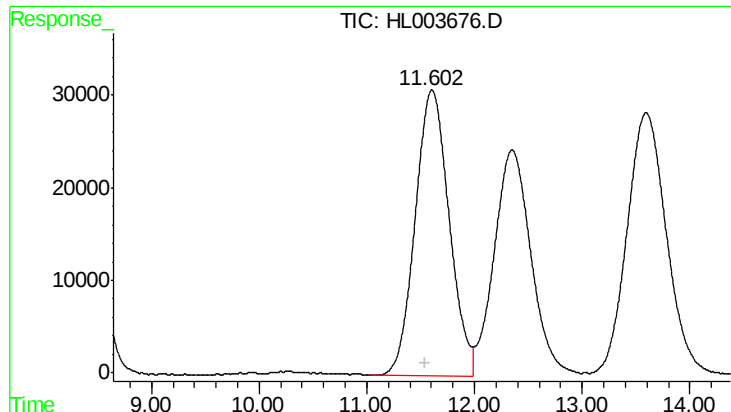

#13 2-Nitrotoluene


R.T.: 11.604 min
Delta R.T.: 0.063 min
Response: 6766774
Conc: 999.06 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

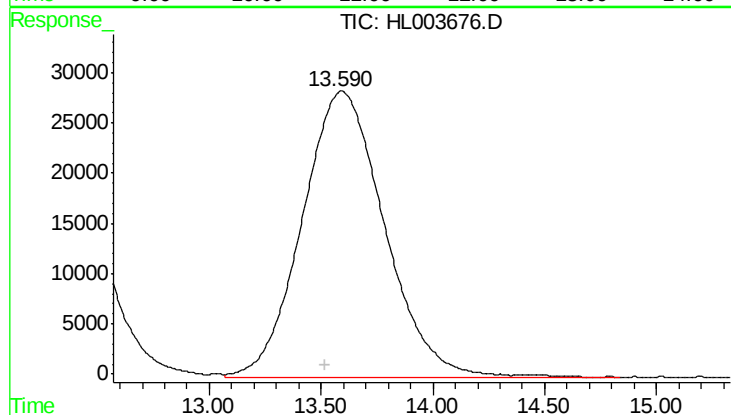


#14 3-Nitrotoluene

R.T.: 13.592 min
Delta R.T.: 0.075 min
Response: 7351109
Conc: 1020.15 ug/L

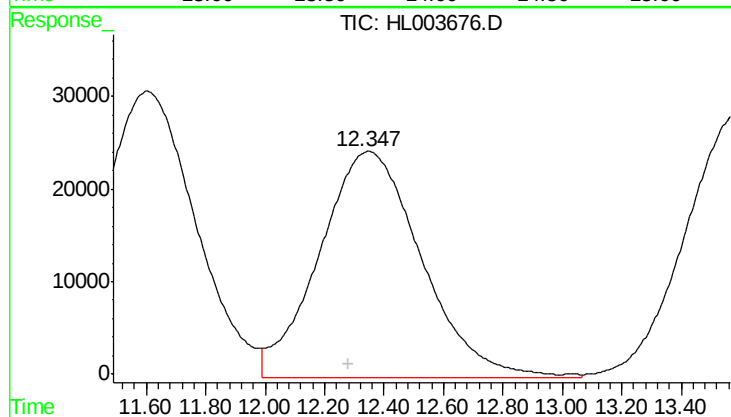


#15 4-Nitrotoluene

R.T.: 12.349 min
Delta R.T.: 0.068 min
Response: 5831552
Conc: 1002.75 ug/L

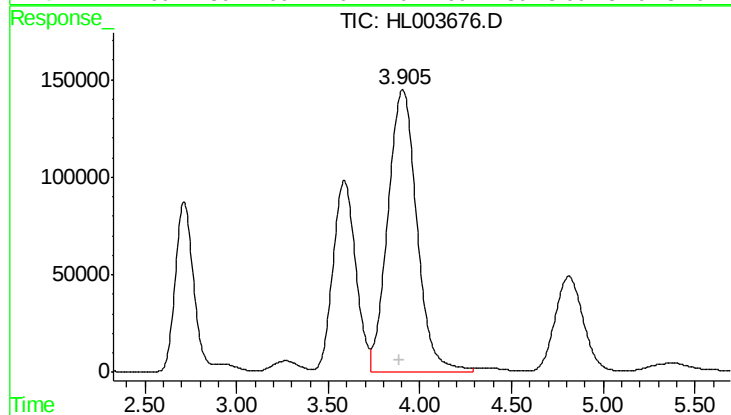

#16 3,5-Dinitroaniline

R.T.: 3.906 min
Delta R.T.: 0.021 min
Response: 15970250
Conc: 1017.14 ug/L

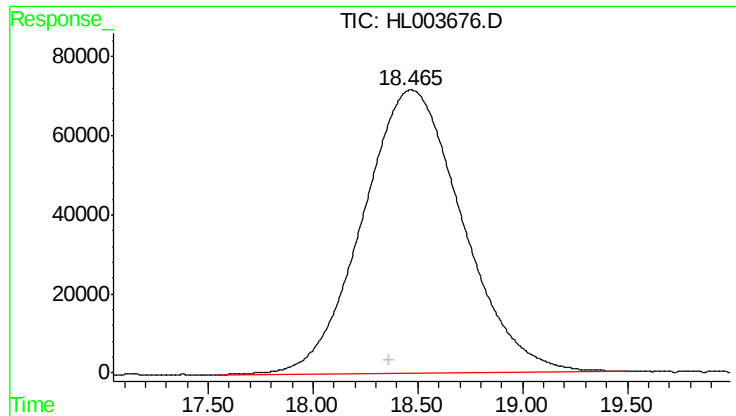

#18 PETN

R.T.: 18.469 min
Delta R.T.: 0.103 min
Response: 23835841
Conc: 2573.86 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV