

Data Path : S:\HPCHEM1\HPLC_L\Data\HL110912\
 Data File : HL003708.D
 Signal(s) : VWD1A.CH
 Acq On : 09-Nov-2012, 19:40
 Operator : HLM
 Sample : D4671-03
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 871

Integration File: events.e
 Quant Time: Nov 16 04:27:06 2012
 Quant Method : S:\HPCHEM1\HPLC_L\methods\HL102412.M
 Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 QLast Update : Thu Oct 25 10:56:40 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.302	517048	96.889 ug/L
Spiked Amount 300.000	Range 37 - 149	Recovery =	32.30%#
Target Compounds			
3) T RDX	1.682	1919537	356.634 ug/L
4) T 1,3,5-Trinitrobenzene	2.616	7389067	622.850 ug/L
6) T 2,4,6-Trinitrotoluene	6.186	5852364	513.601 ug/L
7) T 2-Amino-4,6-dinitroto...	6.595	13338401	1230.283 ug/L
8) T 4-Amino-2,6-dinitroto...	6.870	8572385	1187.952 ug/L
9) T 2,4-Dinitrotoluene	7.708	43527523	2725.913 ug/L
10) T 2,6-Dinitrotoluene	8.035	11818476	1371.236 ug/L
11) T 1,3-Dinitrobenzene	3.450	106020	6.408 ug/L
12) T Nitrobenzene	4.626	5454099	509.625 ug/L
13) T 2-Nitrotoluene	11.080	14128659	2085.986 ug/L
14) T 3-Nitrotoluene	12.975	15882936	2204.150 ug/L
15) T 4-Nitrotoluene	11.787	13098178	2252.271 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_L\Data\HL110912\
Data File : HL003708.D
Signal(s) : VWD1A.CH
Acq On : 09-Nov-2012, 19:40
Operator : HLM
Sample : D4671-03
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
871

Integration File: events.e
Quant Time: Nov 16 04:27:06 2012
Quant Method : S:\HPCHEM1\HPLC_L\methods\HL102412.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Oct 25 10:56:40 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

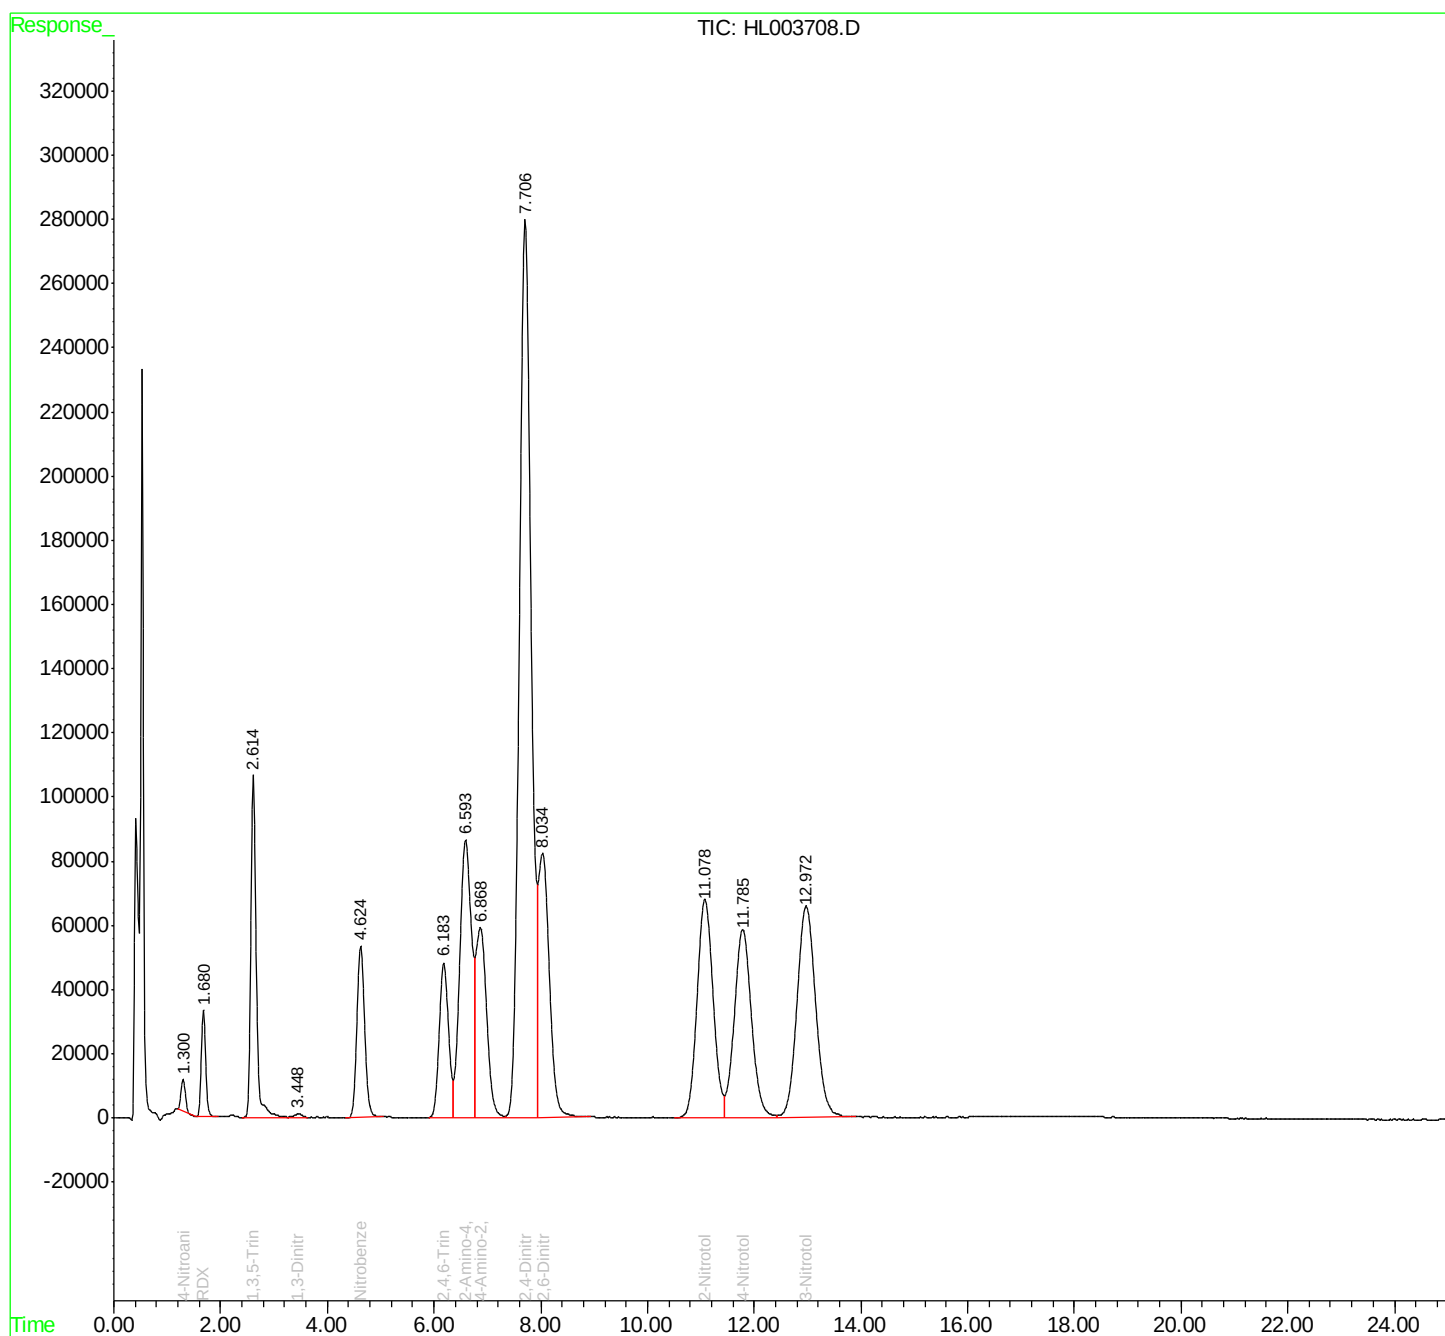


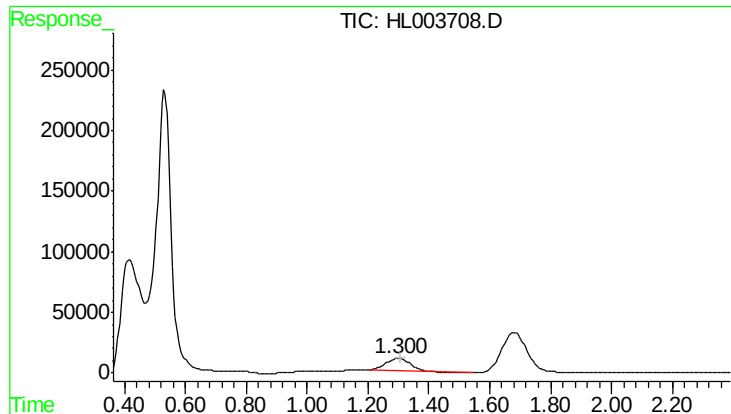

#1 4-Nitroaniline


R.T.: 1.302 min
 Delta R.T.: -0.005 min
 Response: 517048
 Conc: 96.89 ug/L

Instrument :
 HPLC_L
 ClientSampleId :
 871

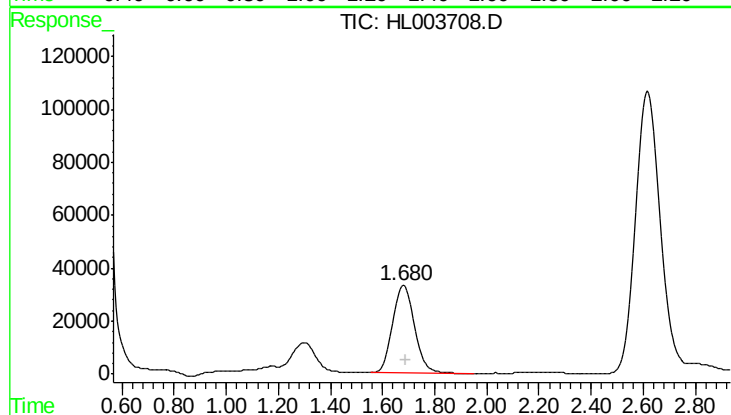


#3 RDX

R.T.: 1.682 min
 Delta R.T.: -0.006 min
 Response: 1919537
 Conc: 356.63 ug/L

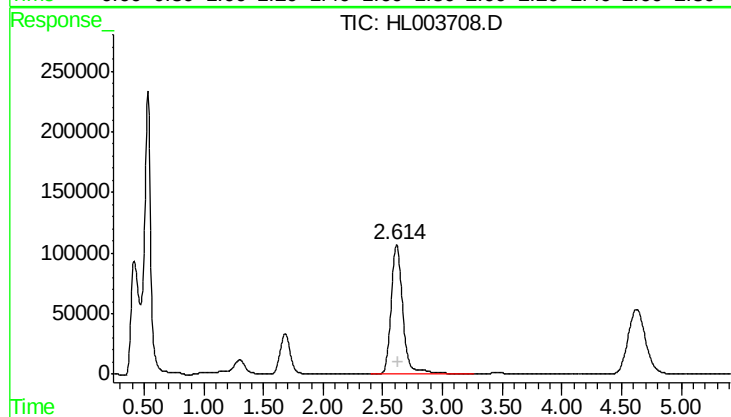


#4 1,3,5-Trinitrobenzene

R.T.: 2.616 min
 Delta R.T.: -0.009 min
 Response: 7389067
 Conc: 622.85 ug/L

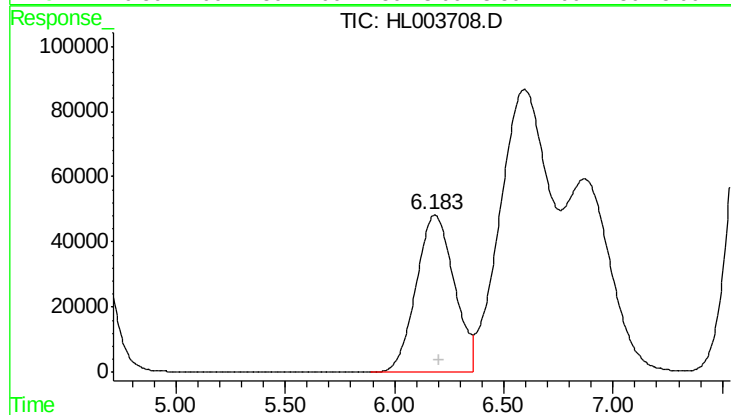

#6 2,4,6-Trinitrotoluene


R.T.: 6.186 min
 Delta R.T.: -0.016 min
 Response: 5852364
 Conc: 513.60 ug/L

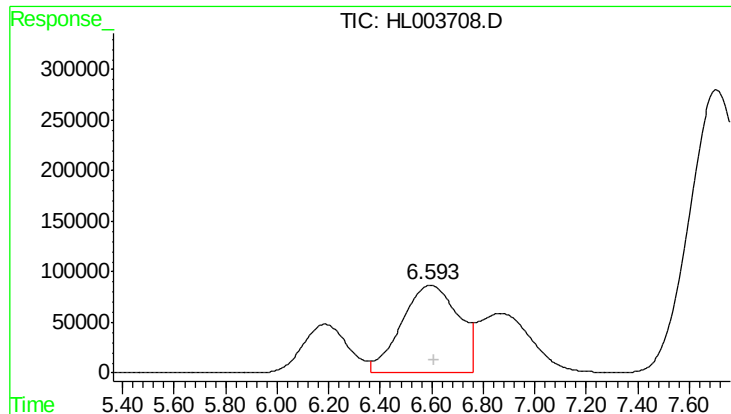

#7 2-Amino-4,6-dinitrotoluene


R.T.: 6.595 min
Delta R.T.: -0.015 min
Response: 13338401
Conc: 1230.28 ug/L

Instrument :
HPLC_L
ClientSampleId :
871

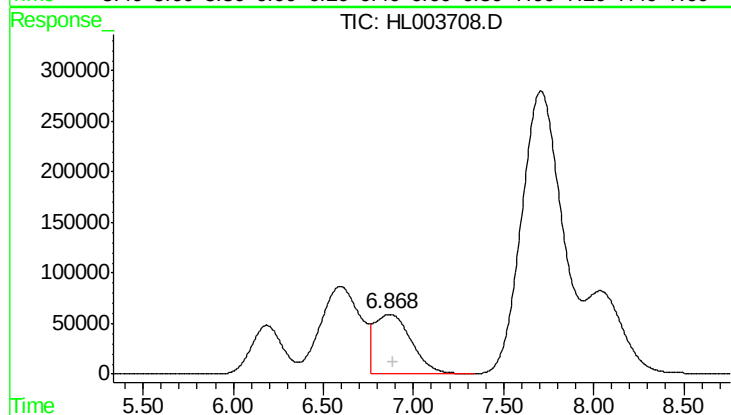


#8 4-Amino-2,6-dinitrotoluene

R.T.: 6.870 min
Delta R.T.: -0.017 min
Response: 8572385
Conc: 1187.95 ug/L

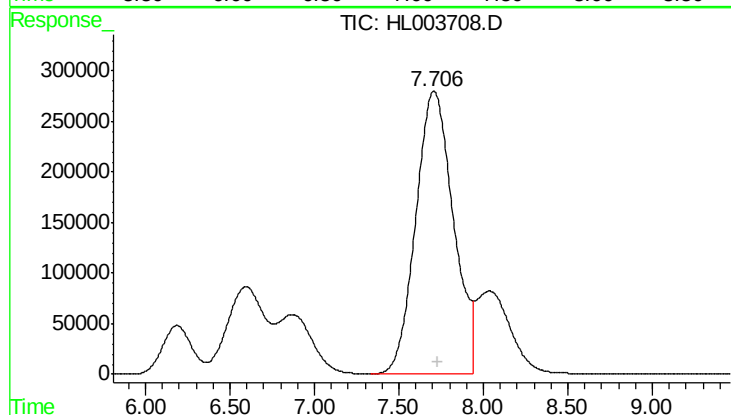


#9 2,4-Dinitrotoluene

R.T.: 7.708 min
Delta R.T.: -0.021 min
Response: 43527523
Conc: 2725.91 ug/L

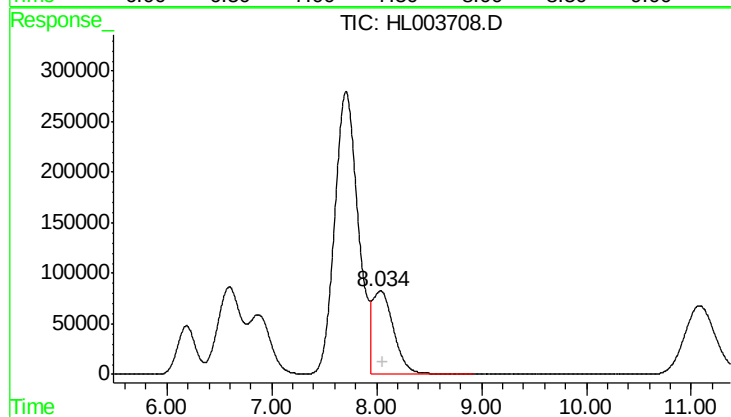

#10 2,6-Dinitrotoluene


R.T.: 8.035 min
Delta R.T.: -0.029 min
Response: 11818476
Conc: 1371.24 ug/L

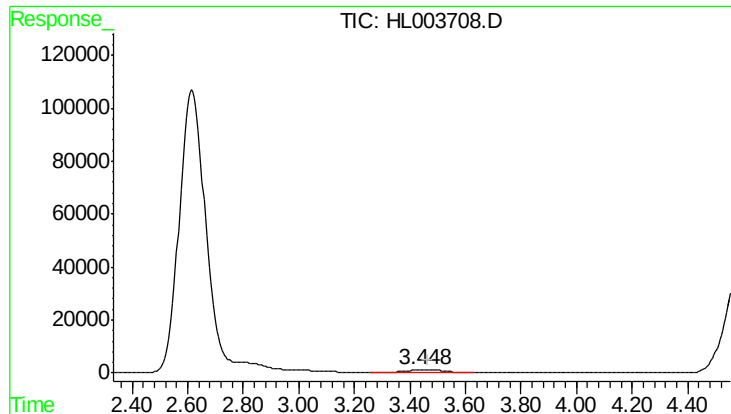

#11 1,3-Dinitrobenzene


R.T.: 3.450 min
Delta R.T.: -0.016 min
Response: 106020
Conc: 6.41 ug/L

Instrument :
HPLC_L
ClientSampleId :
871

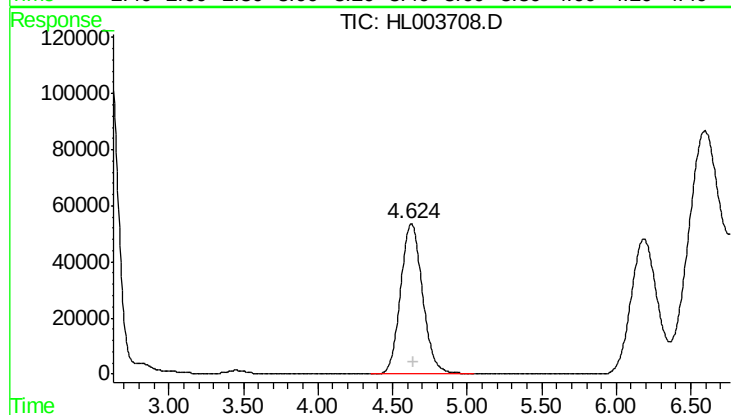


#12 Nitrobenzene

R.T.: 4.626 min
Delta R.T.: -0.014 min
Response: 5454099
Conc: 509.62 ug/L

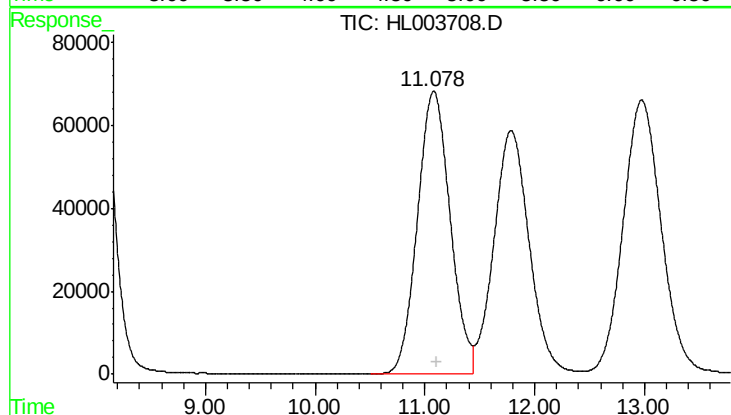


#13 2-Nitrotoluene

R.T.: 11.080 min
Delta R.T.: -0.030 min
Response: 14128659
Conc: 2085.99 ug/L

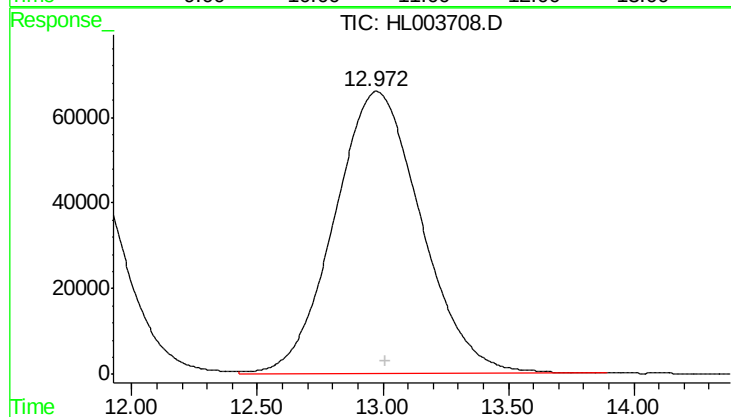

#14 3-Nitrotoluene

R.T.: 12.975 min
Delta R.T.: -0.036 min
Response: 15882936
Conc: 2204.15 ug/L

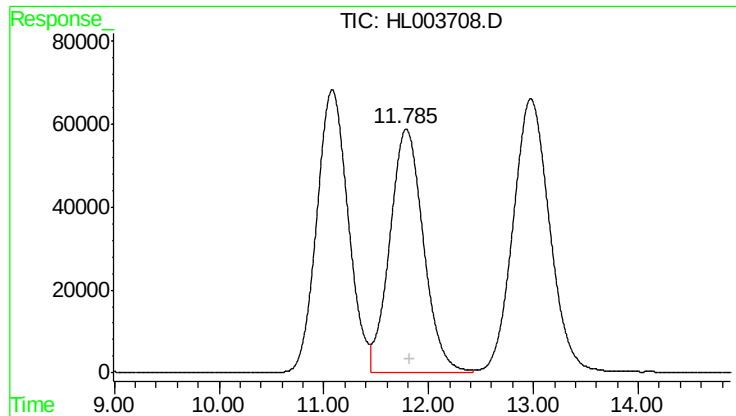

#15 4-Nitrotoluene

R.T.: 11.787 min
Delta R.T.: -0.031 min
Response: 13098178
Conc: 2252.27 ug/L

Instrument :
HPLC_L
ClientSampleId :
871