

Data File : H:\VOL1\HPLC\HPLC L\121113\HL003719.D Vial: 1
Acq On : 13-Nov-2012, 11:40 Operator: HLM
Sample : I.BLK Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Nov 14 13:24 2012 Quant Results File: HL102412.RES

Instrument :
HPLC_L
LabSampleId :
I.BLK

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL102412.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Wed Nov 14 13:24:43 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

16) T	3,5-Dinitroaniline	3.79	55982	3.566 ug/L
-------	--------------------	------	-------	------------

Data File : H:\VOL1\HPLC\HPLC L\121113\HL003719.D

Vial: 1

Acq On : 13-Nov-2012, 11:40

Operator: HLM

Sample : I.BLK

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Nov 14 13:24 2012 Quant Results File: HL102412.RES

Instrument :

HPLC_L

LabSampleId :

I.BLK

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL102412.M (Chemstation Integrator)

Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)

Last Update : Wed Nov 14 13:24:43 2012


Response via : Multiple Level Calibration


DataAcq Meth : 8330AGIP.M

Volume Inj. :

Signal Phase :

Signal Info :

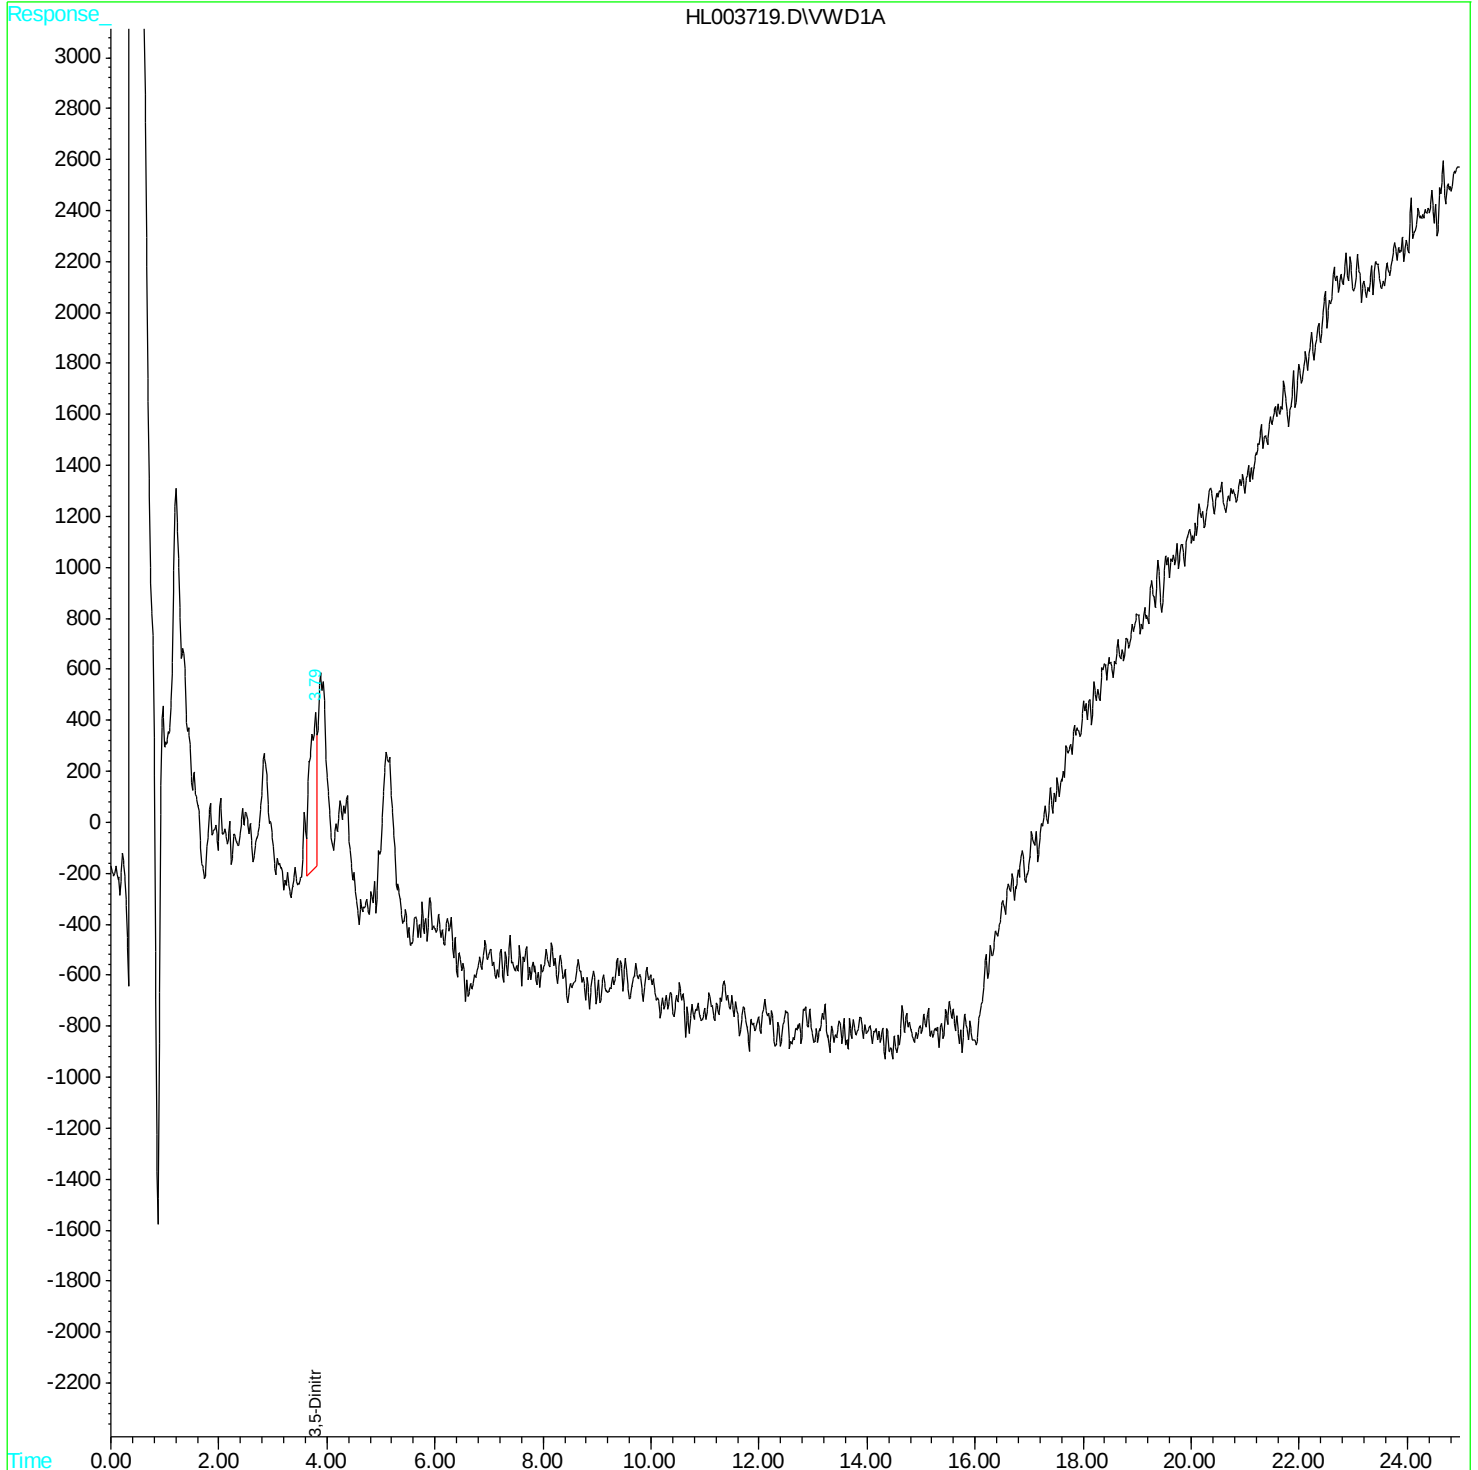

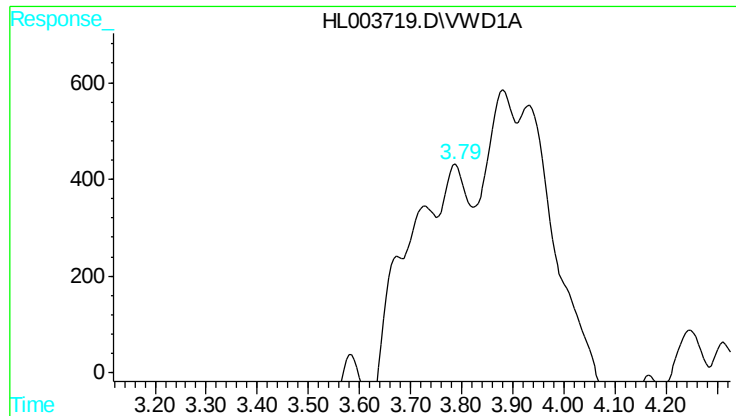

#16 3,5-Dinitroaniline

R.T.: 3.789 min
Delta R.T.: 0.021 min
Response: 55982
Conc: 3.57 ug/L

Instrument :
HPLC_L
LabSampleId :
I.BLK