

Data File : H:\VOL1\HPLC\HPLC L\121113\HL003720.D Vial: 2
 Acq On : 13-Nov-2012, 12:07 Operator: HLM
 Sample : 8330-CCV Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Nov 14 13:24 2012 Quant Results File: HL102412.RES

Instrument :
 HPLC_L
 LabSampleId :
 8330-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL102412.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Wed Nov 14 13:24:43 2012
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.31	3965966	992.566 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 330.86%#

Target Compounds

2) T	HMX	0.89	4241218	1046.969 ug/L
3) T	RDX	1.69	5849530	1086.793 ug/L
4) T	1,3,5-Trinitrobenzene	2.62	6135739	517.203 ug/L
5) T	Tetryl	5.79	8735093	1025.779 ug/L
6) T	2,4,6-Trinitrotoluene	6.20	5806763	509.600 ug/L
7) T	2-Amino-4,6-dinitrotoluene	6.61	5773624	532.537 ug/L
8) T	4-Amino-2,6-dinitrotoluene	6.89	3855482	534.289 ug/L
9) T	2,4-Dinitrotoluene	7.73	8080250	506.026 ug/L
10) T	2,6-Dinitrotoluene	8.06	4386437	508.935 ug/L
11) T	1,3-Dinitrobenzene	3.47	8688929	525.151 ug/L
12) T	Nitrobenzene	4.64	5424196	506.831 ug/L
13) T	2-Nitrotoluene	11.11	6853254	1011.829 ug/L
14) T	3-Nitrotoluene	13.01	7439524	1032.418 ug/L
15) T	4-Nitrotoluene	11.82	5903328	1015.095 ug/L
16) T	3,5-Dinitroaniline	3.77	16456263	1048.096 ug/L
17) T	Nitroglycerin	5.79f	8735093	151609.845 ug/L
18) T	PETN	17.63	23927689	2583.777 ug/L

Data File : H:\VOL1\HPLC\HPLC L\121113\HL003720.D

Vial: 2

Acq On : 13-Nov-2012, 12:07

Operator: HLM

Sample : 8330-CCV

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Nov 14 13:24 2012 Quant Results File: HL102412.RES

Instrument :

HPLC_L

LabSampleId :

8330-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL102412.M (Chemstation Integrator)

Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)

Last Update : Wed Nov 14 13:24:43 2012


Response via : Multiple Level Calibration


DataAcq Meth : 8330AGIP.M

Volume Inj. :

Signal Phase :

Signal Info :

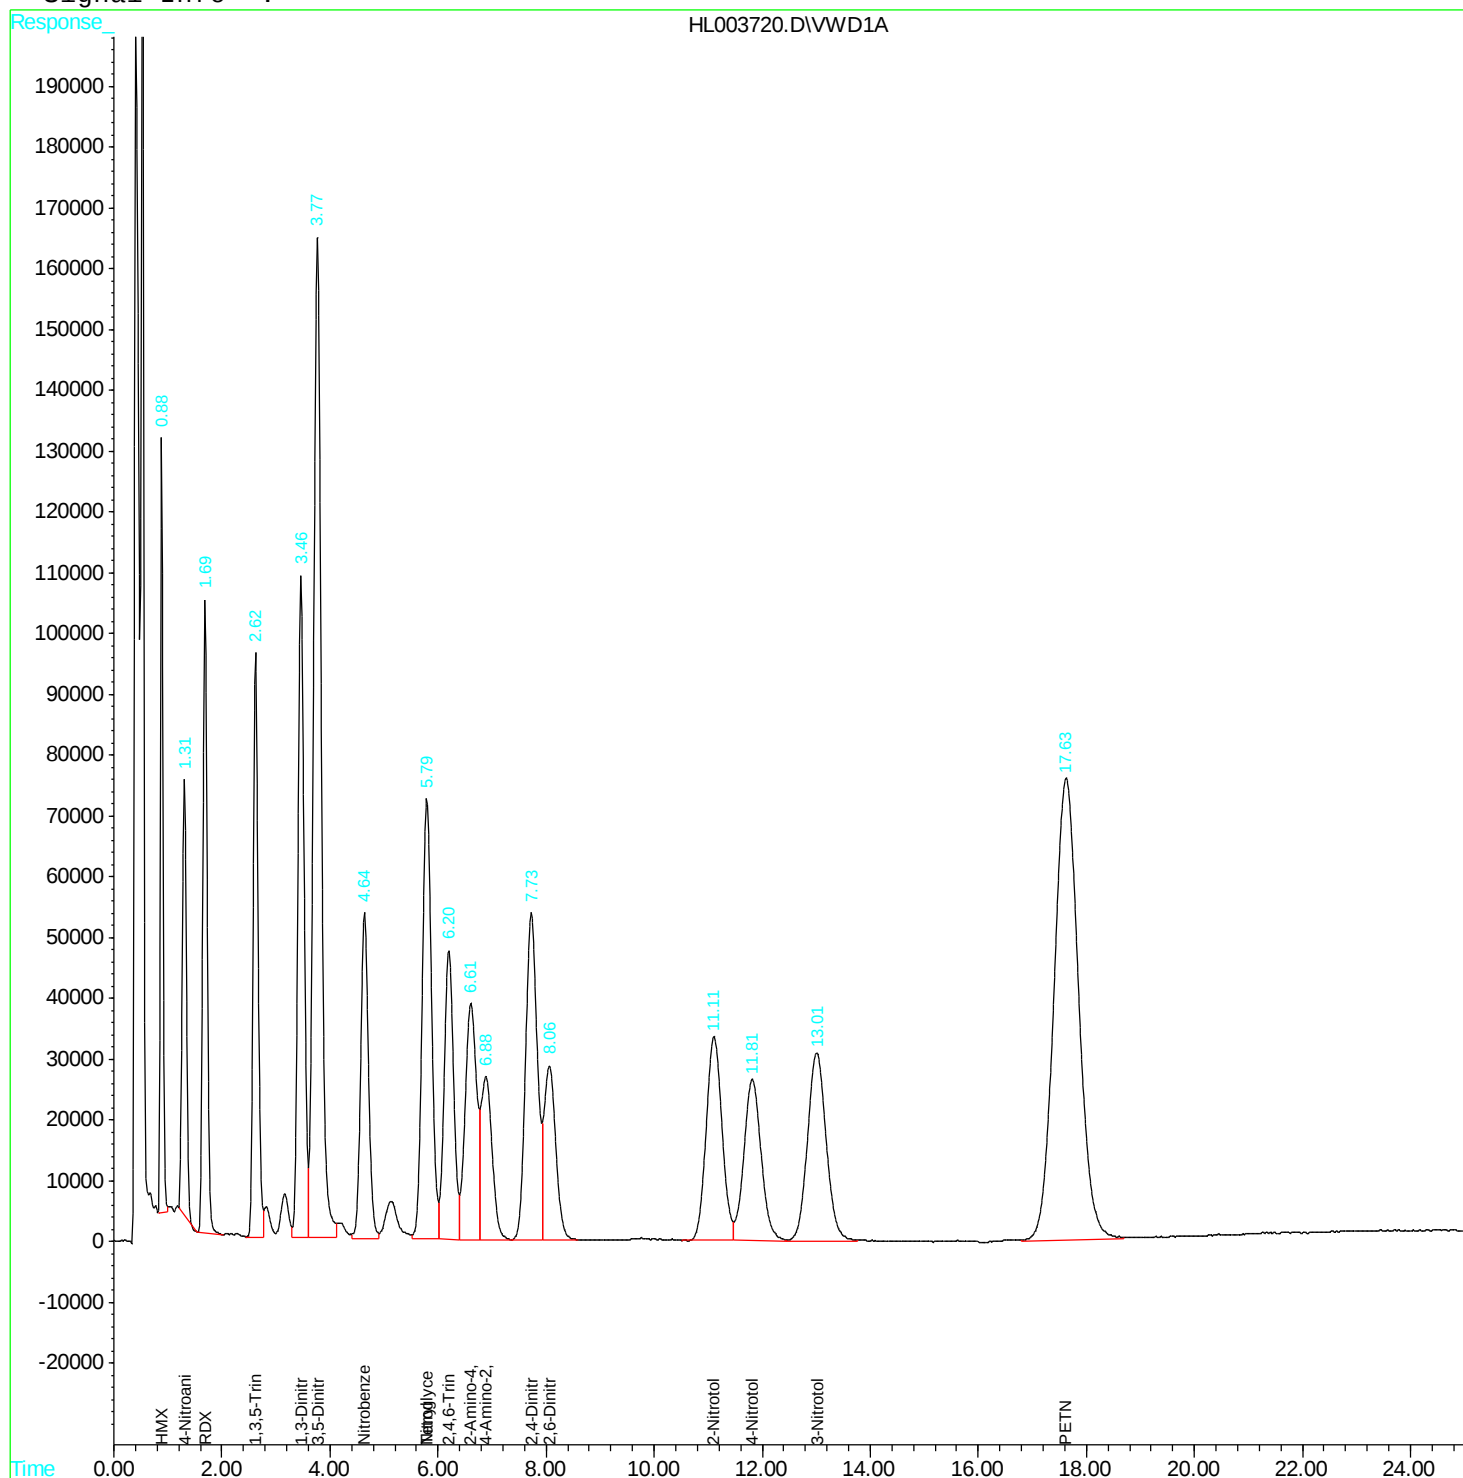


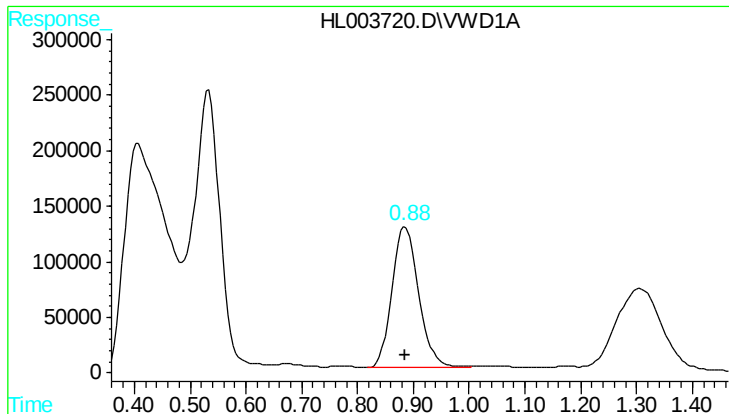

#2 HMX


R.T.: 0.886 min
Delta R.T.: 0.000 min
Response: 4241218
Conc: 1046.97 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

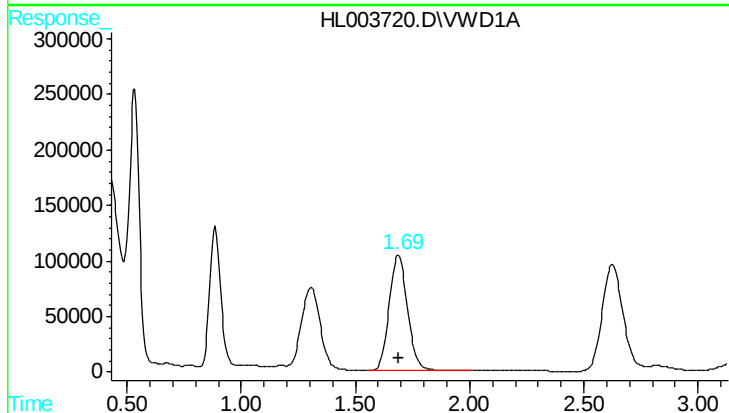


#3 RDX

R.T.: 1.688 min
Delta R.T.: 0.000 min
Response: 5849530
Conc: 1086.79 ug/L

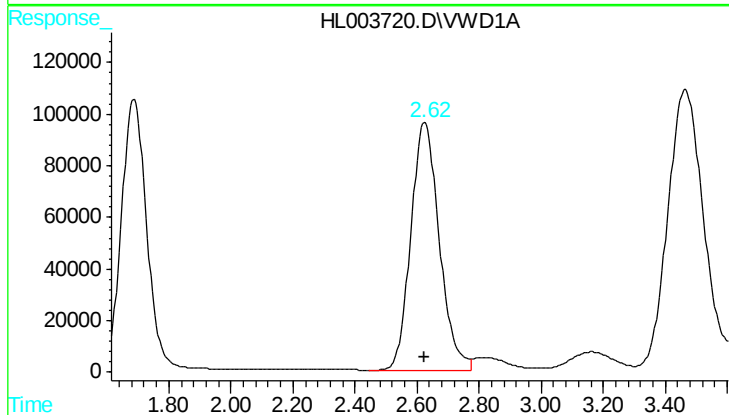


#4 1,3,5-Trinitrobenzene

R.T.: 2.625 min
Delta R.T.: 0.000 min
Response: 6135739
Conc: 517.20 ug/L

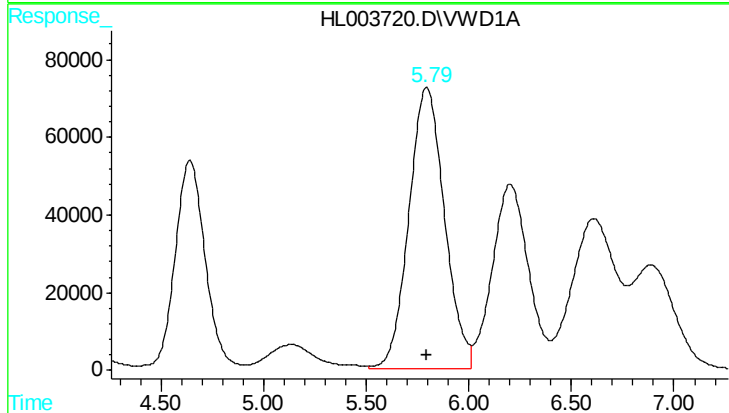

#5 Tetryl


R.T.: 5.794 min
Delta R.T.: 0.000 min
Response: 8735093
Conc: 1025.78 ug/L

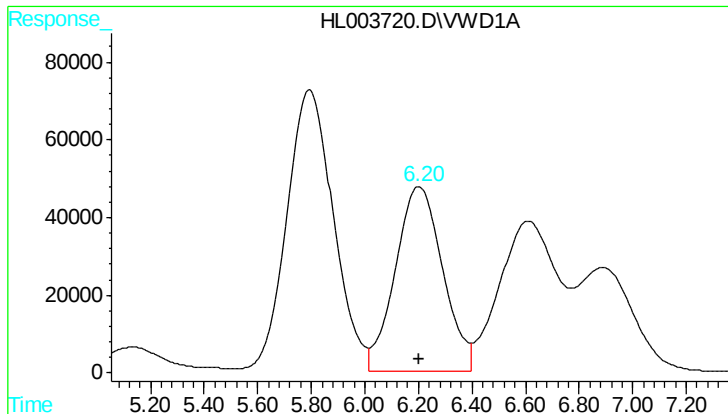

#6 2,4,6-Trinitrotoluene


R.T.: 6.202 min
Delta R.T.: 0.000 min
Response: 5806763
Conc: 509.60 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

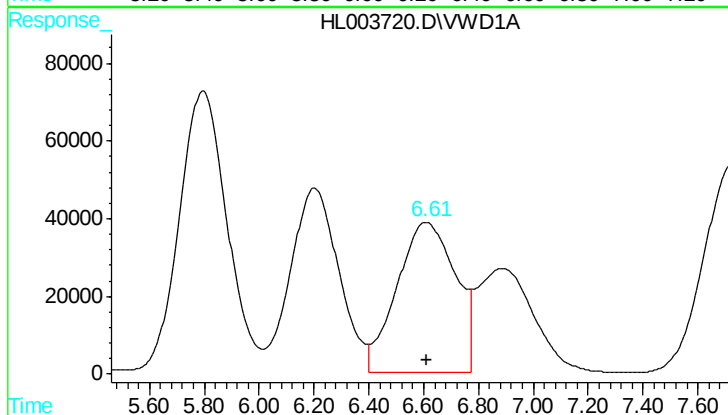


#7 2-Amino-4,6-dinitrotoluene

R.T.: 6.610 min
Delta R.T.: 0.000 min
Response: 5773624
Conc: 532.54 ug/L

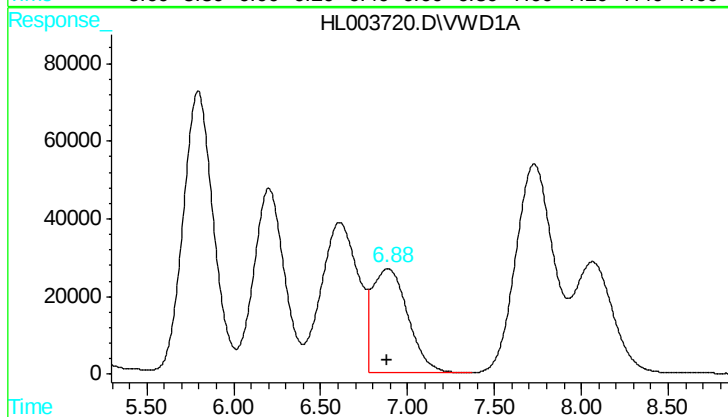


#8 4-Amino-2,6-dinitrotoluene

R.T.: 6.886 min
Delta R.T.: 0.000 min
Response: 3855482
Conc: 534.29 ug/L

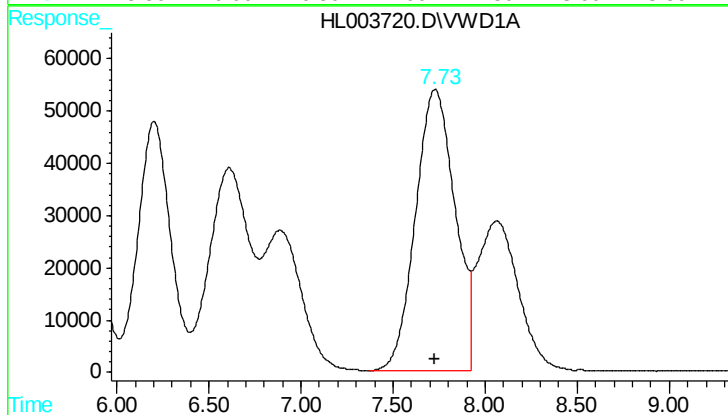

#9 2,4-Dinitrotoluene


R.T.: 7.728 min
Delta R.T.: 0.000 min
Response: 8080250
Conc: 506.03 ug/L

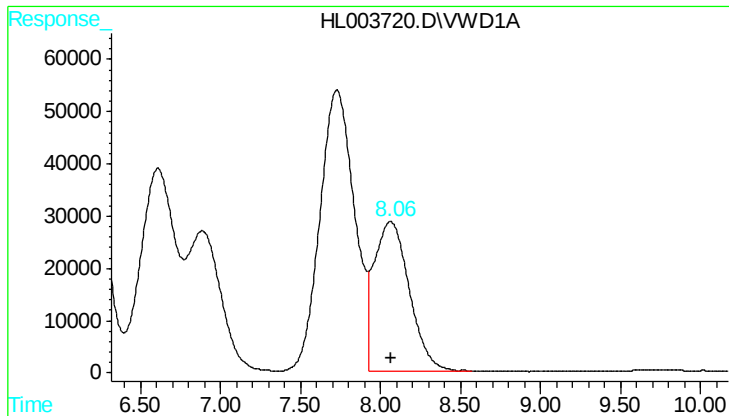

#10 2,6-Dinitrotoluene


R.T.: 8.064 min
Delta R.T.: 0.000 min
Response: 4386437
Conc: 508.94 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

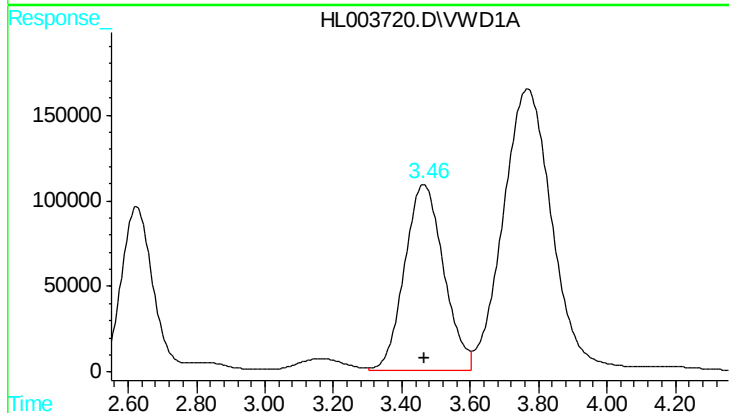


#11 1,3-Dinitrobenzene

R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 8688929
Conc: 525.15 ug/L

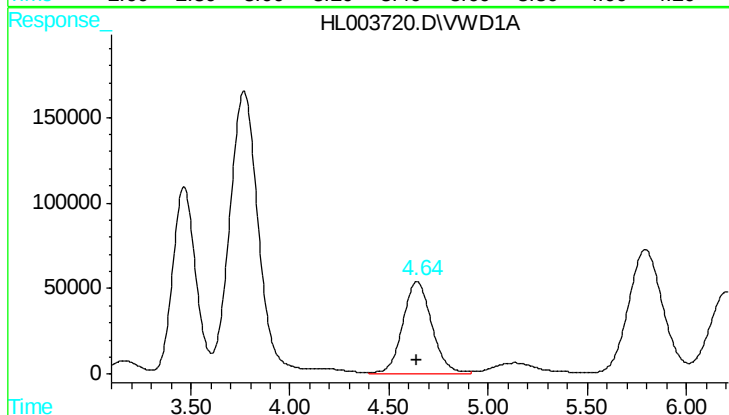


#12 Nitrobenzene

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 5424196
Conc: 506.83 ug/L

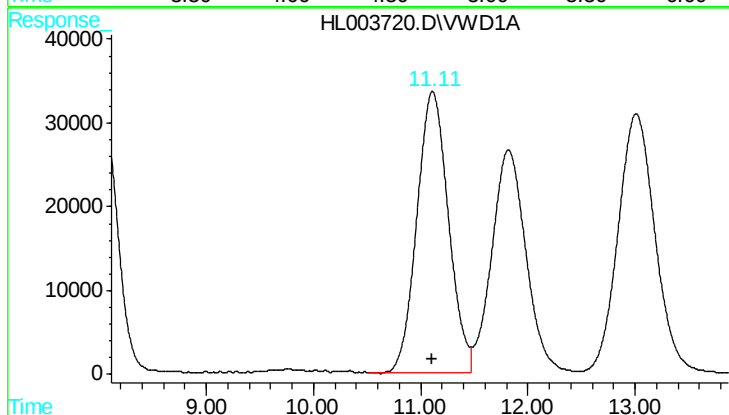

#13 2-Nitrotoluene


R.T.: 11.110 min
Delta R.T.: 0.000 min
Response: 6853254
Conc: 1011.83 ug/L

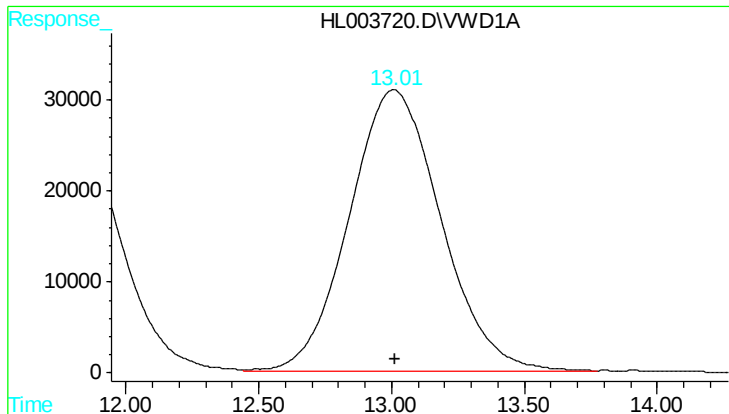

#14 3-Nitrotoluene


R.T.: 13.011 min
 Delta R.T.: 0.000 min
 Response: 7439524
 Conc: 1032.42 ug/L

Instrument :
 HPLC_L
 LabSampleId :
 8330-CCV

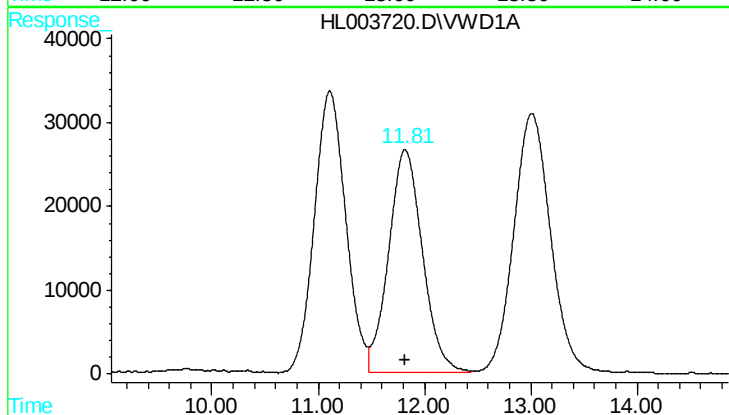


#15 4-Nitrotoluene

R.T.: 11.817 min
 Delta R.T.: 0.000 min
 Response: 5903328
 Conc: 1015.09 ug/L

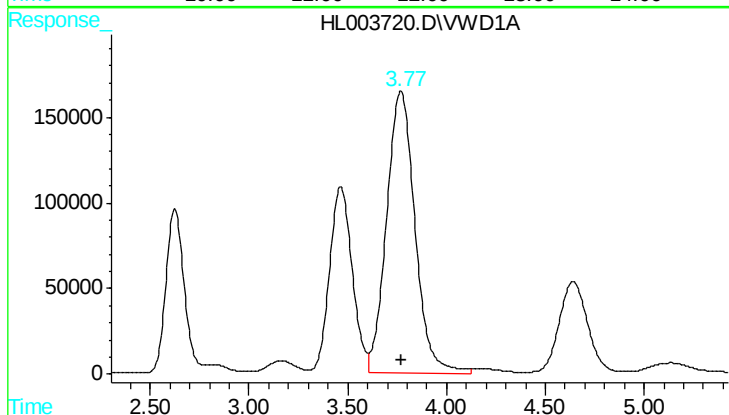


#16 3,5-Dinitroaniline

R.T.: 3.769 min
 Delta R.T.: 0.000 min
 Response: 16456263
 Conc: 1048.10 ug/L

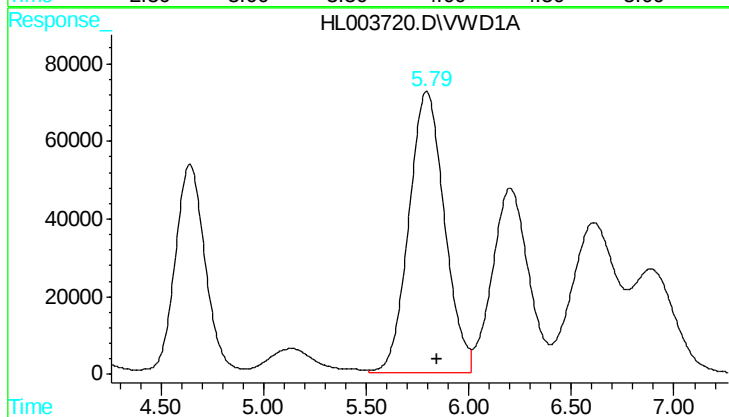

#17 Nitroglycerin

R.T.: 5.794 min
 Delta R.T.: -0.049 min
 Response: 8735093
 Conc: 151609.84 ug/L

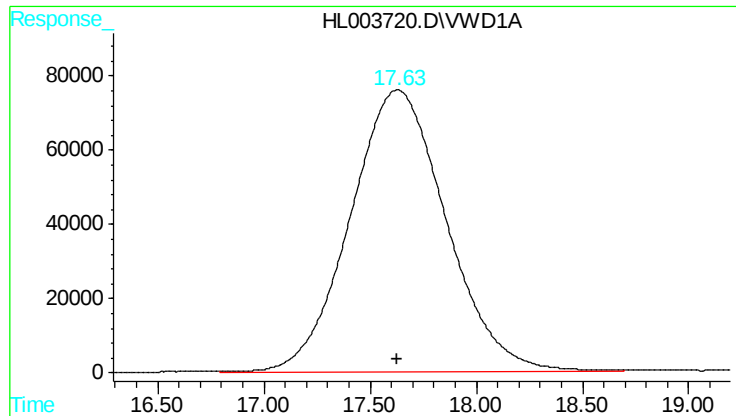

#18 PETN

R.T.: 17.628 min
Delta R.T.: 0.000 min
Response: 23927689
Conc: 2583.78 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV