

Data File : H:\VOL1\HPLC\HPLC L\121113\HL003721.D Vial: 3
Acq On : 13-Nov-2012, 12:34 Operator: HLM
Sample : 8330NG-CCV Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Nov 14 13:25 2012 Quant Results File: HL102412.RES

Instrument :
HPLC_L
LabSampleId :
8330NG-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL102412.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Wed Nov 14 13:24:43 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

5) T	Tetryl	5.84f	614155	72.121 ug/L
16) T	3,5-Dinitroaniline	3.81f	118249	7.531 ug/L
17) T	Nitroglycerin	5.84	614155	10659.521 ug/L

Data File : H:\VOL1\HPLC\HPLC L\121113\HL003721.D

Vial: 3

Acq On : 13-Nov-2012, 12:34

Operator: HLM

Sample : 8330NG-CCV

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Nov 14 13:25 2012 Quant Results File: HL102412.RES

Instrument :

HPLC_L

LabSampleId :

8330NG-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL102412.M (Chemstation Integrator)

Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)

Last Update : Wed Nov 14 13:24:43 2012


Response via : Multiple Level Calibration


DataAcq Meth : 8330AGIP.M

Volume Inj. :

Signal Phase :

Signal Info :

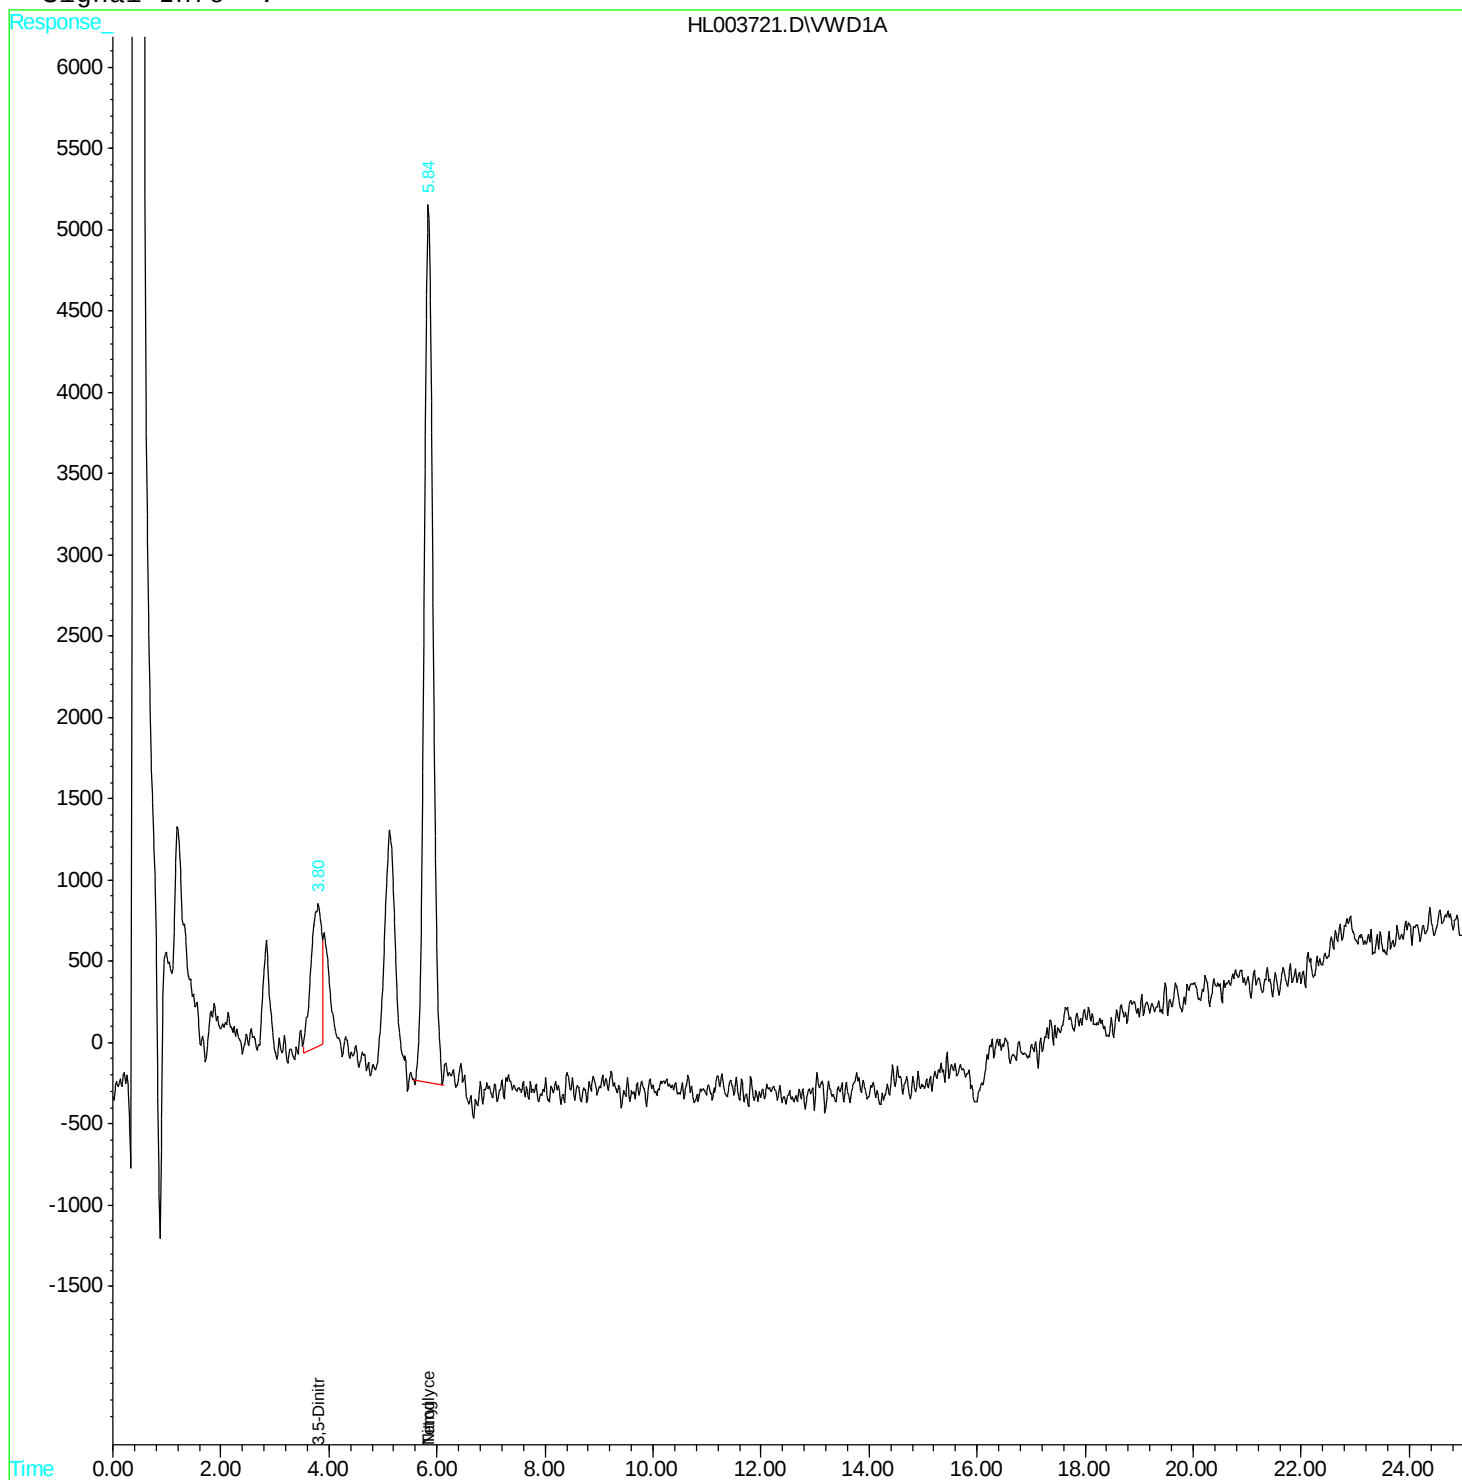


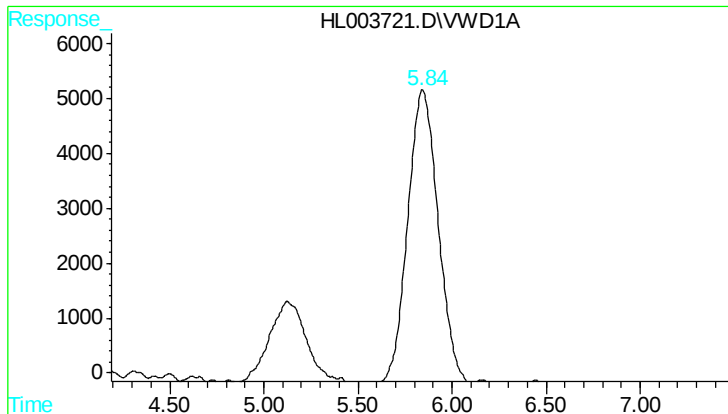

#5 Tetryl


R.T.: 5.843 min
 Delta R.T.: 0.049 min
 Response: 614155
 Conc: 72.12 ug/L

Instrument :
 HPLC_L
 LabSampleId :
 8330NG-CCV

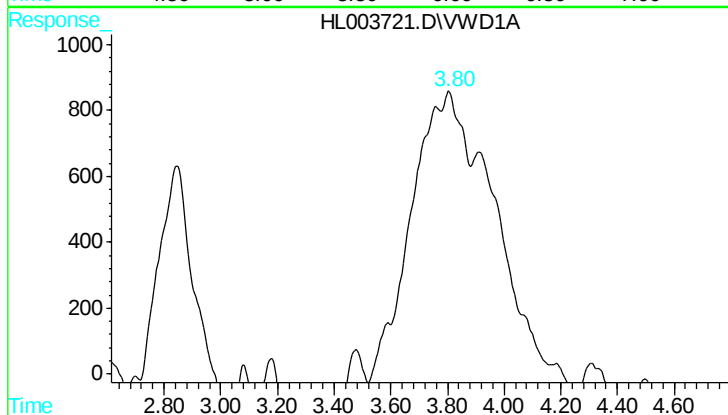

#16 3,5-Dinitroaniline

R.T.: 3.807 min
 Delta R.T.: 0.038 min
 Response: 118249
 Conc: 7.53 ug/L

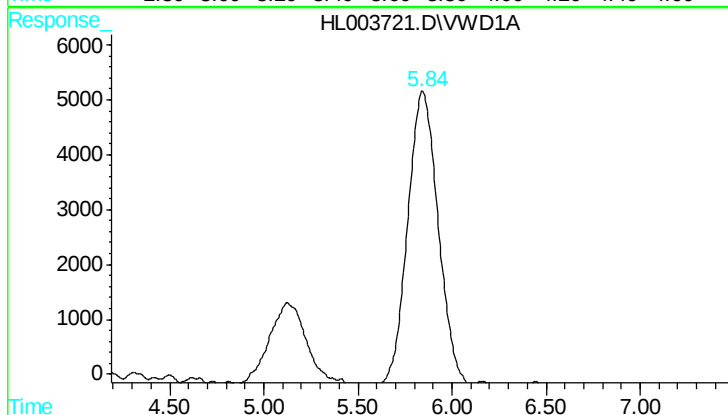

#17 Nitroglycerin

R.T.: 5.843 min
 Delta R.T.: 0.000 min
 Response: 614155
 Conc: 10659.52 ug/L