

Data File : H:\VOL1\HPLC\HPLC L\121113\HL003723.D Vial: 12
 Acq On : 13-Nov-2012, 13:28 Operator: HLM
 Sample : D4671-03DL 2X Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Nov 14 13:25 2012 Quant Results File: HL102412.RES

Instrument :
 HPLC_L
 ClientSampleId :
 871DL

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL102412.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Wed Nov 14 13:24:43 2012
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.30	777367	164.493 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 54.83%

Target Compounds

3) T	RDX	1.68	1124569	208.935 ug/L
4) T	1,3,5-Trinitrobenzene	2.62	4514228	380.520 ug/L
6) T	2,4,6-Trinitrotoluene	6.19	3628351	318.423 ug/L
7) T	2-Amino-4,6-dinitrotoluene	6.60	8476953	781.882 ug/L
8) T	4-Amino-2,6-dinitrotoluene	6.86	4845757	671.520 ug/L
9) T	2,4-Dinitrotoluene	7.71	26949635	1687.722 ug/L
10) T	2,6-Dinitrotoluene	8.03	6961972	807.761 ug/L
11) T	1,3-Dinitrobenzene	3.44f	59823	3.616 ug/L
12) T	Nitrobenzene	4.63	3281191	306.591 ug/L
13) T	2-Nitrotoluene	11.08	8602370	1270.073 ug/L
14) T	3-Nitrotoluene	12.98	9727411	1349.919 ug/L
15) T	4-Nitrotoluene	11.79	7994012	1374.594 ug/L
18) T	PETN	17.49f	163820	17.690 ug/L

Data File : H:\VOL1\HPLC\HPLC L\121113\HL003723.D

Vial: 12

Acq On : 13-Nov-2012, 13:28

Operator: HLM

Sample : D4671-03DL 2X

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Nov 14 13:25 2012 Quant Results File: HL102412.RES

Instrument :

HPLC_L

ClientSampleId :

871DL

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL102412.M (Chemstation Integrator)

Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)

Last Update : Wed Nov 14 13:24:43 2012


Response via : Multiple Level Calibration


DataAcq Meth : 8330AGIP.M

Volume Inj. :

Signal Phase :

Signal Info :

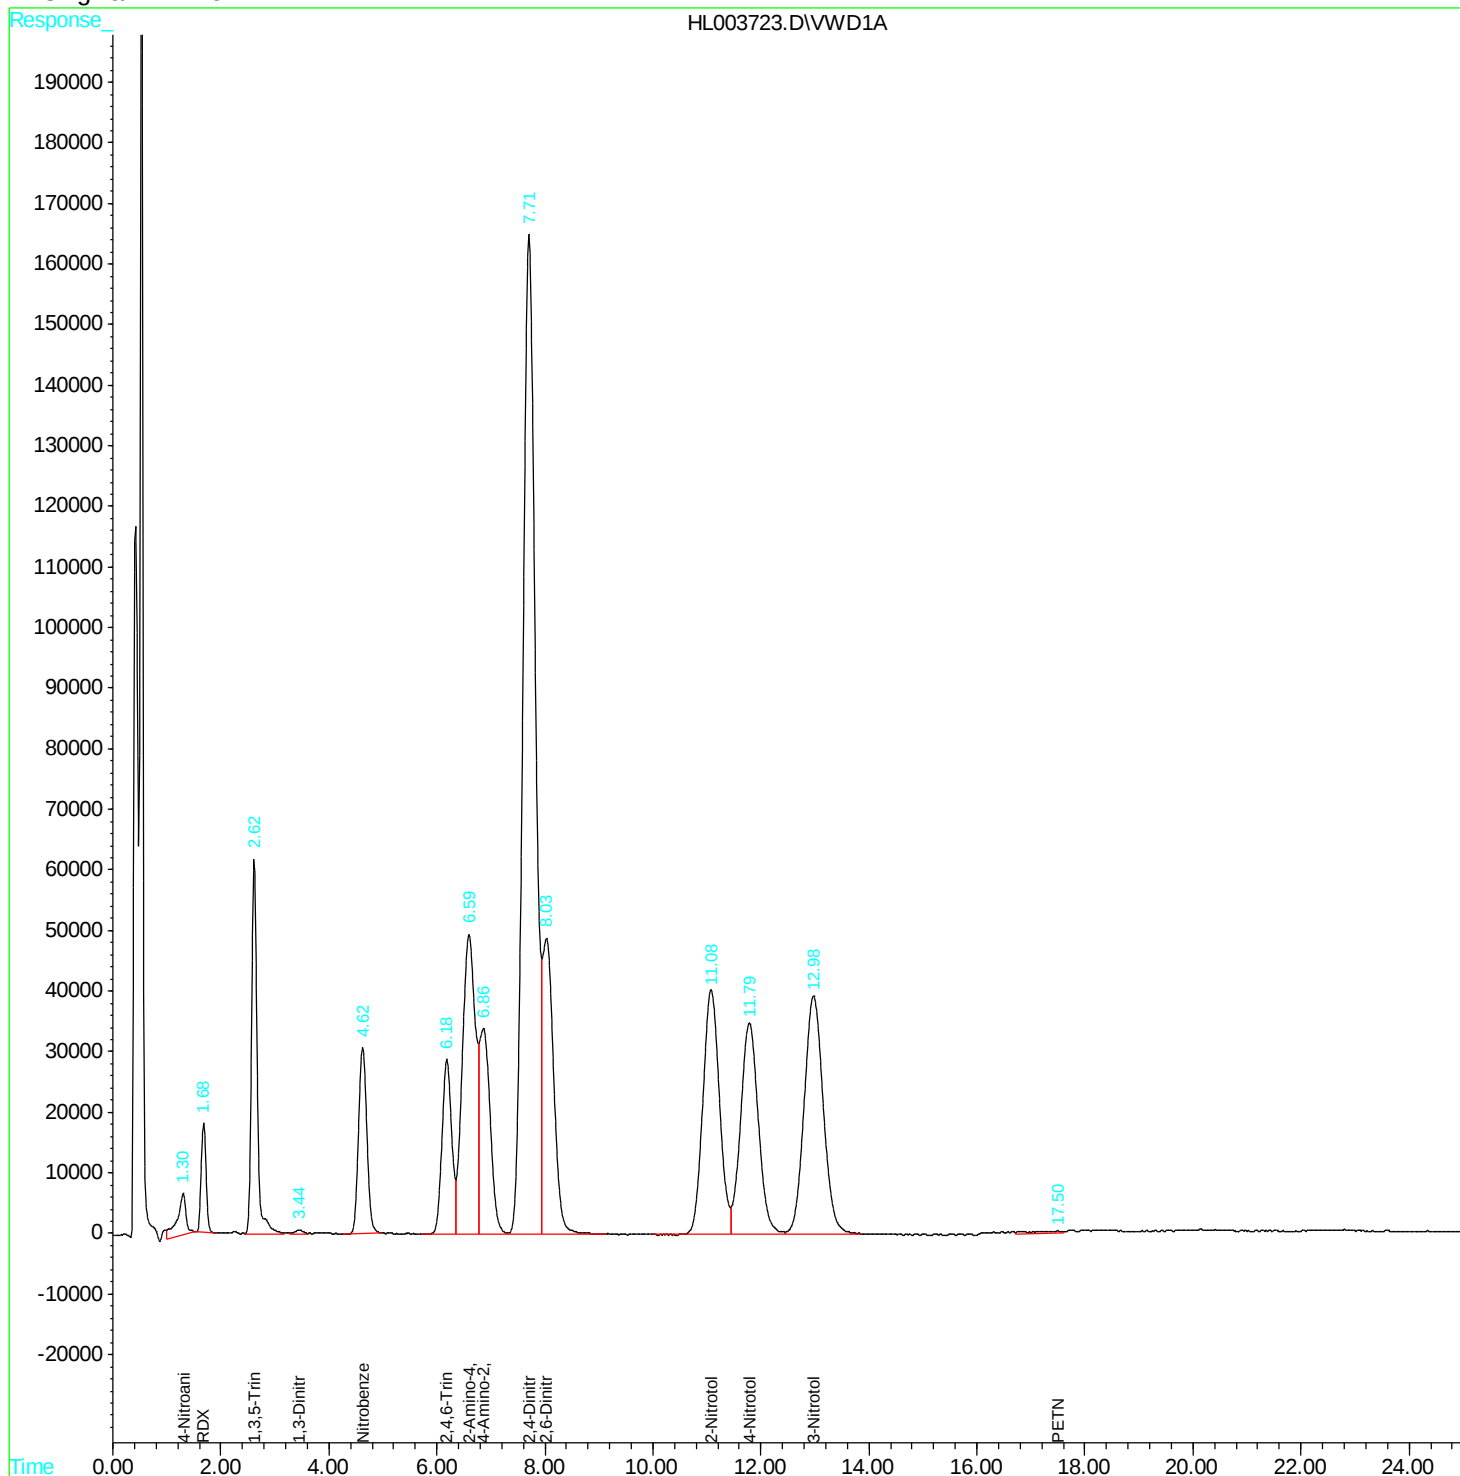


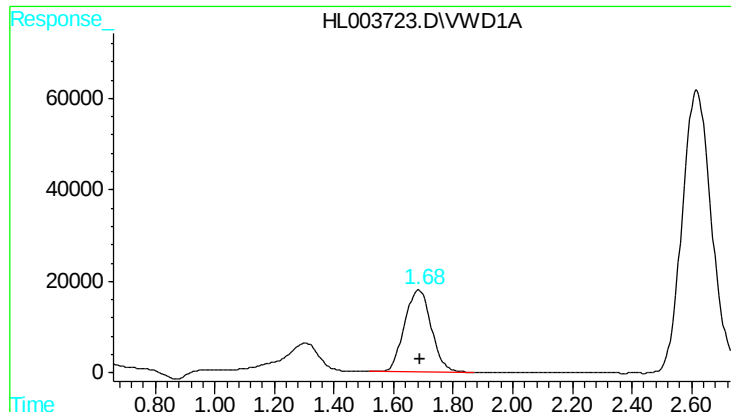

#3 RDX


R.T.: 1.685 min
Delta R.T.: -0.004 min
Response: 1124569
Conc: 208.94 ug/L

Instrument :
HPLC_L
ClientSampleId :
871DL

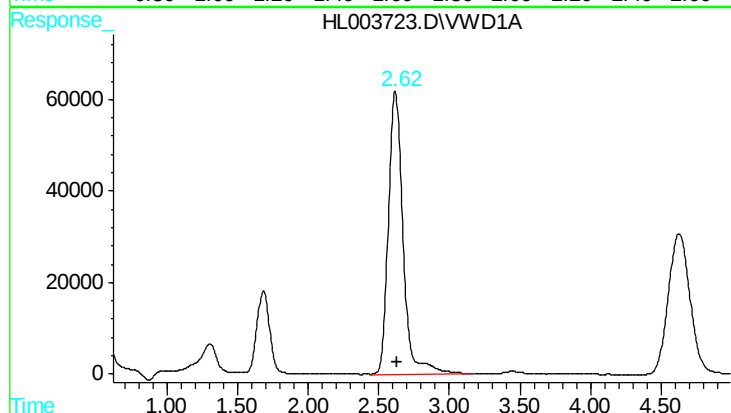


#4 1,3,5-Trinitrobenzene

R.T.: 2.618 min
Delta R.T.: -0.007 min
Response: 4514228
Conc: 380.52 ug/L

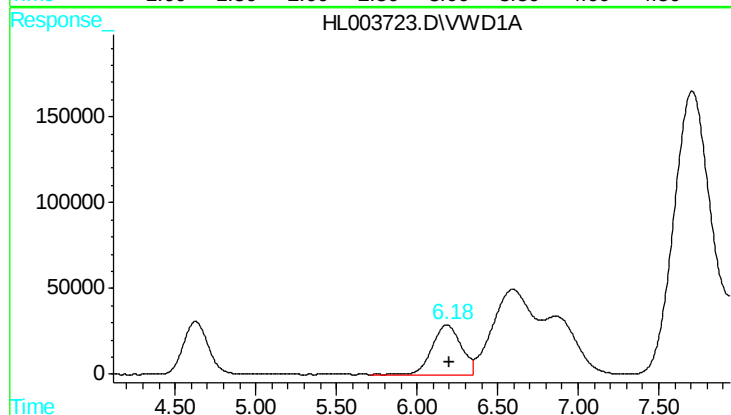


#6 2,4,6-Trinitrotoluene

R.T.: 6.185 min
Delta R.T.: -0.016 min
Response: 3628351
Conc: 318.42 ug/L

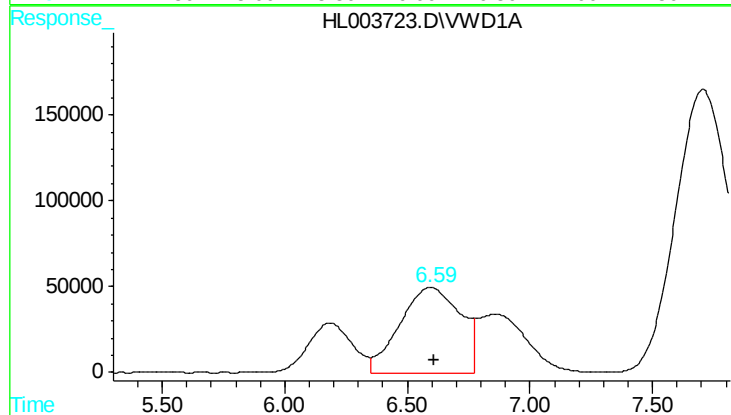

#7 2-Amino-4,6-dinitrotoluene


R.T.: 6.596 min
Delta R.T.: -0.014 min
Response: 8476953
Conc: 781.88 ug/L

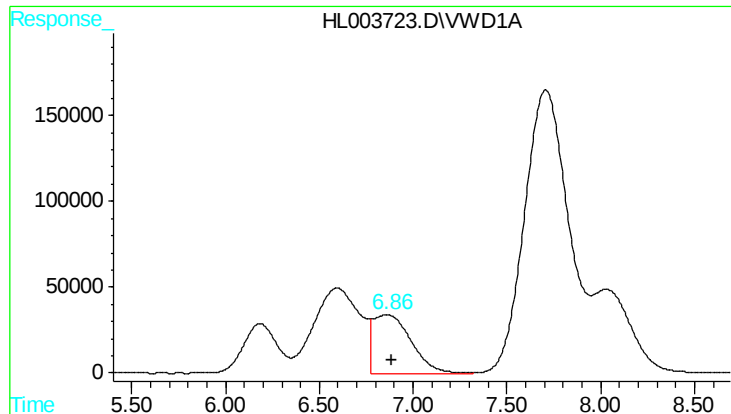

#8 4-Amino-2,6-dinitrotoluene


R.T.: 6.862 min
Delta R.T.: -0.024 min
Response: 4845757
Conc: 671.52 ug/L

Instrument :
HPLC_L
ClientSampleId :
871DL

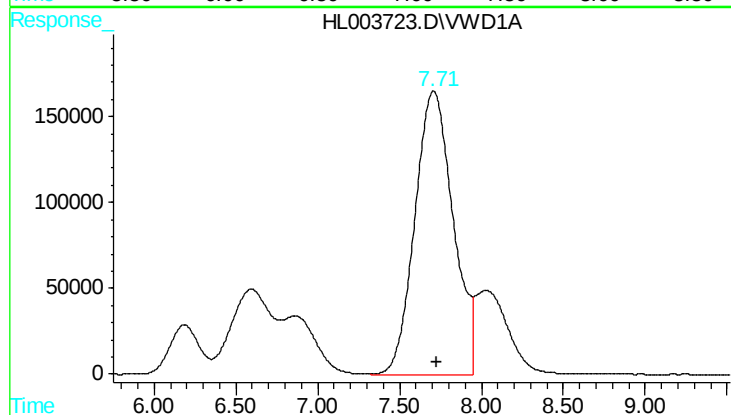


#9 2,4-Dinitrotoluene

R.T.: 7.707 min
Delta R.T.: -0.021 min
Response: 26949635
Conc: 1687.72 ug/L

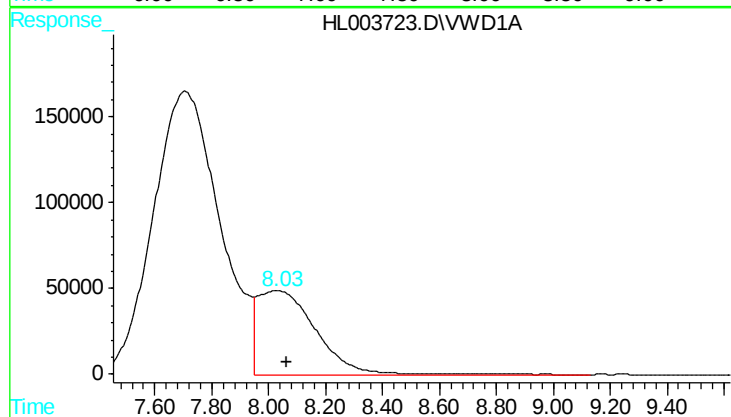


#10 2,6-Dinitrotoluene

R.T.: 8.029 min
Delta R.T.: -0.035 min
Response: 6961972
Conc: 807.76 ug/L

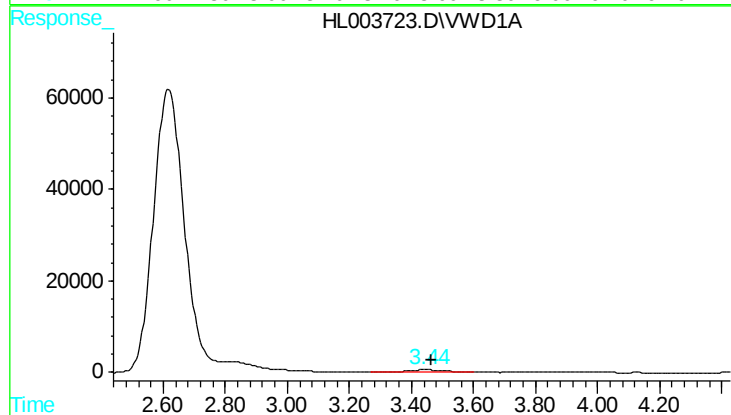

#11 1,3-Dinitrobenzene


R.T.: 3.443 min
Delta R.T.: -0.023 min
Response: 59823
Conc: 3.62 ug/L

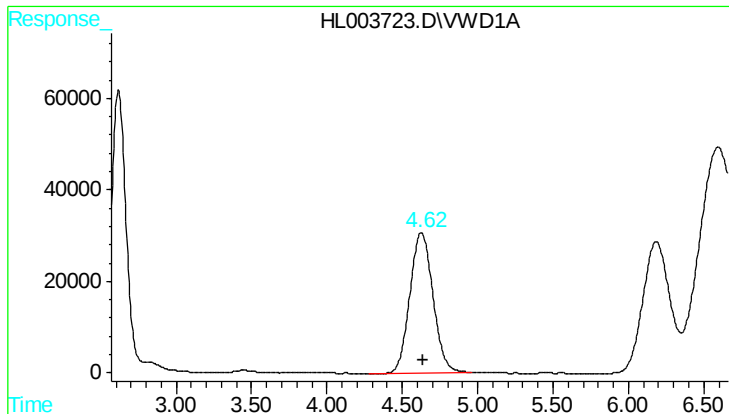

#12 Nitrobenzene


R.T.: 4.627 min
Delta R.T.: -0.014 min
Response: 3281191
Conc: 306.59 ug/L

Instrument :
HPLC_L
ClientSampleId :
871DL

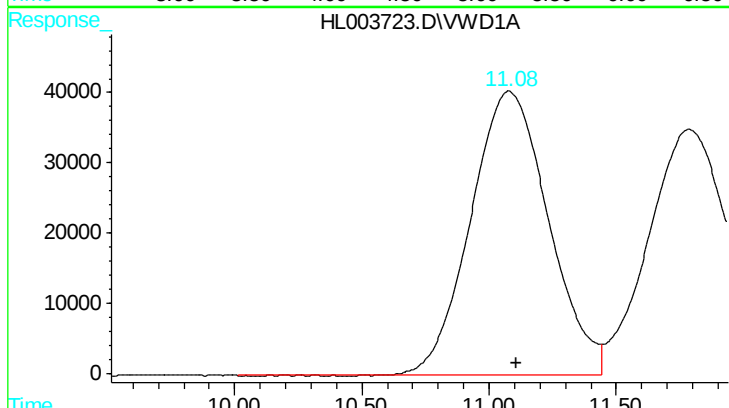


#13 2-Nitrotoluene

R.T.: 11.078 min
Delta R.T.: -0.031 min
Response: 8602370
Conc: 1270.07 ug/L

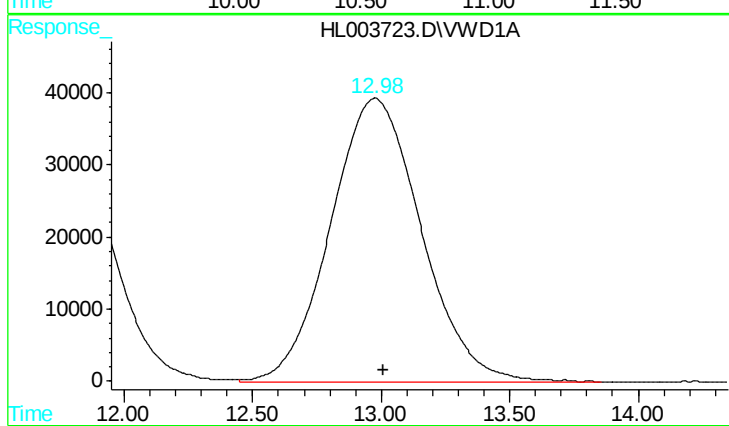


#14 3-Nitrotoluene

R.T.: 12.977 min
Delta R.T.: -0.034 min
Response: 9727411
Conc: 1349.92 ug/L

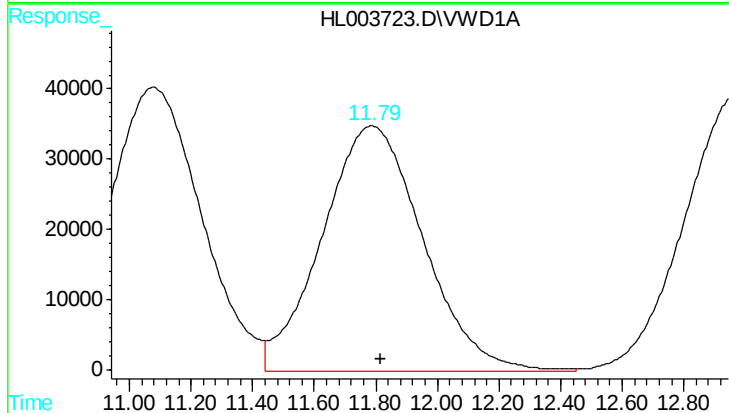

#15 4-Nitrotoluene

R.T.: 11.787 min
Delta R.T.: -0.030 min
Response: 7994012
Conc: 1374.59 ug/L

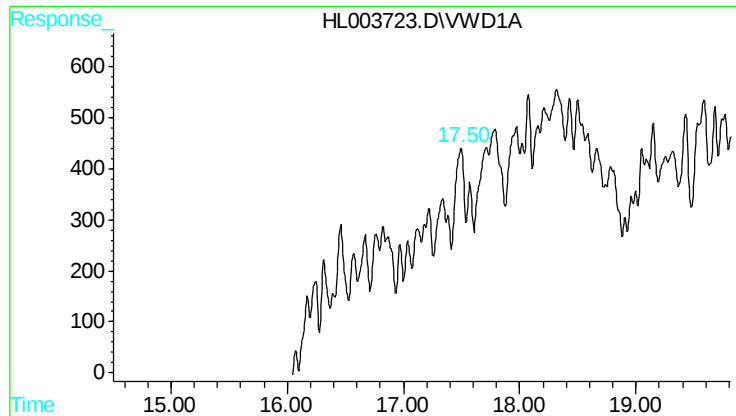

#18 PETN

R.T.: 17.489 min
Delta R.T.: -0.139 min
Response: 163820
Conc: 17.69 ug/L

Instrument :
HPLC_L
ClientSampleId :
871DL