

Data File : H:\VOL1\HPLC\HPLC L\121113\HL003729.D Vial: 23
Acq On : 13-Nov-2012, 16:10 Operator: HLM
Sample : PB66272BS2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Nov 14 13:25 2012 Quant Results File: HL102412.RES

Instrument :
HPLC_L
ClientSampleId :
PB66272BS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL102412.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Wed Nov 14 13:24:43 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.31	1577622	372.318 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 124.11%

Target Compounds

5) T	Tetrvl	5.84f	268956	31.584 ug/L
17) T	Nitroglycerin	5.84	268956	4668.113 ug/L

Data File : H:\VOL1\HPLC\HPLC L\121113\HL003729.D

Vial: 23

Acq On : 13-Nov-2012, 16:10

Operator: HLM

Sample : PB66272BS2

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Nov 14 13:25 2012 Quant Results File: HL102412.RES

Instrument :

HPLC_L

ClientSampleId :

PB66272BS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL102412.M (Chemstation Integrator)

Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)

Last Update : Wed Nov 14 13:24:43 2012


Response via : Multiple Level Calibration


DataAcq Meth : 8330AGIP.M

Volume Inj. :

Signal Phase :

Signal Info :

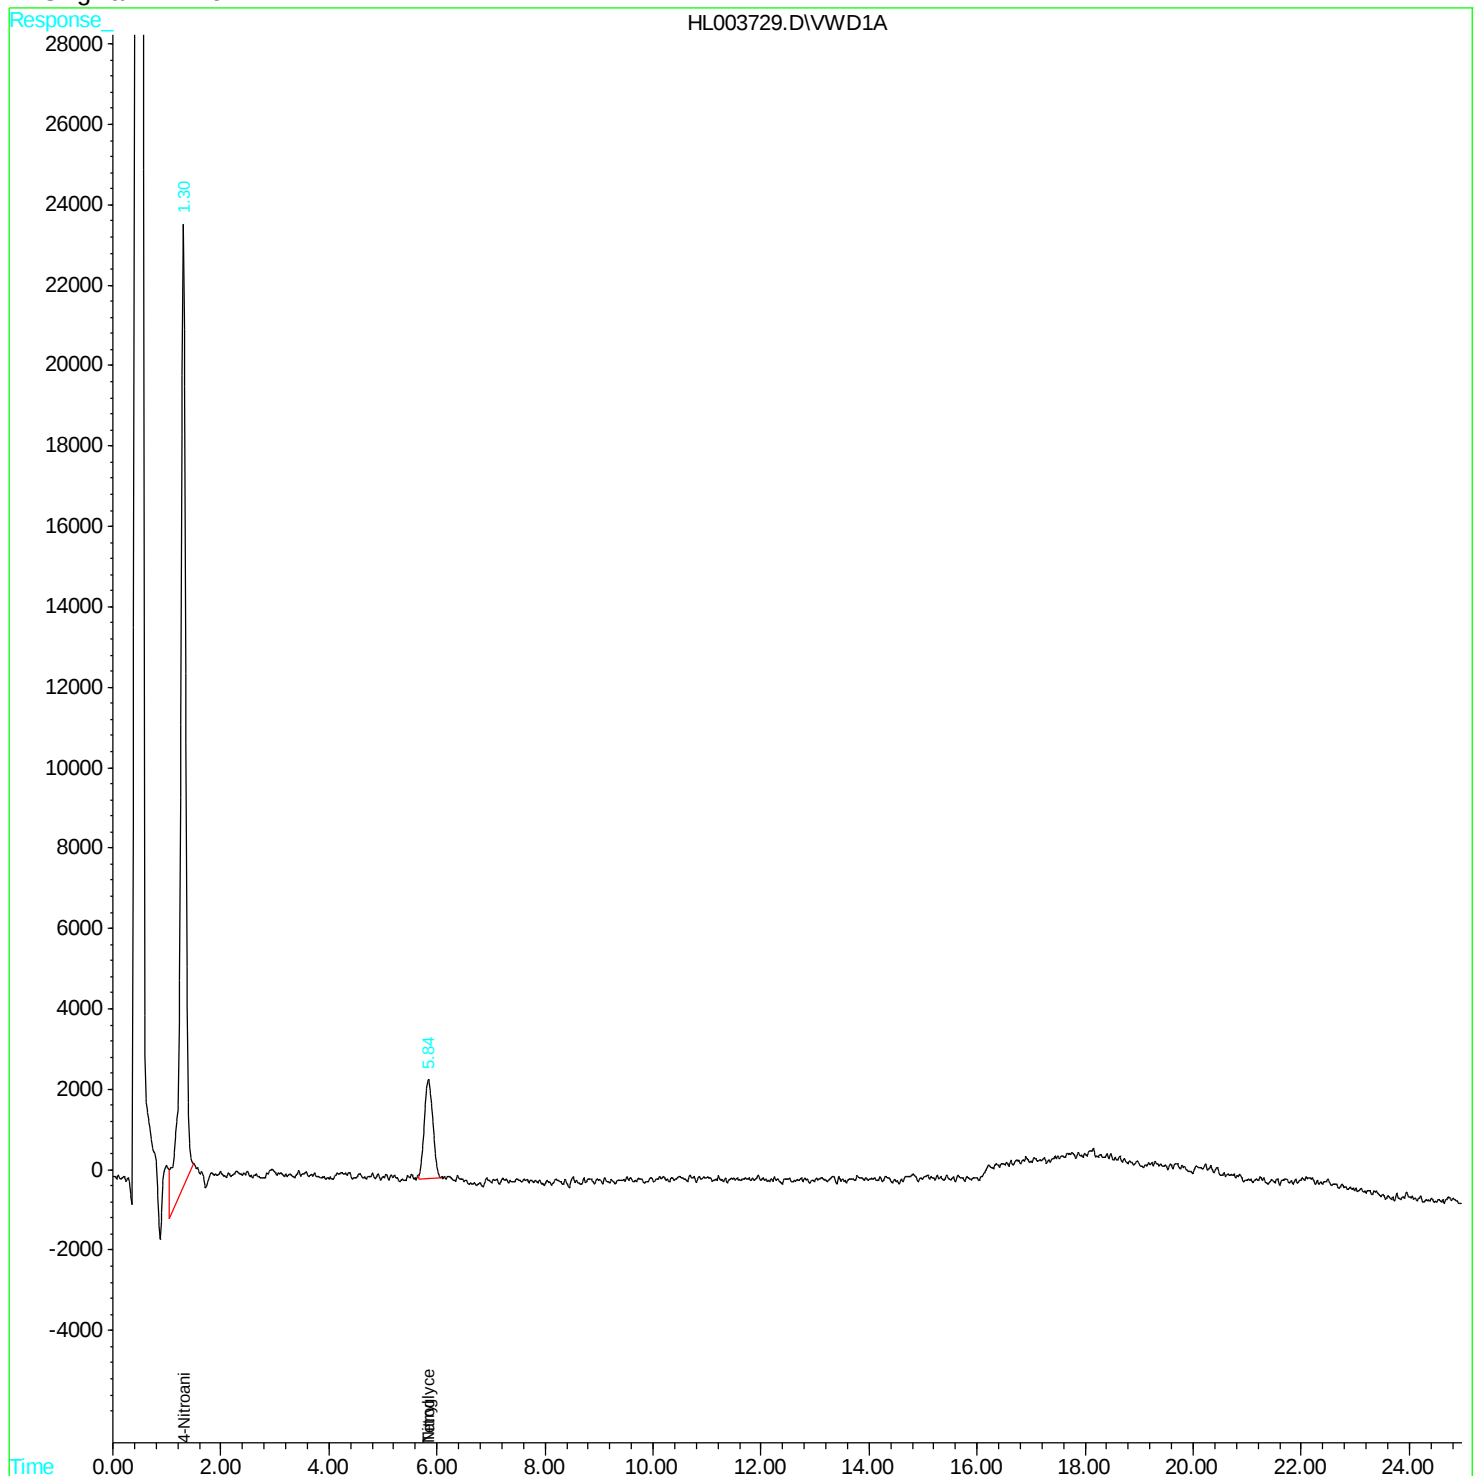


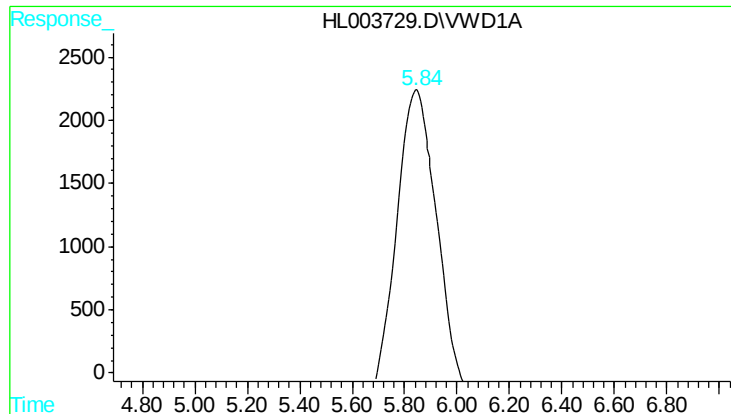

#5 Tetryl

R.T.: 5.844 min
Delta R.T.: 0.050 min
Response: 268956
Conc: 31.58 ug/L

Instrument :
HPLC_L
ClientSampleId :
PB66272BS2

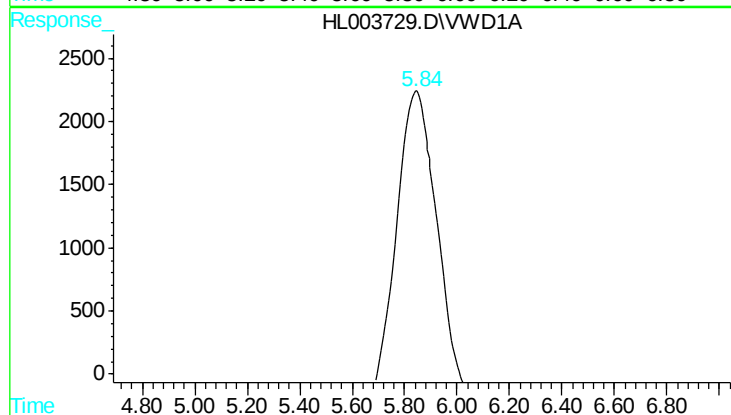

#17 Nitroglycerin

R.T.: 5.844 min
Delta R.T.: 0.000 min
Response: 268956
Conc: 4668.11 ug/L