

Data File : H:\VOL1\HPLC\HPLC L\121113\HL003733.D Vial: 27
Acq On : 13-Nov-2012, 17:57 Operator: HLM
Sample : D4468-08 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Nov 14 13:26 2012 Quant Results File: HL102412.RES

Instrument :
HPLC_L
ClientSampleId :
LOQ Water 2012-4-HPLC

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL102412.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Wed Nov 14 13:24:43 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.30	1625162	384.664 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 128.22%

Target Compounds


5) T	Tetryl	5.84f	113997	13.387 ug/L
17) T	Nitroglycerin	5.84	113997	1978.570 ug/L


Data File : H:\VOL1\HPLC\HPLC L\121113\HL003733.D Vial: 27
Acq On : 13-Nov-2012, 17:57 Operator: HLM
Sample : D4468-08 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Nov 14 13:26 2012 Quant Results File: HL102412.RES

Instrument :
HPLC_L
ClientSampleId :
LOQ Water 2012-4-HPLC

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL102412.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Wed Nov 14 13:24:43 2012
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

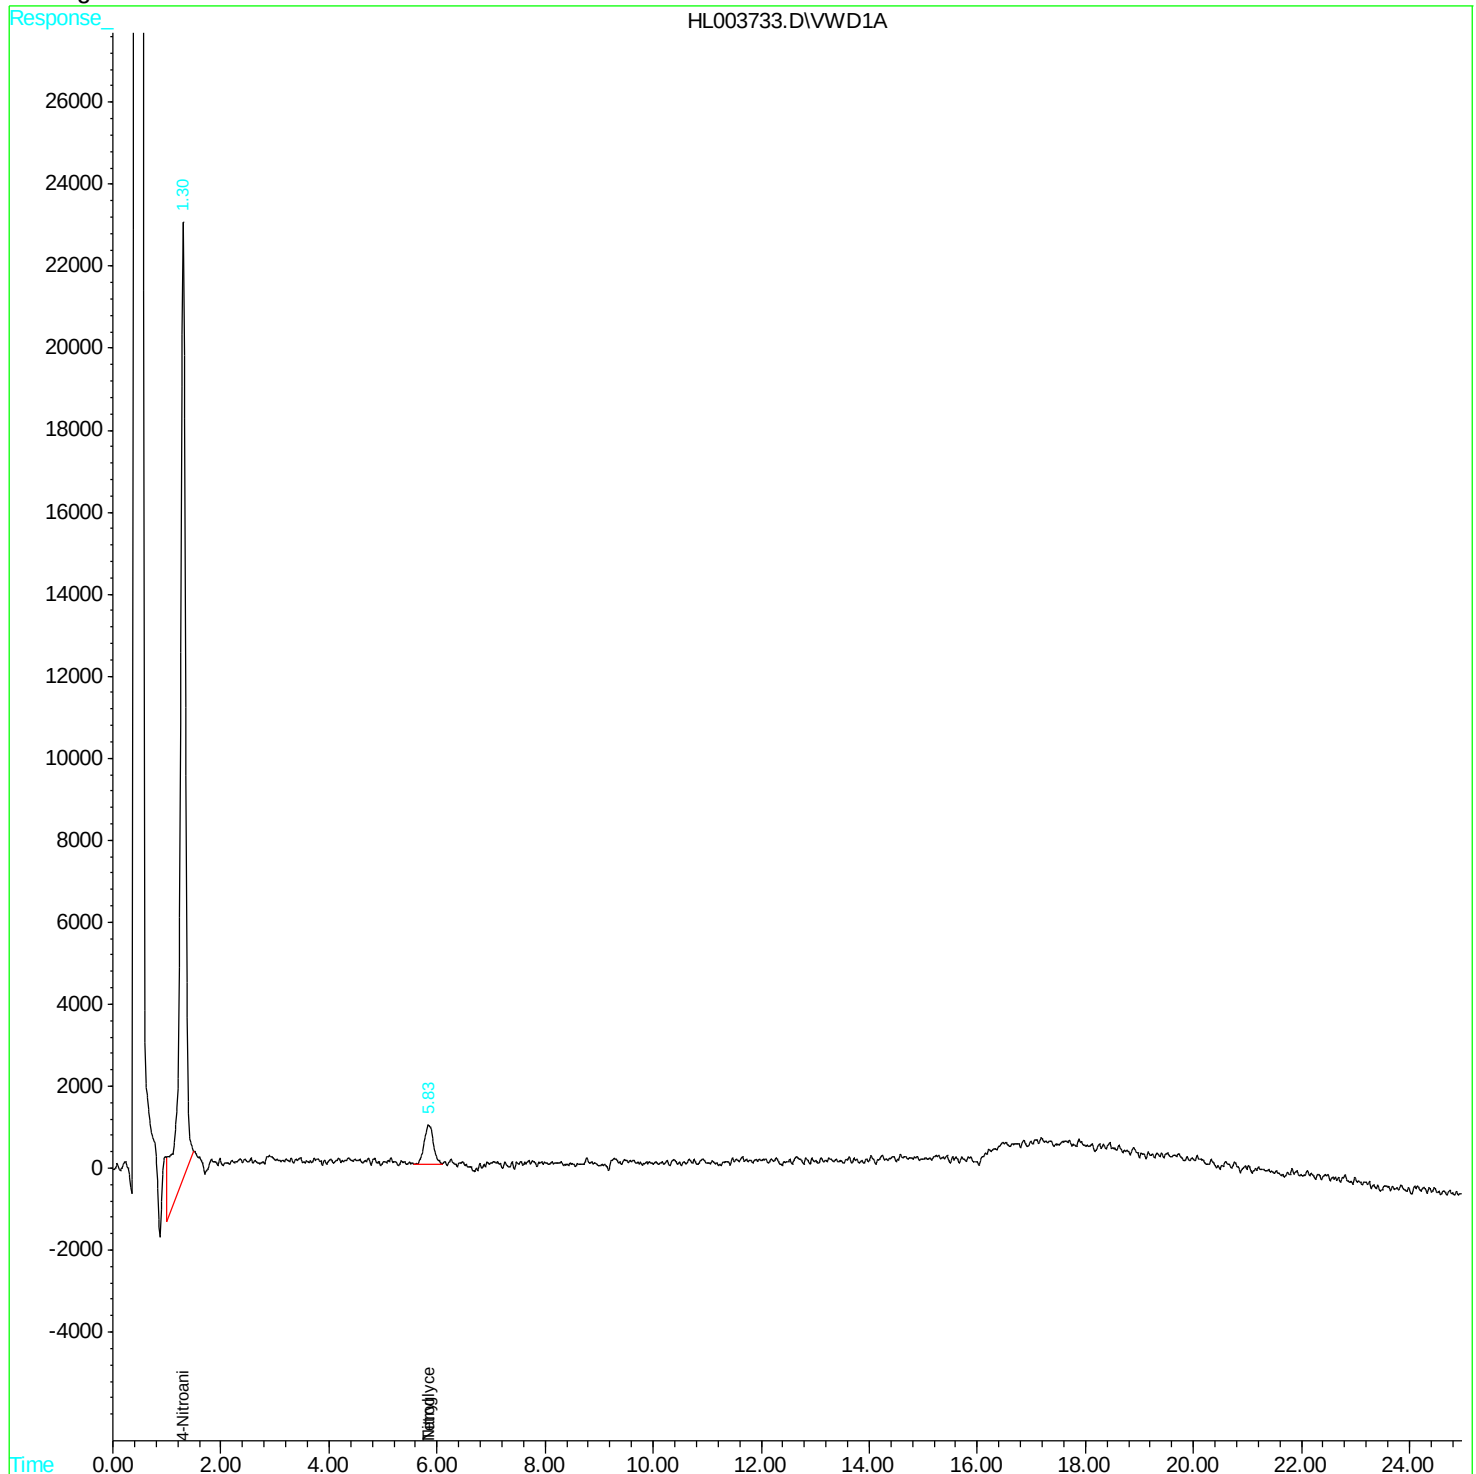


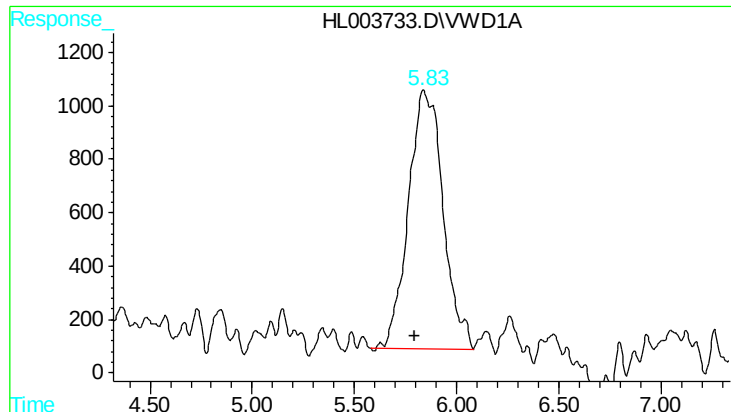

#5 Tetryl

R.T.: 5.837 min
Delta R.T.: 0.043 min
Response: 113997
Conc: 13.39 ug/L

Instrument :
HPLC_L
ClientSampleId :
LOQ Water 2012-4-HPLC

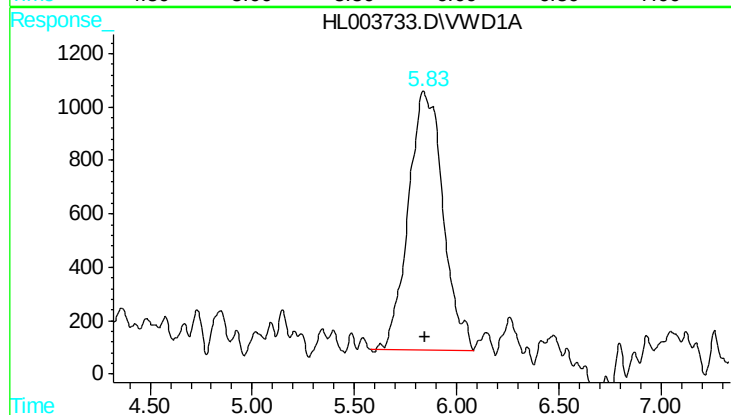

#17 Nitroglycerin

R.T.: 5.837 min
Delta R.T.: -0.006 min
Response: 113997
Conc: 1978.57 ug/L