

Data File : H:\VOL1\HPLC\HPLC L\121113\HL003734.D Vial: 1
Acq On : 13-Nov-2012, 18:24 Operator: HLM
Sample : I.BLK Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Nov 14 13:26 2012 Quant Results File: HL102412.RES

Instrument :
HPLC_L
ClientSampleId :
I.BLK

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL102412.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Wed Nov 14 13:24:43 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

16) T	3,5-Dinitroaniline	3.78	139572	8.889 ug/L
-------	--------------------	------	--------	------------


Quantitation Report


Data File : H:\VOL1\HPLC\HPLC L\121113\HL003734.D Vial: 1
 Acq On : 13-Nov-2012, 18:24 Operator: HLM
 Sample : I.BLK Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Nov 14 13:26 2012 Quant Results File: HL102412.RES

Instrument :
 HPLC_L
 ClientSampleId :
 I.BLK

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL102412.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Wed Nov 14 13:24:43 2012
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

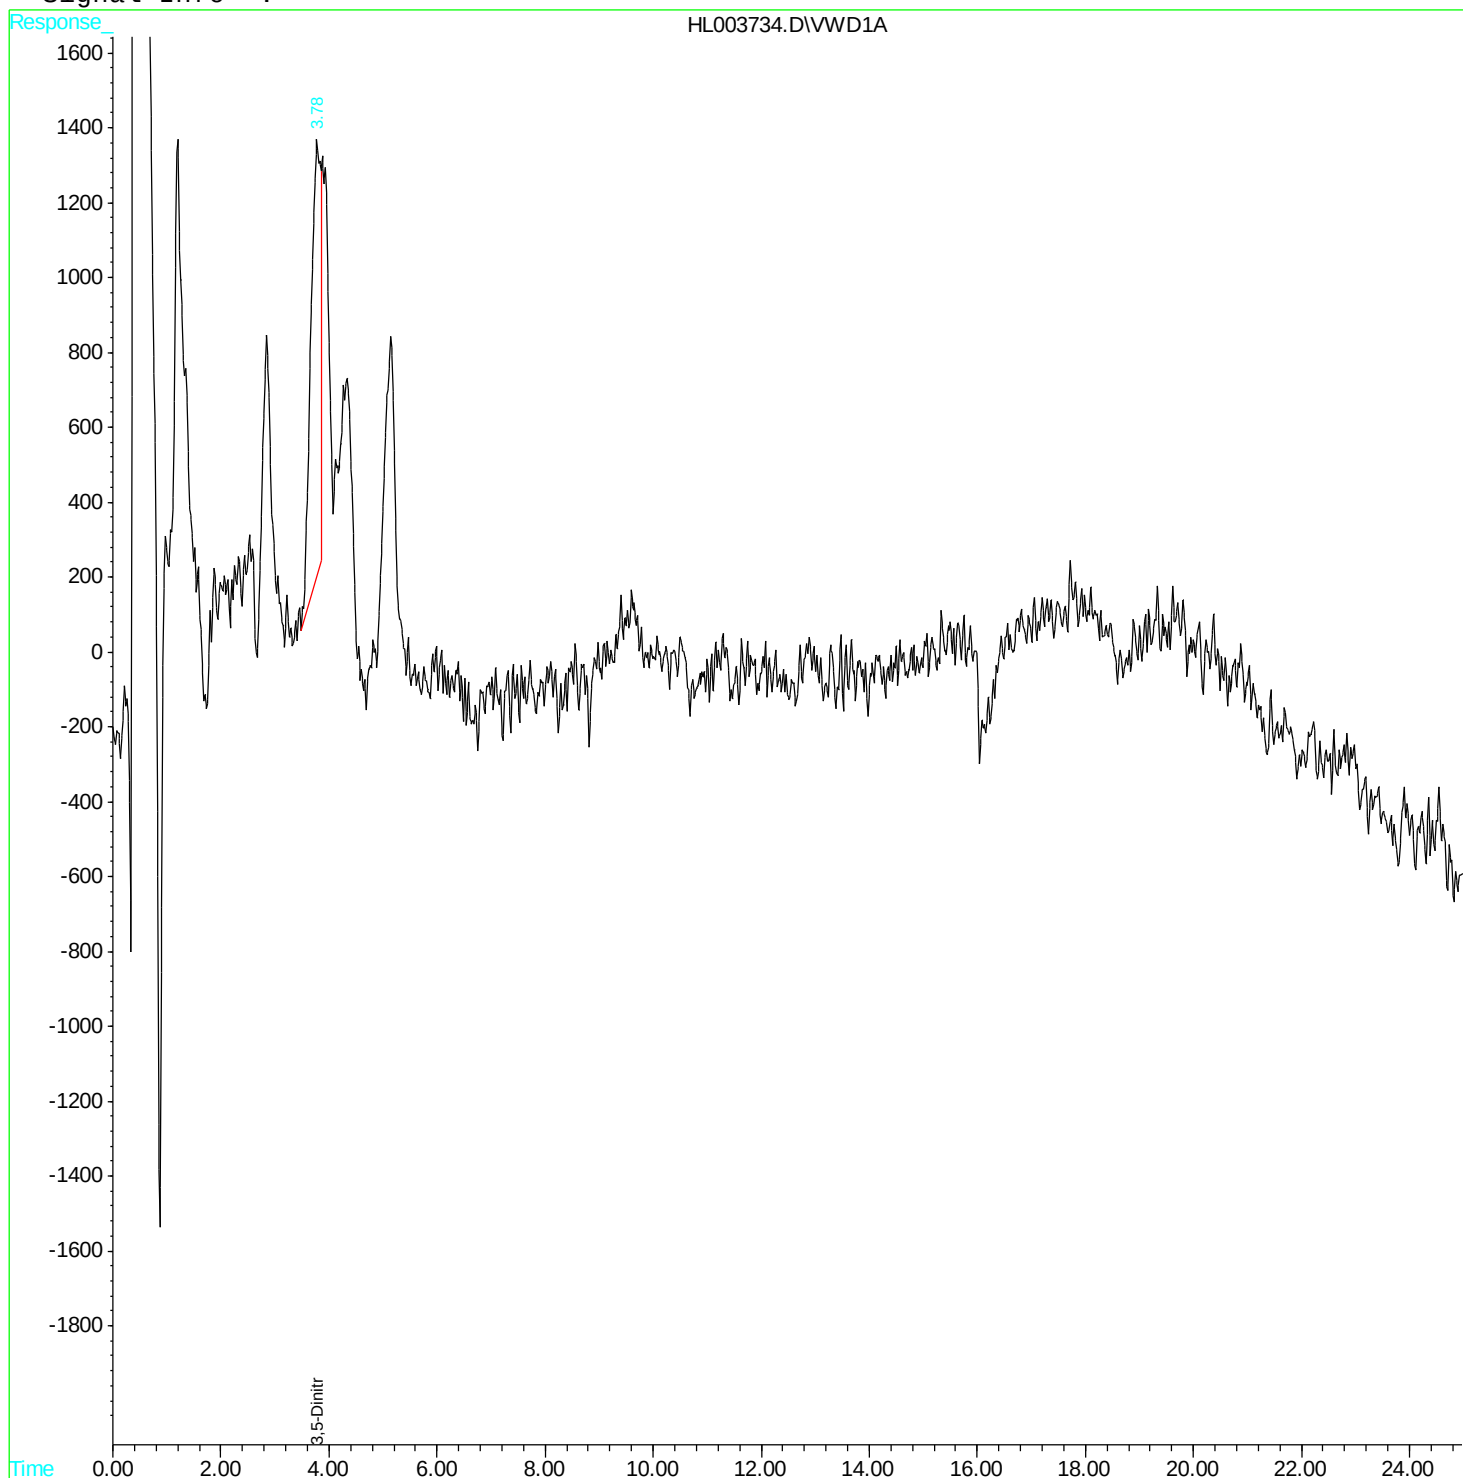

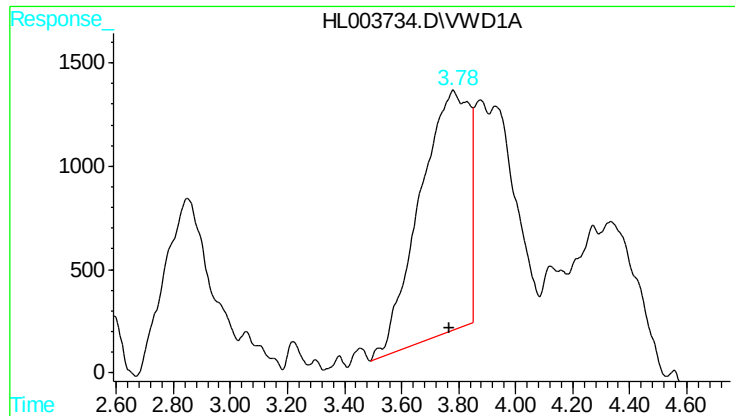

#16 3,5-Dinitroaniline

R.T.: 3.782 min
Delta R.T.: 0.013 min
Response: 139572
Conc: 8.89 ug/L

Instrument :
HPLC_L
ClientSampleId :
I.BLK