

Data File : H:\VOL1\HPLC\HPLC L\121113\HL003735.D Vial: 2
 Acq On : 13-Nov-2012, 18:52 Operator: HLM
 Sample : 8330-CCV Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Nov 14 13:26 2012 Quant Results File: HL102412.RES

Instrument :
 HPLC_L
 ClientSampleId :
 8330-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL102412.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Wed Nov 14 13:24:43 2012
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.31	3960561	991.162 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 330.39%#

Target Compounds

2) T	HMX	0.88	4237135	1045.969 ug/L
3) T	RDX	1.69	5851353	1087.131 ug/L
4) T	1,3,5-Trinitrobenzene	2.62	6132684	516.945 ug/L
5) T	Tetryl	5.79	8653891	1016.243 ug/L
6) T	2,4,6-Trinitrotoluene	6.20	5818596	510.638 ug/L
7) T	2-Amino-4,6-dinitrotoluene	6.61	5740866	529.516 ug/L
8) T	4-Amino-2,6-dinitrotoluene	6.89	3845392	532.890 ug/L
9) T	2,4-Dinitrotoluene	7.73	8083254	506.214 ug/L
10) T	2,6-Dinitrotoluene	8.06	4420723	512.913 ug/L
11) T	1,3-Dinitrobenzene	3.46	8698271	525.715 ug/L
12) T	Nitrobenzene	4.64	5399650	504.537 ug/L
13) T	2-Nitrotoluene	11.11	6830597	1008.484 ug/L
14) T	3-Nitrotoluene	13.01	7390392	1025.600 ug/L
15) T	4-Nitrotoluene	11.82	5897809	1014.146 ug/L
16) T	3,5-Dinitroaniline	3.77	16499670	1050.860 ug/L
17) T	Nitroglycerin	5.79f	8653891	150200.481 ug/L
18) T	PETN	17.63	24068666	2599.000 ug/L

Data File : H:\VOL1\HPLC\HPLC L\121113\HL003735.D

Vial: 2

Acq On : 13-Nov-2012, 18:52

Operator: HLM

Sample : 8330-CCV

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Nov 14 13:26 2012 Quant Results File: HL102412.RES

Instrument :

HPLC_L

ClientSampleId :

8330-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL102412.M (Chemstation Integrator)

Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)

Last Update : Wed Nov 14 13:24:43 2012


Response via : Multiple Level Calibration


DataAcq Meth : 8330AGIP.M

Volume Inj. :

Signal Phase :

Signal Info :

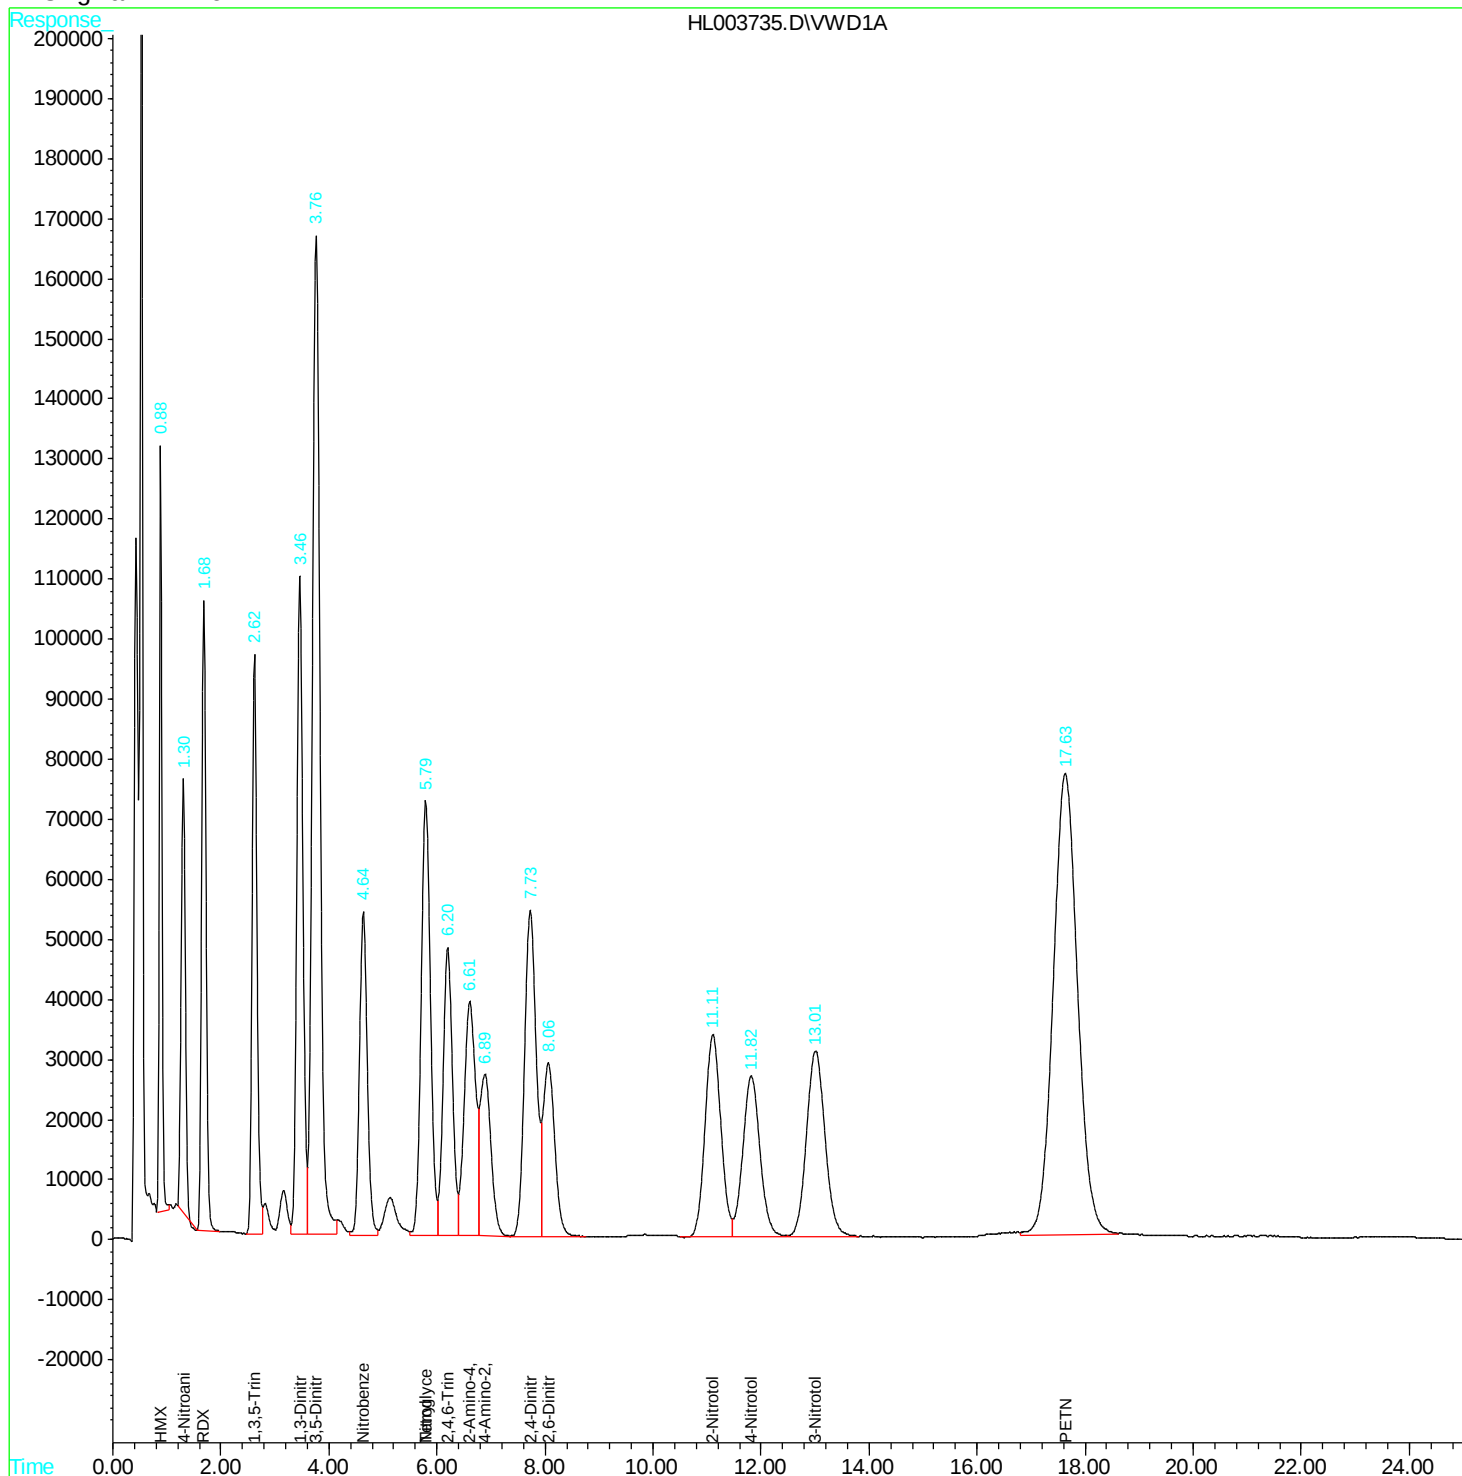


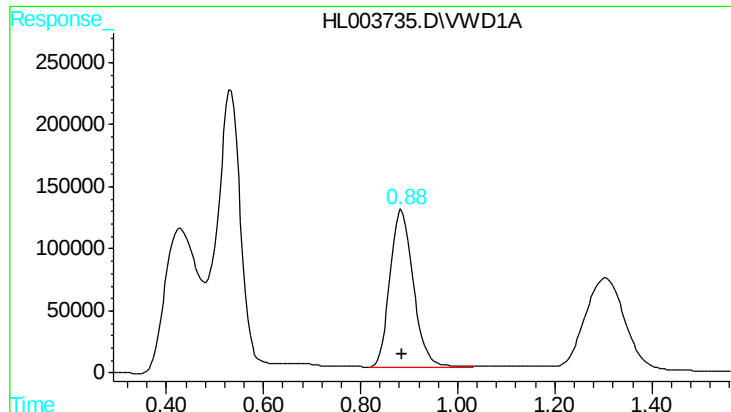

#2 HMX


R.T.: 0.884 min
Delta R.T.: -0.001 min
Response: 4237135
Conc: 1045.97 ug/L

Instrument :
HPLC_L
ClientSampleId :
8330-CCV

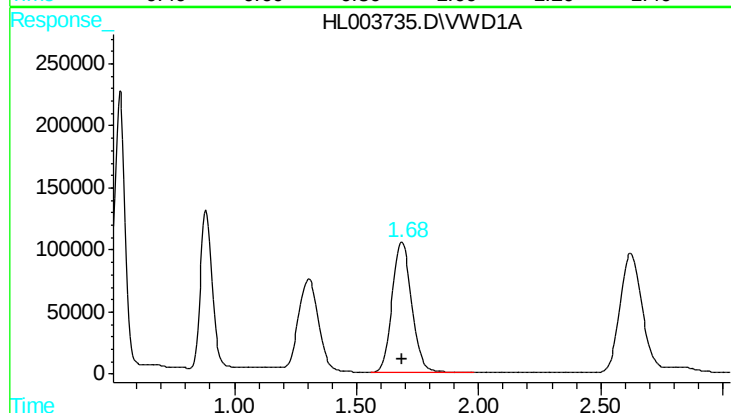


#3 RDX

R.T.: 1.686 min
Delta R.T.: -0.002 min
Response: 5851353
Conc: 1087.13 ug/L

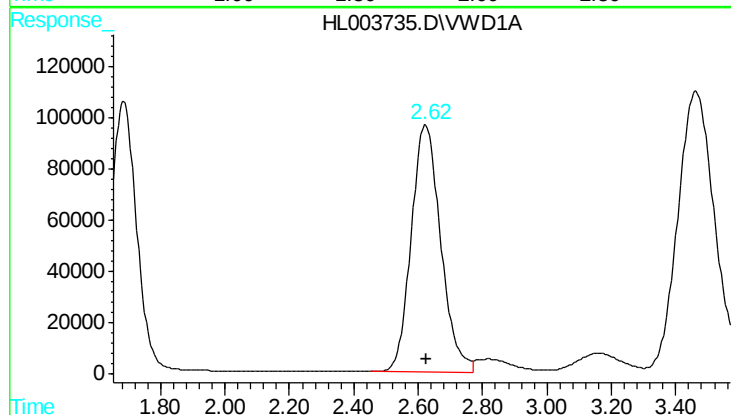


#4 1,3,5-Trinitrobenzene

R.T.: 2.623 min
Delta R.T.: -0.002 min
Response: 6132684
Conc: 516.95 ug/L

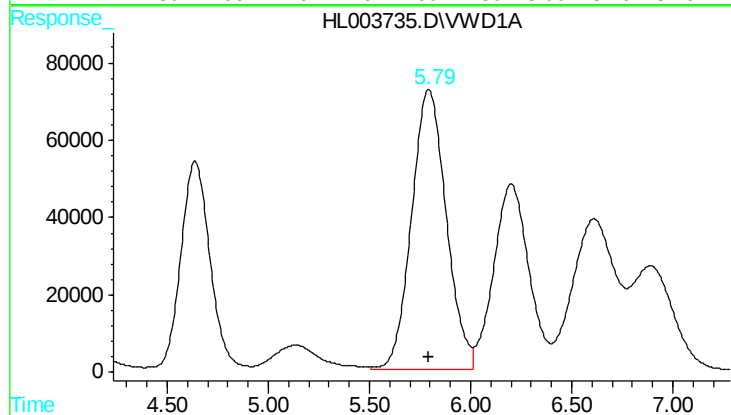

#5 Tetryl


R.T.: 5.793 min
Delta R.T.: -0.001 min
Response: 8653891
Conc: 1016.24 ug/L

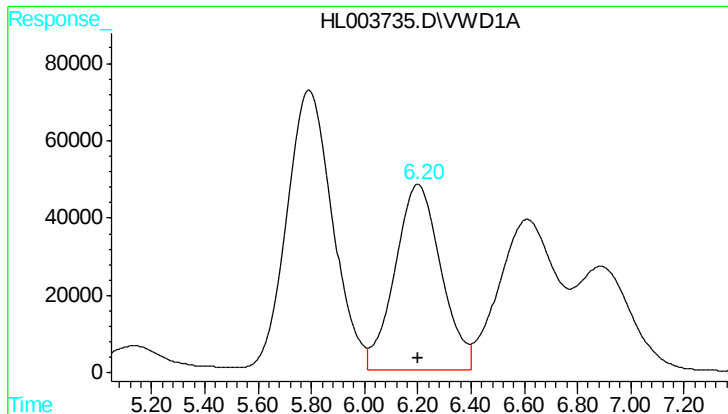

#6 2,4,6-Trinitrotoluene


R.T.: 6.201 min
Delta R.T.: 0.000 min
Response: 5818596
Conc: 510.64 ug/L

Instrument :
HPLC_L
ClientSampleId :
8330-CCV

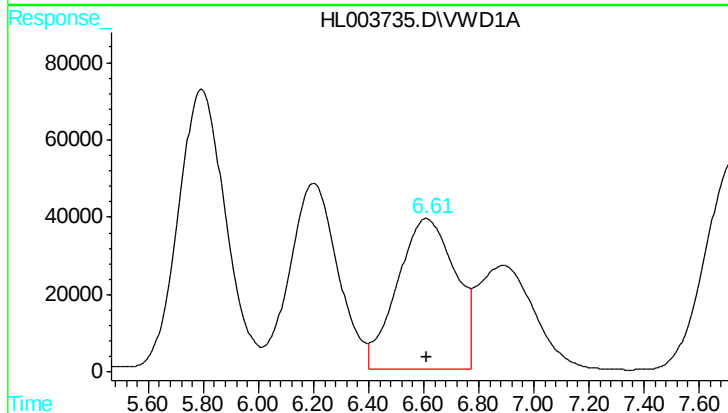


#7 2-Amino-4,6-dinitrotoluene

R.T.: 6.611 min
Delta R.T.: 0.001 min
Response: 5740866
Conc: 529.52 ug/L

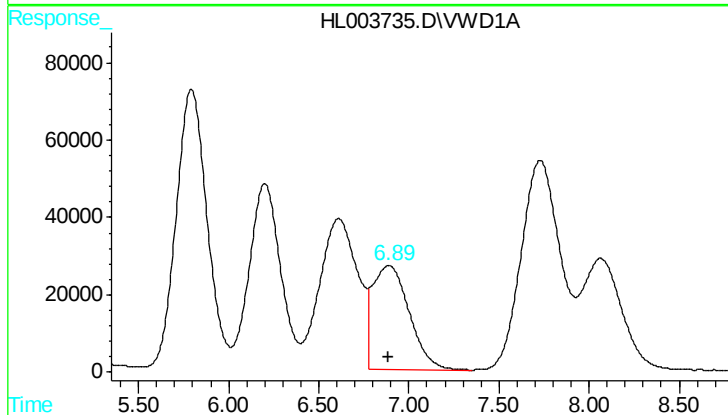


#8 4-Amino-2,6-dinitrotoluene

R.T.: 6.890 min
Delta R.T.: 0.003 min
Response: 3845392
Conc: 532.89 ug/L

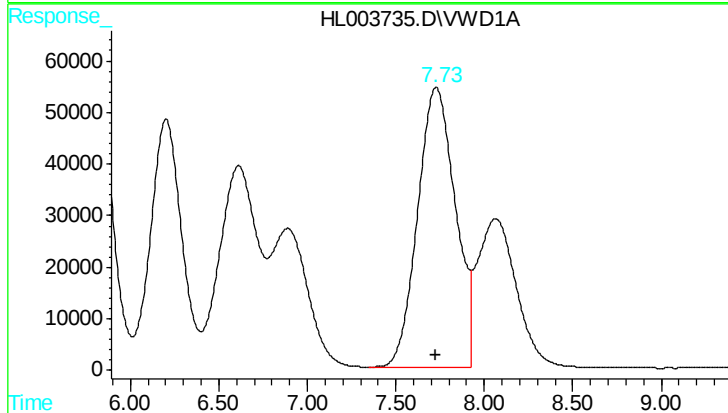

#9 2,4-Dinitrotoluene


R.T.: 7.729 min
Delta R.T.: 0.000 min
Response: 8083254
Conc: 506.21 ug/L

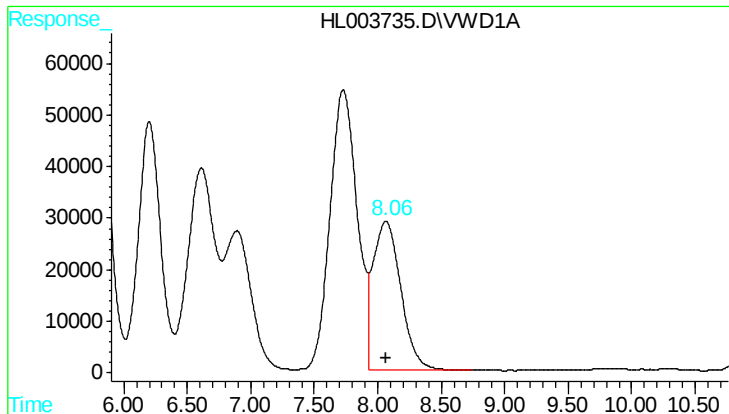

#10 2,6-Dinitrotoluene


R.T.: 8.064 min
Delta R.T.: 0.000 min
Response: 4420723
Conc: 512.91 ug/L

Instrument :
HPLC_L
ClientSampleId :
8330-CCV

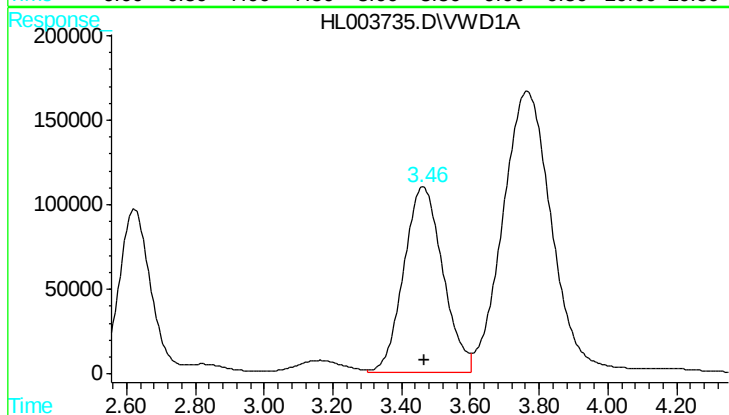


#11 1,3-Dinitrobenzene

R.T.: 3.463 min
Delta R.T.: -0.002 min
Response: 8698271
Conc: 525.72 ug/L

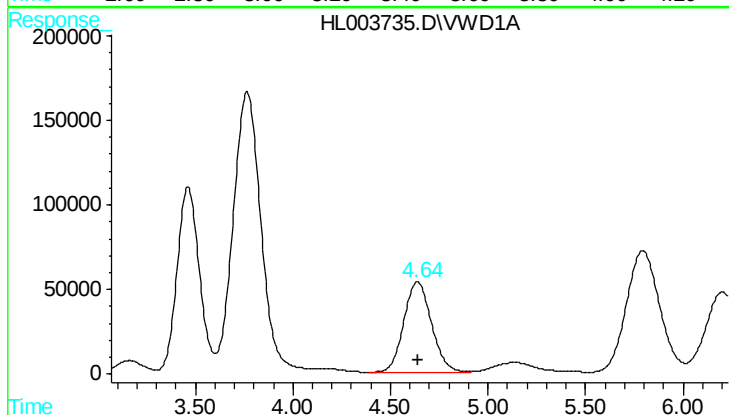


#12 Nitrobenzene

R.T.: 4.638 min
Delta R.T.: -0.003 min
Response: 5399650
Conc: 504.54 ug/L

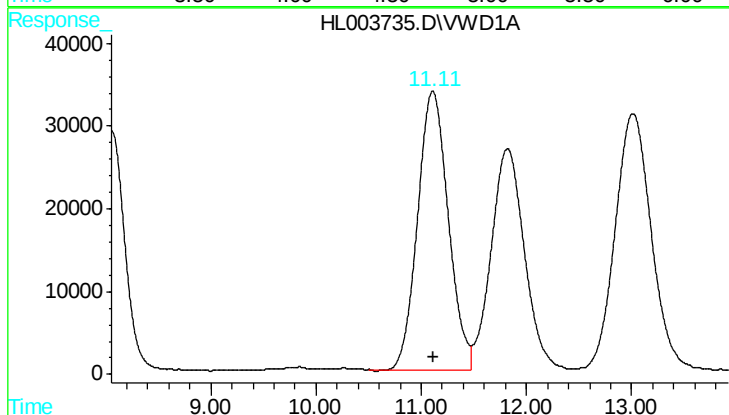

#13 2-Nitrotoluene


R.T.: 11.109 min
Delta R.T.: 0.000 min
Response: 6830597
Conc: 1008.48 ug/L

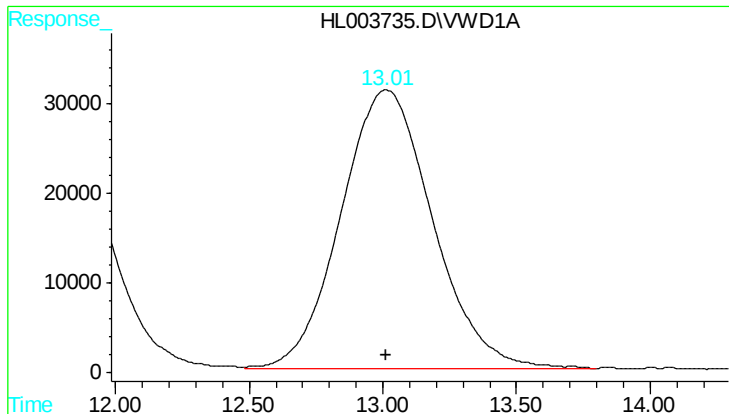

#14 3-Nitrotoluene


R.T.: 13.011 min
Delta R.T.: 0.000 min
Response: 7390392
Conc: 1025.60 ug/L

Instrument :
HPLC_L
ClientSampleId :
8330-CCV

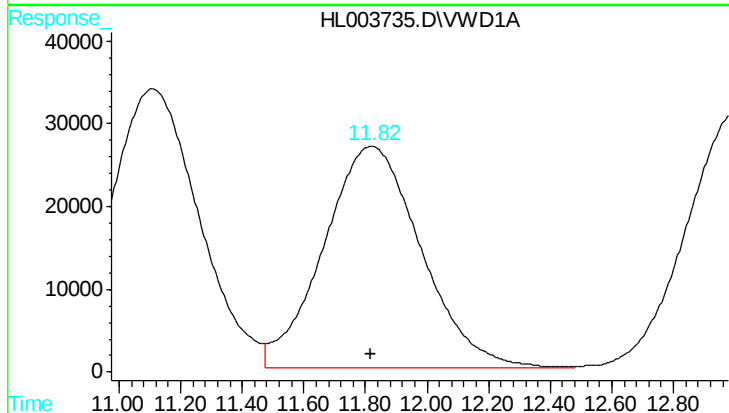


#15 4-Nitrotoluene

R.T.: 11.821 min
Delta R.T.: 0.003 min
Response: 5897809
Conc: 1014.15 ug/L

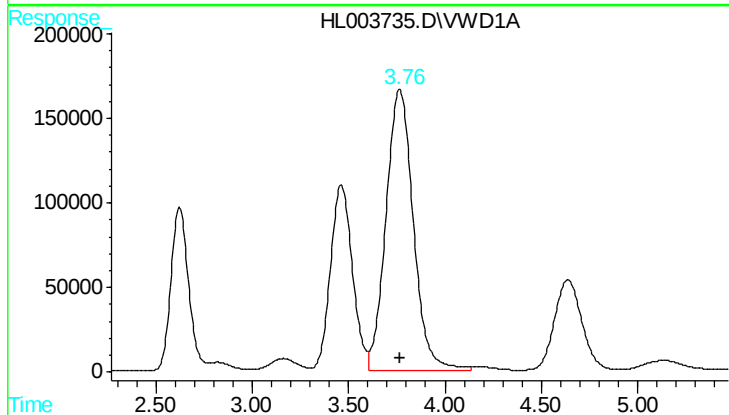


#16 3,5-Dinitroaniline

R.T.: 3.766 min
Delta R.T.: -0.003 min
Response: 16499670
Conc: 1050.86 ug/L

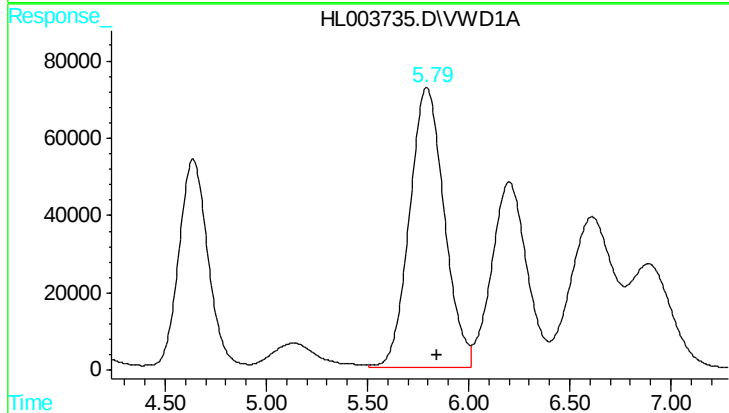

#17 Nitroglycerin

R.T.: 5.793 min
Delta R.T.: -0.050 min
Response: 8653891
Conc: 150200.48 ug/L

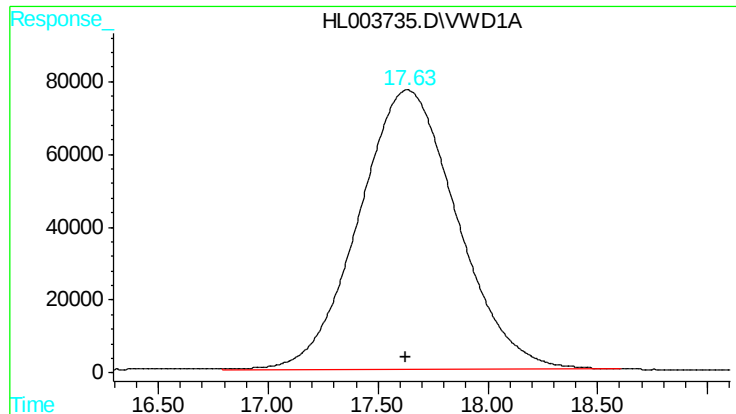

#18 PETN

R.T.: 17.634 min
Delta R.T.: 0.007 min
Response: 24068666
Conc: 2599.00 ug/L

Instrument :
HPLC_L
ClientSampleId :
8330-CCV