

Data File : H:\VOL1\HPLC\HPLC L\121113\HL003736.D Vial: 3
Acq On : 13-Nov-2012, 19:19 Operator: HLM
Sample : 8330NG-CCV Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Nov 14 13:26 2012 Quant Results File: HL102412.RES

Instrument :
HPLC_L
ClientSampleId :
8330NG-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL102412.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Wed Nov 14 13:24:43 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

5) T	Tetryl	5.84f	625727	73.480 ug/L
16) T	3,5-Dinitroaniline	3.78	113920	7.256 ug/L
17) T	Nitroglycerin	5.84	625727	10860.379 ug/L


Quantitation Report


Data File : H:\VOL1\HPLC\HPLC L\121113\HL003736.D Vial: 3
 Acq On : 13-Nov-2012, 19:19 Operator: HLM
 Sample : 8330NG-CCV Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Nov 14 13:26 2012 Quant Results File: HL102412.RES

Instrument :
 HPLC_L
 ClientSampleId :
 8330NG-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL102412.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Wed Nov 14 13:24:43 2012
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

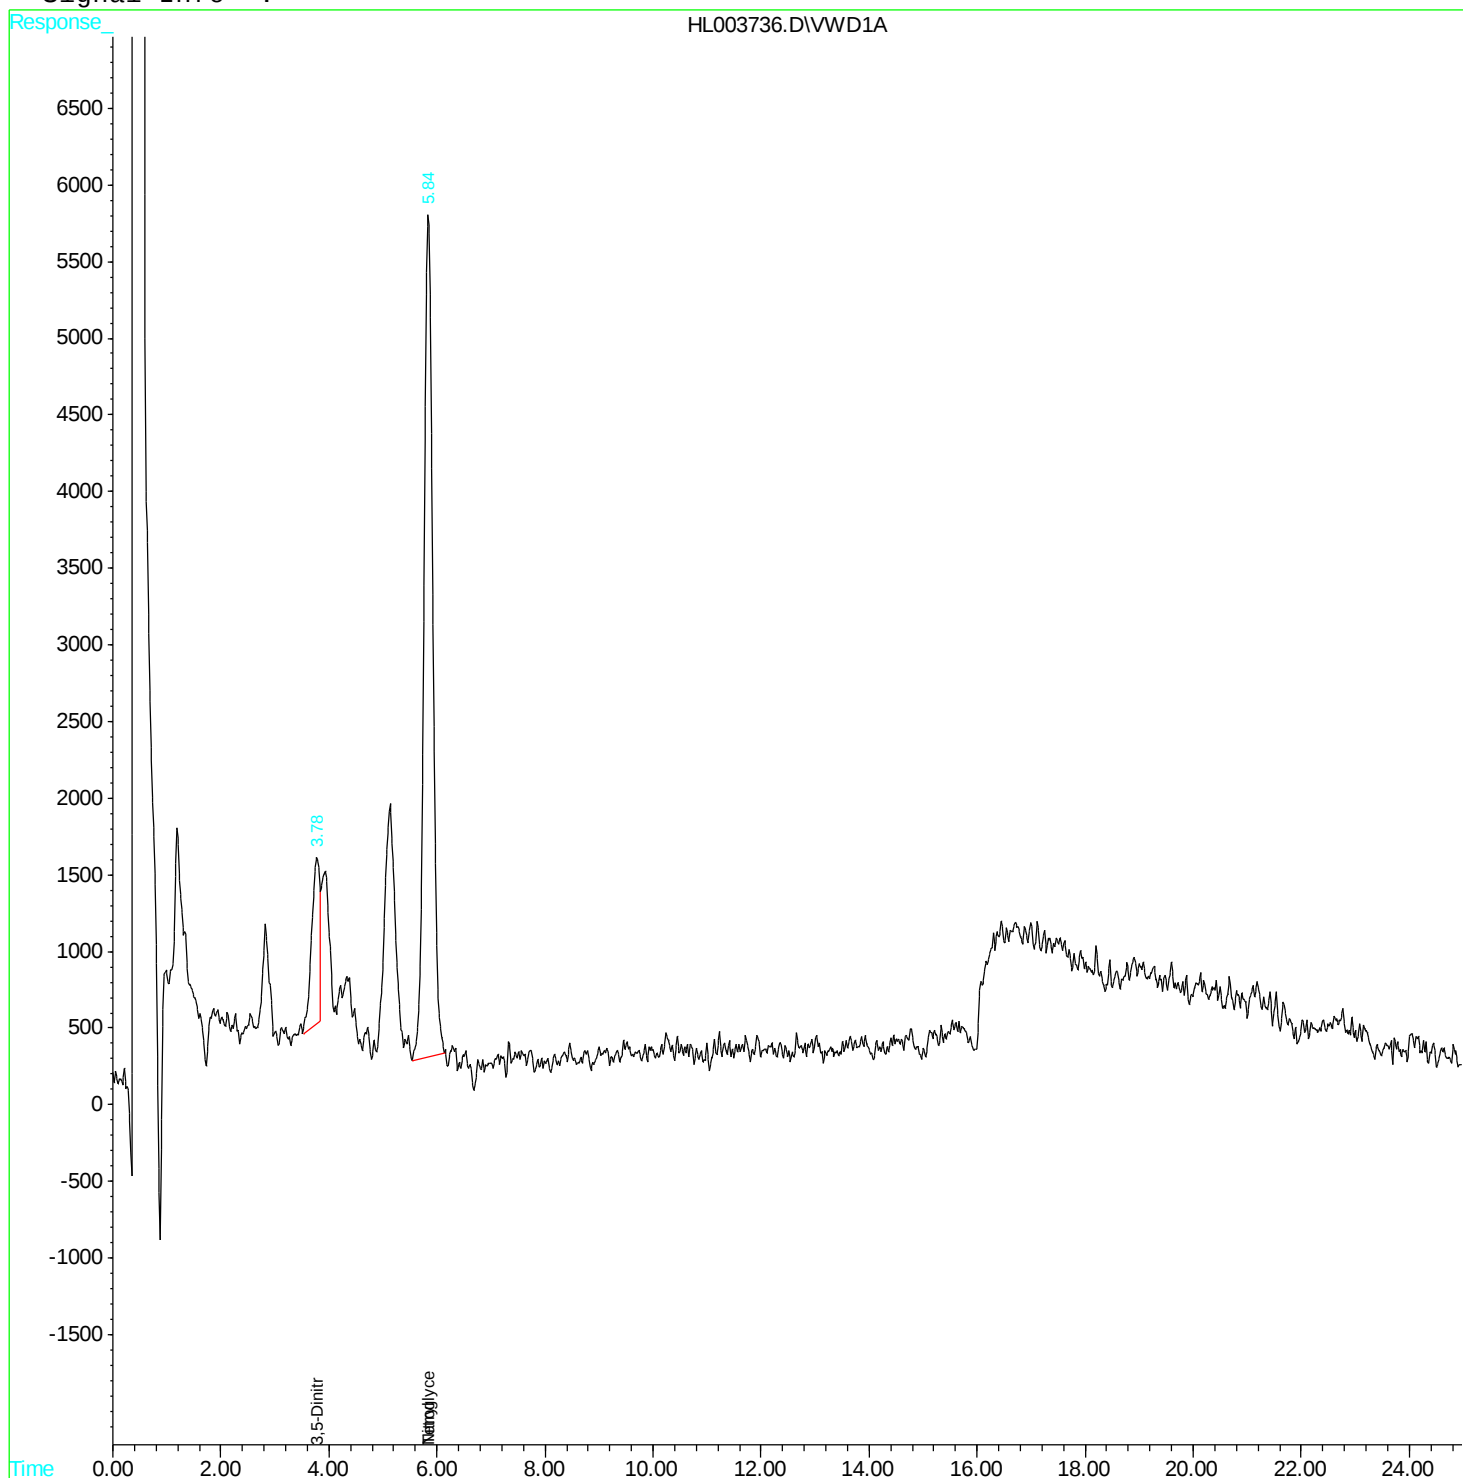


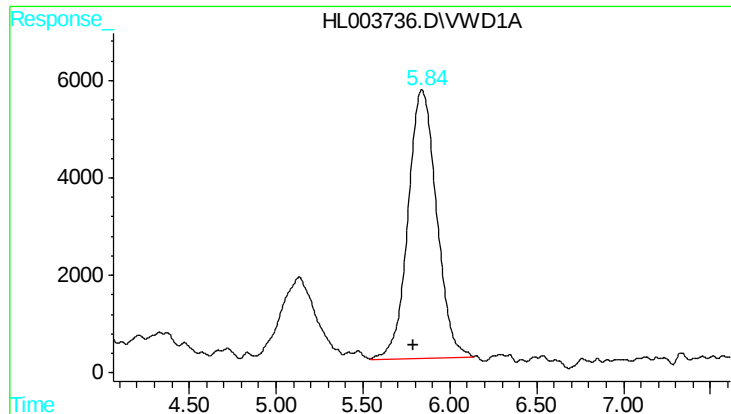

#5 Tetryl


R.T.: 5.839 min
Delta R.T.: 0.045 min
Response: 625727
Conc: 73.48 ug/L

Instrument :
HPLC_L
ClientSampleId :
8330NG-CCV

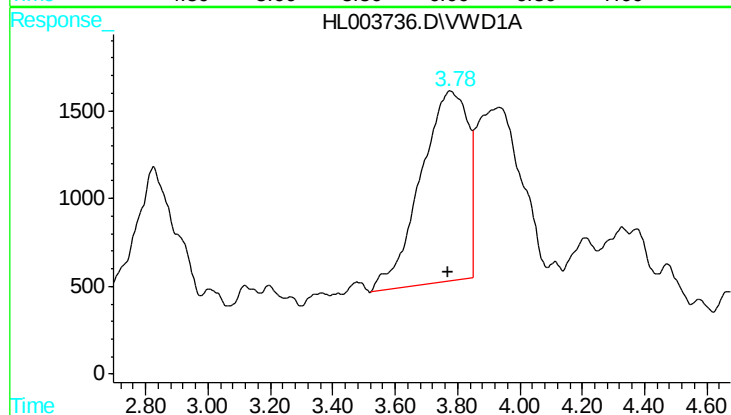

#16 3,5-Dinitroaniline

R.T.: 3.777 min
Delta R.T.: 0.009 min
Response: 113920
Conc: 7.26 ug/L

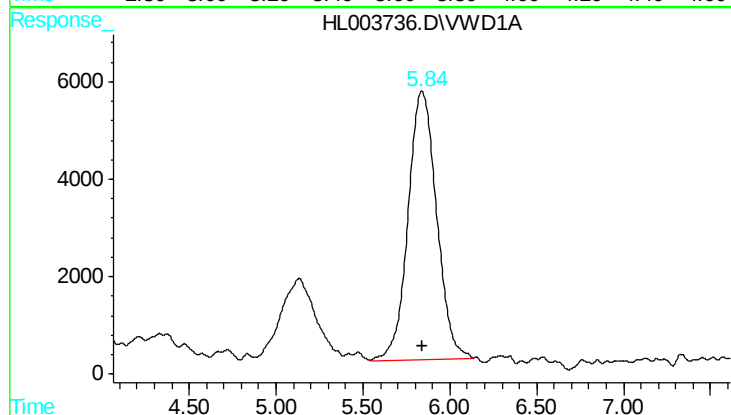

#17 Nitroglycerin

R.T.: 5.839 min
Delta R.T.: -0.004 min
Response: 625727
Conc: 10860.38 ug/L