

Data Path : S:\HPCHEM1\HPLC_L\Data\HL111312\
 Data File : HL003720.D
 Signal(s) : VWD1A.CH
 Acq On : 13-Nov-2012, 12:07
 Operator : HLM
 Sample : 8330-CCV
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 HPLC_L
 LabSampleId :
 8330-CCV

Integration File: events.e
 Quant Time: Nov 17 00:37:24 2012
 Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL102412.M
 Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 QLast Update : Wed Nov 14 13:24:43 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.307	3965966	992.566 ug/L
Spiked Amount 300.000	Range 37 - 149	Recovery	= 330.86%#
Target Compounds			
2) T HMX	0.886	4241218	1046.969 ug/L
3) T RDX	1.688	5849530	1086.793 ug/L
4) T 1,3,5-Trinitrobenzene	2.625	6135739	517.203 ug/L
5) T Tetryl	5.794	8735093	1025.779 ug/L
6) T 2,4,6-Trinitrotoluene	6.202	5806763	509.600 ug/L
7) T 2-Amino-4,6-dinitroto...	6.610	5773624	532.537 ug/L
8) T 4-Amino-2,6-dinitroto...	6.886	3855482	534.289 ug/L
9) T 2,4-Dinitrotoluene	7.728	8080250	506.026 ug/L
10) T 2,6-Dinitrotoluene	8.064	4386437	508.935 ug/L
11) T 1,3-Dinitrobenzene	3.465	8688929	525.151 ug/L
12) T Nitrobenzene	4.641	5424196	506.831 ug/L
13) T 2-Nitrotoluene	11.110	6853254	1011.829 ug/L
14) T 3-Nitrotoluene	13.011	7439524	1032.418 ug/L
15) T 4-Nitrotoluene	11.817	5903328	1015.095 ug/L
16) T 3,5-Dinitroaniline	3.769	16456263	1048.096 ug/L
18) T PETN	17.628	23927689	2583.777 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_L\Data\HL111312\
Data File : HL003720.D
Signal(s) : VWD1A.CH
Acq On : 13-Nov-2012, 12:07
Operator : HLM
Sample : 8330-CCV
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
LabSampleId :
8330-CCV

Integration File: events.e
Quant Time: Nov 17 00:37:24 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL102412.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Wed Nov 14 13:24:43 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

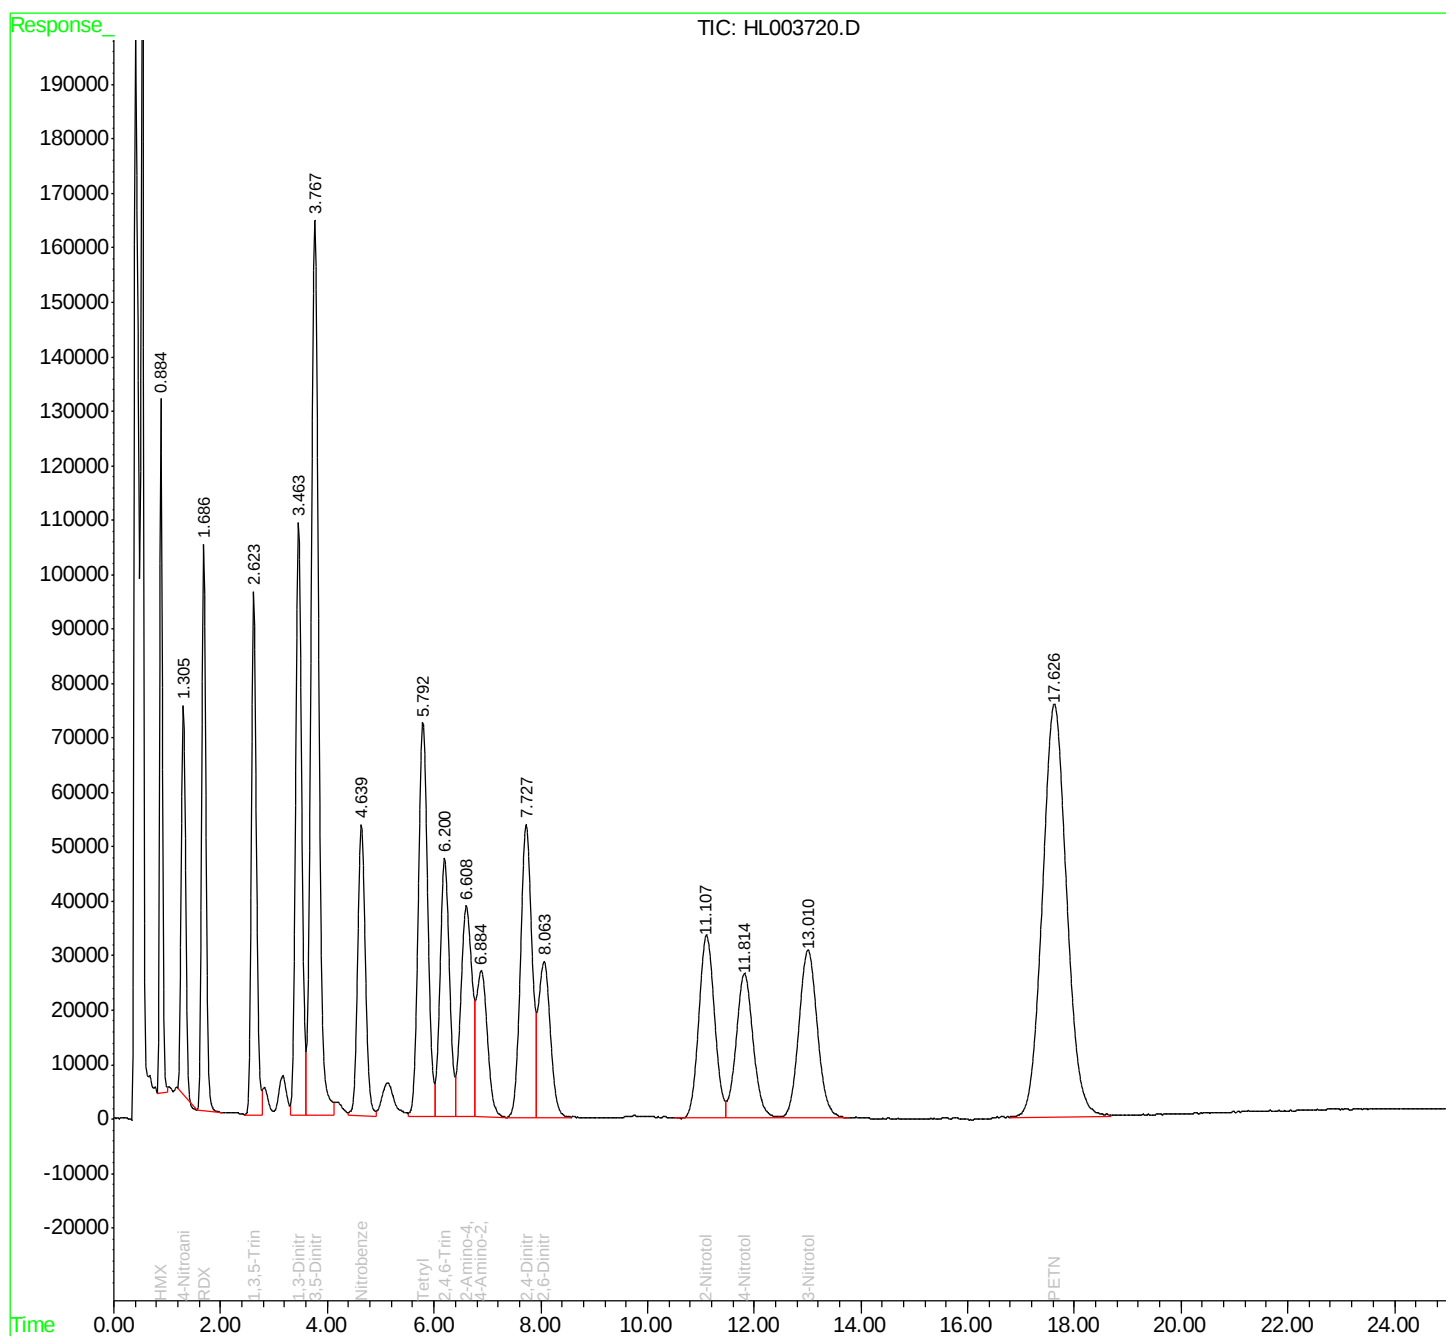


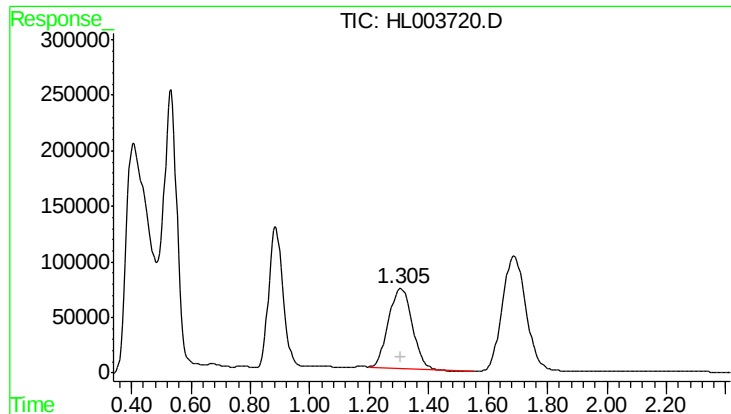

#1 4-Nitroaniline


R.T.: 1.307 min
Delta R.T.: 0.000 min
Response: 3965966
Conc: 992.57 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

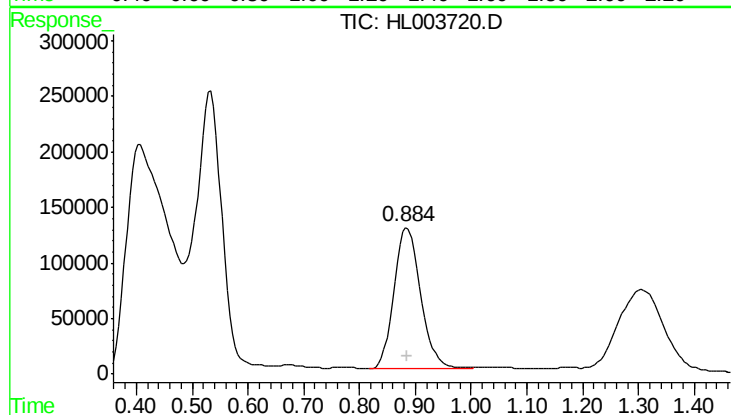


#2 HMX

R.T.: 0.886 min
Delta R.T.: 0.000 min
Response: 4241218
Conc: 1046.97 ug/L

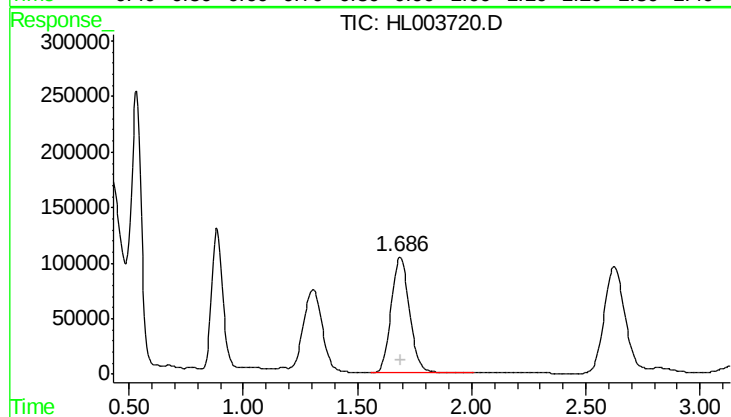


#3 RDX

R.T.: 1.688 min
Delta R.T.: 0.000 min
Response: 5849530
Conc: 1086.79 ug/L

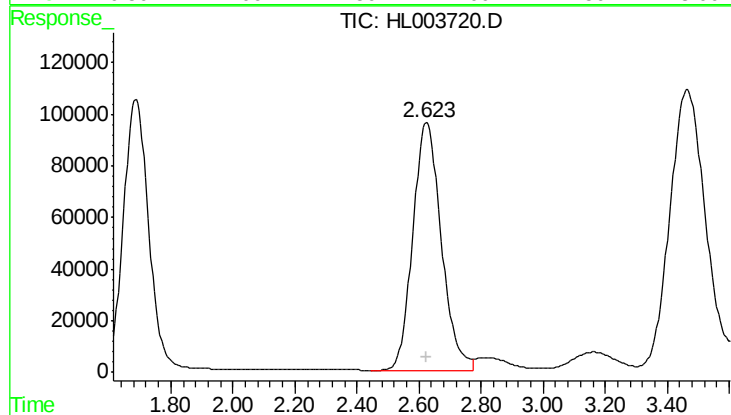

#4 1,3,5-Trinitrobenzene


R.T.: 2.625 min
Delta R.T.: 0.000 min
Response: 6135739
Conc: 517.20 ug/L

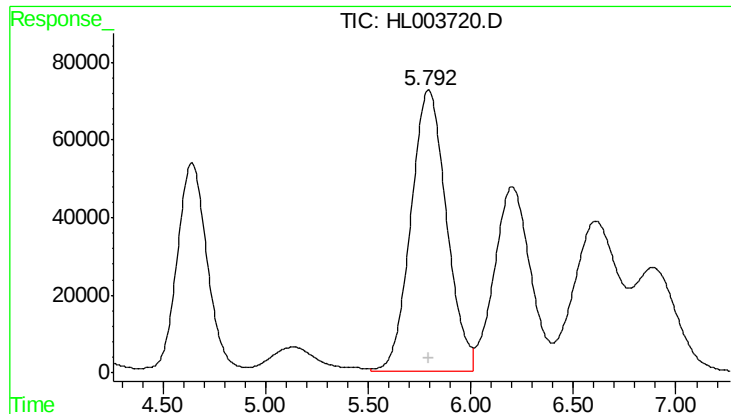

#5 Tetryl


R.T.: 5.794 min
Delta R.T.: 0.000 min
Response: 8735093
Conc: 1025.78 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

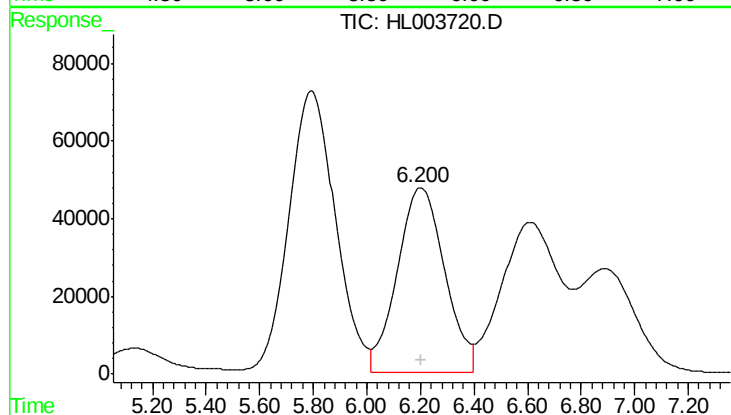


#6 2,4,6-Trinitrotoluene

R.T.: 6.202 min
Delta R.T.: 0.000 min
Response: 5806763
Conc: 509.60 ug/L

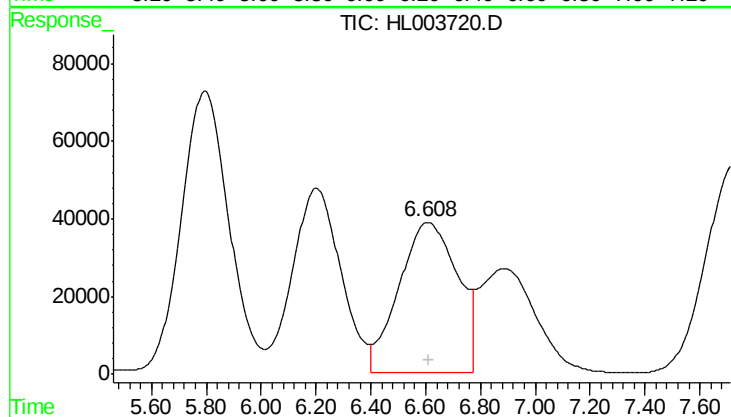


#7 2-Amino-4,6-dinitrotoluene

R.T.: 6.610 min
Delta R.T.: 0.000 min
Response: 5773624
Conc: 532.54 ug/L

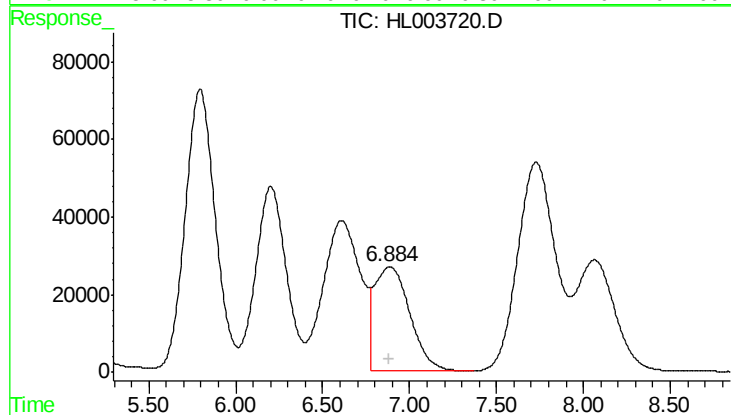

#8 4-Amino-2,6-dinitrotoluene


R.T.: 6.886 min
Delta R.T.: 0.000 min
Response: 3855482
Conc: 534.29 ug/L

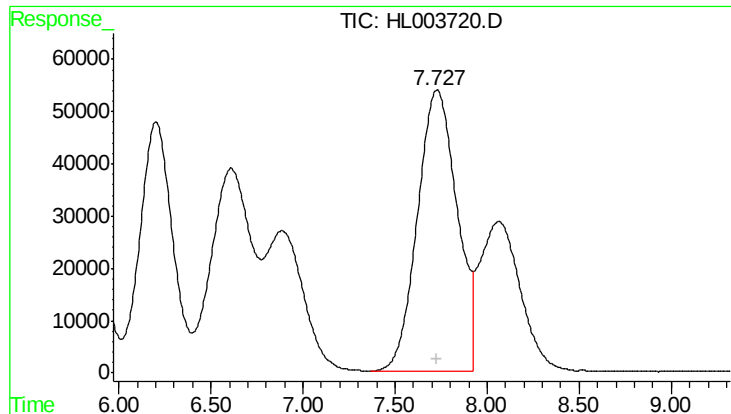

#9 2,4-Dinitrotoluene


R.T.: 7.728 min
Delta R.T.: 0.000 min
Response: 8080250
Conc: 506.03 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

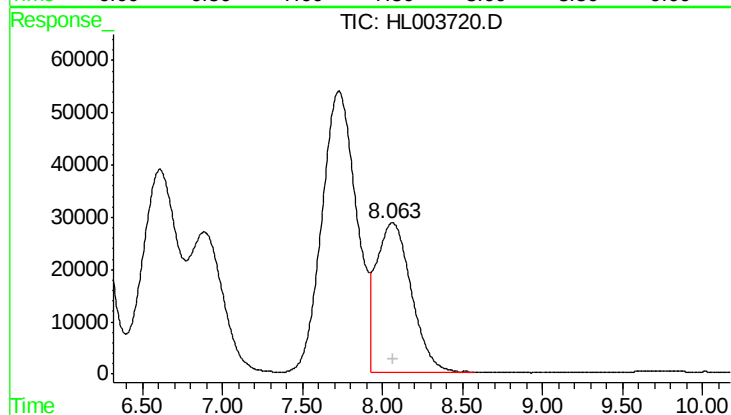


#10 2,6-Dinitrotoluene

R.T.: 8.064 min
Delta R.T.: 0.000 min
Response: 4386437
Conc: 508.94 ug/L

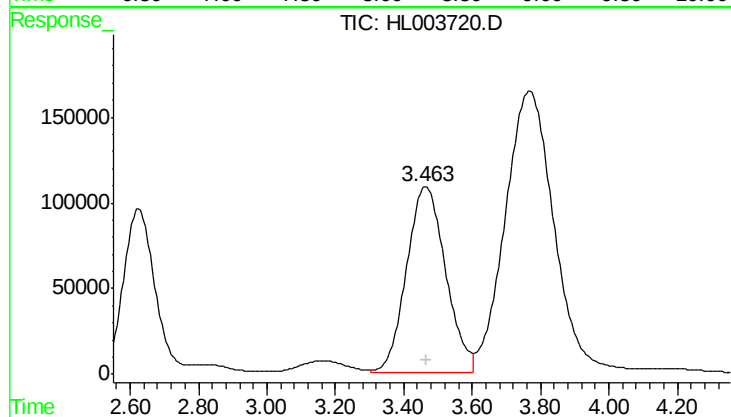


#11 1,3-Dinitrobenzene

R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 8688929
Conc: 525.15 ug/L

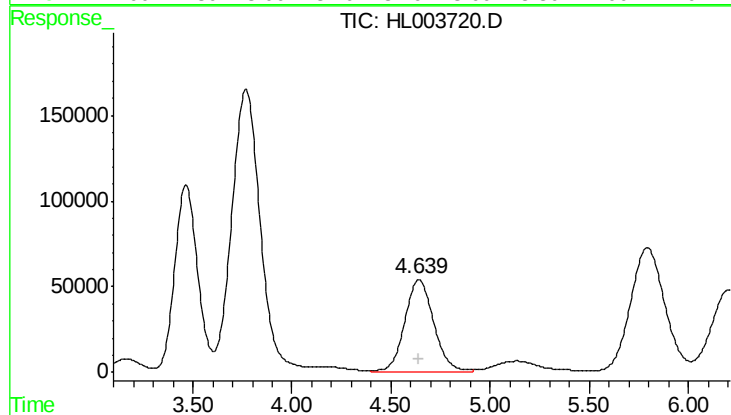

#12 Nitrobenzene


R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 5424196
Conc: 506.83 ug/L

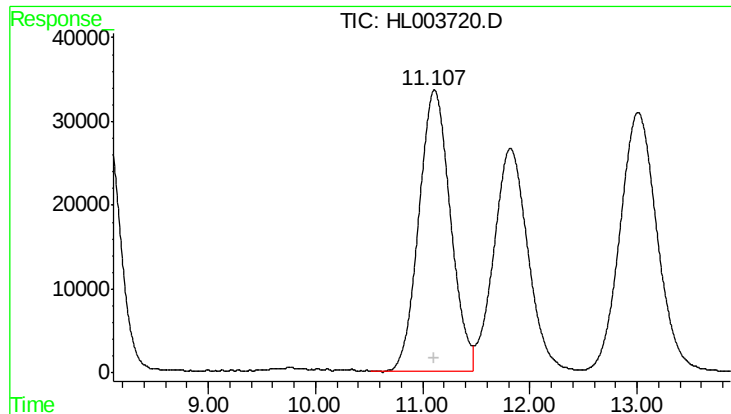

#13 2-Nitrotoluene


R.T.: 11.110 min
 Delta R.T.: 0.000 min
 Response: 6853254
 Conc: 1011.83 ug/L

Instrument :
 HPLC_L
 LabSampleId :
 8330-CCV

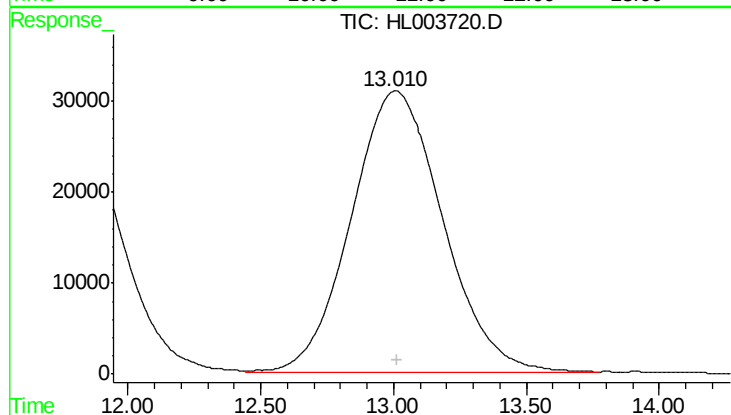


#14 3-Nitrotoluene

R.T.: 13.011 min
 Delta R.T.: 0.000 min
 Response: 7439524
 Conc: 1032.42 ug/L

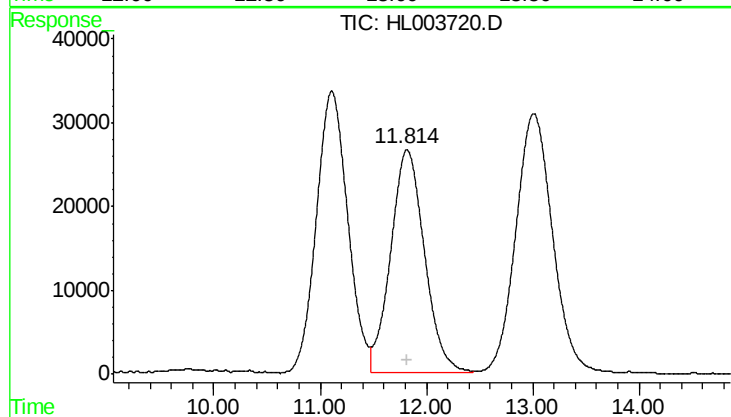


#15 4-Nitrotoluene

R.T.: 11.817 min
 Delta R.T.: 0.000 min
 Response: 5903328
 Conc: 1015.09 ug/L

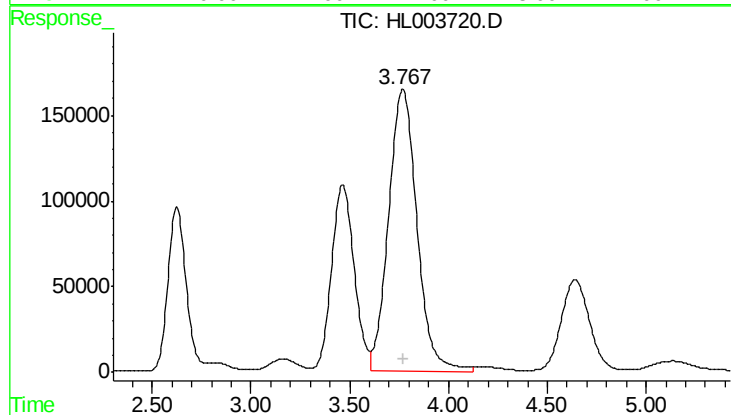

#16 3,5-Dinitroaniline

R.T.: 3.769 min
 Delta R.T.: 0.000 min
 Response: 16456263
 Conc: 1048.10 ug/L

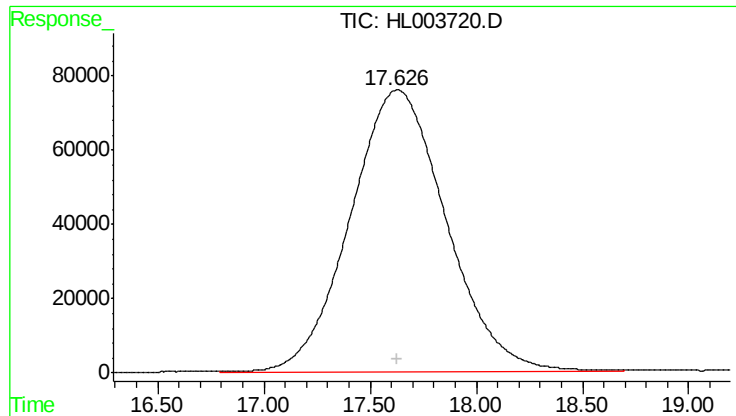

#18 PETN

R.T.: 17.628 min
Delta R.T.: 0.000 min
Response: 23927689
Conc: 2583.78 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV