

Data Path : S:\HPCHEM1\HPLC_L\Data\HL111312\
 Data File : HL003722.D
 Signal(s) : VWD1A.CH
 Acq On : 13-Nov-2012, 13:01
 Operator : HLM
 Sample : D4671-01DL 2X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :
 871DL

Integration File: events.e
 Quant Time: Nov 17 00:37:34 2012
 Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL102412.M
 Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 QLast Update : Wed Nov 14 13:24:43 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.310	287908	37.381 ug/L m
Spiked Amount 300.000	Range 37 - 149	Recovery =	12.46%#
Target Compounds			
3) T RDX	1.688	988932	183.735 ug/L
4) T 1,3,5-Trinitrobenzene	2.623	3737124	315.015 ug/L
6) T 2,4,6-Trinitrotoluene	6.198	3100483	272.097 ug/L
7) T 2-Amino-4,6-dinitroto...	6.608	7219050	665.858 ug/L
8) T 4-Amino-2,6-dinitroto...	6.881	4346751	602.368 ug/L
9) T 2,4-Dinitrotoluene	7.724	23343095	1461.862 ug/L
10) T 2,6-Dinitrotoluene	8.049	6120146	710.088 ug/L
11) T 1,3-Dinitrobenzene	3.480	47690	2.882 ug/L
12) T Nitrobenzene	4.636	2892915	270.311 ug/L
13) T 2-Nitrotoluene	11.101	7564148	1116.787 ug/L
14) T 3-Nitrotoluene	13.002	8546608	1186.053 ug/L
15) T 4-Nitrotoluene	11.811	7045066	1211.420 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_L\Data\HL111312\
Data File : HL003722.D
Signal(s) : VWD1A.CH
Acq On : 13-Nov-2012, 13:01
Operator : HLM
Sample : D4671-01DL 2X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
871DL

Integration File: events.e
Quant Time: Nov 17 00:37:34 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL102412.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Wed Nov 14 13:24:43 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

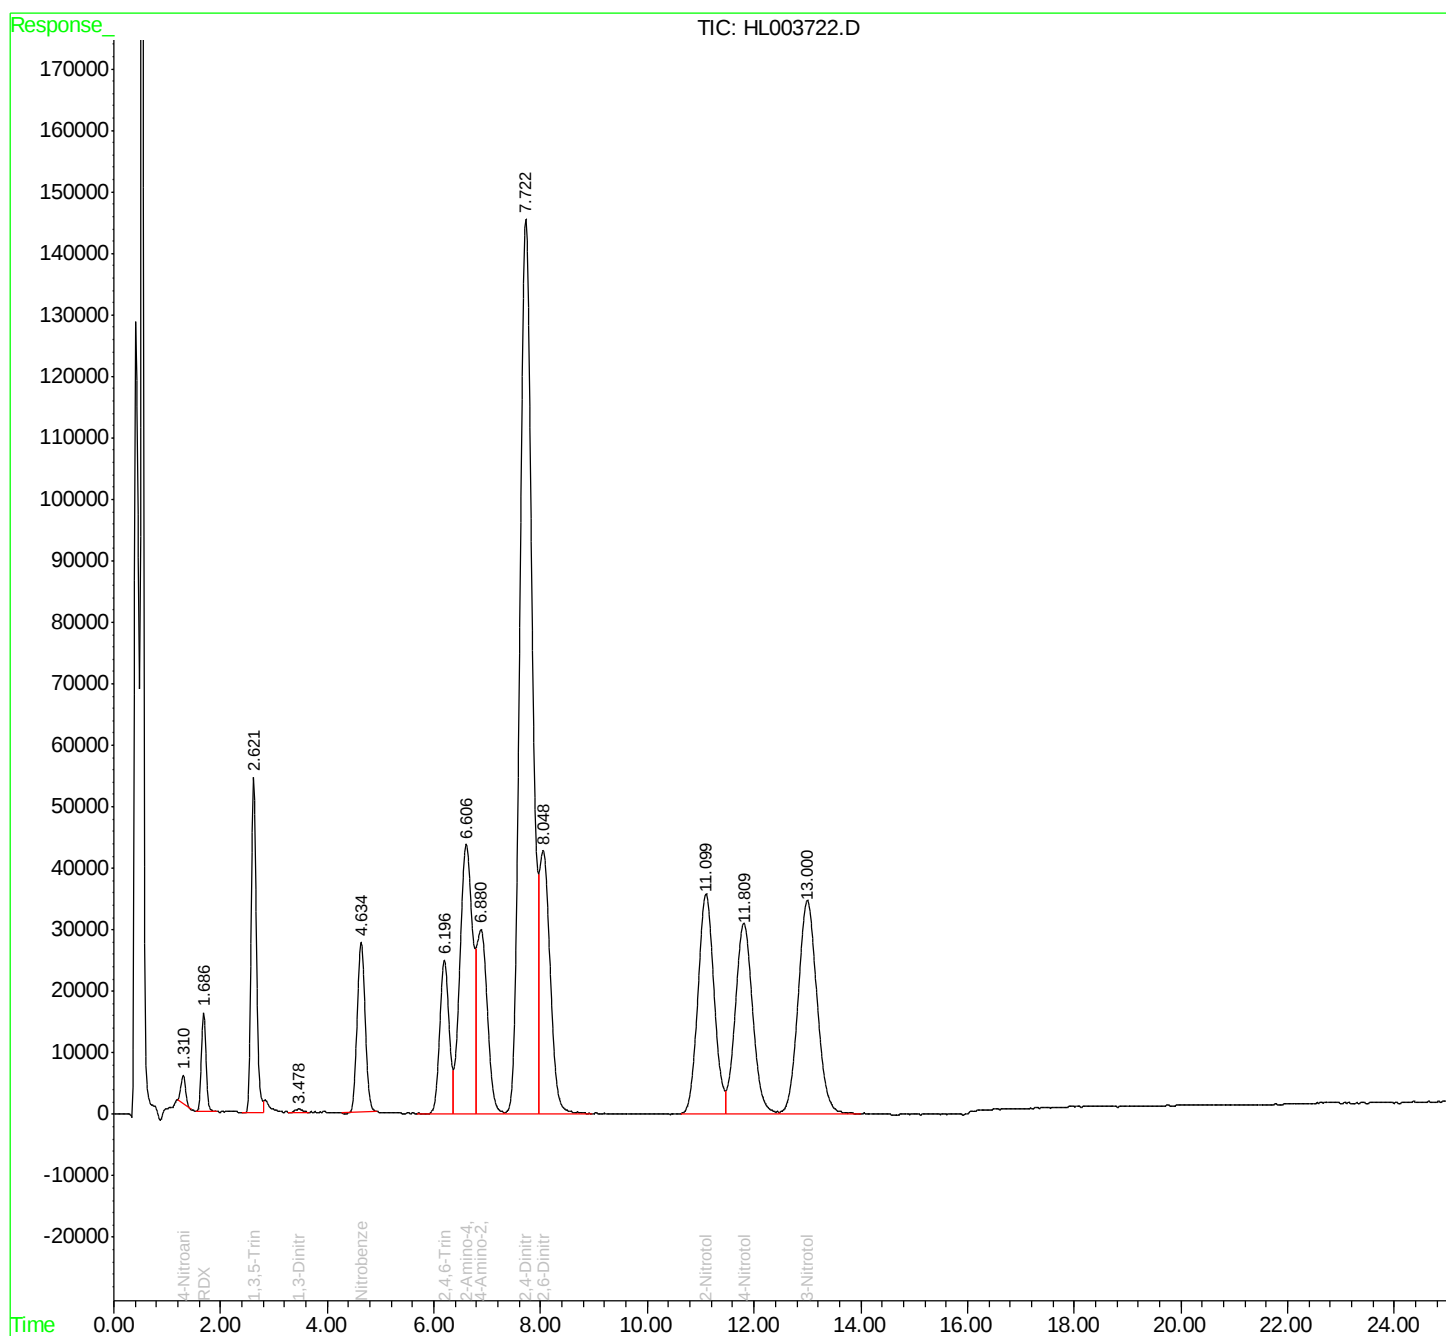


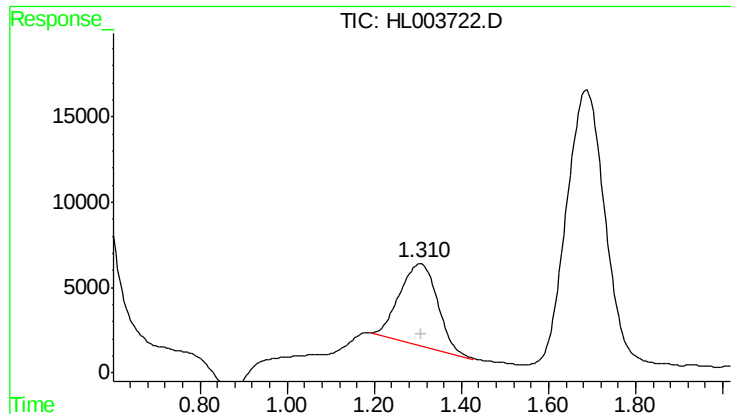

#1 4-Nitroaniline


R.T.: 1.310 min
 Delta R.T.: 0.002 min
 Response: 287908
 Conc: 37.38 ug/L

Instrument :
 HPLC_L
 ClientSampleId :
 871DL

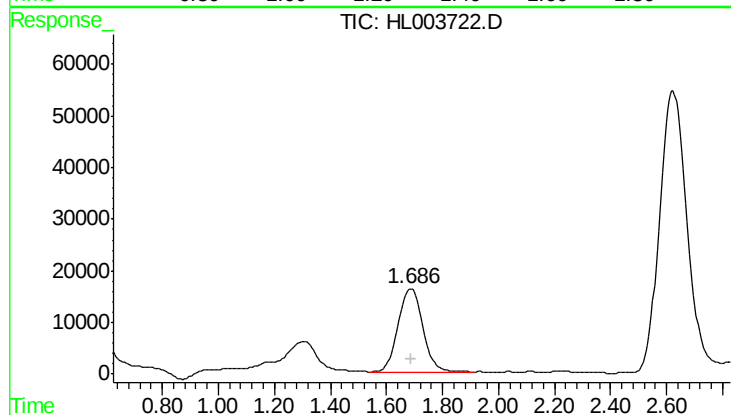


#3 RDX

R.T.: 1.688 min
 Delta R.T.: 0.000 min
 Response: 988932
 Conc: 183.73 ug/L

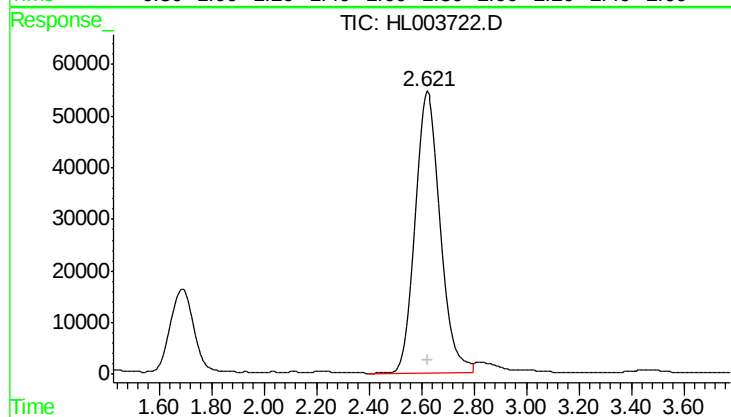


#4 1,3,5-Trinitrobenzene

R.T.: 2.623 min
 Delta R.T.: -0.002 min
 Response: 3737124
 Conc: 315.02 ug/L

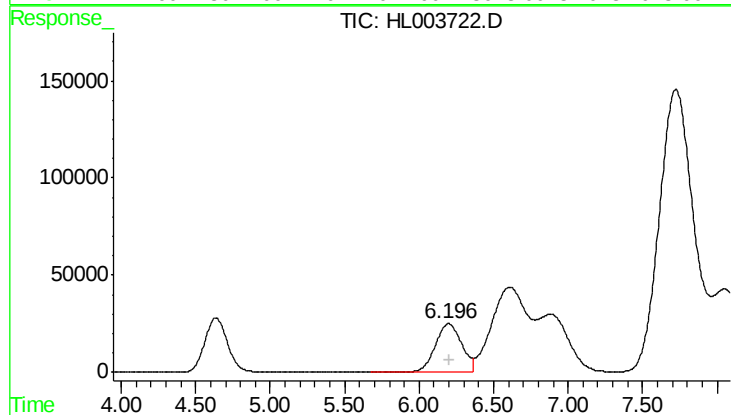

#6 2,4,6-Trinitrotoluene


R.T.: 6.198 min
 Delta R.T.: -0.004 min
 Response: 3100483
 Conc: 272.10 ug/L

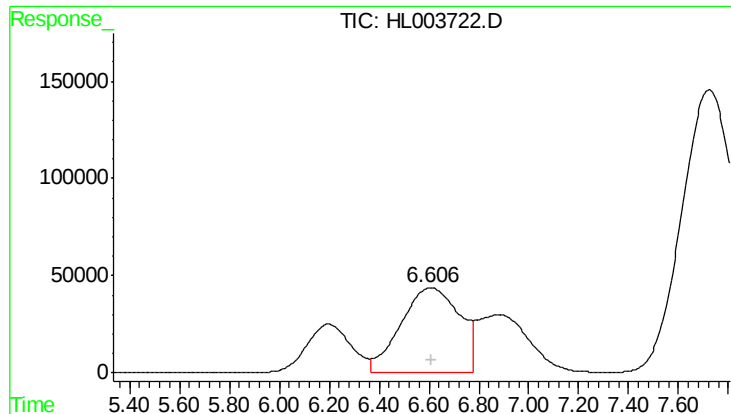

#7 2-Amino-4,6-dinitrotoluene


R.T.: 6.608 min
Delta R.T.: -0.002 min
Response: 7219050
Conc: 665.86 ug/L

Instrument :
HPLC_L
ClientSampleId :
871DL

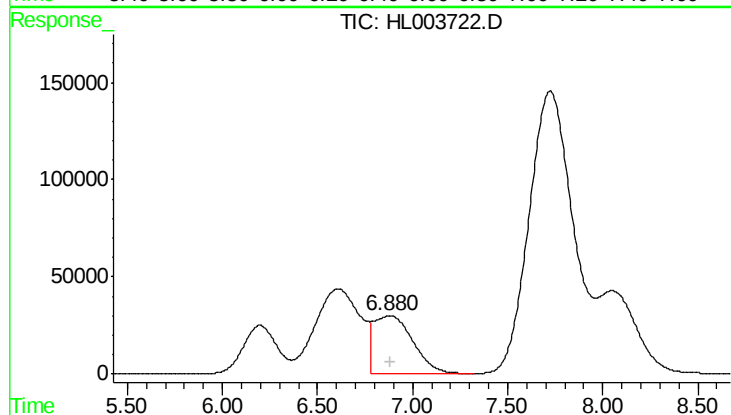


#8 4-Amino-2,6-dinitrotoluene

R.T.: 6.881 min
Delta R.T.: -0.005 min
Response: 4346751
Conc: 602.37 ug/L

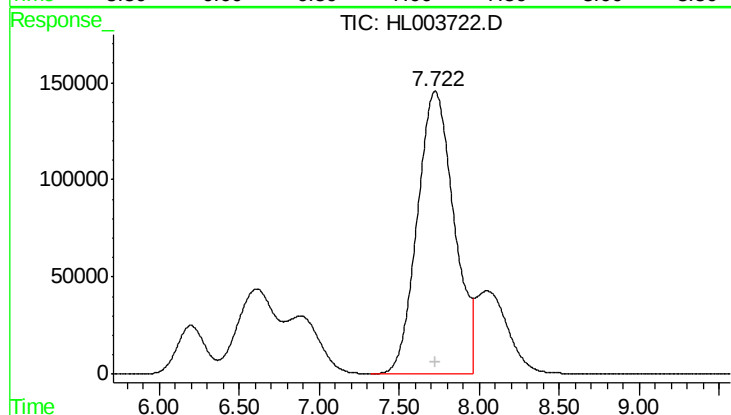


#9 2,4-Dinitrotoluene

R.T.: 7.724 min
Delta R.T.: -0.005 min
Response: 23343095
Conc: 1461.86 ug/L

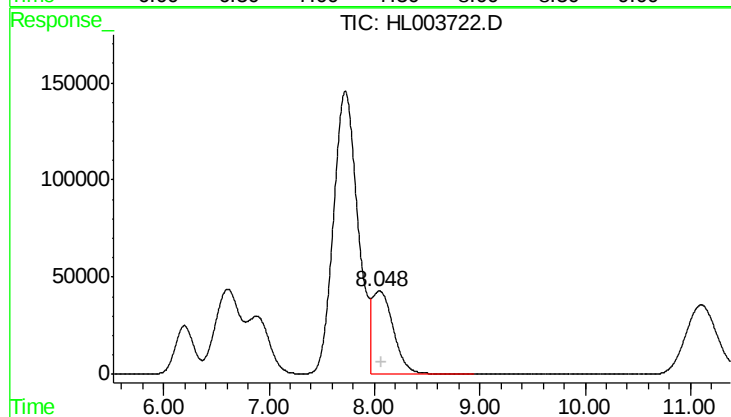

#10 2,6-Dinitrotoluene


R.T.: 8.049 min
Delta R.T.: -0.015 min
Response: 6120146
Conc: 710.09 ug/L

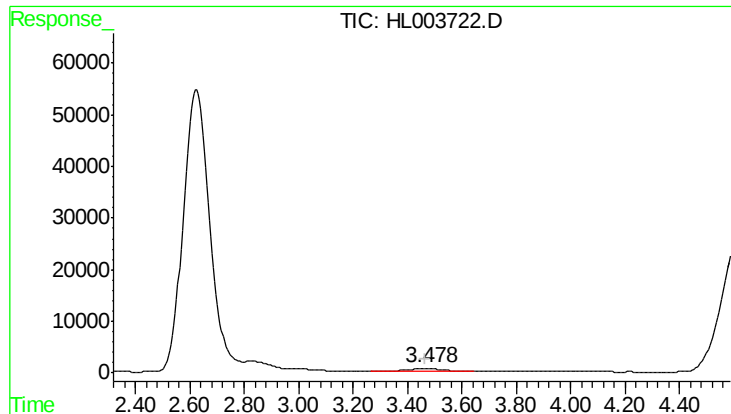

#11 1,3-Dinitrobenzene


R.T.: 3.480 min
Delta R.T.: 0.015 min
Response: 47690
Conc: 2.88 ug/L

Instrument :
HPLC_L
ClientSampleId :
871DL

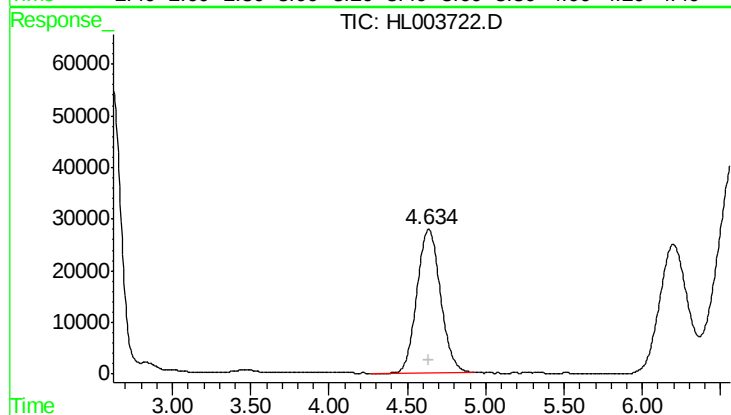


#12 Nitrobenzene

R.T.: 4.636 min
Delta R.T.: -0.004 min
Response: 2892915
Conc: 270.31 ug/L

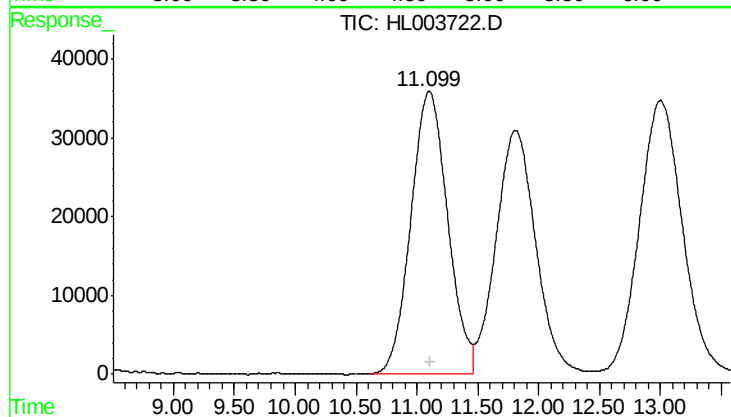


#13 2-Nitrotoluene

R.T.: 11.101 min
Delta R.T.: -0.008 min
Response: 7564148
Conc: 1116.79 ug/L

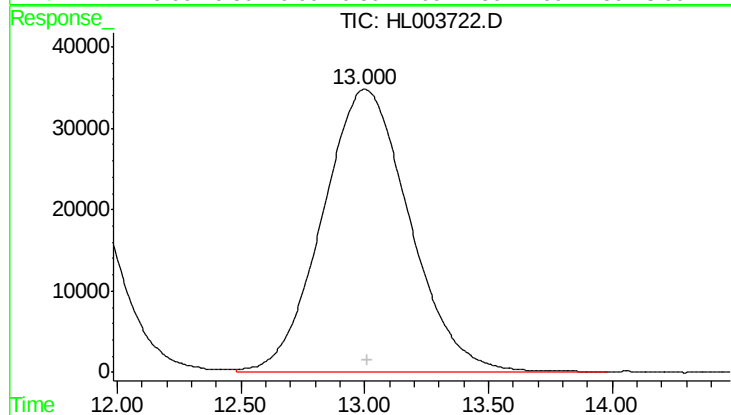

#14 3-Nitrotoluene

R.T.: 13.002 min
Delta R.T.: -0.009 min
Response: 8546608
Conc: 1186.05 ug/L

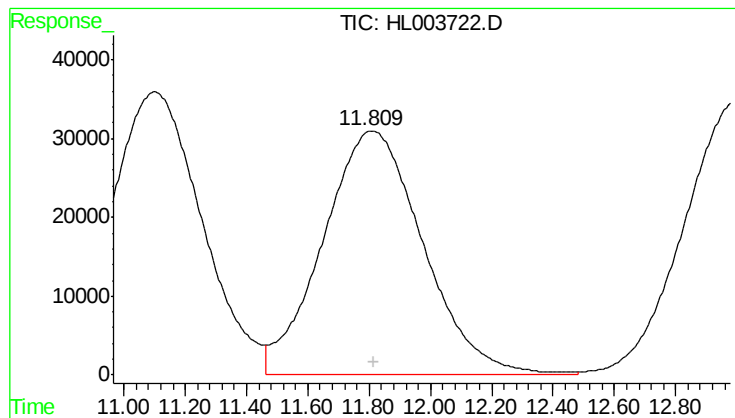

#15 4-Nitrotoluene

R.T.: 11.811 min
Delta R.T.: -0.007 min
Response: 7045066
Conc: 1211.42 ug/L

Instrument :
HPLC_L
ClientSampleId :
871DL