

Data File : H:\VOL1\HPLC\HPLC L\121115\HL003745.D Vial: 26
Acq On : 15-Nov-2012, 16:32 Operator: HLM
Sample : D4468-07 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Nov 16 16:17 2012 Quant Results File: HL102412.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL102412.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Fri Nov 16 16:16:22 2012
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.38	1276785	294.191 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 98.06%

Target Compounds


17) T	Nitroglycerin	6.30	53460	927.871 ug/L
-------	---------------	------	-------	--------------


Quantitation Report

Data File : H:\VOL1\HPLC\HPLC L\121115\HL003745.D Vial: 26
 Acq On : 15-Nov-2012, 16:32 Operator: HLM
 Sample : D4468-07 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Nov 16 16:17 2012 Quant Results File: HL102412.RES

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL102412.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Fri Nov 16 16:16:22 2012
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

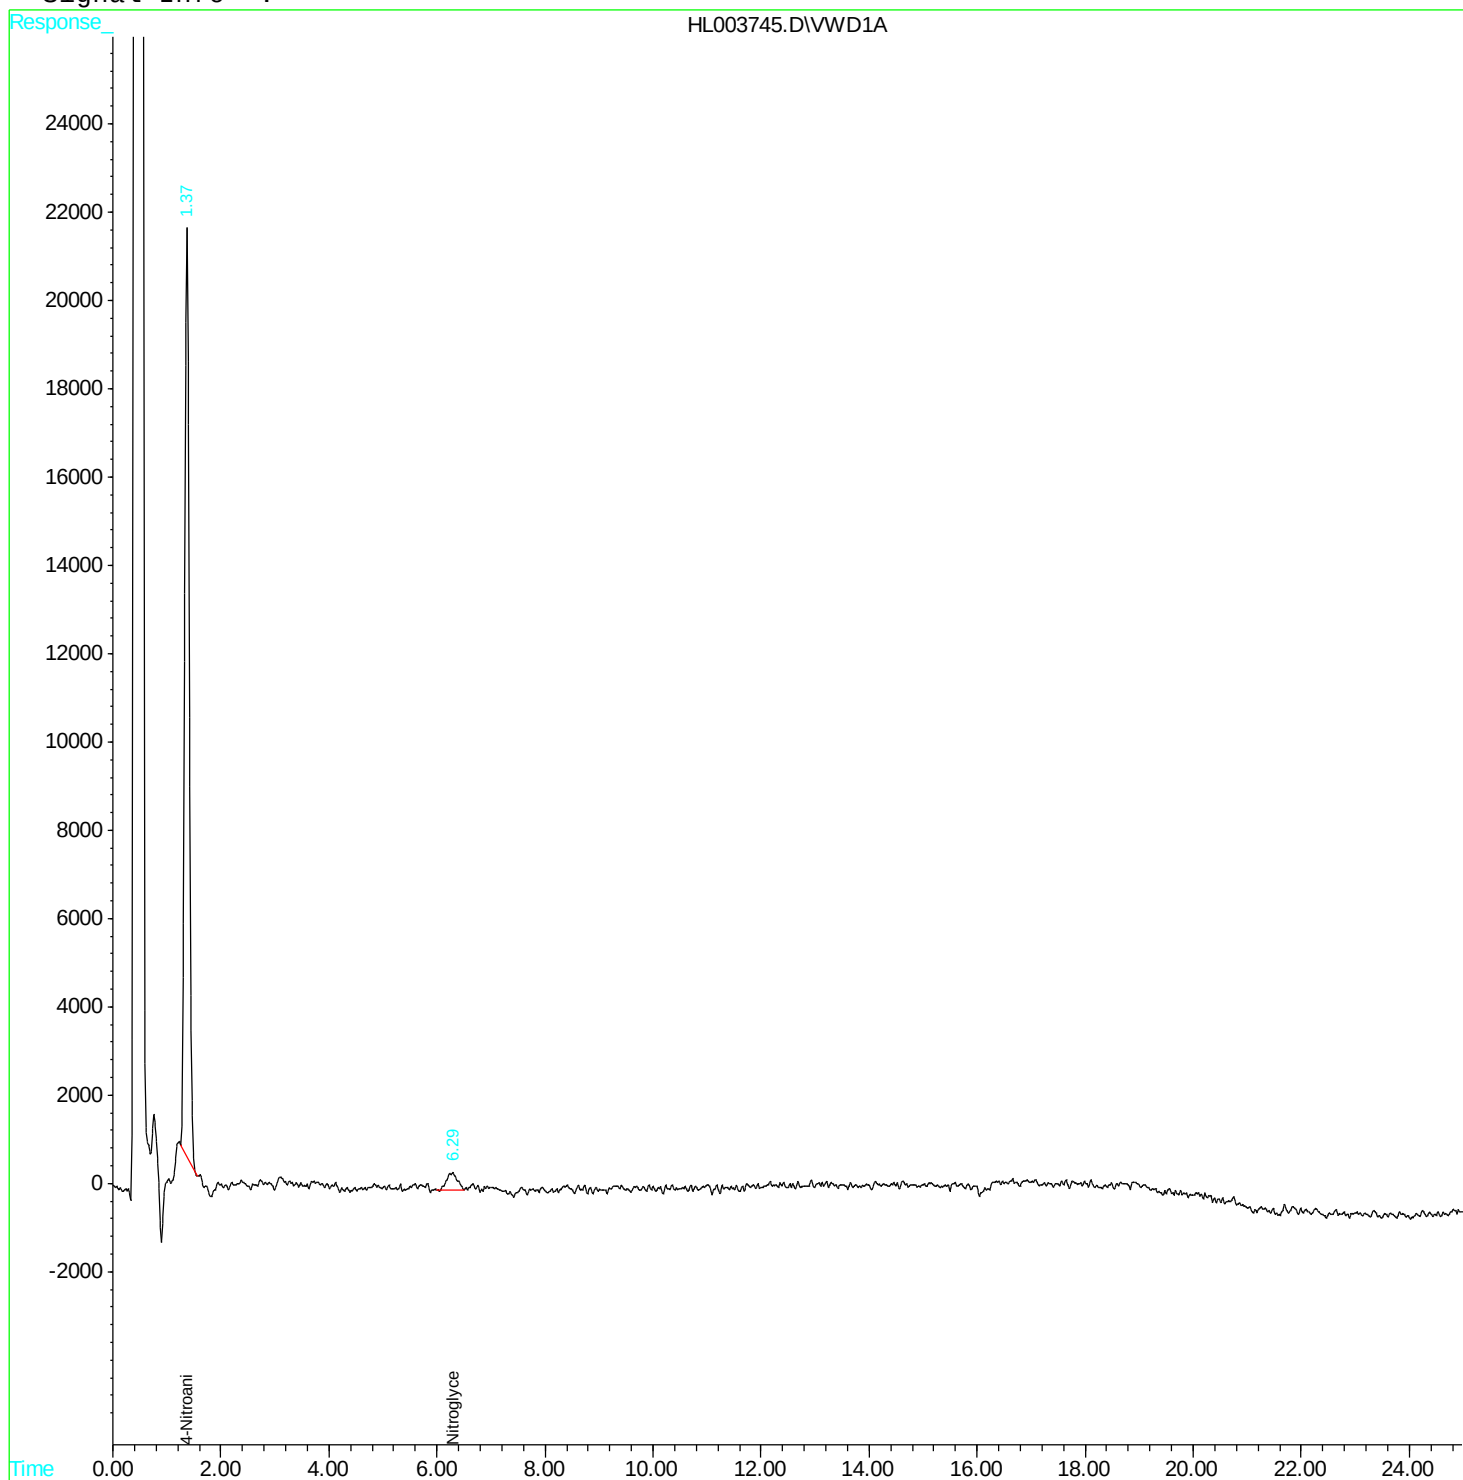

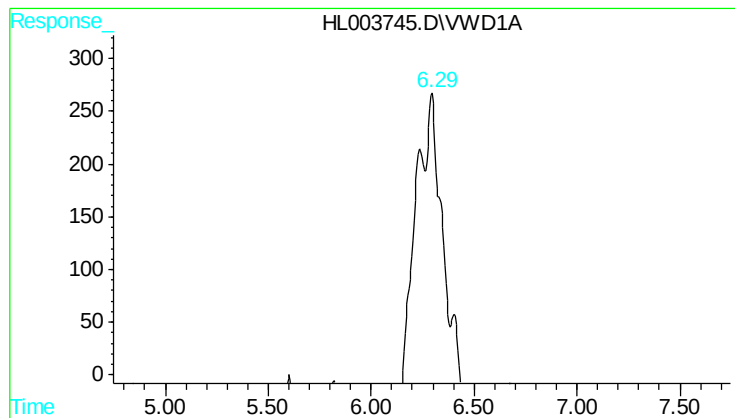

#17 Nitroglycerin

R.T.: 6.296 min
Delta R.T.: 0.024 min
Response: 53460
Conc: 927.87 ug/L