

Data Path : S:\HPCHEM1\HPLC_L\Data\HL111912\
Data File : HL003787.D
Signal(s) : VWD1A.CH
Acq On : 19-Nov-2012, 16:50
Operator : HLM
Sample : 8330-CCV
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
LabSampleId :
8330-CCV

Integration File: events.e
Quant Time: Nov 22 04:04:19 2012
Quant Method : S:\HPCHEM1\HPLC_L\methods\HL102412.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Oct 25 10:56:40 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
8) T	4-Amino-2,6-dinitroto...	6.829f	5597040	775.632 ug/L
9) T	2,4-Dinitrotoluene	7.652f	3640805	228.006 ug/L
14) T	3-Nitrotoluene	13.125f	5605981	777.969 ug/L
16) T	3,5-Dinitroaniline	3.732f	8368599	532.994 ug/L
18) T	PETN	17.606	121008	13.067 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_L\Data\HL111912\
Data File : HL003787.D
Signal(s) : VWD1A.CH
Acq On : 19-Nov-2012, 16:50
Operator : HLM
Sample : 8330-CCV
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
LabSampleId :
8330-CCV

Integration File: events.e
Quant Time: Nov 22 04:04:19 2012
Quant Method : S:\HPCHEM1\HPLC_L\methods\HL102412.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Oct 25 10:56:40 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

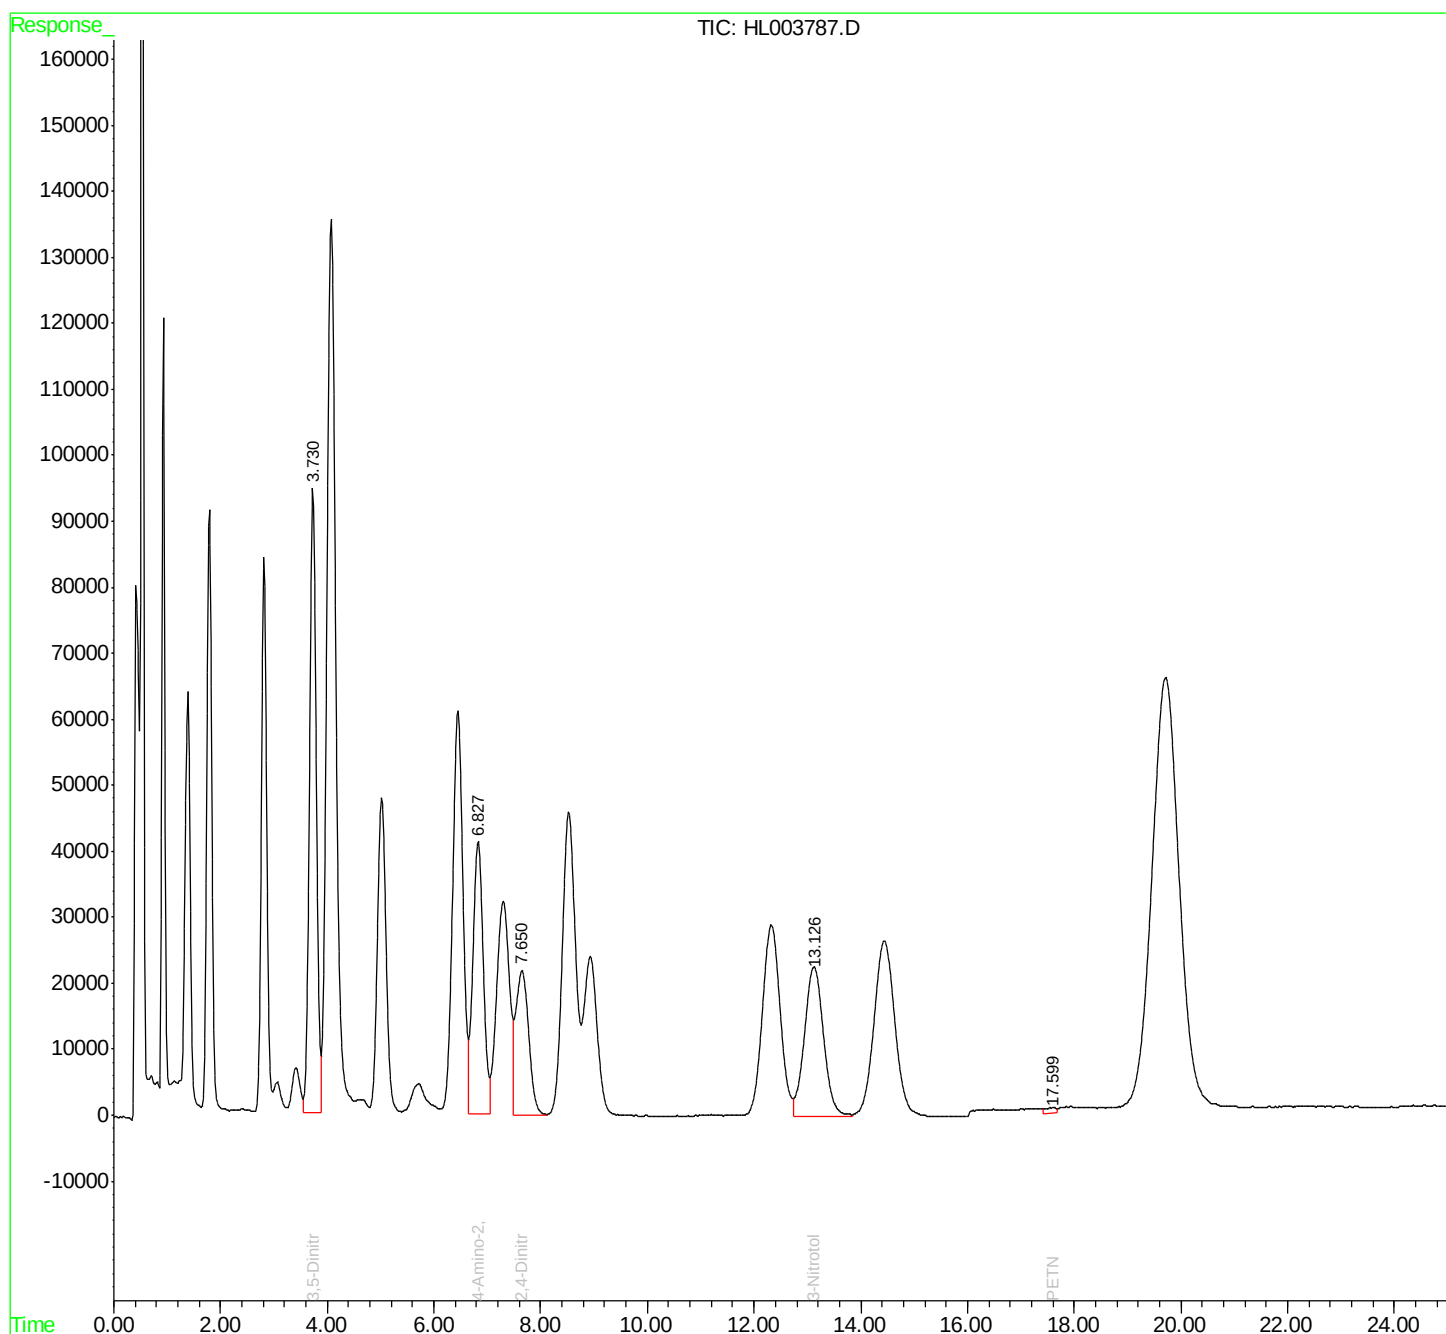


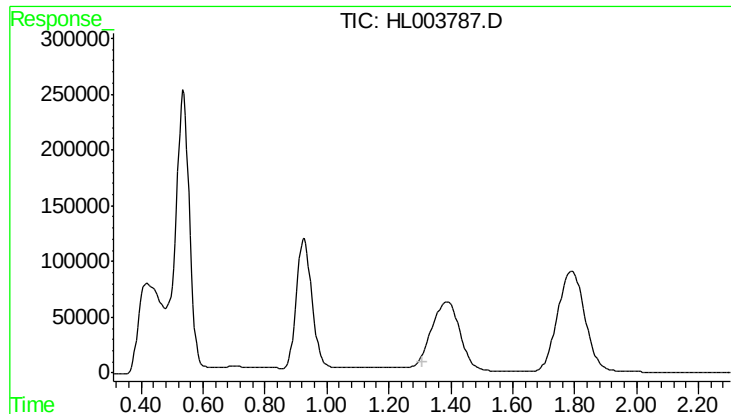

#1 4-Nitroaniline


R.T.: 0.000 min
Exp R.T.: 1.307 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
LabSampleId :
8330-CCV

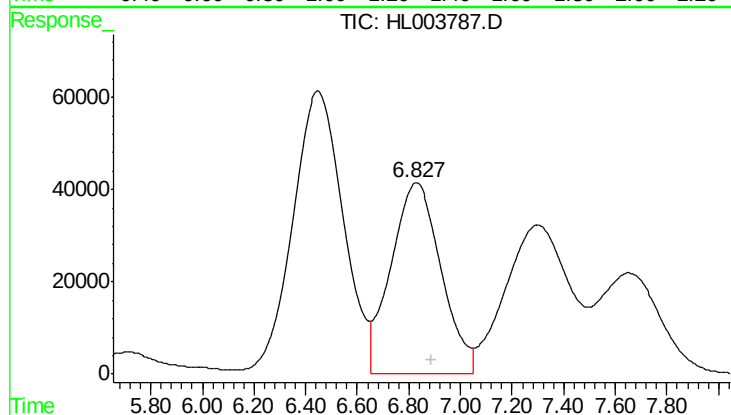


#8 4-Amino-2,6-dinitrotoluene

R.T.: 6.829 min
Delta R.T.: -0.058 min
Response: 5597040
Conc: 775.63 ug/L

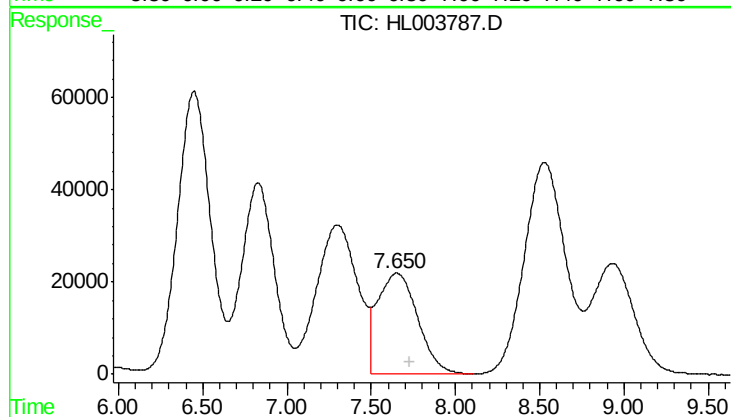


#9 2,4-Dinitrotoluene

R.T.: 7.652 min
Delta R.T.: -0.076 min
Response: 3640805
Conc: 228.01 ug/L

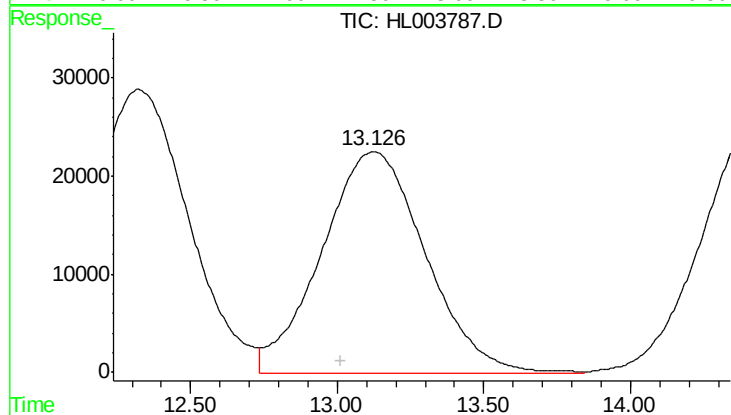

#14 3-Nitrotoluene


R.T.: 13.125 min
Delta R.T.: 0.114 min
Response: 5605981
Conc: 777.97 ug/L

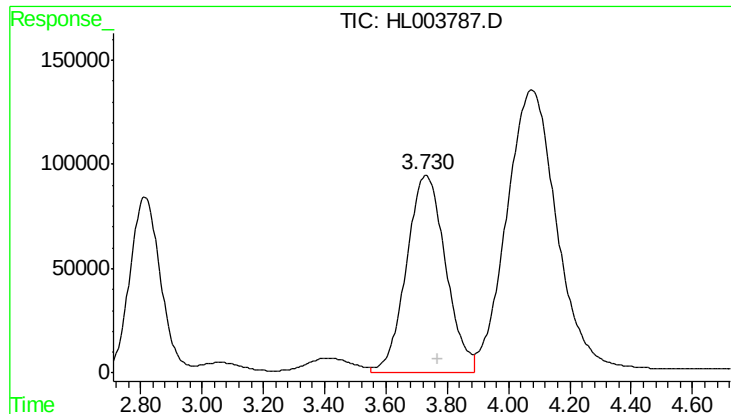

#16 3,5-Dinitroaniline

R.T.: 3.732 min
Delta R.T.: -0.037 min
Response: 8368599
Conc: 532.99 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

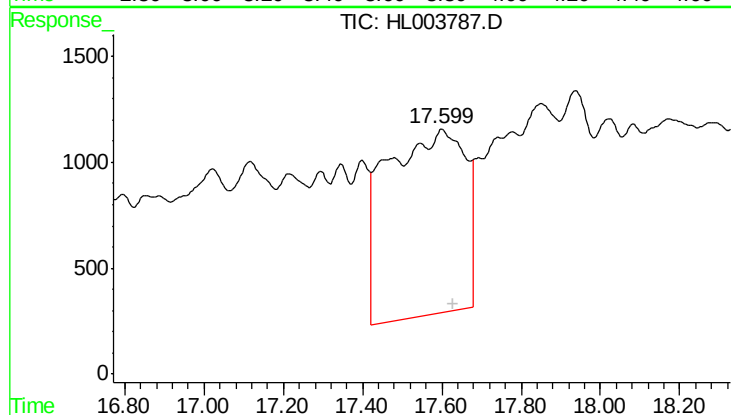

#18 PETN

R.T.: 17.606 min
Delta R.T.: -0.022 min
Response: 121008
Conc: 13.07 ug/L