

Data Path : S:\HPCHEM1\HPLC_L\Data\HL111912\
Data File : HL003790.D
Signal(s) : VWD1A.CH
Acq On : 19-Nov-2012, 18:11
Operator : HLM
Sample : D4768-01MS1
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :

Integration File: events.e
Quant Time: Nov 22 04:04:40 2012
Quant Method : S:\HPCHEM1\HPLC_L\methods\HL102412.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Oct 25 10:56:40 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
8) T	4-Amino-2,6-dinitroto...	6.836f	1253256	173.675 ug/L
9) T	2,4-Dinitrotoluene	7.671f	674774	42.258 ug/L
14) T	3-Nitrotoluene	13.125f	509190	70.663 ug/L
16) T	3,5-Dinitroaniline	3.740f	1340092	85.350 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_L\Data\HL111912\
Data File : HL003790.D
Signal(s) : VWD1A.CH
Acq On : 19-Nov-2012, 18:11
Operator : HLM
Sample : D4768-01MS1
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :

Integration File: events.e
Quant Time: Nov 22 04:04:40 2012
Quant Method : S:\HPCHEM1\HPLC_L\methods\HL102412.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Oct 25 10:56:40 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

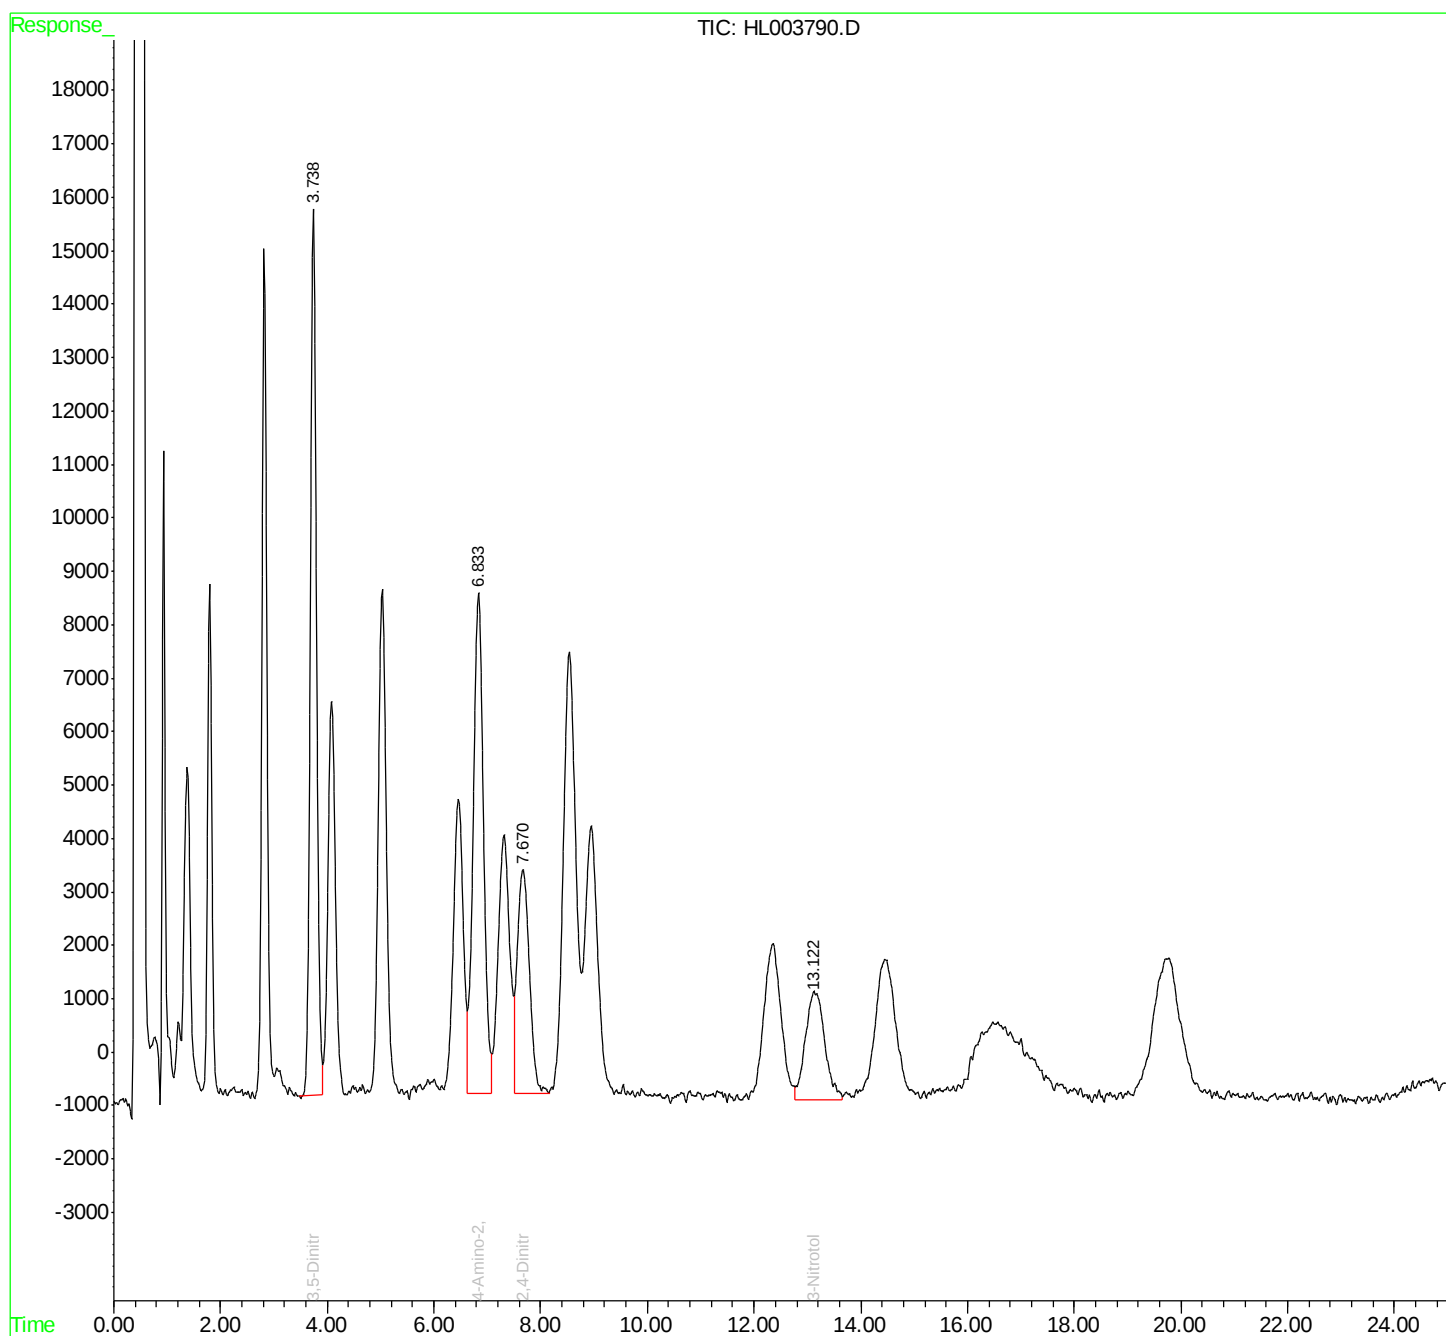


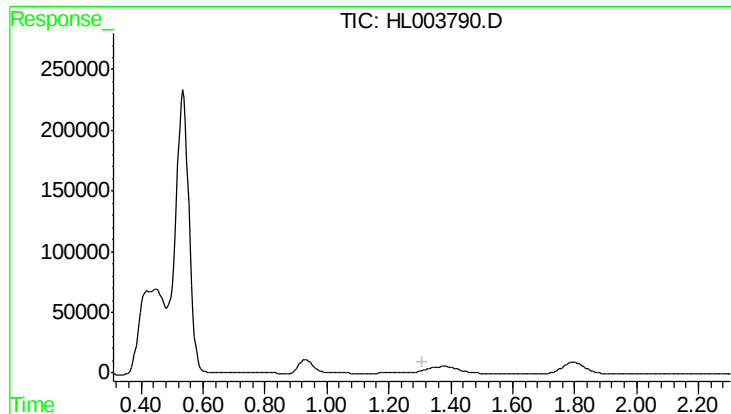

#1 4-Nitroaniline


R.T.: 0.000 min
Exp R.T.: 1.307 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
ClientSampleId :

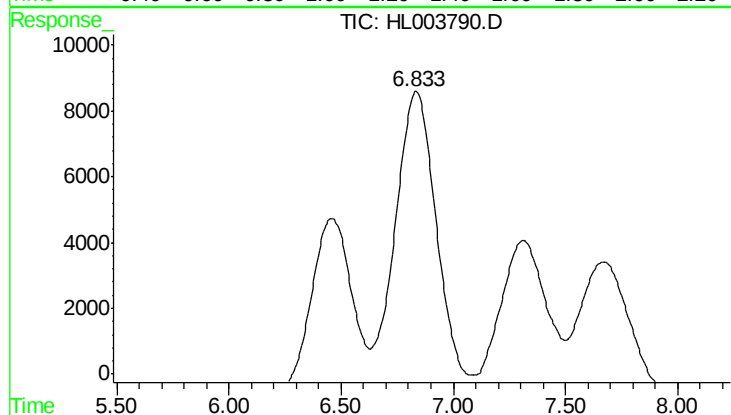


#8 4-Amino-2,6-dinitrotoluene

R.T.: 6.836 min
Delta R.T.: -0.051 min
Response: 1253256
Conc: 173.67 ug/L

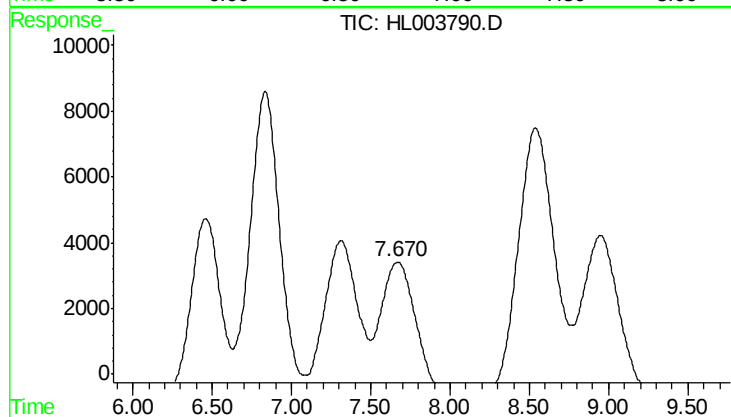


#9 2,4-Dinitrotoluene

R.T.: 7.671 min
Delta R.T.: -0.058 min
Response: 674774
Conc: 42.26 ug/L

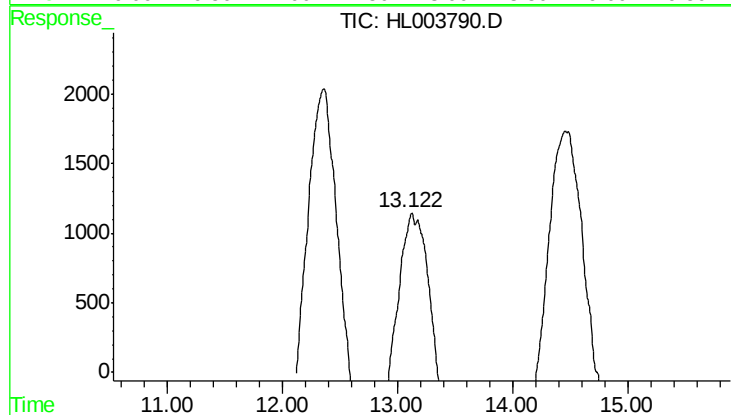

#14 3-Nitrotoluene

R.T.: 13.125 min
Delta R.T.: 0.113 min
Response: 509190
Conc: 70.66 ug/L

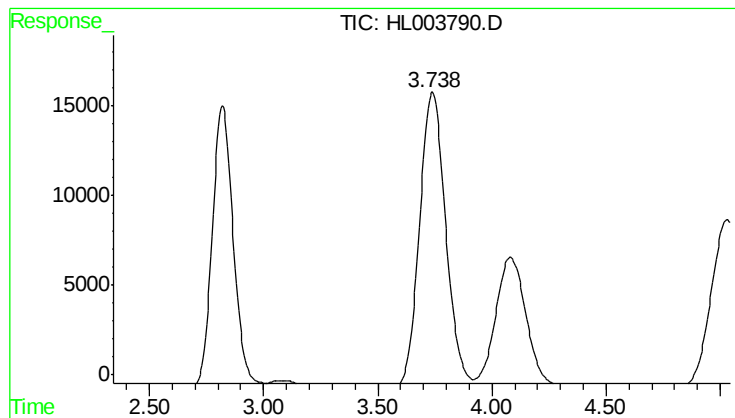

#16 3,5-Dinitroaniline

R.T.: 3.740 min
Delta R.T.: -0.028 min
Response: 1340092
Conc: 85.35 ug/L

Instrument :
HPLC_L
ClientSampleId :