

Data Path : S:\HPCHEM1\HPLC_L\Data\HL111912\
Data File : HL003796.D
Signal(s) : VWD1A.CH
Acq On : 19-Nov-2012, 20:53
Operator : HLM
Sample : 8330-CCV
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :

Integration File: events.e
Quant Time: Nov 22 04:05:21 2012
Quant Method : S:\HPCHEM1\HPLC_L\methods\HL102412.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Oct 25 10:56:40 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
8) T	4-Amino-2,6-dinitroto...	6.832f	5615694	778.217 ug/L
9) T	2,4-Dinitrotoluene	7.658f	3612439	226.229 ug/L
14) T	3-Nitrotoluene	13.128f	5615199	779.248 ug/L
16) T	3,5-Dinitroaniline	3.736f	8395628	534.716 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_L\Data\HL111912\
Data File : HL003796.D
Signal(s) : VWD1A.CH
Acq On : 19-Nov-2012, 20:53
Operator : HLM
Sample : 8330-CCV
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :

Integration File: events.e
Quant Time: Nov 22 04:05:21 2012
Quant Method : S:\HPCHEM1\HPLC_L\methods\HL102412.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Oct 25 10:56:40 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

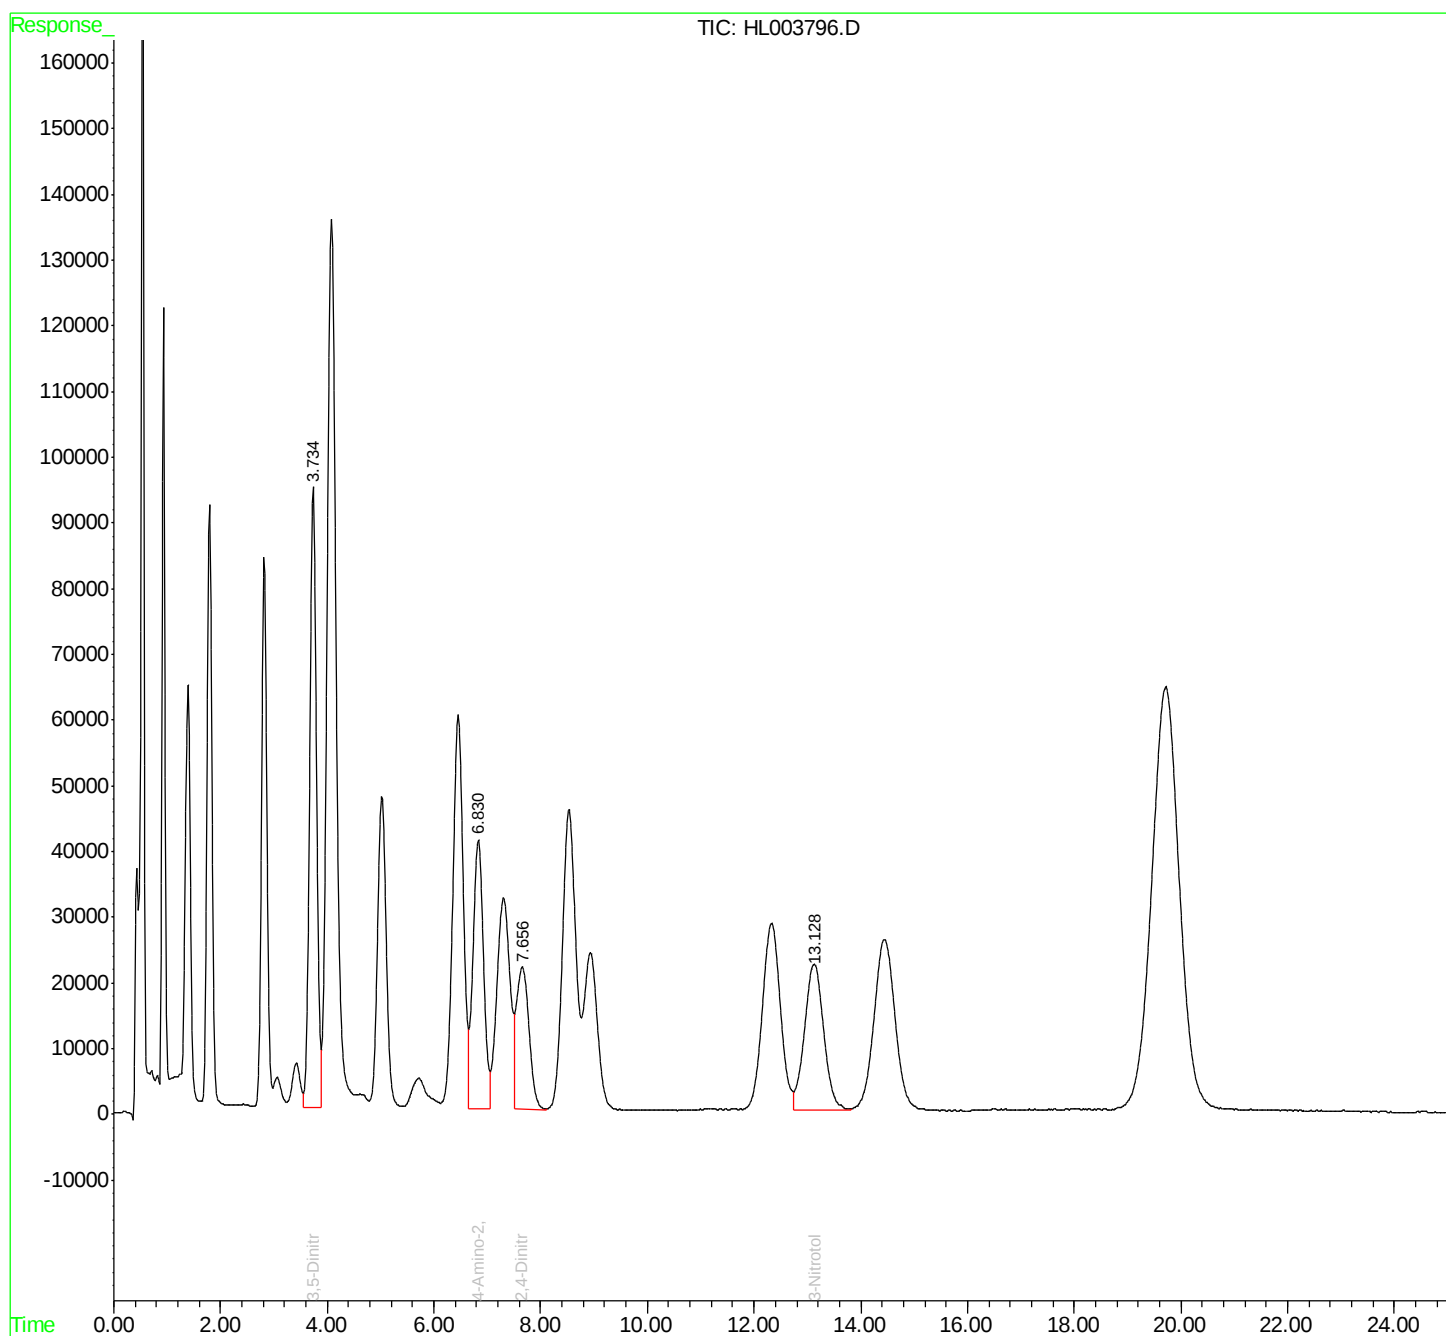


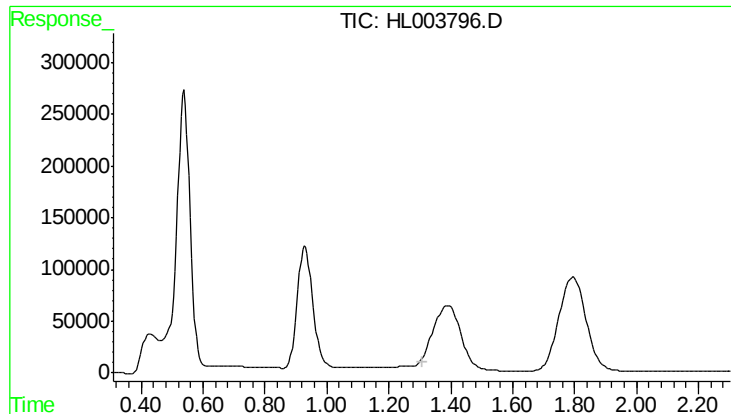

#1 4-Nitroaniline


R.T.: 0.000 min
Exp R.T.: 1.307 min
Response: 0
Conc: N.D.

Instrument :
HPLC_L
ClientSampleId :

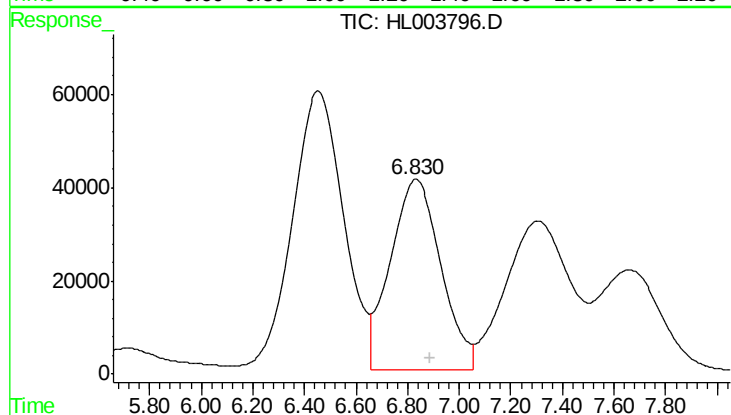


#8 4-Amino-2,6-dinitrotoluene

R.T.: 6.832 min
Delta R.T.: -0.054 min
Response: 5615694
Conc: 778.22 ug/L

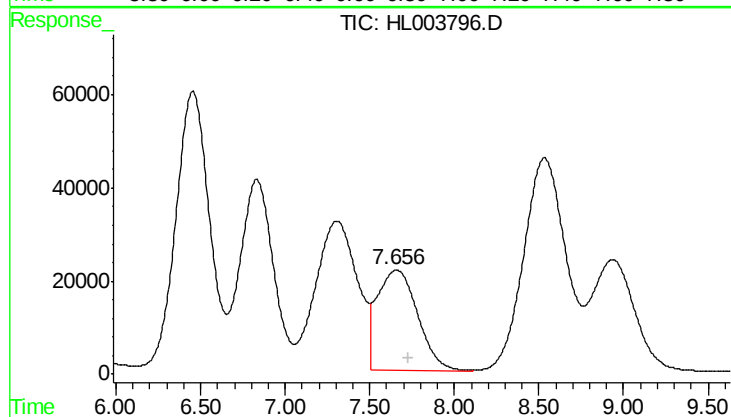


#9 2,4-Dinitrotoluene

R.T.: 7.658 min
Delta R.T.: -0.070 min
Response: 3612439
Conc: 226.23 ug/L

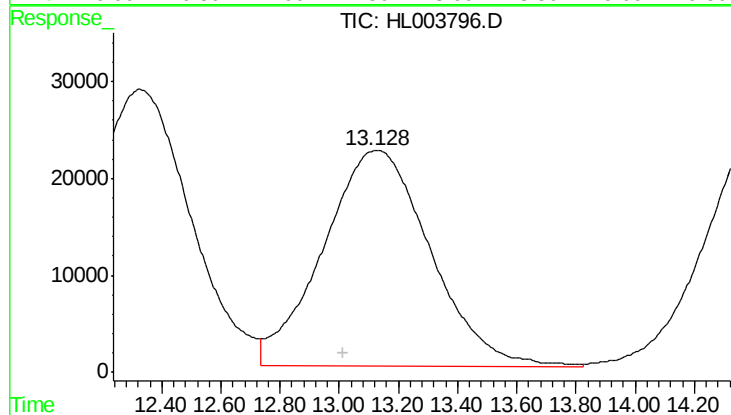

#14 3-Nitrotoluene

R.T.: 13.128 min
Delta R.T.: 0.117 min
Response: 5615199
Conc: 779.25 ug/L

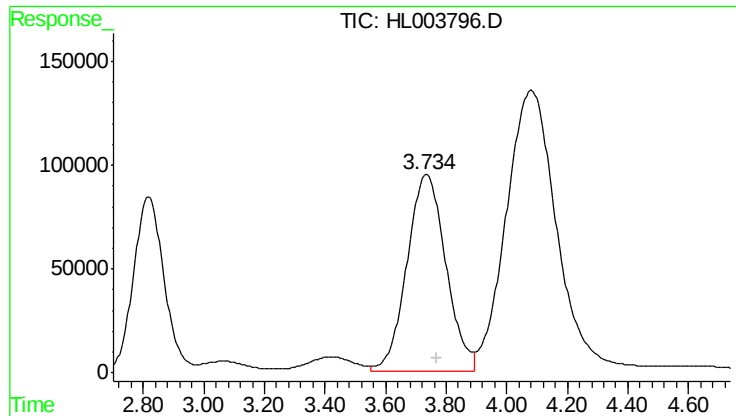

#16 3,5-Dinitroaniline

R.T.: 3.736 min
Delta R.T.: -0.033 min
Response: 8395628
Conc: 534.72 ug/L

Instrument :
HPLC_L
ClientSampleId :