

Data File : H:\VOL1\HPLC\HPLC L\121119\HL003787.D Vial: 2
 Acq On : 19-Nov-2012, 16:50 Operator: HLM
 Sample : 8330-CCV Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Nov 19 19:02 2012 Quant Results File: HL102412.RES

Instrument :
 HPLC_L
 LabSampleId :
 8330-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL102412.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Mon Nov 19 19:01:42 2012
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.39	3759927	939.058 ug/L
Spiked Amount 300.000 Range 37 - 149		Recovery	=	313.02%#

Target Compounds

2) T	HMX	0.93	4045622	999.035 ug/L
3) T	RDX	1.79	5633334	1046.625 ug/L
4) T	1,3,5-Trinitrobenzene	2.81	5820864	490.661 ug/L
5) T	Tetryl	6.45	8290456	973.564 ug/L
6) T	2,4,6-Trinitrotoluene	6.83	5597040	491.194 ug/L
7) T	2-Amino-4,6-dinitrotoluene	7.30	5501087	507.399 ug/L
8) T	4-Amino-2,6-dinitrotoluene	7.65	3640805	504.539 ug/L
9) T	2,4-Dinitrotoluene	8.53	7803346	488.685 ug/L
10) T	2,6-Dinitrotoluene	8.93	4229509	490.728 ug/L
11) T	1,3-Dinitrobenzene	3.73	8368599	505.790 ug/L
12) T	Nitrobenzene	5.02	5327820	497.826 ug/L
13) T	2-Nitrotoluene	12.32	6688391	987.488 ug/L
14) T	3-Nitrotoluene	14.44	7171877	995.275 ug/L
15) T	4-Nitrotoluene	13.13	5605981	963.965 ug/L
16) T	3,5-Dinitroaniline	4.08	15679129	998.600 ug/L
18) T	PETN	19.72	23251477	2510.758 ug/L

Data File : H:\VOL1\HPLC\HPLC L\121119\HL003787.D

Vial: 2

Acq On : 19-Nov-2012, 16:50

Operator: HLM

Sample : 8330-CCV

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Nov 19 19:02 2012 Quant Results File: HL102412.RES

Instrument :

HPLC_L

LabSampleId :

8330-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL102412.M (Chemstation Integrator)

Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)

Last Update : Mon Nov 19 19:01:42 2012


Response via : Multiple Level Calibration


DataAcq Meth : 8330AGIP.M

Volume Inj. :

Signal Phase :

Signal Info :

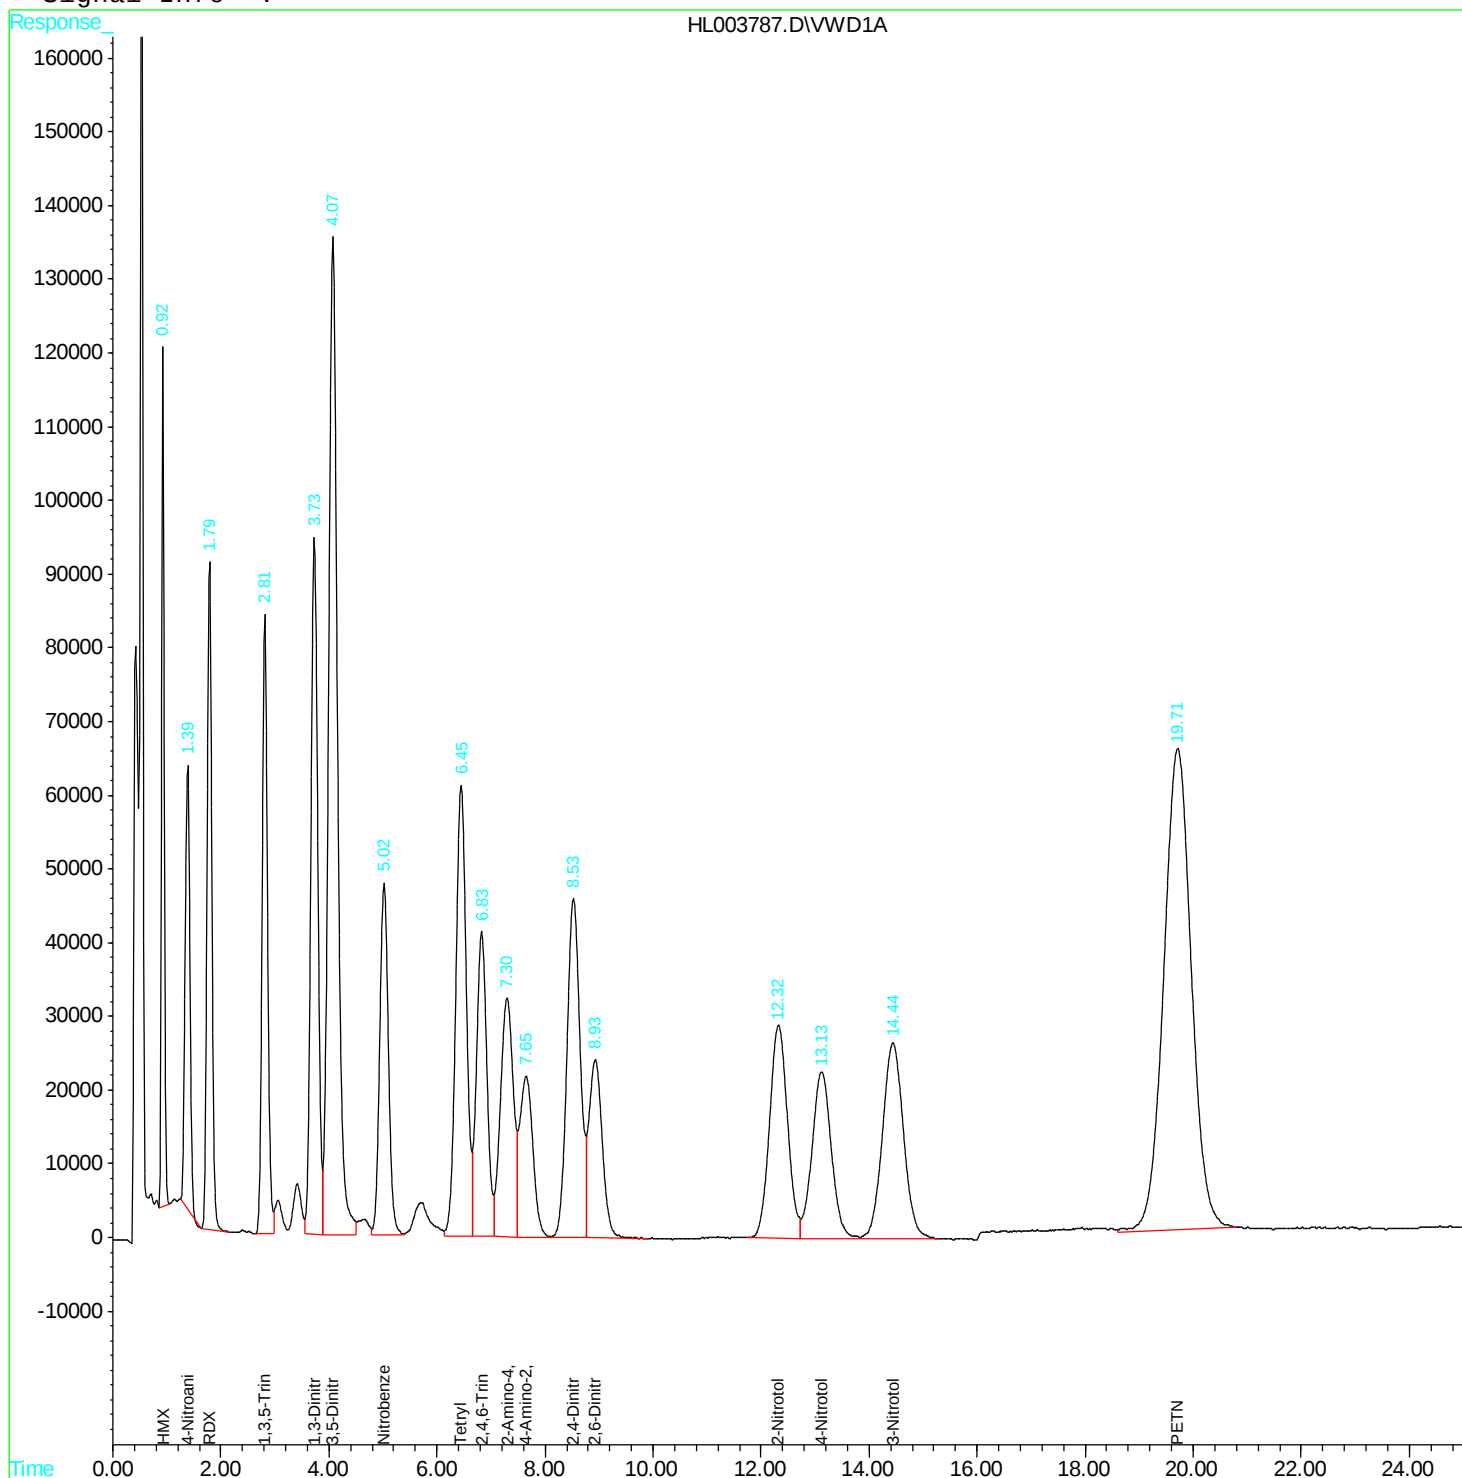


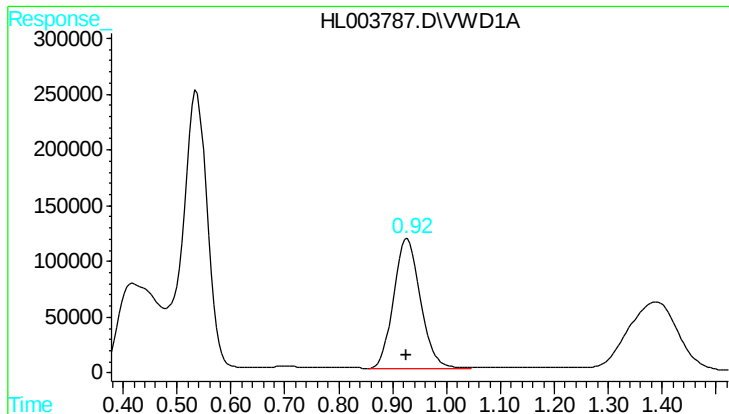

#2 HMX


R.T.: 0.927 min
Delta R.T.: 0.001 min
Response: 4045622
Conc: 999.04 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

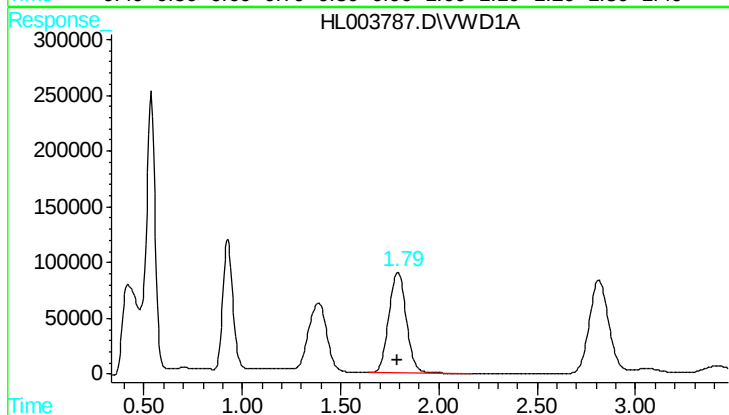


#3 RDX

R.T.: 1.792 min
Delta R.T.: 0.001 min
Response: 5633334
Conc: 1046.63 ug/L

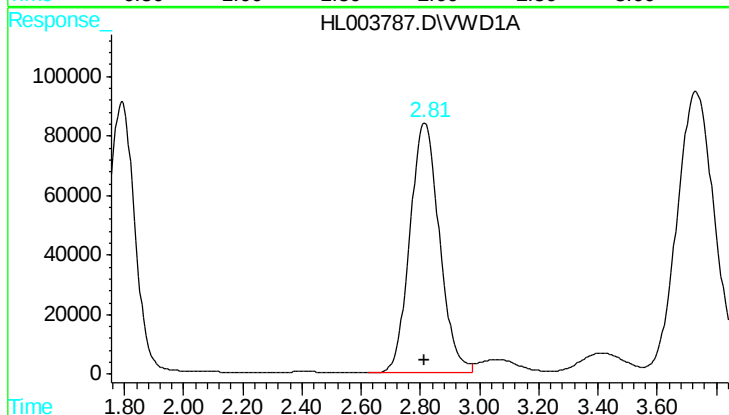


#4 1,3,5-Trinitrobenzene

R.T.: 2.815 min
Delta R.T.: 0.001 min
Response: 5820864
Conc: 490.66 ug/L

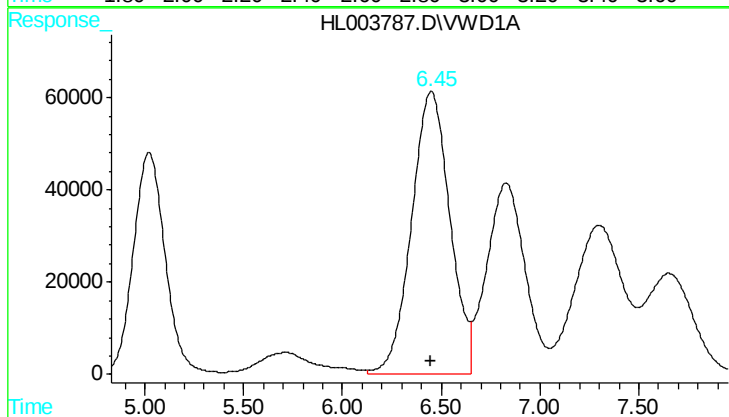

#5 Tetryl


R.T.: 6.449 min
Delta R.T.: 0.003 min
Response: 8290456
Conc: 973.56 ug/L

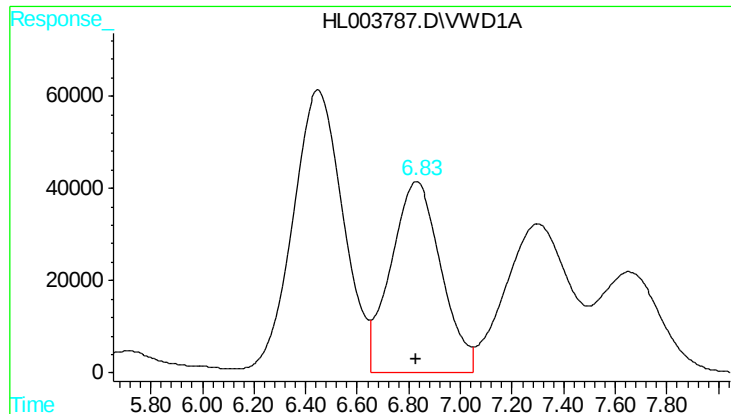

#6 2,4,6-Trinitrotoluene


R.T.: 6.829 min
Delta R.T.: 0.003 min
Response: 5597040
Conc: 491.19 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

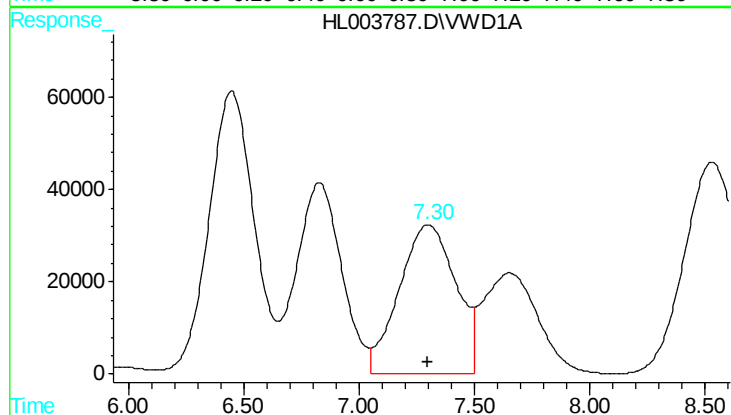


#7 2-Amino-4,6-dinitrotoluene

R.T.: 7.300 min
Delta R.T.: 0.003 min
Response: 5501087
Conc: 507.40 ug/L

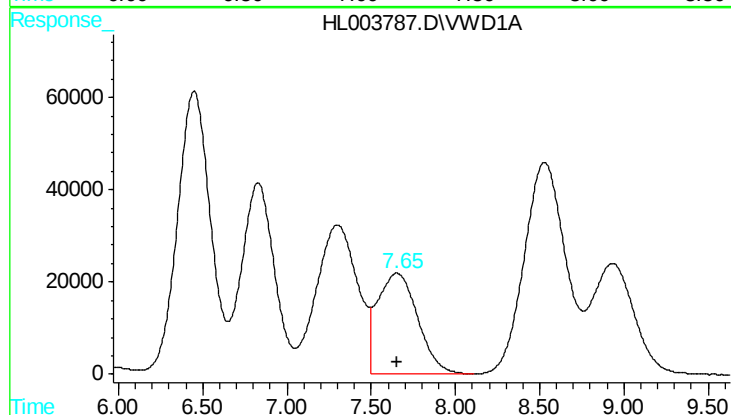


#8 4-Amino-2,6-dinitrotoluene

R.T.: 7.652 min
Delta R.T.: 0.000 min
Response: 3640805
Conc: 504.54 ug/L

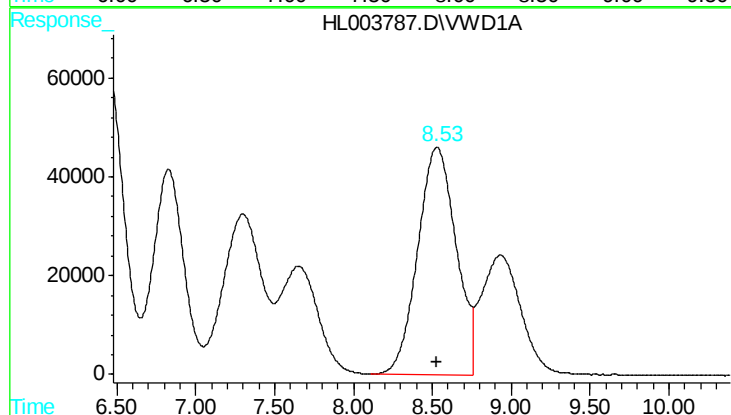

#9 2,4-Dinitrotoluene


R.T.: 8.529 min
Delta R.T.: 0.002 min
Response: 7803346
Conc: 488.68 ug/L

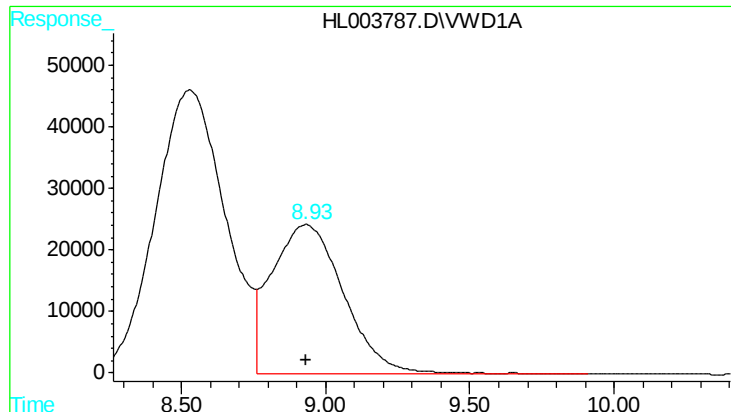

#10 2,6-Dinitrotoluene


R.T.: 8.932 min
Delta R.T.: 0.002 min
Response: 4229509
Conc: 490.73 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

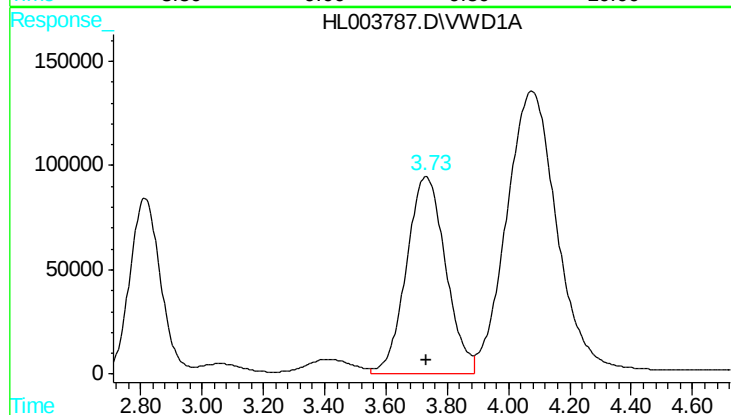


#11 1,3-Dinitrobenzene

R.T.: 3.732 min
Delta R.T.: 0.001 min
Response: 8368599
Conc: 505.79 ug/L

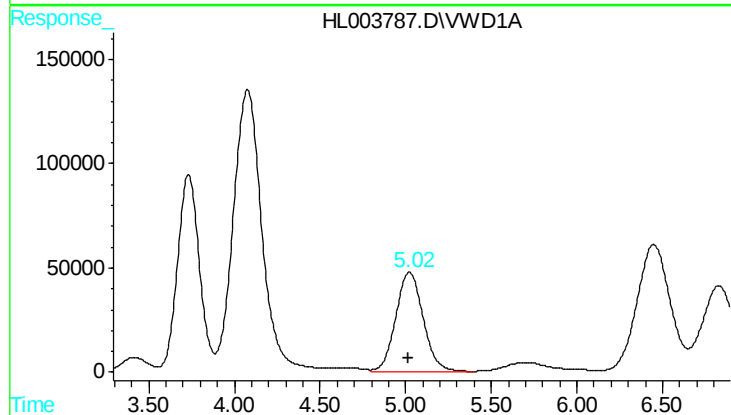


#12 Nitrobenzene

R.T.: 5.022 min
Delta R.T.: 0.002 min
Response: 5327820
Conc: 497.83 ug/L

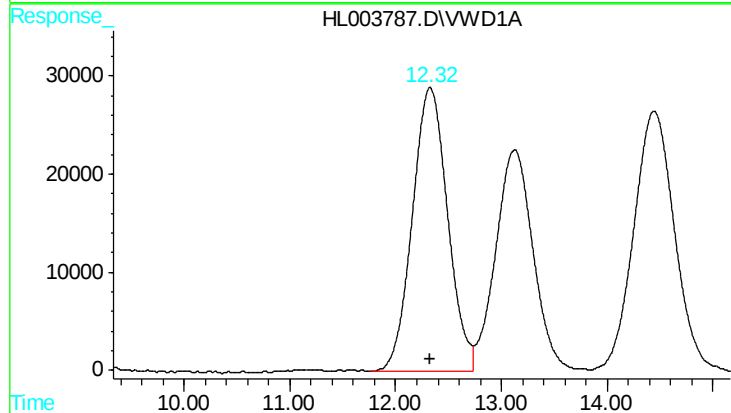

#13 2-Nitrotoluene


R.T.: 12.323 min
Delta R.T.: 0.000 min
Response: 6688391
Conc: 987.49 ug/L

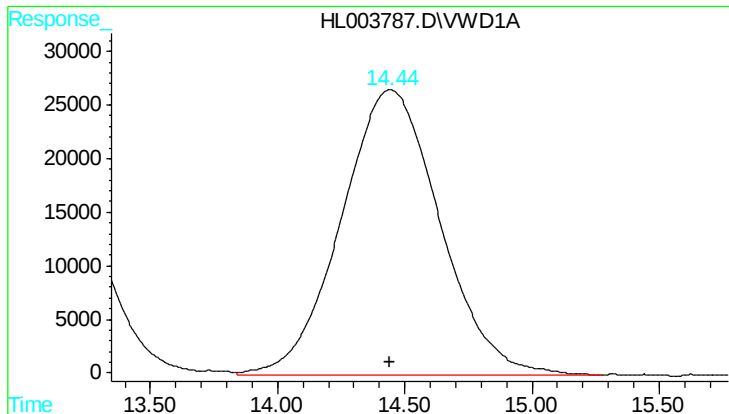

#14 3-Nitrotoluene


R.T.: 14.444 min
Delta R.T.: 0.001 min
Response: 7171877
Conc: 995.28 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

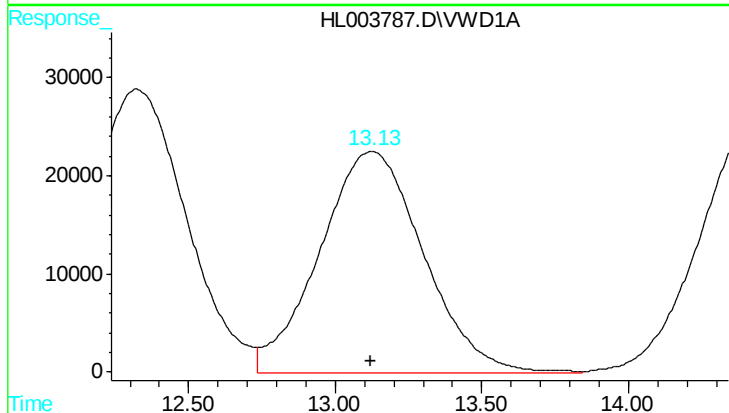


#15 4-Nitrotoluene

R.T.: 13.125 min
Delta R.T.: 0.004 min
Response: 5605981
Conc: 963.97 ug/L

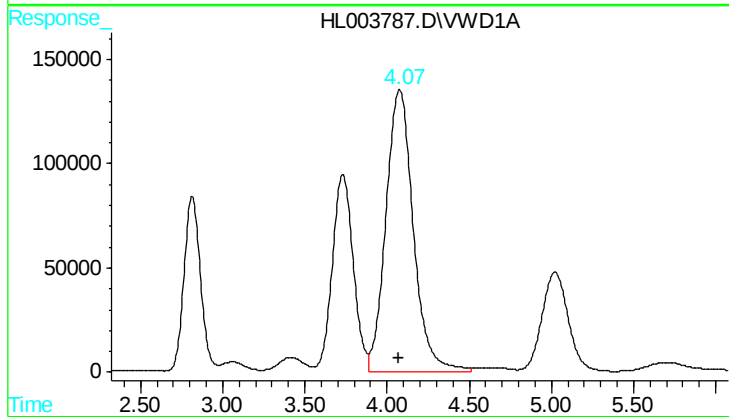

#16 3,5-Dinitroaniline

R.T.: 4.077 min
Delta R.T.: 0.002 min
Response: 15679129
Conc: 998.60 ug/L

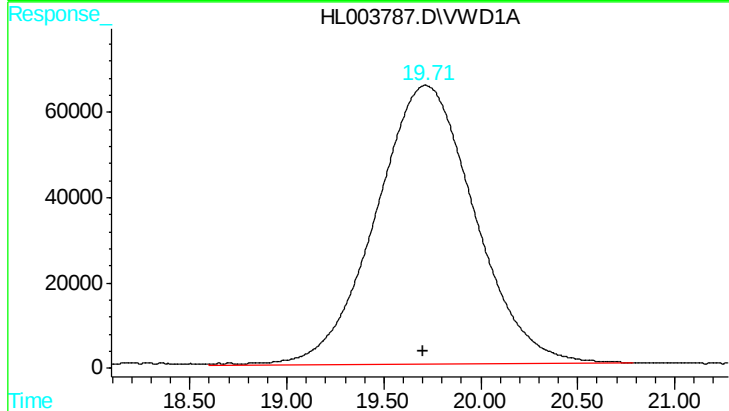

#18 PETN

R.T.: 19.716 min
Delta R.T.: 0.010 min
Response: 23251477
Conc: 2510.76 ug/L