

Data Path : S:\HPCHEM1\HPLC_L\Data\HL111912\
 Data File : HL003796.D
 Signal(s) : VWD1A.CH
 Acq On : 19-Nov-2012, 20:53
 Operator : HLM
 Sample : 8330-CCV
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 HPLC_L
 ClientSampleId :

Integration File: events.e
 Quant Time: Nov 22 03:50:50 2012
 Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL102412.M
 Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 QLast Update : Tue Nov 20 11:37:40 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.392	4323873	1085.514 ug/L
Spiked Amount 300.000	Range 37 - 149	Recovery	= 361.84%#
Target Compounds			
2) T HMX	0.930	4137660	1021.591 ug/L
3) T RDX	1.795	5612704	1042.792 ug/L
4) T 1,3,5-Trinitrobenzene	2.818	5837946	492.101 ug/L
5) T Tetryl	6.454	8242312	967.910 ug/L
6) T 2,4,6-Trinitrotoluene	6.832	5615694	492.831 ug/L
7) T 2-Amino-4,6-dinitroto...	7.305	5513495	508.544 ug/L
8) T 4-Amino-2,6-dinitroto...	7.658	3612439	500.608 ug/L
9) T 2,4-Dinitrotoluene	8.533	7839576	490.954 ug/L
10) T 2,6-Dinitrotoluene	8.936	4195393	486.769 ug/L
11) T 1,3-Dinitrobenzene	3.736	8395628	507.424 ug/L
12) T Nitrobenzene	5.025	5342334	499.182 ug/L
13) T 2-Nitrotoluene	12.328	6665780	984.150 ug/L
14) T 3-Nitrotoluene	14.446	7195514	998.555 ug/L
15) T 4-Nitrotoluene	13.128	5615199	965.550 ug/L
16) T 3,5-Dinitroaniline	4.081	15745885	1002.852 ug/L
18) T PETN	19.720	23005224	2484.167 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_L\Data\HL111912\
Data File : HL003796.D
Signal(s) : VWD1A.CH
Acq On : 19-Nov-2012, 20:53
Operator : HLM
Sample : 8330-CCV
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :

Integration File: events.e
Quant Time: Nov 22 03:50:50 2012
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL102412.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Tue Nov 20 11:37:40 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

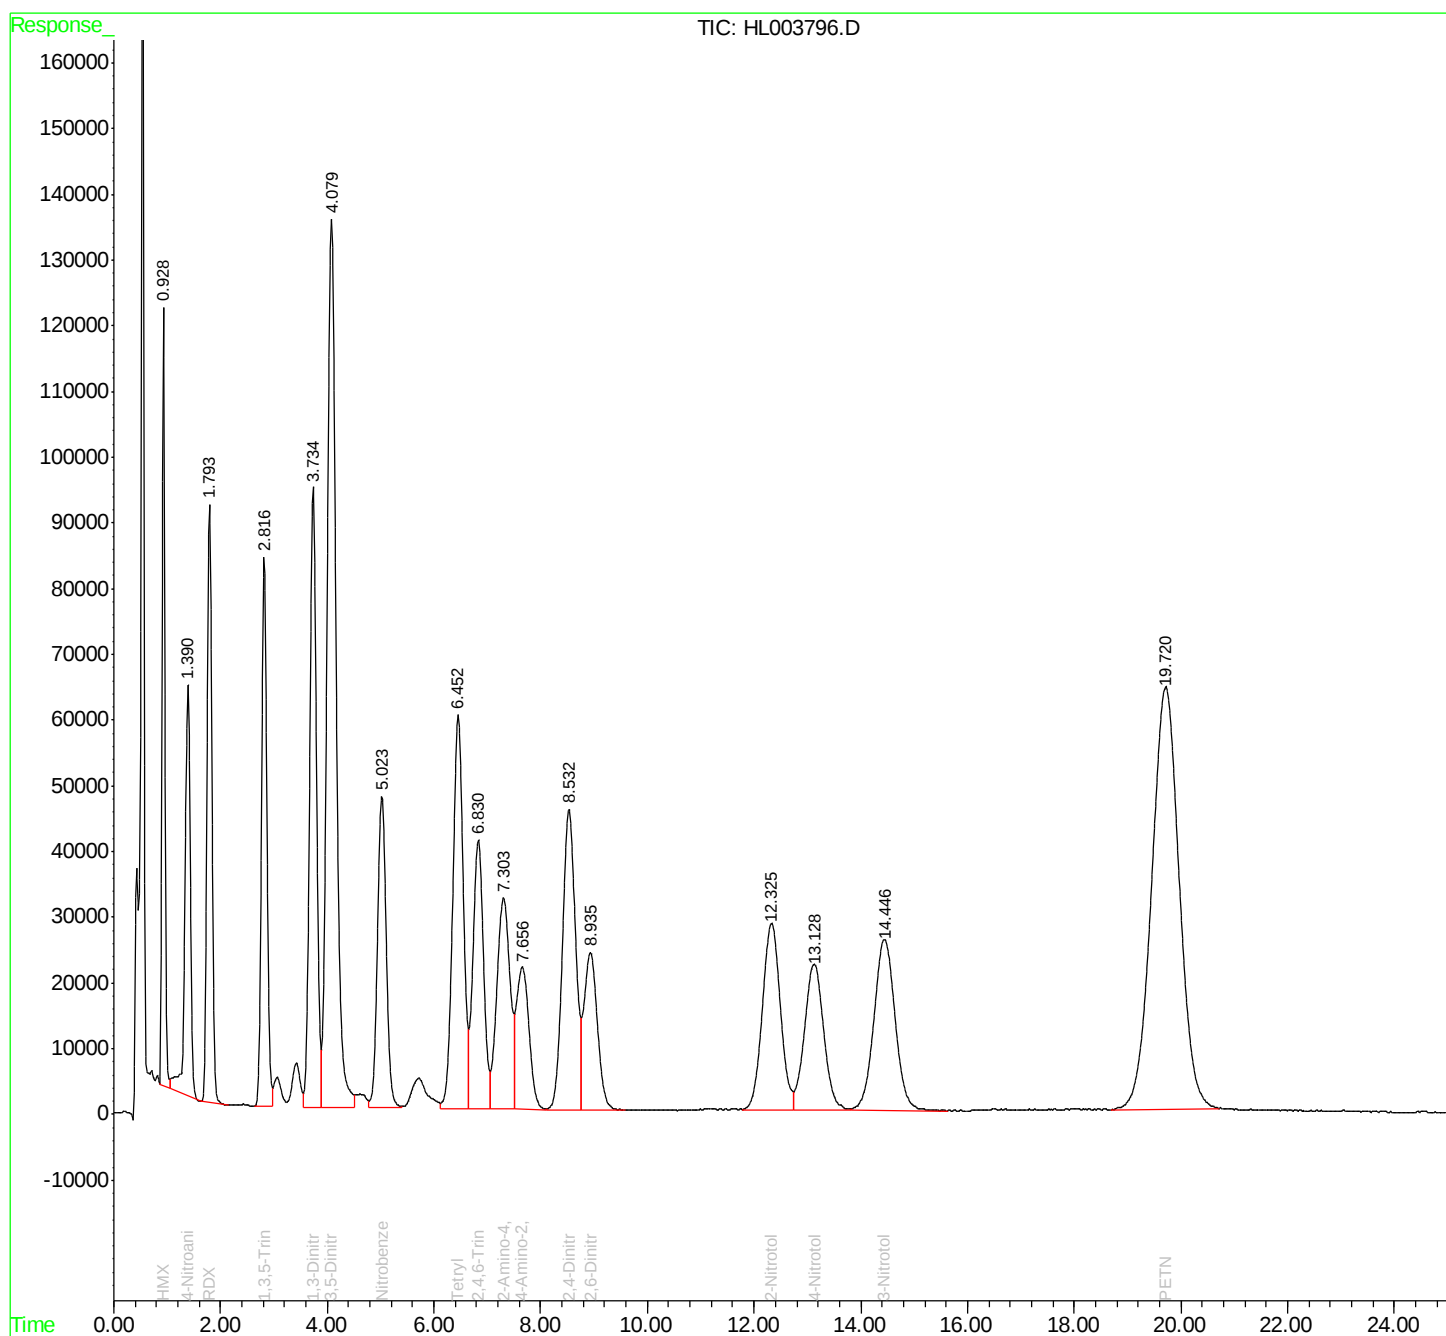


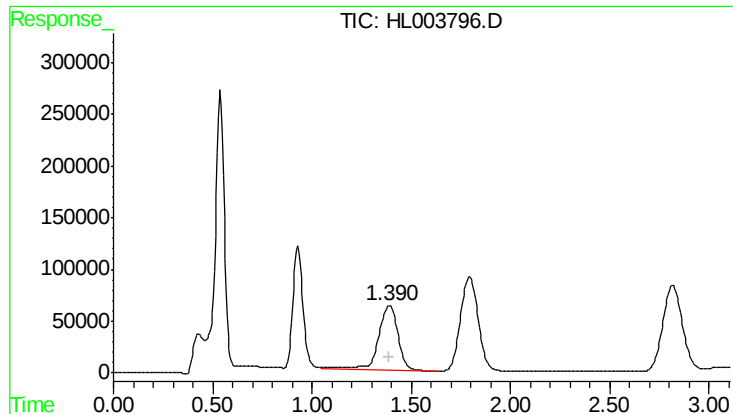

#1 4-Nitroaniline


R.T.: 1.392 min
Delta R.T.: 0.003 min
Response: 4323873
Conc: 1085.51 ug/L

Instrument :
HPLC_L
ClientSampleId :

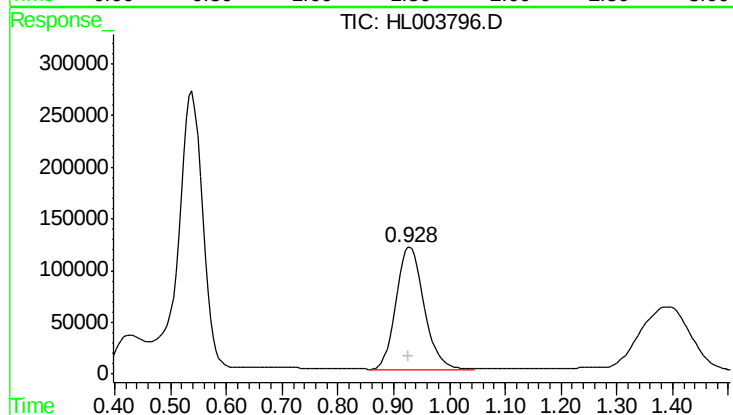


#2 HMX

R.T.: 0.930 min
Delta R.T.: 0.003 min
Response: 4137660
Conc: 1021.59 ug/L

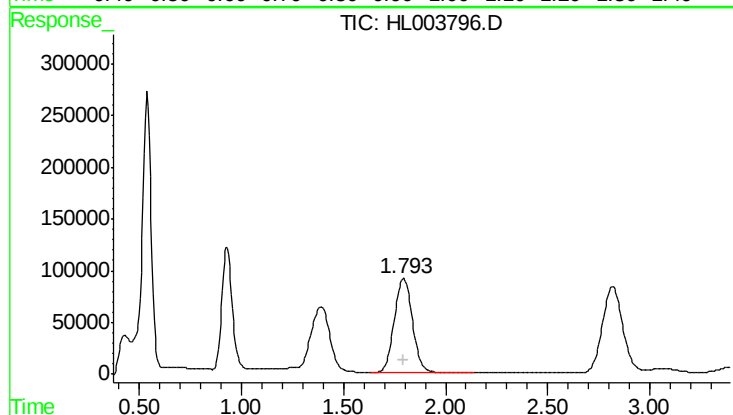


#3 RDX

R.T.: 1.795 min
Delta R.T.: 0.004 min
Response: 5612704
Conc: 1042.79 ug/L

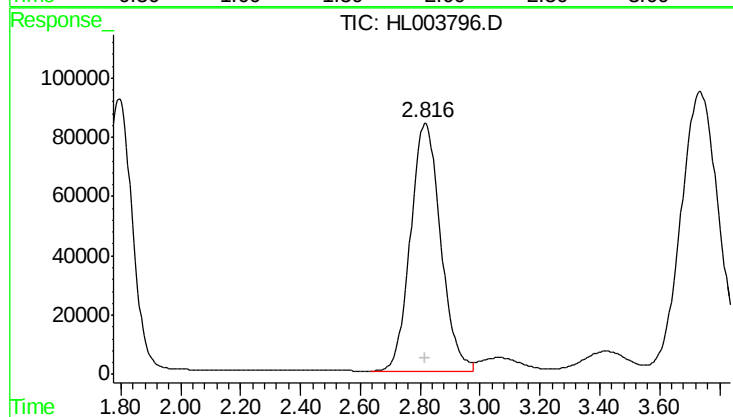

#4 1,3,5-Trinitrobenzene


R.T.: 2.818 min
Delta R.T.: 0.004 min
Response: 5837946
Conc: 492.10 ug/L

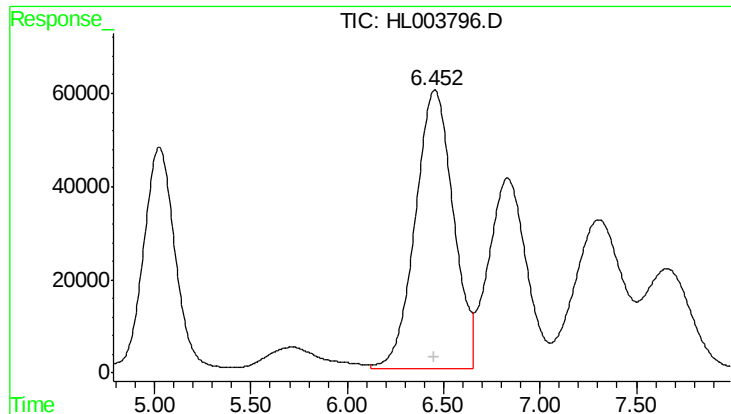

#5 Tetryl


R.T.: 6.454 min
Delta R.T.: 0.006 min
Response: 8242312
Conc: 967.91 ug/L

Instrument :
HPLC_L
ClientSampleId :

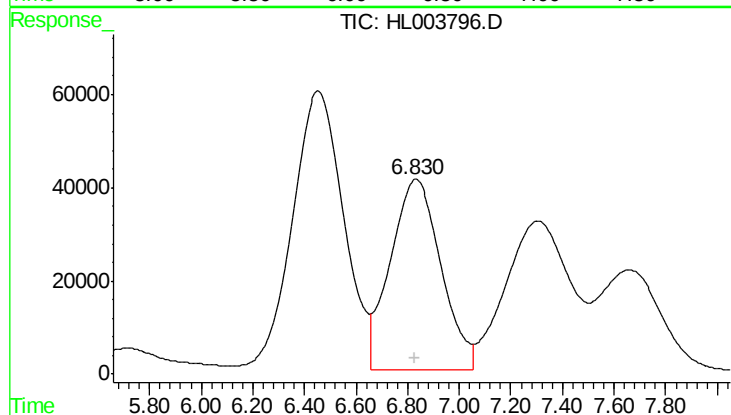


#6 2,4,6-Trinitrotoluene

R.T.: 6.832 min
Delta R.T.: 0.003 min
Response: 5615694
Conc: 492.83 ug/L

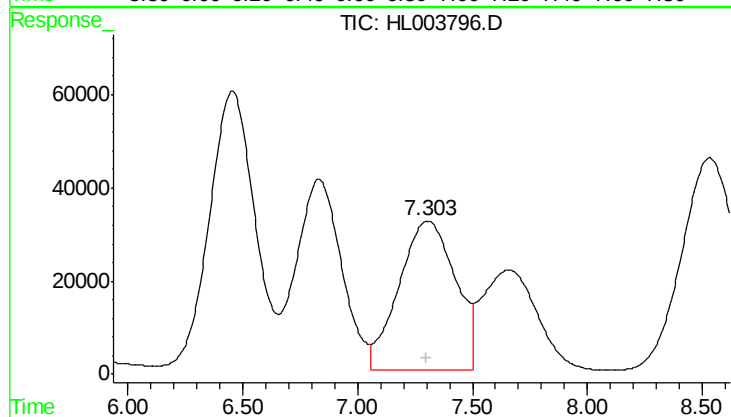


#7 2-Amino-4,6-dinitrotoluene

R.T.: 7.305 min
Delta R.T.: 0.006 min
Response: 5513495
Conc: 508.54 ug/L

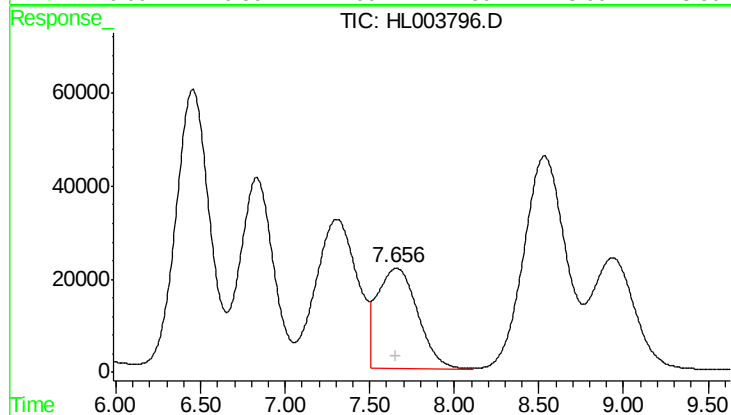

#8 4-Amino-2,6-dinitrotoluene


R.T.: 7.658 min
Delta R.T.: 0.006 min
Response: 3612439
Conc: 500.61 ug/L

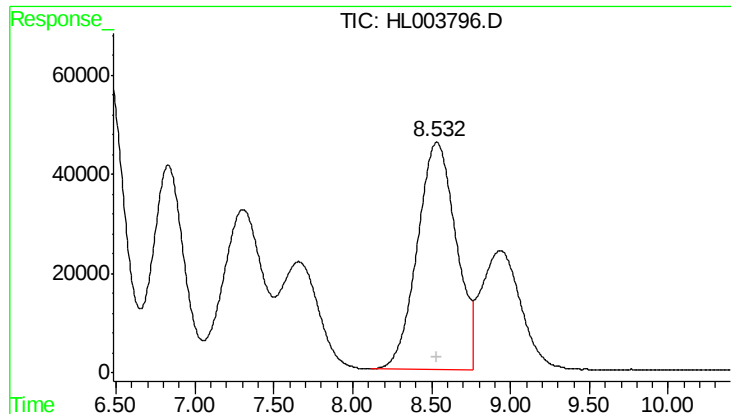

#9 2,4-Dinitrotoluene


R.T.: 8.533 min
Delta R.T.: 0.004 min
Response: 7839576
Conc: 490.95 ug/L

Instrument :
HPLC_L
ClientSampleId :

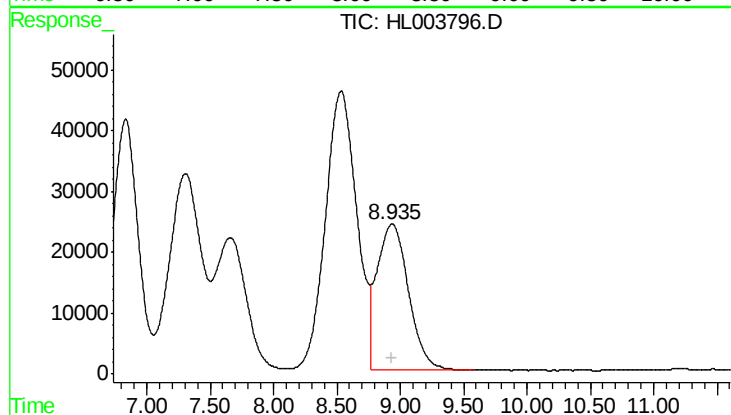


#10 2,6-Dinitrotoluene

R.T.: 8.936 min
Delta R.T.: 0.004 min
Response: 4195393
Conc: 486.77 ug/L

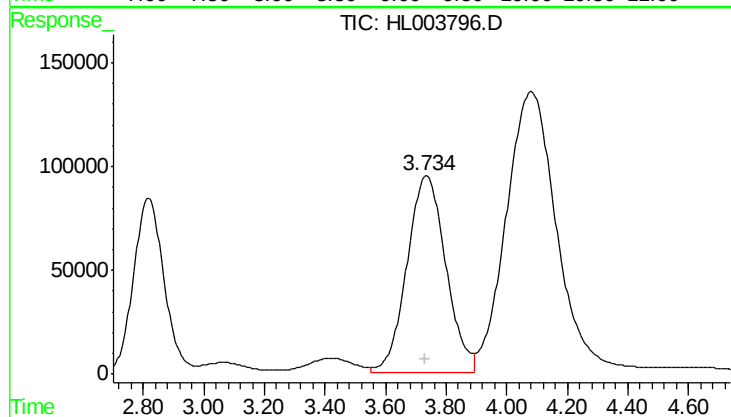


#11 1,3-Dinitrobenzene

R.T.: 3.736 min
Delta R.T.: 0.004 min
Response: 8395628
Conc: 507.42 ug/L

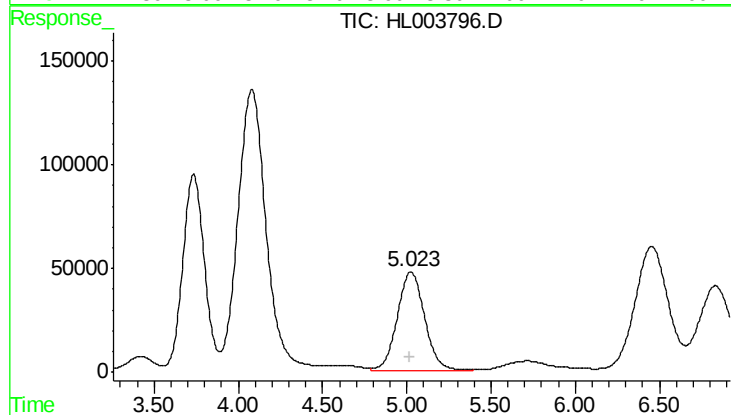

#12 Nitrobenzene


R.T.: 5.025 min
Delta R.T.: 0.003 min
Response: 5342334
Conc: 499.18 ug/L

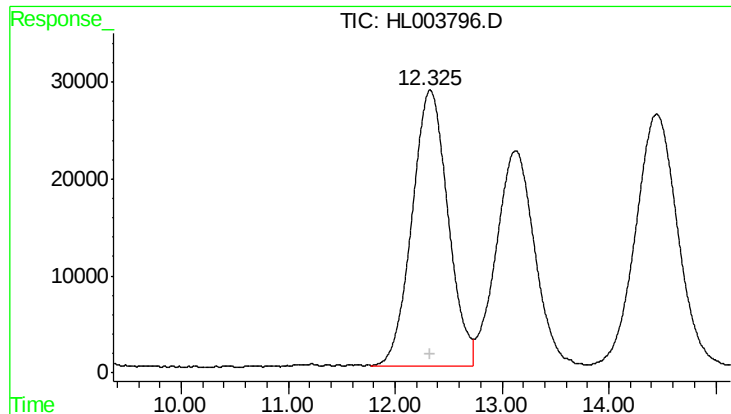

#13 2-Nitrotoluene


R.T.: 12.328 min
Delta R.T.: 0.005 min
Response: 6665780
Conc: 984.15 ug/L

Instrument :
HPLC_L
ClientSampleId :

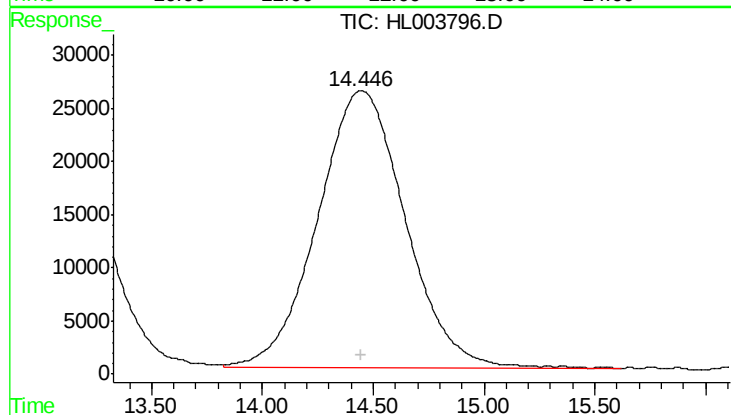


#14 3-Nitrotoluene

R.T.: 14.446 min
Delta R.T.: 0.003 min
Response: 7195514
Conc: 998.56 ug/L

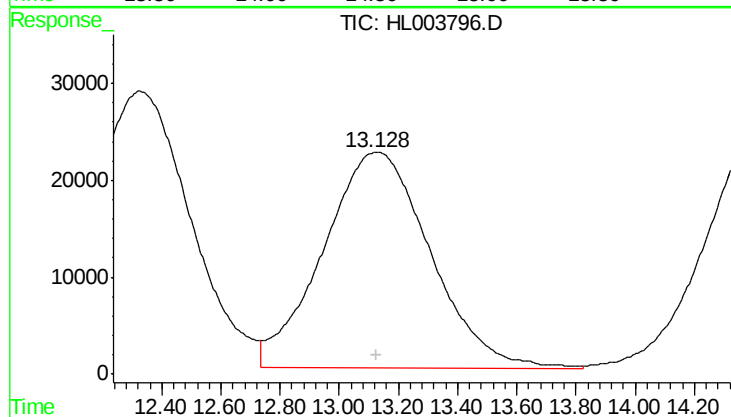


#15 4-Nitrotoluene

R.T.: 13.128 min
Delta R.T.: 0.003 min
Response: 5615199
Conc: 965.55 ug/L

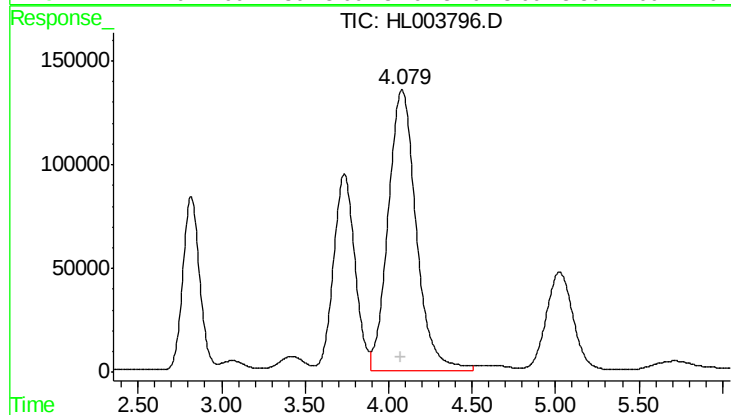

#16 3,5-Dinitroaniline

R.T.: 4.081 min
Delta R.T.: 0.005 min
Response: 15745885
Conc: 1002.85 ug/L

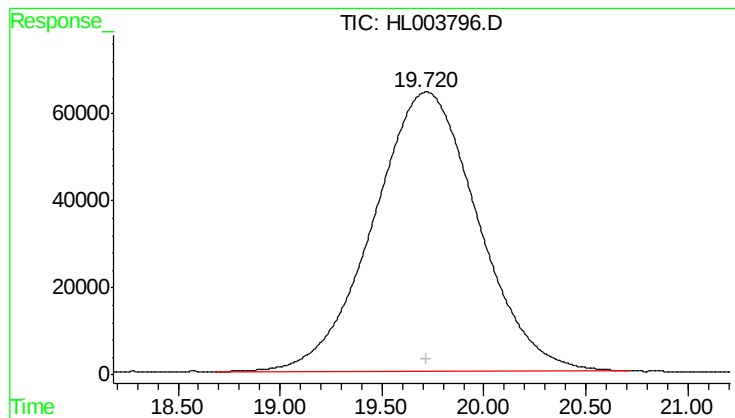

#18 PETN

R.T.: 19.720 min
Delta R.T.: 0.004 min
Response: 23005224
Conc: 2484.17 ug/L

Instrument :
HPLC_L
ClientSampleId :