

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003869.D Vial: 13
 Acq On : 31-Dec-2012, 22:33 Operator: HLM
 Sample : 8330-ICV Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Jan 2 11:24 2013 Quant Results File: HL123112.RES

Instrument :
 HPLC_L
 ClientSampleId :
 ICVHL123112

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Wed Jan 02 11:22:54 2013
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
2) T HMX	0.91	5524674	1305.289 ug/L
3) T RDX	1.74	5539332	1021.349 ug/L
4) T 1,3,5-Trinitrobenzene	2.72	12330193	1040.669 ug/L
5) T Tetrvl	6.15	8949905	1003.610 ug/L
6) T 2,4,6-Trinitrotoluene	6.53	11812168	1008.048 ug/L
7) T 2-Amino-4,6-dinitrotoluene	6.99	11037752	978.605 ug/L
8) T 4-Amino-2,6-dinitrotoluene	7.31	7395379	1010.248 ug/L
9) T 2,4-Dinitrotoluene	8.16	15190429	974.839 ug/L
10) T 2,6-Dinitrotoluene	8.53	8474847	978.924 ug/L
11) T 1,3-Dinitrobenzene	3.60	16690387	985.798 ug/L
12) T Nitrobenzene	4.84	10535508	981.072 ug/L
13) T 2-Nitrotoluene	11.77	6919882	1044.833 ug/L
14) T 3-Nitrotoluene	13.78	7357292	1034.496 ug/L
15) T 4-Nitrotoluene	12.53	5748983	1047.740 ug/L
16) T 3,5-Dinitroaniline	3.93	13777595	864.928 ug/L
17) T Nitroglycerin	6.15f	8949905	159562.654 ug/L
18) T PETN	18.74	8896092	969.563 ug/L

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003869.D

Vial: 13

Acq On : 31-Dec-2012, 22:33

Operator: HLM

Sample : 8330-ICV

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Jan 2 11:24 2013 Quant Results File: HL123112.RES

Instrument :

HPLC_L

ClientSampleId :

ICVHL123112

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)

Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)

Last Update : Wed Jan 02 11:22:54 2013


Response via : Multiple Level Calibration


DataAcq Meth : 8330AGIP.M

Volume Inj. :

Signal Phase :

Signal Info :

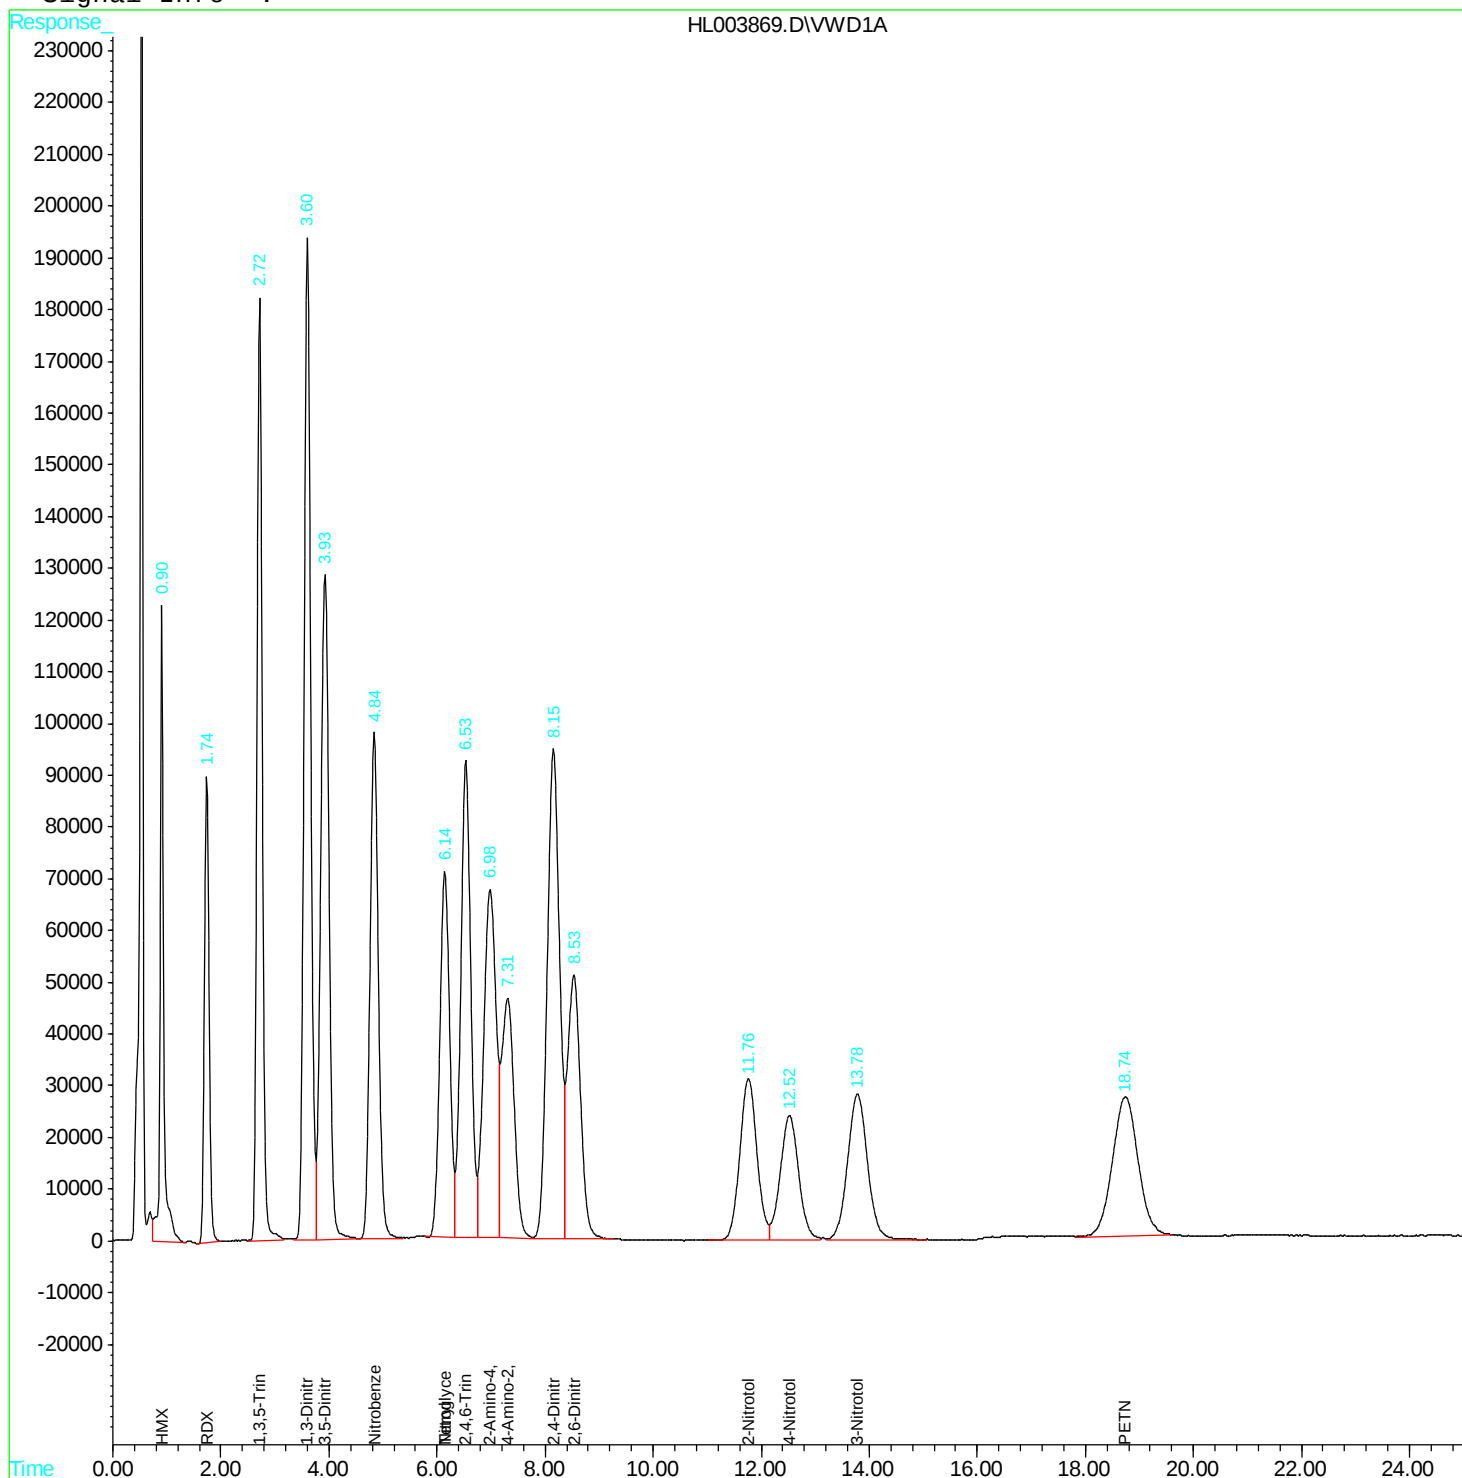


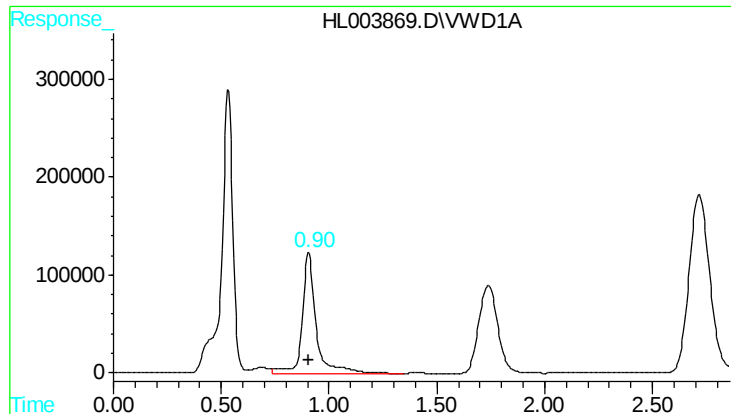

#2 HMX


R.T.: 0.905 min
Delta R.T.: -0.002 min
Response: 5524674
Conc: 1305.29 ug/L

Instrument :
HPLC_L
ClientSampleId :
ICVHL123112

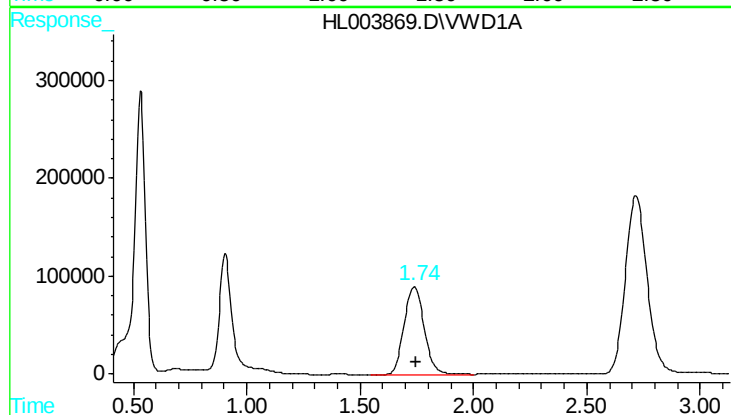


#3 RDX

R.T.: 1.740 min
Delta R.T.: -0.007 min
Response: 5539332
Conc: 1021.35 ug/L

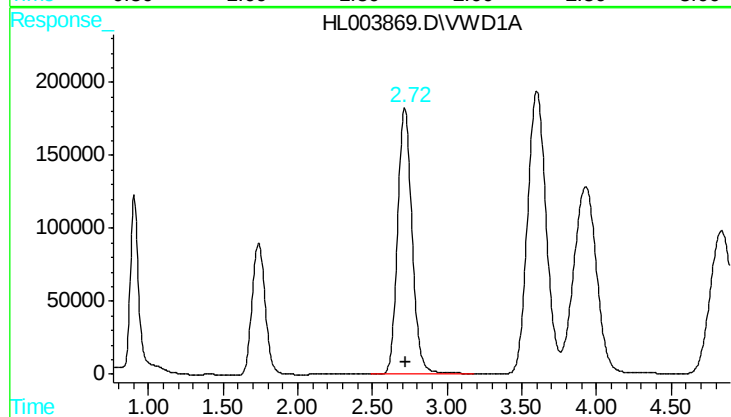


#4 1,3,5-Trinitrobenzene

R.T.: 2.717 min
Delta R.T.: -0.010 min
Response: 12330193
Conc: 1040.67 ug/L

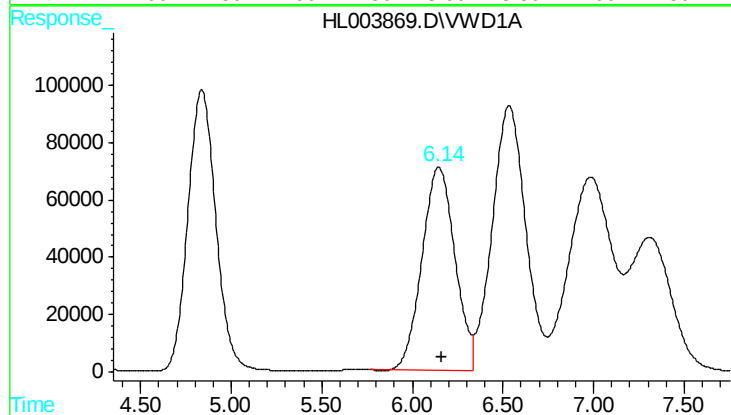

#5 Tetryl


R.T.: 6.145 min
Delta R.T.: -0.017 min
Response: 8949905
Conc: 1003.61 ug/L

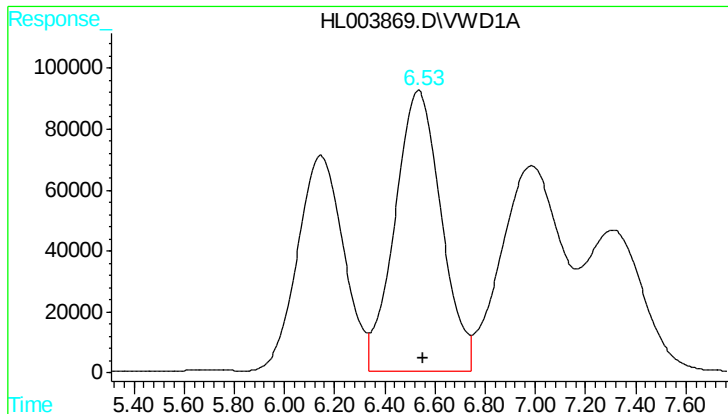

#6 2,4,6-Trinitrotoluene


R.T.: 6.534 min
Delta R.T.: -0.021 min
Response: 11812168
Conc: 1008.05 ug/L

Instrument :
HPLC_L
ClientSampleId :
ICVHL123112

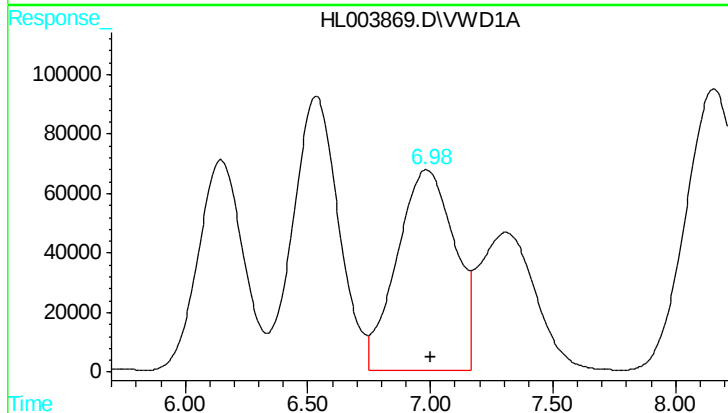


#7 2-Amino-4,6-dinitrotoluene

R.T.: 6.985 min
Delta R.T.: -0.016 min
Response: 11037752
Conc: 978.61 ug/L

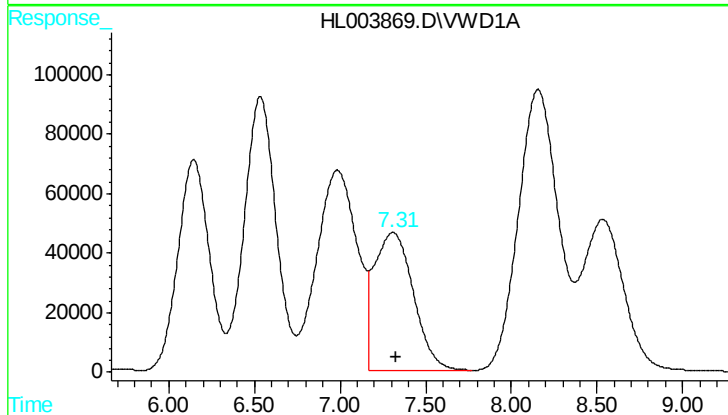


#8 4-Amino-2,6-dinitrotoluene

R.T.: 7.309 min
Delta R.T.: -0.018 min
Response: 7395379
Conc: 1010.25 ug/L

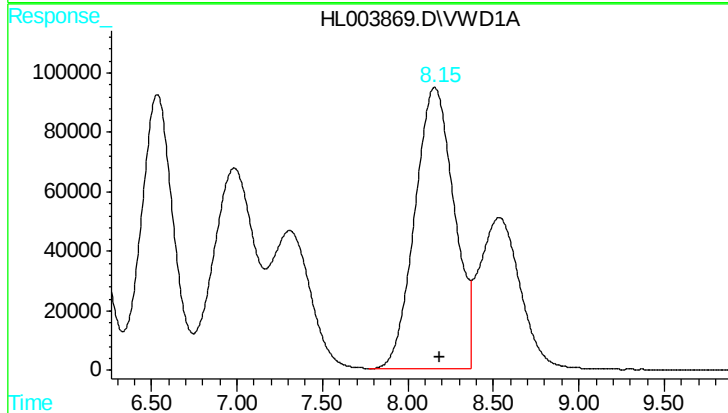

#9 2,4-Dinitrotoluene


R.T.: 8.156 min
Delta R.T.: -0.027 min
Response: 15190429
Conc: 974.84 ug/L

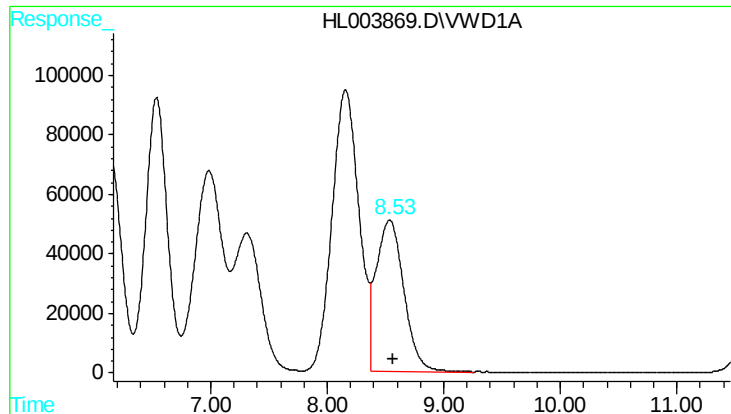

#10 2,6-Dinitrotoluene


R.T.: 8.534 min
Delta R.T.: -0.026 min
Response: 8474847
Conc: 978.92 ug/L

Instrument :
HPLC_L
ClientSampleId :
ICVHL123112

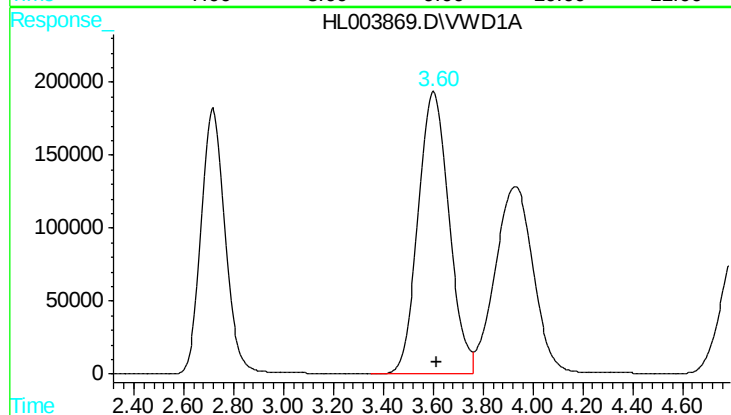


#11 1,3-Dinitrobenzene

R.T.: 3.602 min
Delta R.T.: -0.013 min
Response: 16690387
Conc: 985.80 ug/L

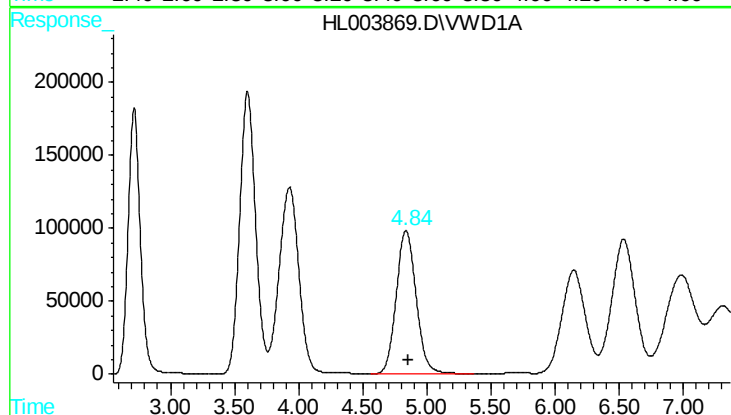


#12 Nitrobenzene

R.T.: 4.838 min
Delta R.T.: -0.017 min
Response: 10535508
Conc: 981.07 ug/L

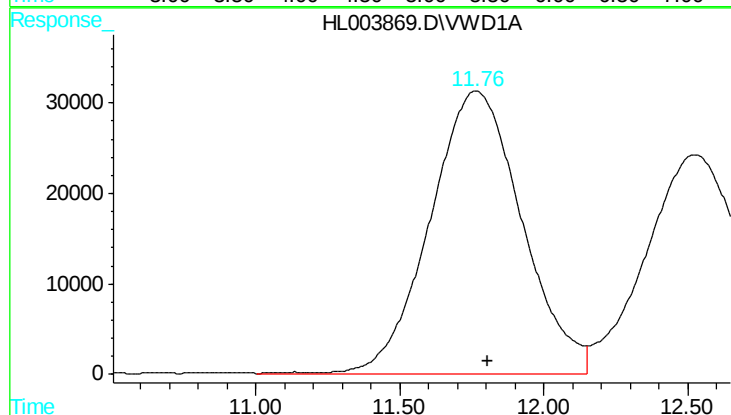

#13 2-Nitrotoluene


R.T.: 11.765 min
Delta R.T.: -0.041 min
Response: 6919882
Conc: 1044.83 ug/L

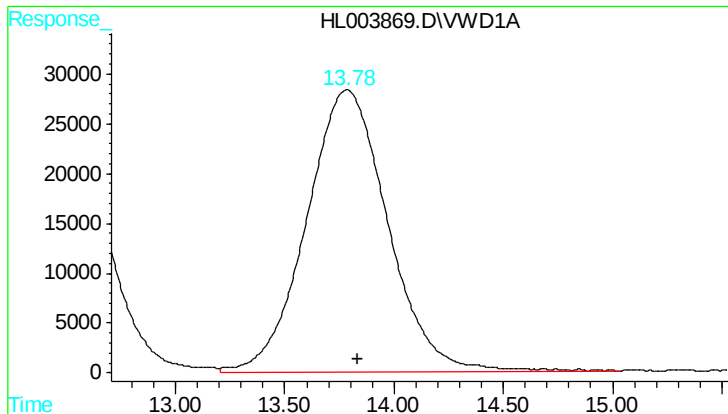

#14 3-Nitrotoluene


R.T.: 13.785 min
Delta R.T.: -0.047 min
Response: 7357292
Conc: 1034.50 ug/L

Instrument :
HPLC_L
ClientSampleId :
ICVHL123112

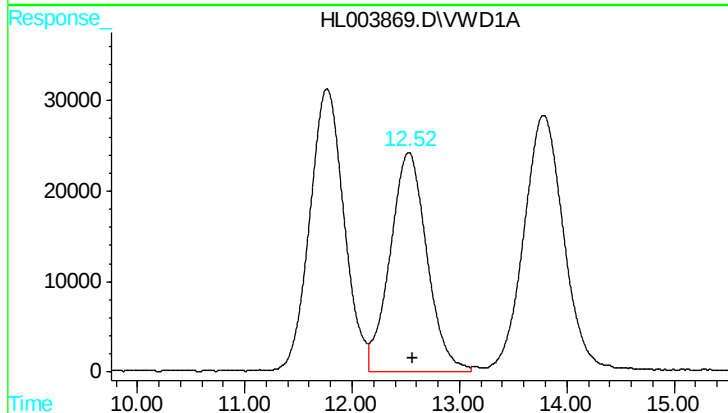


#15 4-Nitrotoluene

R.T.: 12.527 min
Delta R.T.: -0.044 min
Response: 5748983
Conc: 1047.74 ug/L

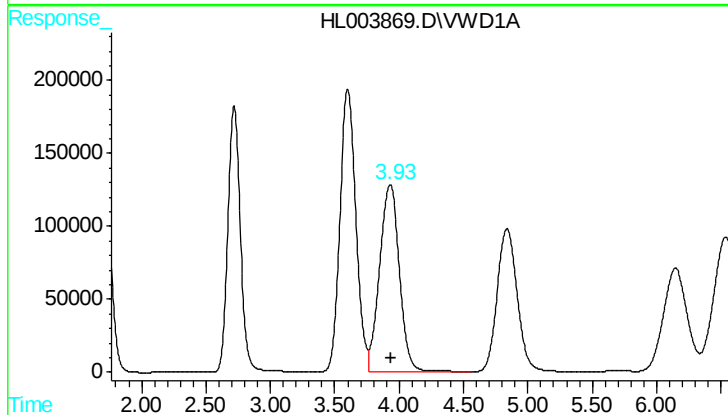


#16 3,5-Dinitroaniline

R.T.: 3.930 min
Delta R.T.: -0.013 min
Response: 13777595
Conc: 864.93 ug/L

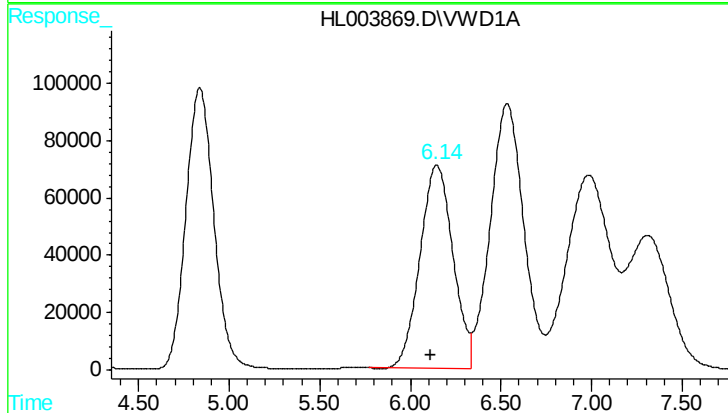

#17 Nitroglycerin

R.T.: 6.145 min
Delta R.T.: 0.032 min
Response: 8949905
Conc: 159562.65 ug/L

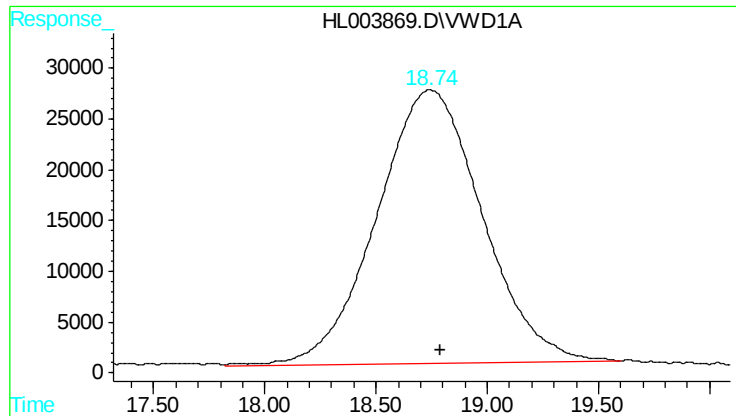

#18 PETN

R.T.: 18.743 min
Delta R.T.: -0.046 min
Response: 8896092
Conc: 969.56 ug/L

Instrument :
HPLC_L
ClientSampleId :
ICVHL123112