

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003877.D Vial: 25  
Acq On : 01-Jan-2013, 02:09 Operator: HLM  
Sample : PB67689BSD2 Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : events.e  
Quant Time: Jan 2 11:25 2013 Quant Results File: HL123112.RES

Instrument :  
HPLC\_L  
ClientSampleId :  
PB67689BSD2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)  
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)  
Last Update : Wed Jan 02 11:22:54 2013  
Response via : Initial Calibration  
DataAcq Meth : 8330AGIP.M

Volume Inj. :  
Signal Phase :  
Signal Info :

| Compound | R.T. | Response | Conc Units |
|----------|------|----------|------------|
|----------|------|----------|------------|

-----  
System Monitoring Compounds

|               |                |       |          |                    |
|---------------|----------------|-------|----------|--------------------|
| 1) S          | 4-Nitroaniline | 1.35  | 1196451  | 307.766 ug/L       |
| Spiked Amount | 300.000        | Range | 37 - 149 | Recovery = 102.59% |

Target Compounds


|       |               |       |        |               |
|-------|---------------|-------|--------|---------------|
| 3) T  | RDX           | 1.73f | 37498  | 6.914 ug/L    |
| 5) T  | Tetryl        | 6.13  | 272900 | 30.602 ug/L   |
| 17) T | Nitroglycerin | 6.13  | 272900 | 4865.378 ug/L |


Data File : H:\VOL1\HPLC\HPLC L\121231\HL003877.D Vial: 25  
Acq On : 01-Jan-2013, 02:09 Operator: HLM  
Sample : PB67689BSD2 Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : events.e  
Quant Time: Jan 2 11:25 2013 Quant Results File: HL123112.RES

Instrument :  
HPLC\_L  
ClientSampleId :  
PB67689BSD2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)  
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)  
Last Update : Wed Jan 02 11:22:54 2013  
Response via : Multiple Level Calibration  
DataAcq Meth : 8330AGIP.M

Volume Inj. :  
Signal Phase :  
Signal Info :

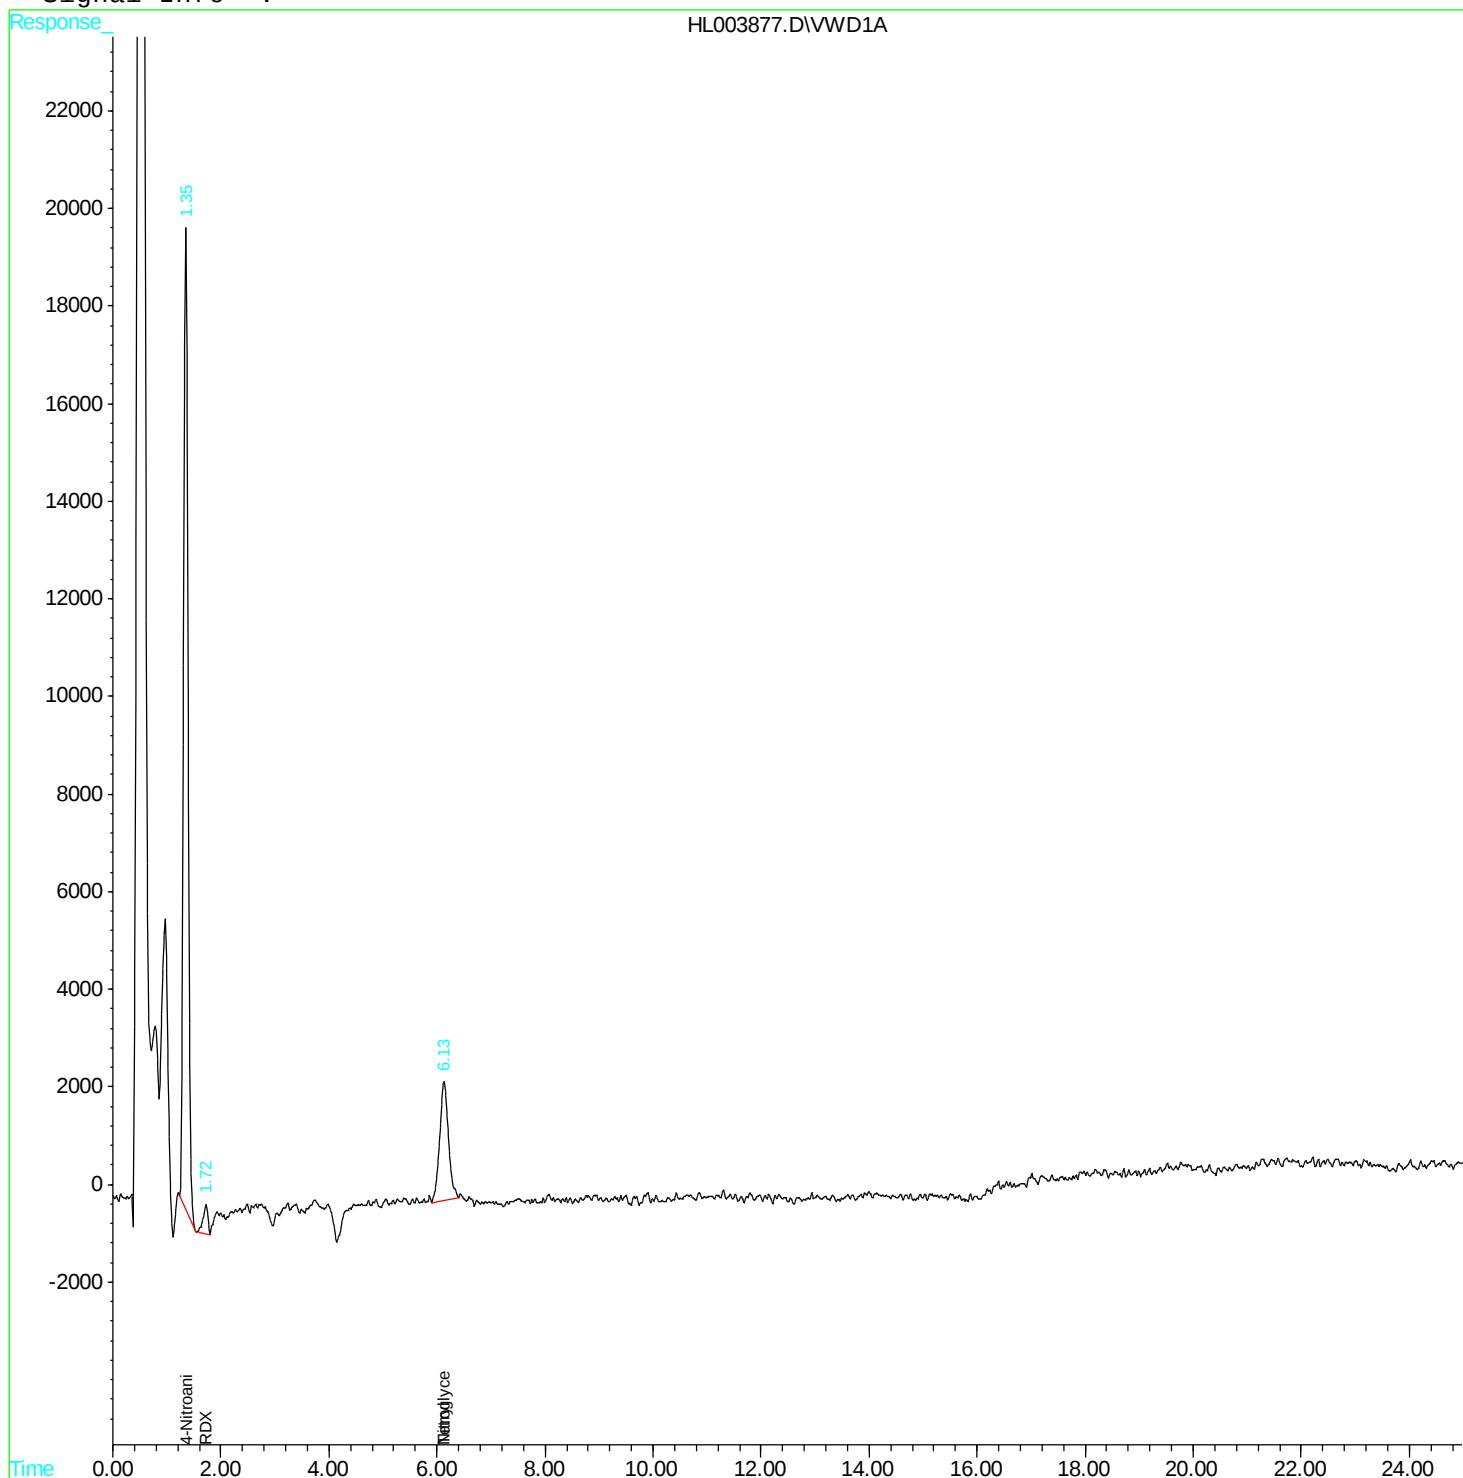


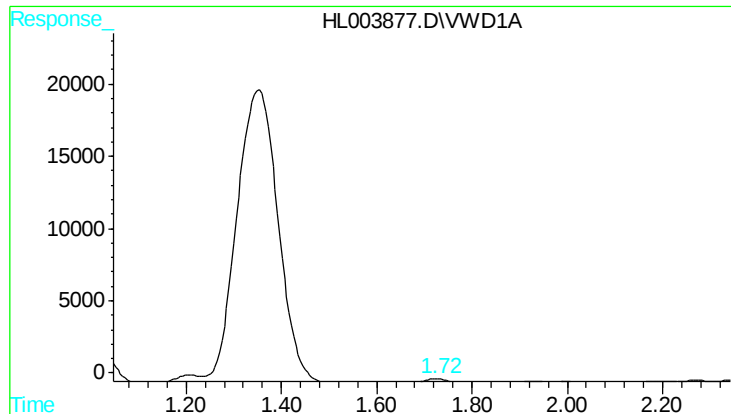

#3 RDX


R.T.: 1.725 min  
Delta R.T.: -0.021 min  
Response: 37498  
Conc: 6.91 ug/L

Instrument :  
HPLC\_L  
ClientSampleId :  
PB67689BSD2

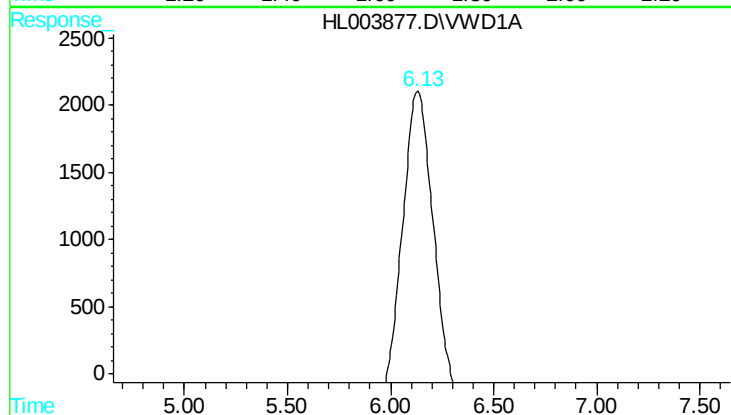

#5 Tetryl

R.T.: 6.133 min  
Delta R.T.: -0.029 min  
Response: 272900  
Conc: 30.60 ug/L

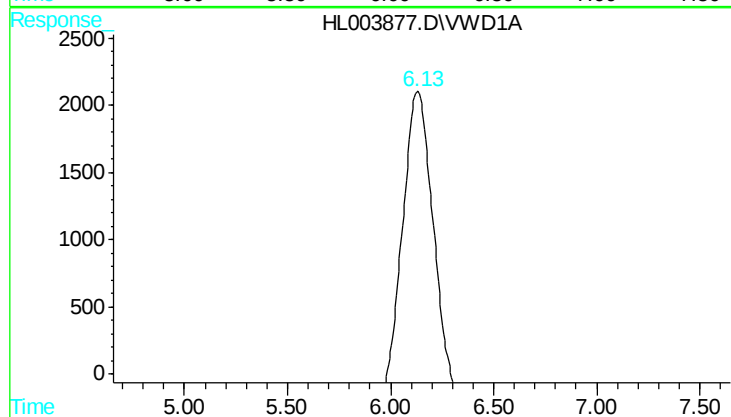

#17 Nitroglycerin

R.T.: 6.133 min  
Delta R.T.: 0.019 min  
Response: 272900  
Conc: 4865.38 ug/L