

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003882.D Vial: 30
Acq On : 01-Jan-2013, 04:23 Operator: HLM
Sample : PB67726BS2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Jan 2 11:25 2013 Quant Results File: HL123112.RES

Instrument :
HPLC_L
ClientSampleId :
PB67726BS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Wed Jan 02 11:22:54 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.35	633350	162.918 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 54.31%

Target Compounds


5) T	Tetrvl	6.12f	167537	18.787 ug/L
17) T	Nitroglycerin	6.12	167537	2986.924 ug/L


Data File : H:\VOL1\HPLC\HPLC L\121231\HL003882.D Vial: 30
Acq On : 01-Jan-2013, 04:23 Operator: HLM
Sample : PB67726BS2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Jan 2 11:25 2013 Quant Results File: HL123112.RES

Instrument :
HPLC_L
ClientSampleId :
PB67726BS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Wed Jan 02 11:22:54 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

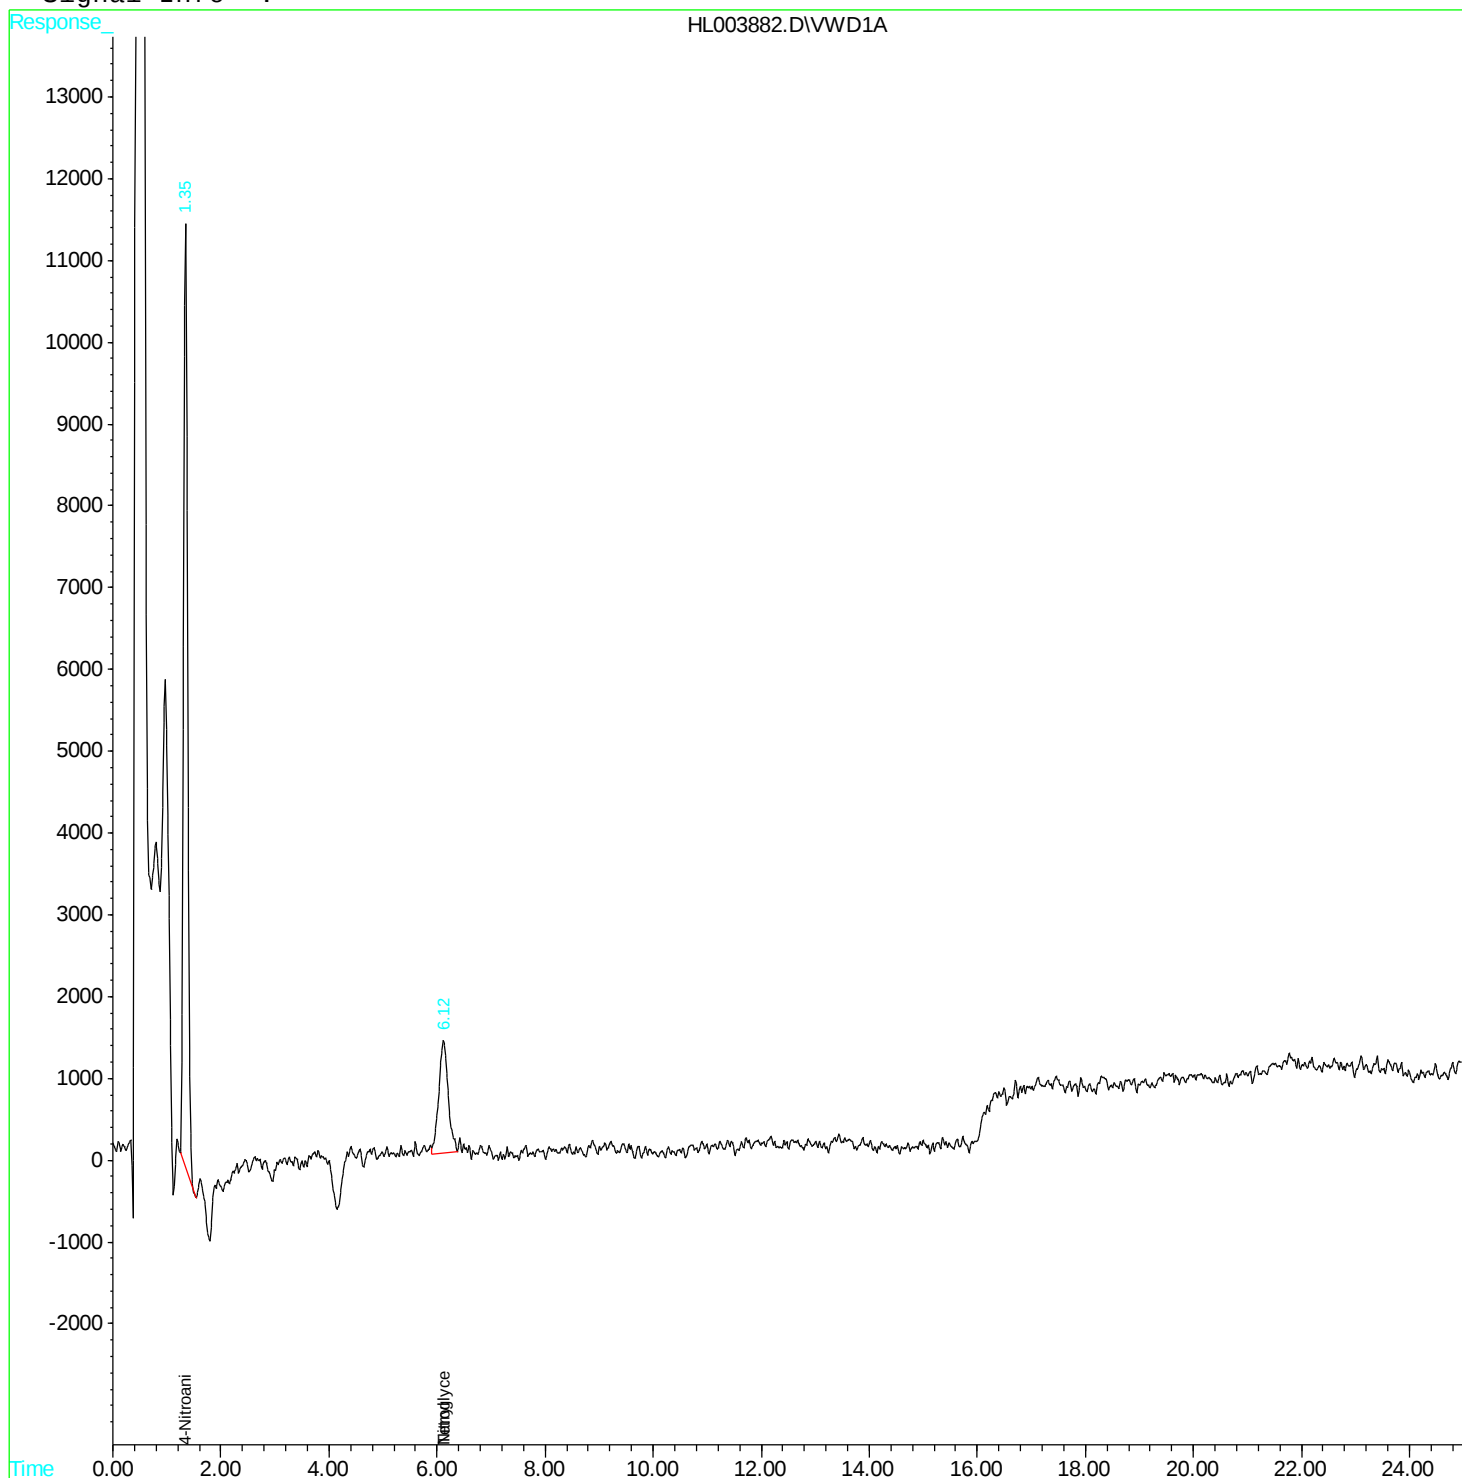


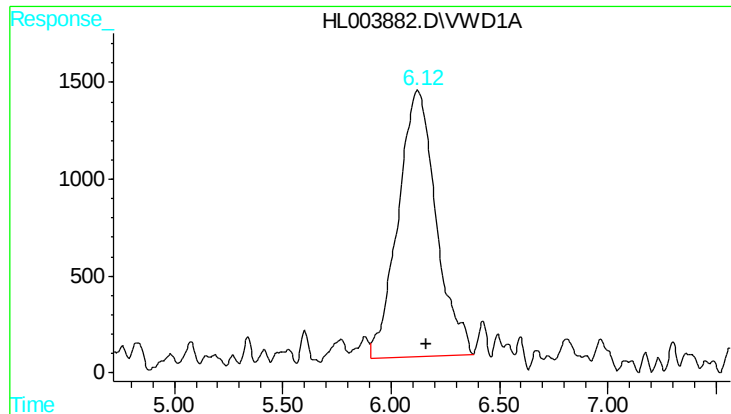

#5 Tetryl

R.T.: 6.122 min
Delta R.T.: -0.040 min
Response: 167537
Conc: 18.79 ug/L

Instrument :
HPLC_L
ClientSampleId :
PB67726BS2

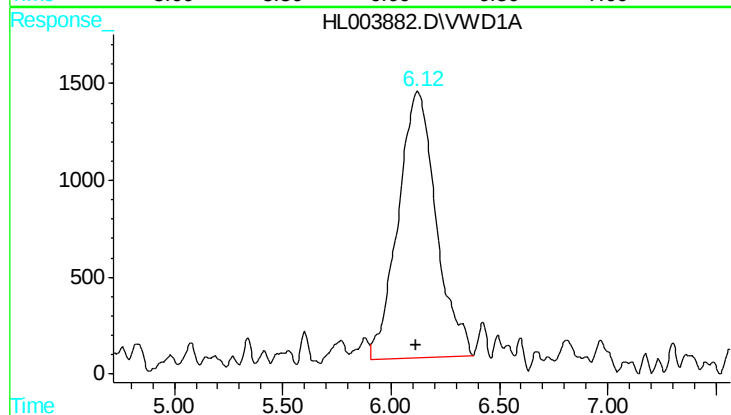

#17 Nitroglycerin

R.T.: 6.122 min
Delta R.T.: 0.009 min
Response: 167537
Conc: 2986.92 ug/L