

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003884.D Vial: 2
 Acq On : 01-Jan-2013, 05:17 Operator: HLM
 Sample : 8330-CCV Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Jan 2 11:25 2013 Quant Results File: HL123112.RES

Instrument :
 HPLC_L
 LabSampleId :
 8330-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Wed Jan 02 11:22:54 2013
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.35	3871454	995.865 ug/L
Spiked Amount 300.000		Range 37 - 149	Recovery	= 331.96%#

Target Compounds

2) T	HMX	0.91	4378854	1015.059 ug/L
3) T	RDX	1.75	5583929	1029.572 ug/L
4) T	1,3,5-Trinitrobenzene	2.72	5800680	489.578 ug/L
5) T	Tetryl	6.16	8408007	942.843 ug/L
6) T	2,4,6-Trinitrotoluene	6.54	5546153	473.308 ug/L
7) T	2-Amino-4,6-dinitrotoluene	7.00	5497849	487.438 ug/L
8) T	4-Amino-2,6-dinitrotoluene	7.32	3640331	497.288 ug/L
9) T	2,4-Dinitrotoluene	8.16	7716592	495.209 ug/L
10) T	2,6-Dinitrotoluene	8.54	4212339	486.565 ug/L
11) T	1,3-Dinitrobenzene	3.61	8324936	491.703 ug/L
12) T	Nitrobenzene	4.84	5297077	493.267 ug/L
13) T	2-Nitrotoluene	11.77	6652149	1004.408 ug/L
14) T	3-Nitrotoluene	13.79	7060501	992.765 ug/L
15) T	4-Nitrotoluene	12.52	5610237	1022.454 ug/L
16) T	3,5-Dinitroaniline	3.94	15874382	996.559 ug/L
17) T	Nitroglycerin	6.16f	8408007	149901.468 ug/L
18) T	PETN	18.76	23206126	2529.179 ug/L

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003884.D

Vial: 2

Acq On : 01-Jan-2013, 05:17

Operator: HLM

Sample : 8330-CCV

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Jan 2 11:25 2013 Quant Results File: HL123112.RES

Instrument :

HPLC_L

LabSampleId :

8330-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)

Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)

Last Update : Wed Jan 02 11:22:54 2013


Response via : Multiple Level Calibration


DataAcq Meth : 8330AGIP.M

Volume Inj. :

Signal Phase :

Signal Info :

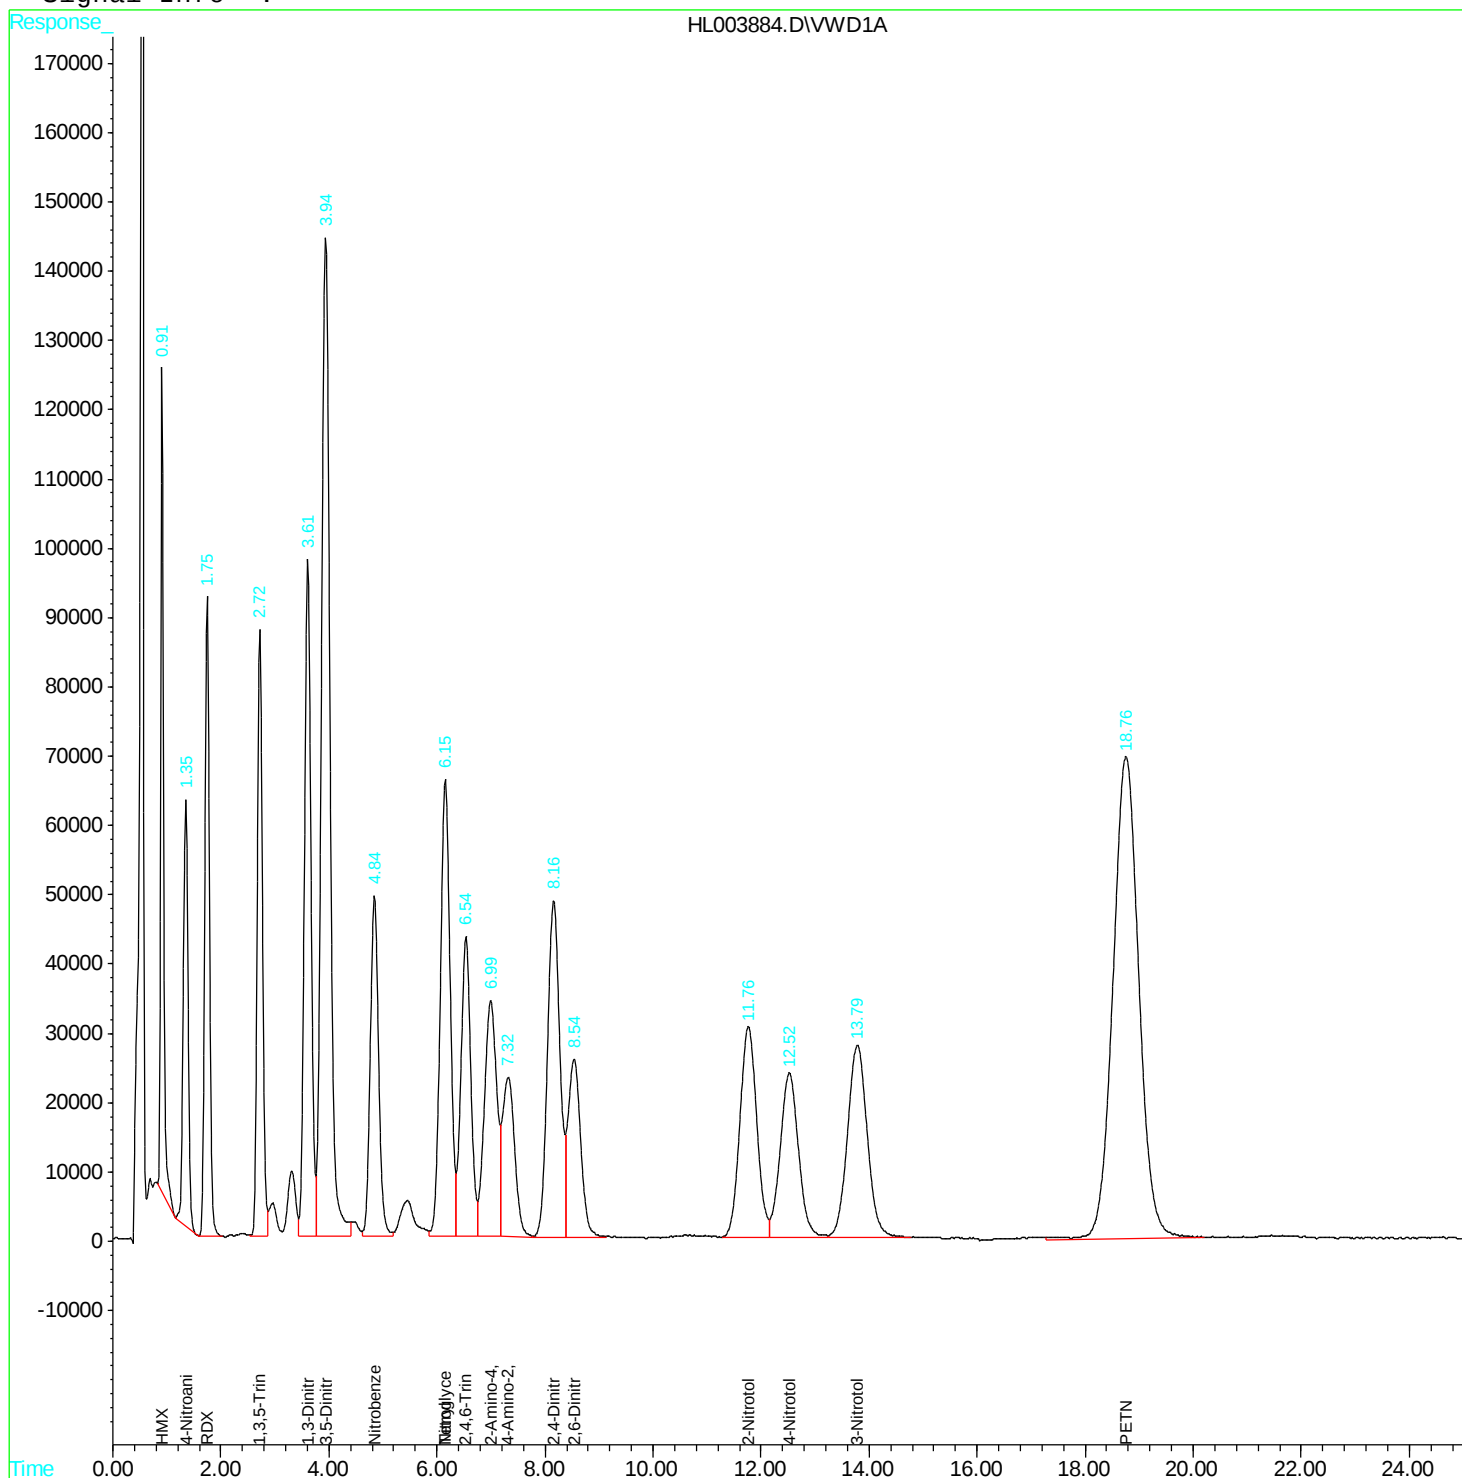


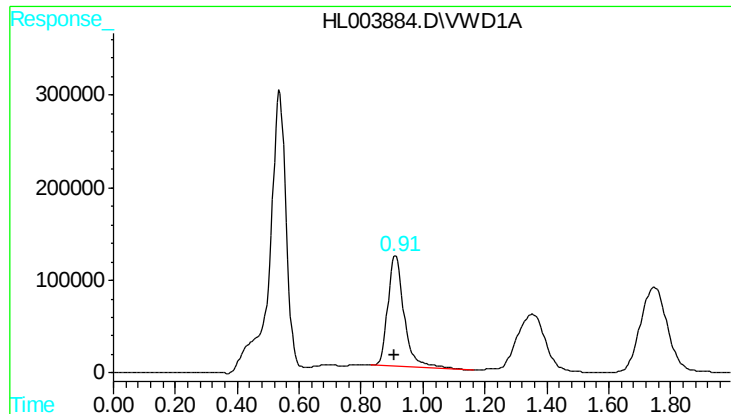

#2 HMX


R.T.: 0.911 min
Delta R.T.: 0.004 min
Response: 4378854
Conc: 1015.06 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

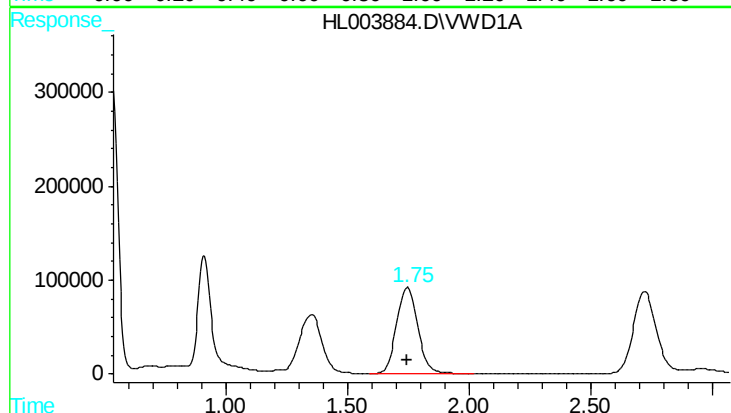


#3 RDX

R.T.: 1.748 min
Delta R.T.: 0.000 min
Response: 5583929
Conc: 1029.57 ug/L

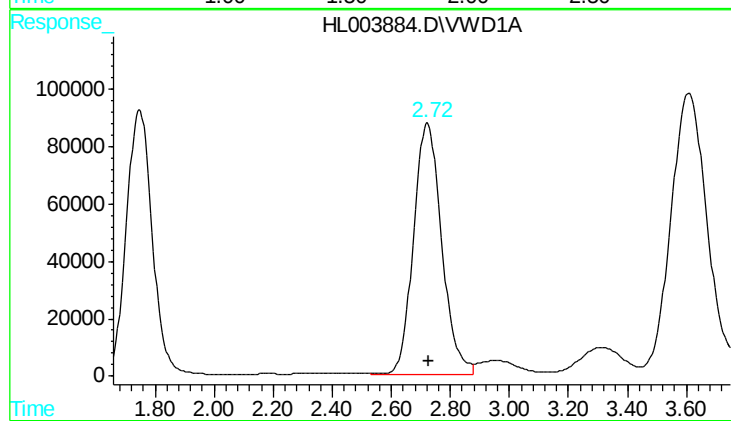


#4 1,3,5-Trinitrobenzene

R.T.: 2.723 min
Delta R.T.: -0.005 min
Response: 5800680
Conc: 489.58 ug/L

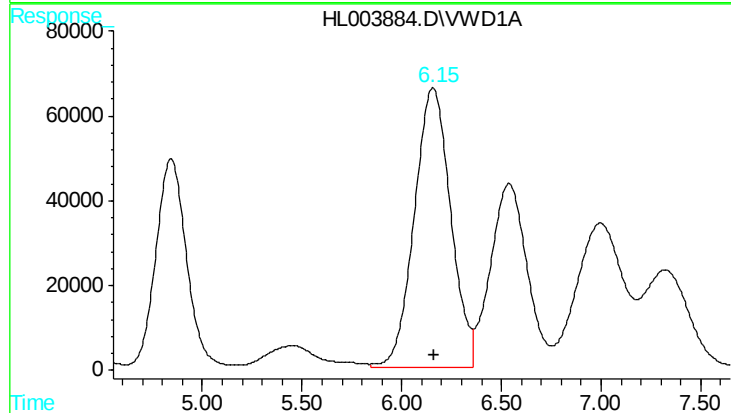

#5 Tetryl


R.T.: 6.156 min
Delta R.T.: -0.006 min
Response: 8408007
Conc: 942.84 ug/L

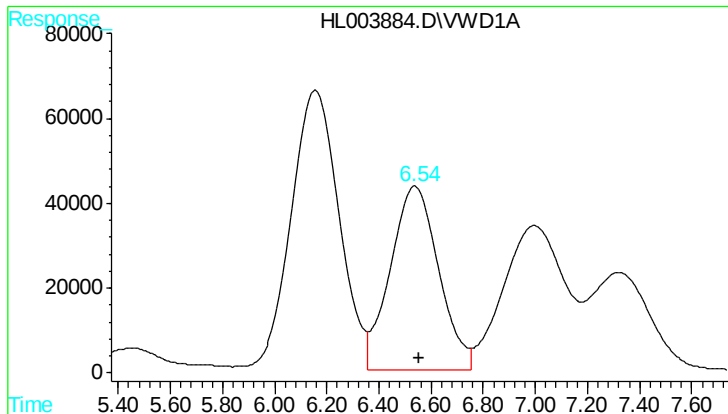

#6 2,4,6-Trinitrotoluene


R.T.: 6.538 min
Delta R.T.: -0.017 min
Response: 5546153
Conc: 473.31 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

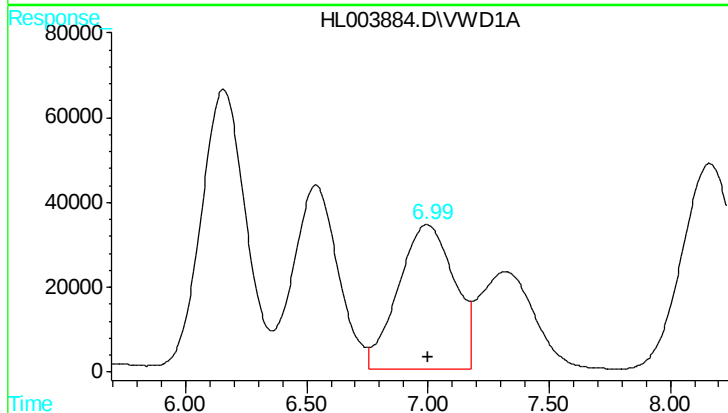


#7 2-Amino-4,6-dinitrotoluene

R.T.: 6.997 min
Delta R.T.: -0.005 min
Response: 5497849
Conc: 487.44 ug/L

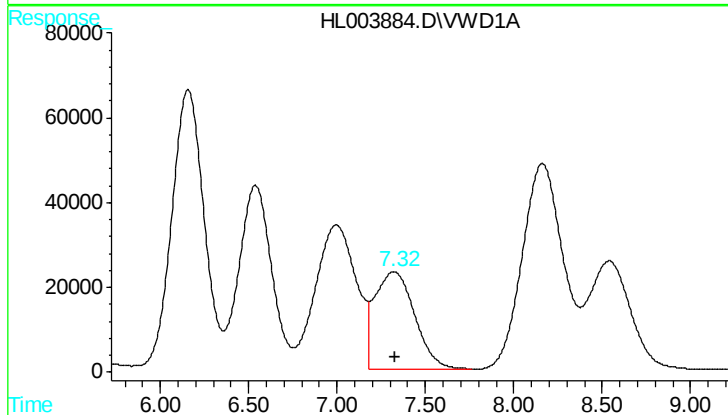


#8 4-Amino-2,6-dinitrotoluene

R.T.: 7.322 min
Delta R.T.: -0.006 min
Response: 3640331
Conc: 497.29 ug/L

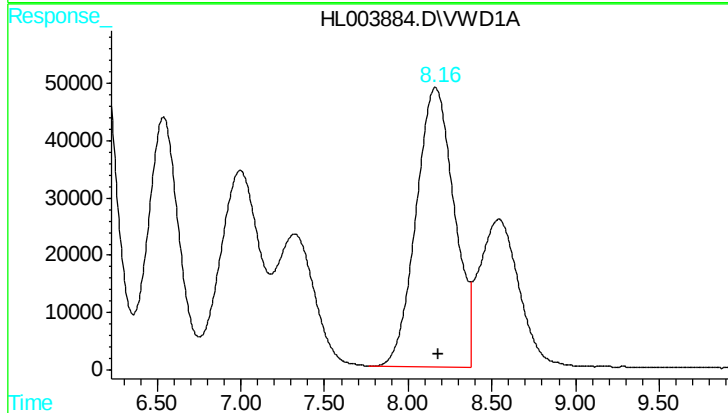

#9 2,4-Dinitrotoluene


R.T.: 8.162 min
Delta R.T.: -0.021 min
Response: 7716592
Conc: 495.21 ug/L

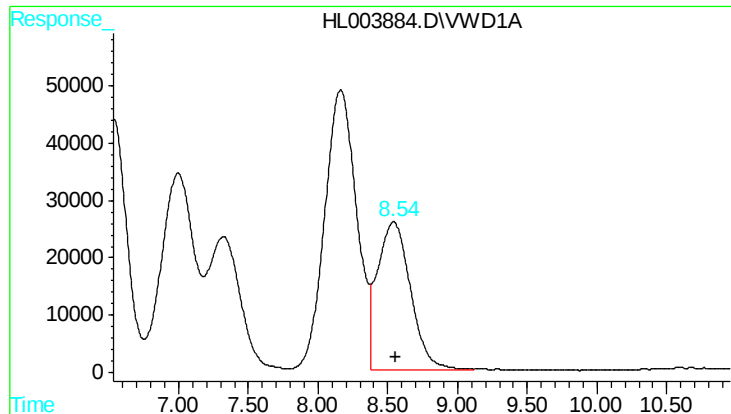

#10 2,6-Dinitrotoluene


R.T.: 8.541 min
Delta R.T.: -0.020 min
Response: 4212339
Conc: 486.56 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

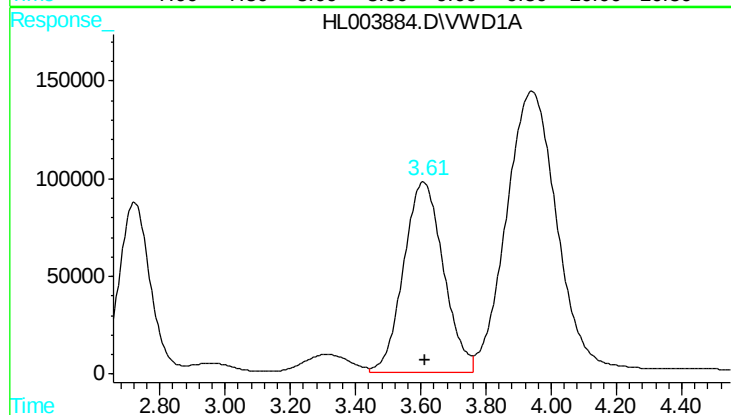


#11 1,3-Dinitrobenzene

R.T.: 3.609 min
Delta R.T.: -0.006 min
Response: 8324936
Conc: 491.70 ug/L

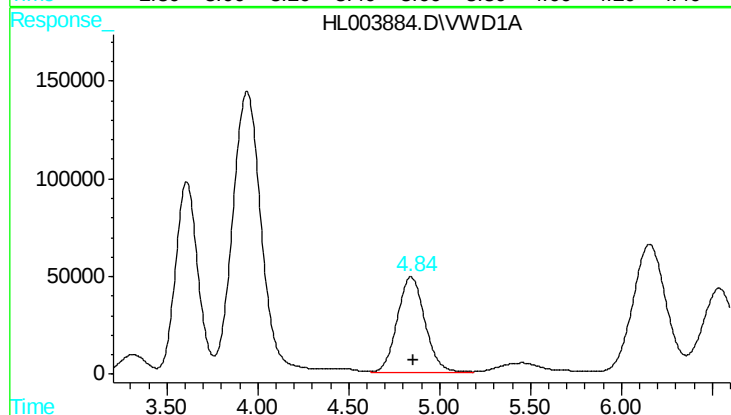


#12 Nitrobenzene

R.T.: 4.843 min
Delta R.T.: -0.012 min
Response: 5297077
Conc: 493.27 ug/L

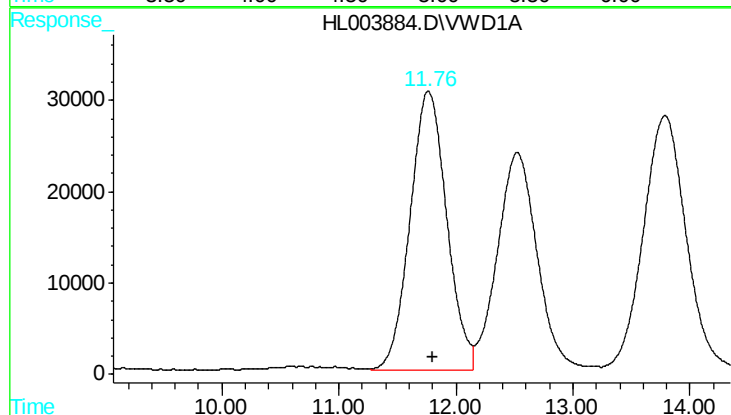

#13 2-Nitrotoluene


R.T.: 11.765 min
Delta R.T.: -0.041 min
Response: 6652149
Conc: 1004.41 ug/L

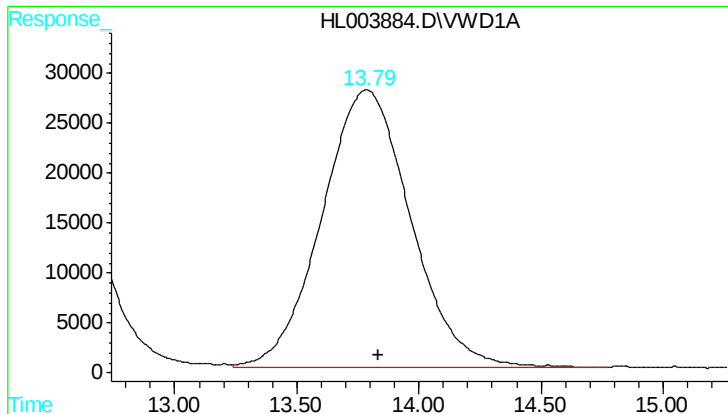

#14 3-Nitrotoluene


R.T.: 13.788 min
Delta R.T.: -0.044 min
Response: 7060501
Conc: 992.76 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

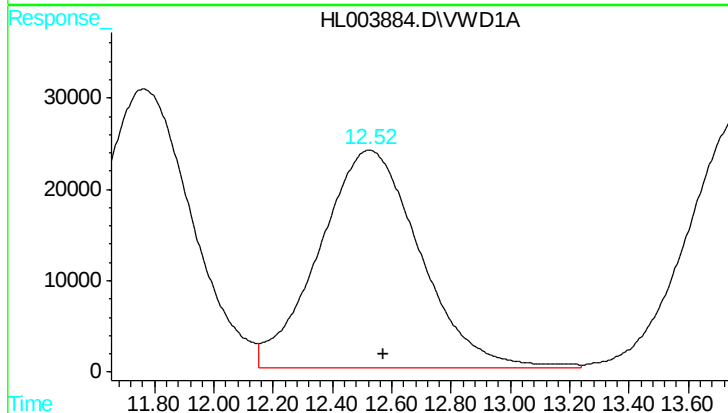


#15 4-Nitrotoluene

R.T.: 12.524 min
Delta R.T.: -0.046 min
Response: 5610237
Conc: 1022.45 ug/L

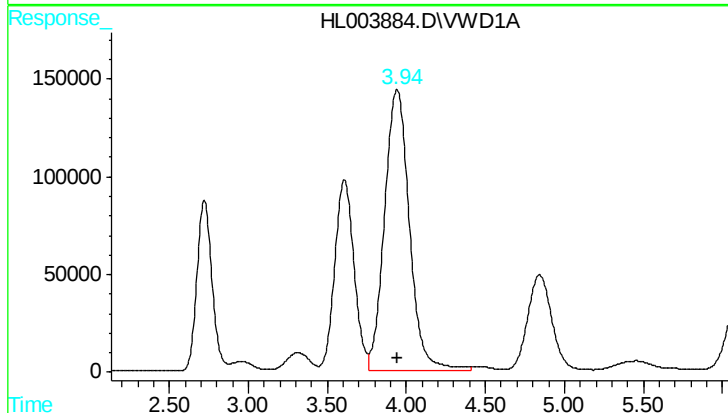


#16 3,5-Dinitroaniline

R.T.: 3.941 min
Delta R.T.: 0.000 min
Response: 15874382
Conc: 996.56 ug/L

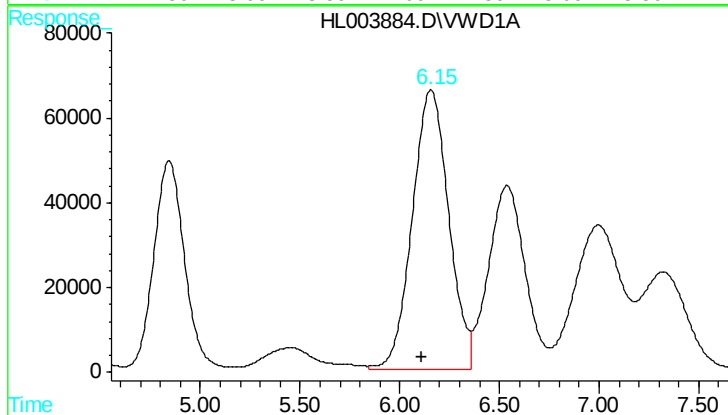

#17 Nitroglycerin

R.T.: 6.156 min
Delta R.T.: 0.043 min
Response: 8408007
Conc: 149901.47 ug/L

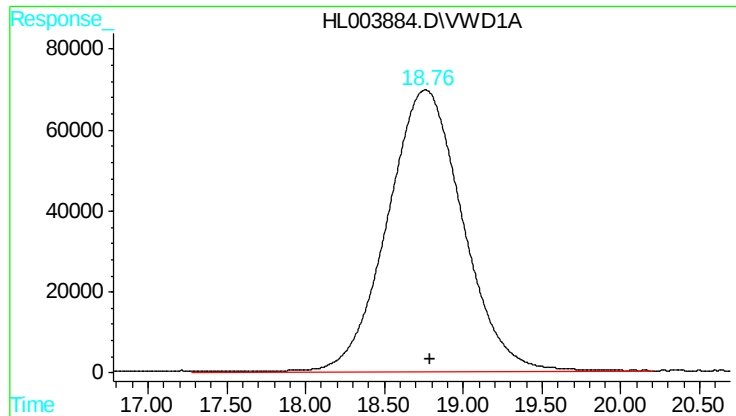

#18 PETN

R.T.: 18.759 min
Delta R.T.: -0.030 min
Response: 23206126
Conc: 2529.18 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV