

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003889.D Vial: 34
 Acq On : 01-Jan-2013, 07:32 Operator: HLM
 Sample : D5263-03MS2 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Jan 2 11:26 2013 Quant Results File: HL123112.RES

Instrument :
 HPLC_L
 ClientSampleId :
 C04-SD-36MS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Wed Jan 02 11:22:54 2013
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S 4-Nitroaniline	1.35	565561	145.481 ug/L
Spiked Amount 300.000	Range 37 - 149	Recovery	= 48.49%

Target Compounds

5) T Tetrvl	6.12f	151417	16.979 ug/L
17) T Nitroglycerin	6.12	151417	2699.517 ug/L


Quantitation Report


Data File : H:\VOL1\HPLC\HPLC L\121231\HL003889.D Vial: 34
 Acq On : 01-Jan-2013, 07:32 Operator: HLM
 Sample : D5263-03MS2 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Jan 2 11:26 2013 Quant Results File: HL123112.RES

Instrument :
 HPLC_L
 ClientSampleId :
 C04-SD-36MS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Wed Jan 02 11:22:54 2013
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

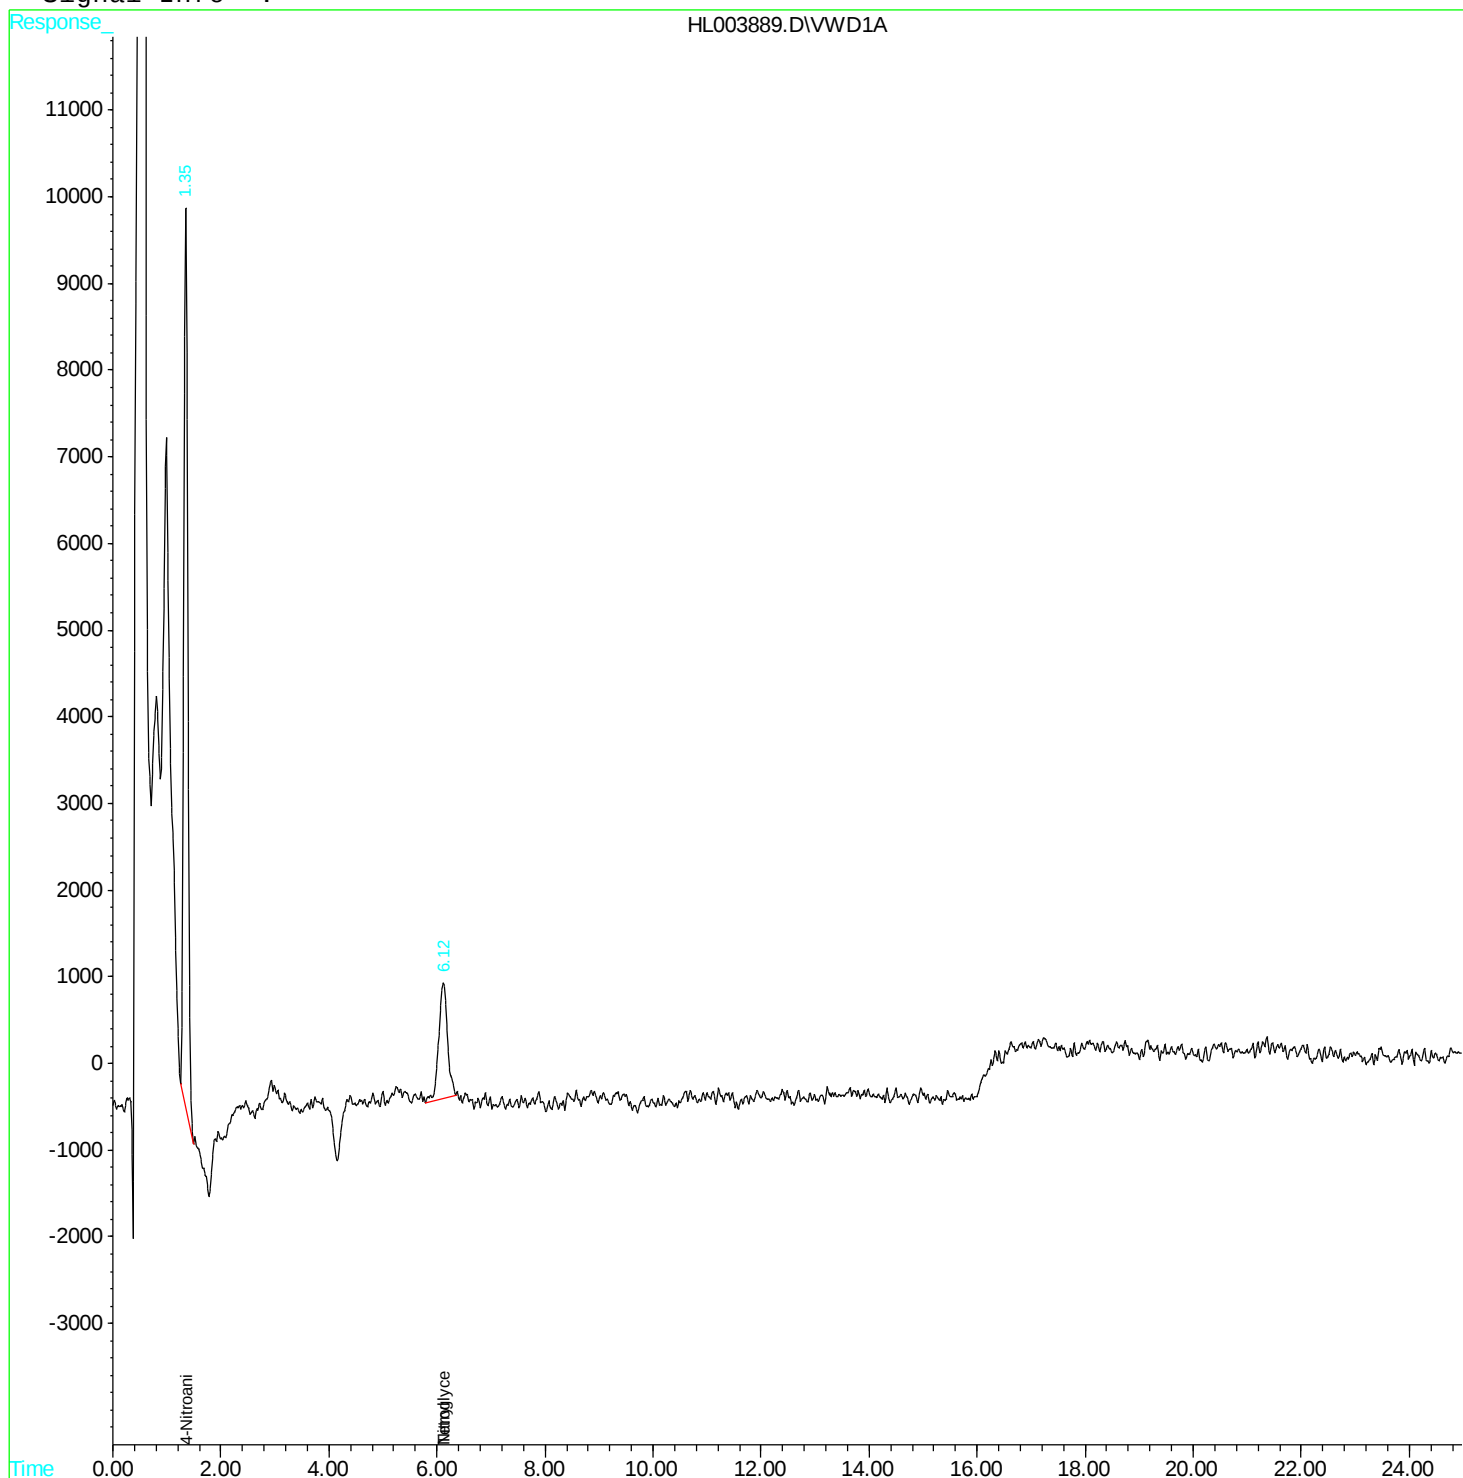


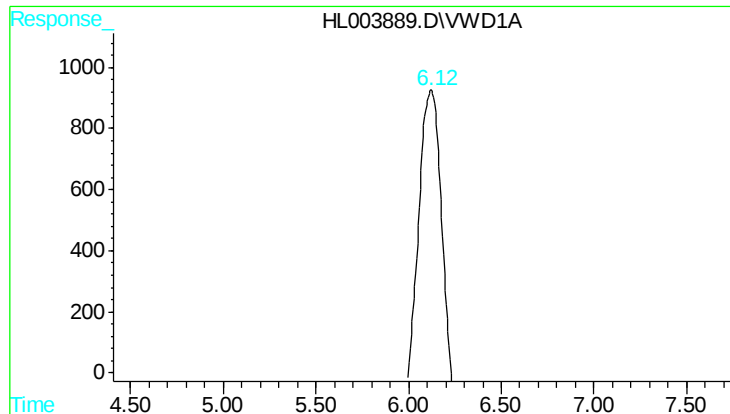

#5 Tetryl

R.T.: 6.124 min
Delta R.T.: -0.038 min
Response: 151417
Conc: 16.98 ug/L

Instrument :
HPLC_L
ClientSampleId :
C04-SD-36MS2

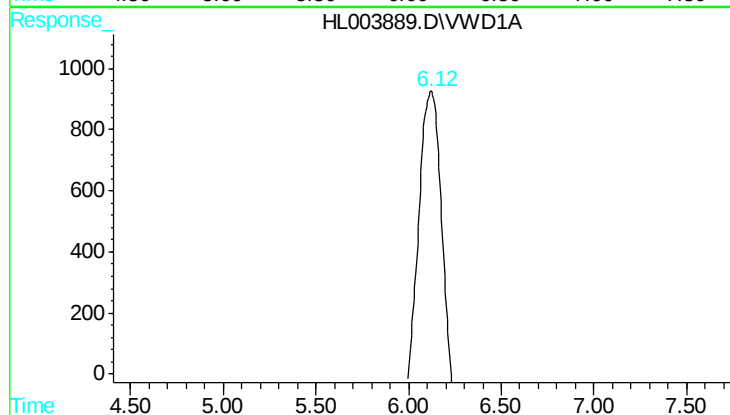

#17 Nitroglycerin

R.T.: 6.124 min
Delta R.T.: 0.011 min
Response: 151417
Conc: 2699.52 ug/L