

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003891.D Vial: 36
Acq On : 01-Jan-2013, 08:26 Operator: HLM
Sample : D5263-04MSD2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Jan 2 11:26 2013 Quant Results File: HL123112.RES

Instrument :
HPLC_L
ClientSampleId :
C04-SD-36MSD2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Wed Jan 02 11:22:54 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.35	613791	157.887 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 52.63%

Target Compounds

5) T	Tetryl	6.12f	157864	17.702 ug/L
17) T	Nitroglycerin	6.12	157864	2814.474 ug/L


Quantitation Report


Data File : H:\VOL1\HPLC\HPLC L\121231\HL003891.D Vial: 36
 Acq On : 01-Jan-2013, 08:26 Operator: HLM
 Sample : D5263-04MSD2 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Jan 2 11:26 2013 Quant Results File: HL123112.RES

Instrument :
 HPLC_L
 ClientSampleId :
 C04-SD-36MSD2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Wed Jan 02 11:22:54 2013
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

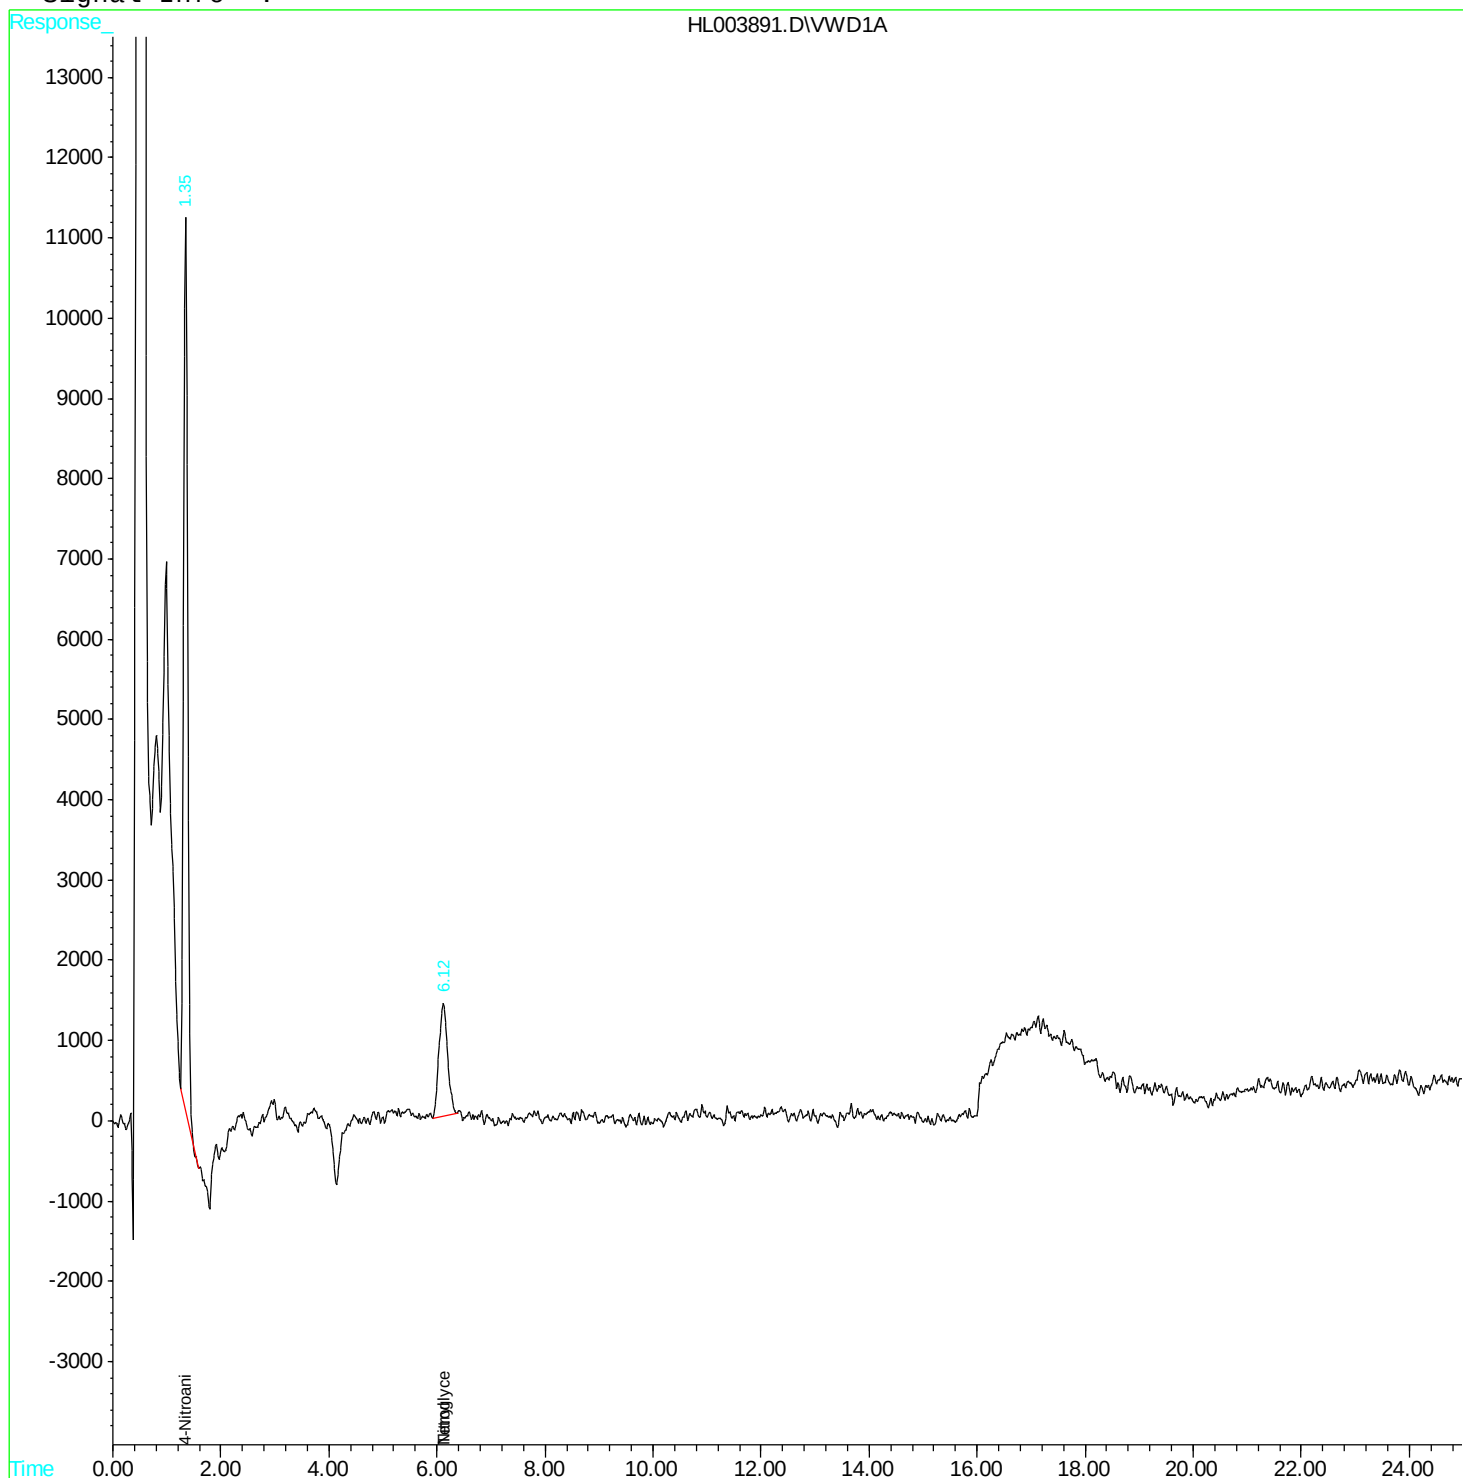


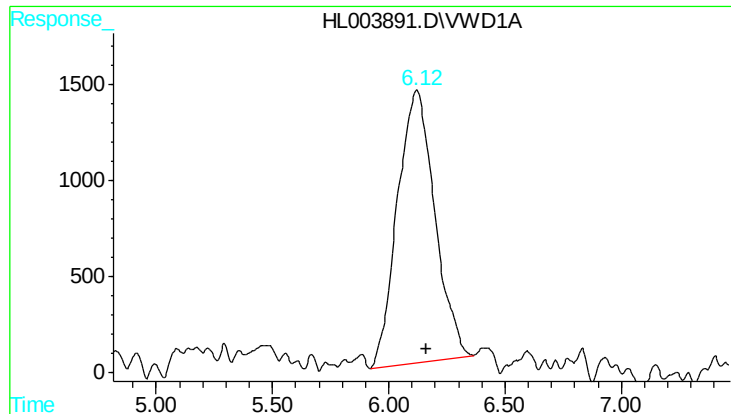

#5 Tetryl

R.T.: 6.122 min
Delta R.T.: -0.040 min
Response: 157864
Conc: 17.70 ug/L

Instrument :
HPLC_L
ClientSampleId :
C04-SD-36MSD2

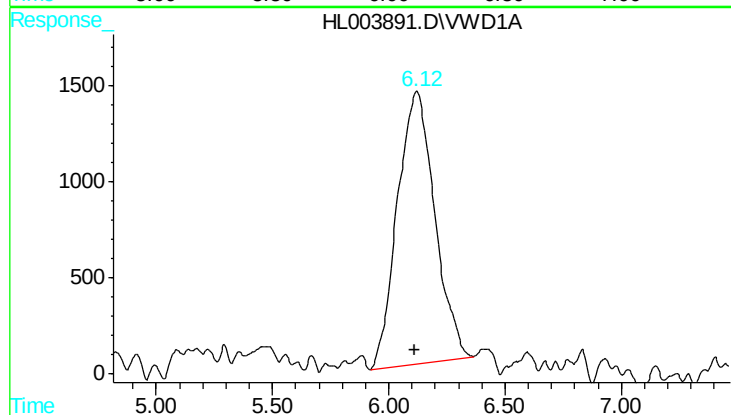

#17 Nitroglycerin

R.T.: 6.122 min
Delta R.T.: 0.008 min
Response: 157864
Conc: 2814.47 ug/L