

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003897.D Vial: 2
 Acq On : 01-Jan-2013, 11:07 Operator: HLM
 Sample : 8330-CCV Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Jan 2 11:26 2013 Quant Results File: HL123112.RES

Instrument :
 HPLC_L
 LabSampleId :
 8330-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Wed Jan 02 11:22:54 2013
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.35	3746797	963.799 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 321.27%#

Target Compounds

2) T	HMX	0.91	4436020	1029.539 ug/L
3) T	RDX	1.75	5632310	1038.493 ug/L
4) T	1,3,5-Trinitrobenzene	2.72	5743694	484.768 ug/L
5) T	Tetryl	6.16	8334564	934.608 ug/L
6) T	2,4,6-Trinitrotoluene	6.54	5539101	472.706 ug/L
7) T	2-Amino-4,6-dinitrotoluene	7.00	5525256	489.868 ug/L
8) T	4-Amino-2,6-dinitrotoluene	7.32	3686656	503.617 ug/L
9) T	2,4-Dinitrotoluene	8.16	7804318	500.839 ug/L
10) T	2,6-Dinitrotoluene	8.54	4318361	498.811 ug/L
11) T	1,3-Dinitrobenzene	3.61	8314913	491.111 ug/L
12) T	Nitrobenzene	4.84	5314479	494.887 ug/L
13) T	2-Nitrotoluene	11.77	6604336	997.189 ug/L
14) T	3-Nitrotoluene	13.79	7035159	989.202 ug/L
15) T	4-Nitrotoluene	12.53	5548743	1011.247 ug/L
16) T	3,5-Dinitroaniline	3.94	15842321	994.547 ug/L
17) T	Nitroglycerin	6.16f	8334564	148592.098 ug/L
18) T	PETN	18.79	22904152	2496.268 ug/L

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003897.D

Vial: 2

Acq On : 01-Jan-2013, 11:07

Operator: HLM

Sample : 8330-CCV

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Jan 2 11:26 2013 Quant Results File: HL123112.RES

Instrument :

HPLC_L

LabSampleId :

8330-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)

Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)

Last Update : Wed Jan 02 11:22:54 2013


Response via : Multiple Level Calibration


DataAcq Meth : 8330AGIP.M

Volume Inj. :

Signal Phase :

Signal Info :

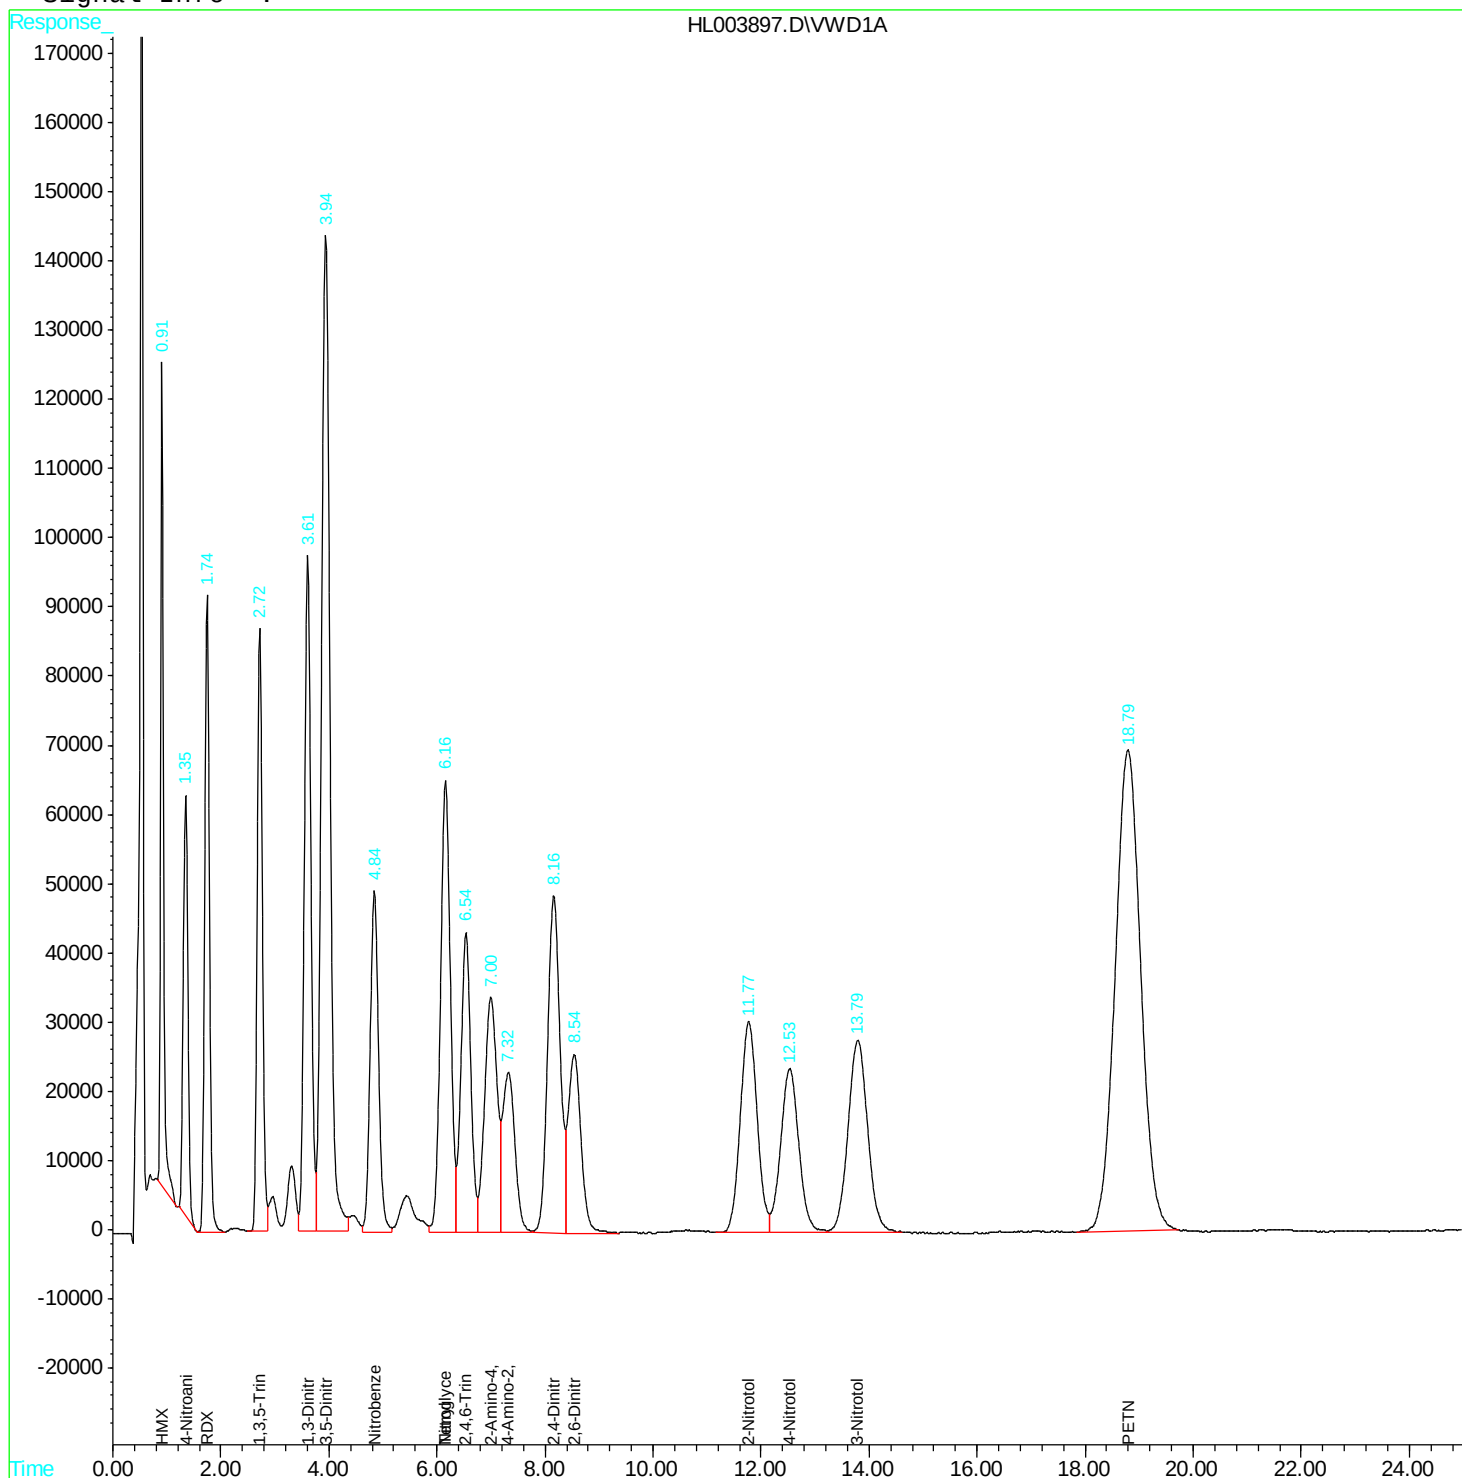


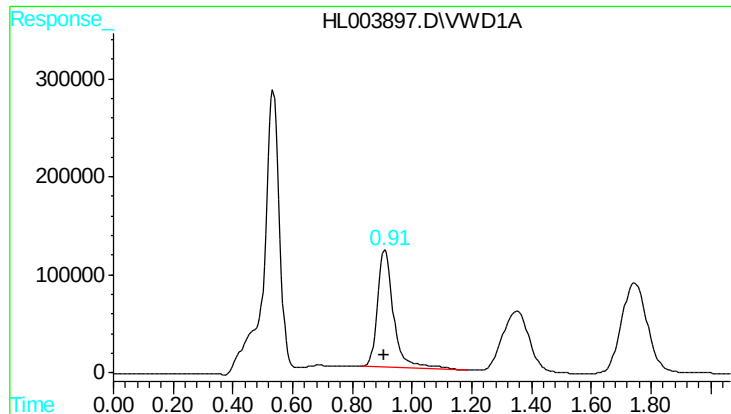

#2 HMX


R.T.: 0.909 min
Delta R.T.: 0.002 min
Response: 4436020
Conc: 1029.54 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

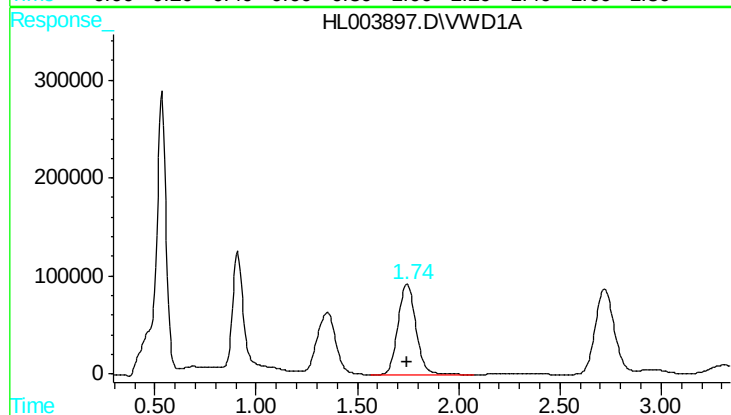


#3 RDX

R.T.: 1.746 min
Delta R.T.: 0.000 min
Response: 5632310
Conc: 1038.49 ug/L

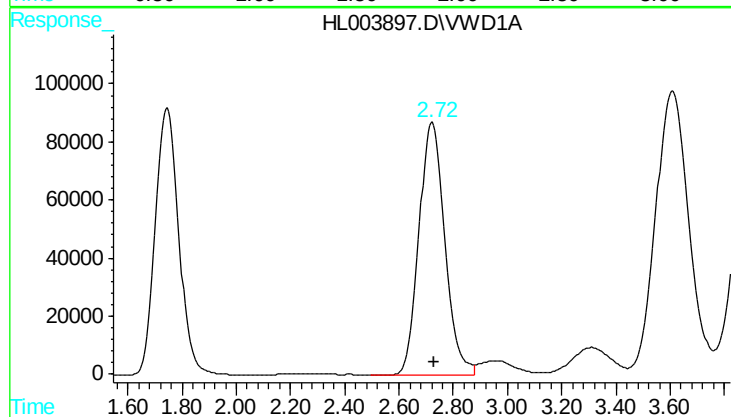


#4 1,3,5-Trinitrobenzene

R.T.: 2.721 min
Delta R.T.: -0.006 min
Response: 5743694
Conc: 484.77 ug/L

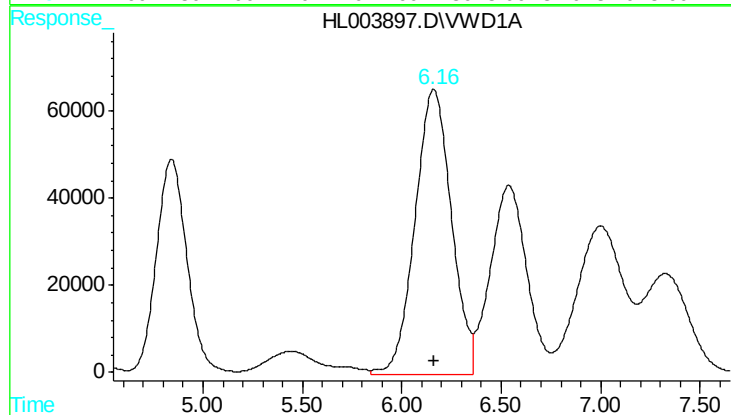

#5 Tetryl


R.T.: 6.160 min
Delta R.T.: -0.002 min
Response: 8334564
Conc: 934.61 ug/L

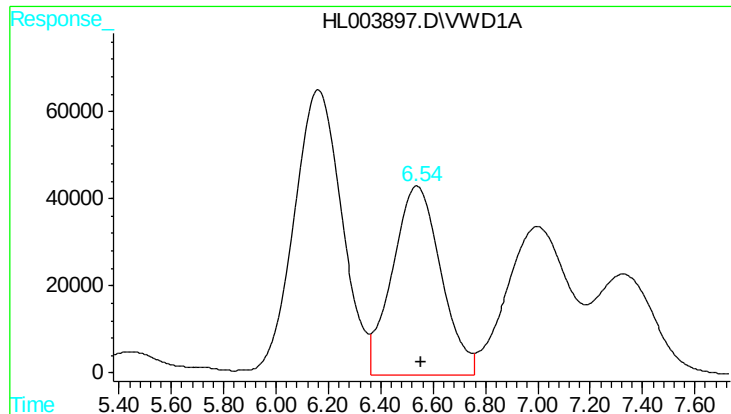

#6 2,4,6-Trinitrotoluene


R.T.: 6.539 min
Delta R.T.: -0.017 min
Response: 5539101
Conc: 472.71 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

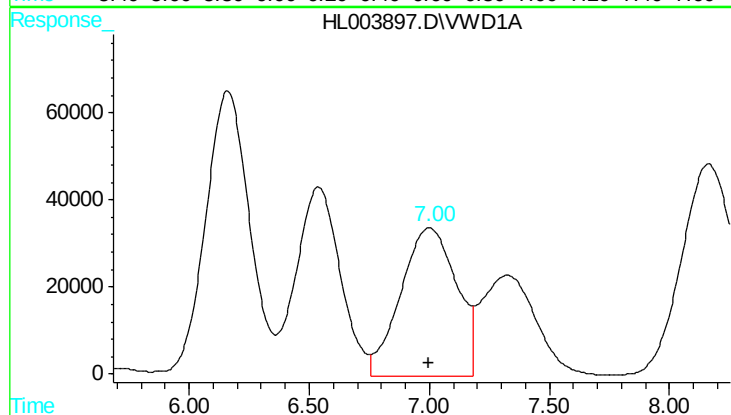


#7 2-Amino-4,6-dinitrotoluene

R.T.: 7.001 min
Delta R.T.: 0.000 min
Response: 5525256
Conc: 489.87 ug/L

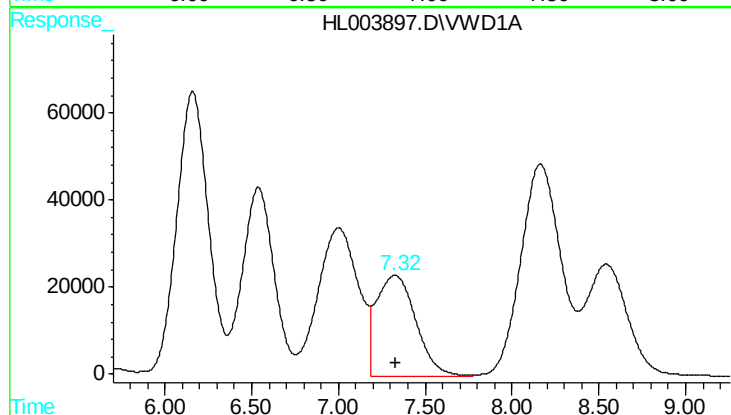


#8 4-Amino-2,6-dinitrotoluene

R.T.: 7.324 min
Delta R.T.: -0.003 min
Response: 3686656
Conc: 503.62 ug/L

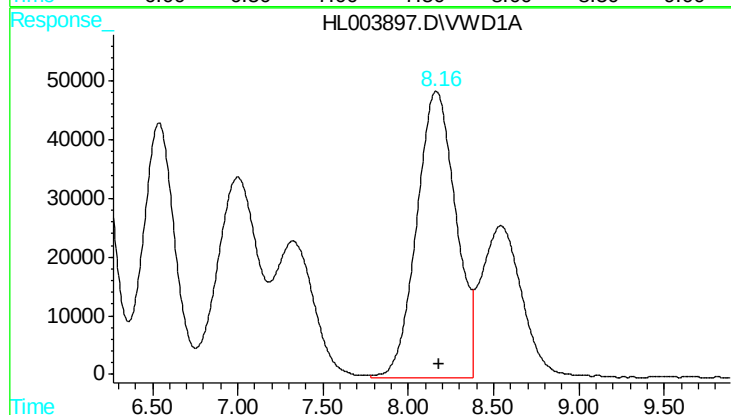

#9 2,4-Dinitrotoluene


R.T.: 8.164 min
Delta R.T.: -0.019 min
Response: 7804318
Conc: 500.84 ug/L

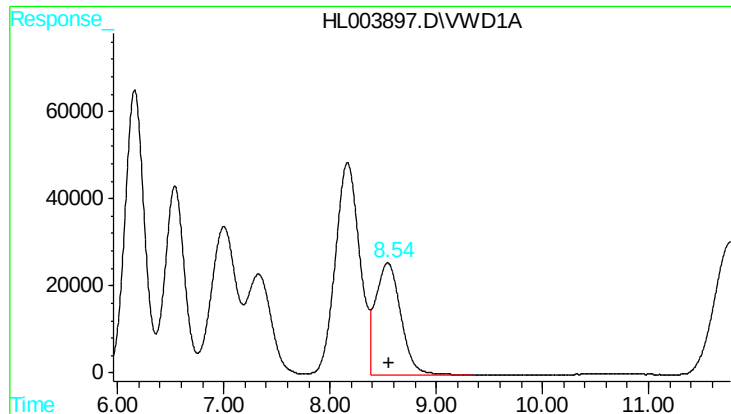

#10 2,6-Dinitrotoluene


R.T.: 8.543 min
Delta R.T.: -0.018 min
Response: 4318361
Conc: 498.81 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

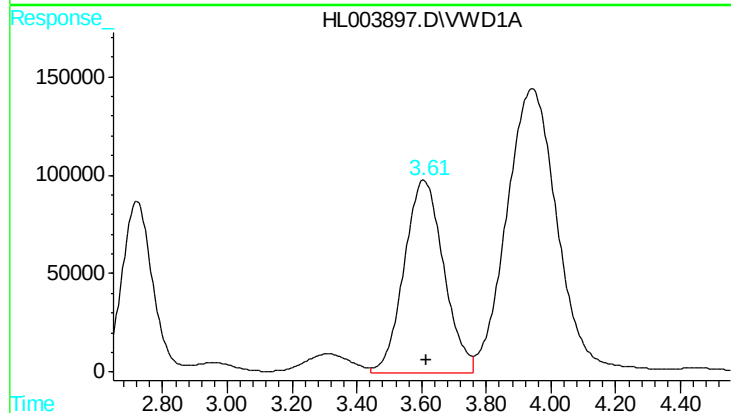


#11 1,3-Dinitrobenzene

R.T.: 3.608 min
Delta R.T.: -0.007 min
Response: 8314913
Conc: 491.11 ug/L

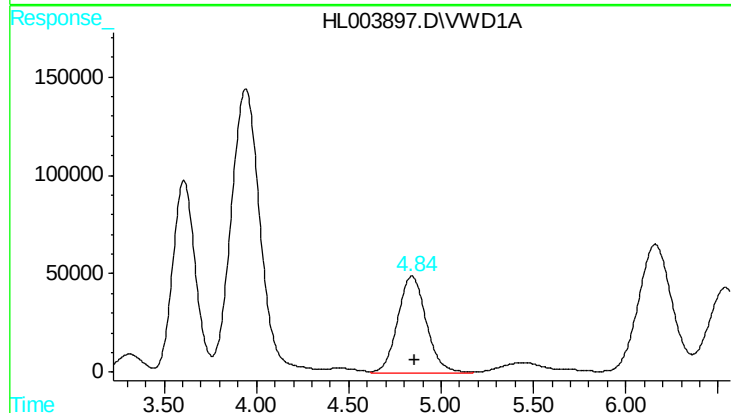


#12 Nitrobenzene

R.T.: 4.842 min
Delta R.T.: -0.013 min
Response: 5314479
Conc: 494.89 ug/L

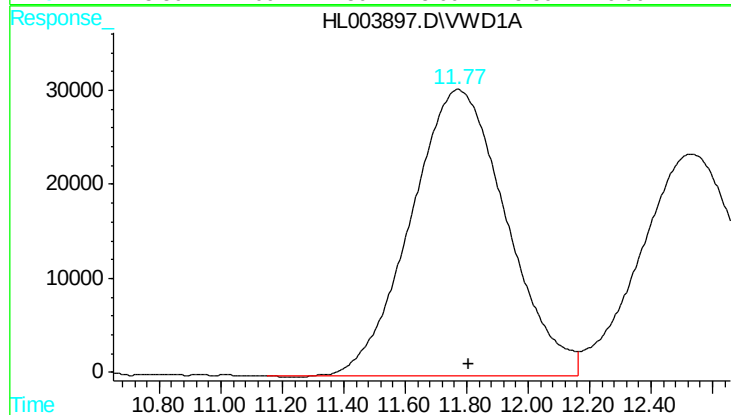

#13 2-Nitrotoluene


R.T.: 11.773 min
Delta R.T.: -0.033 min
Response: 6604336
Conc: 997.19 ug/L

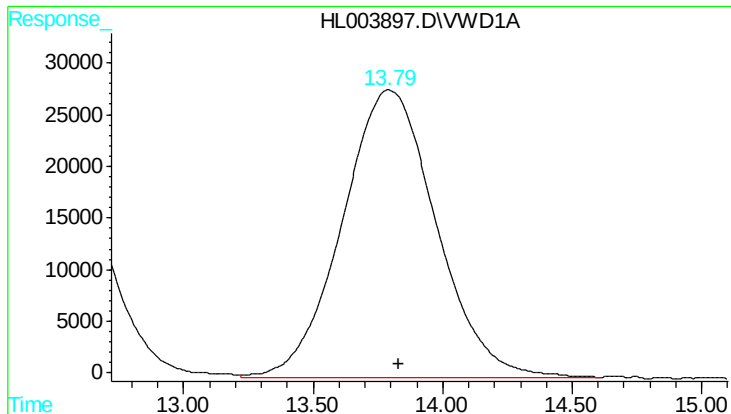

#14 3-Nitrotoluene


R.T.: 13.793 min
Delta R.T.: -0.039 min
Response: 7035159
Conc: 989.20 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

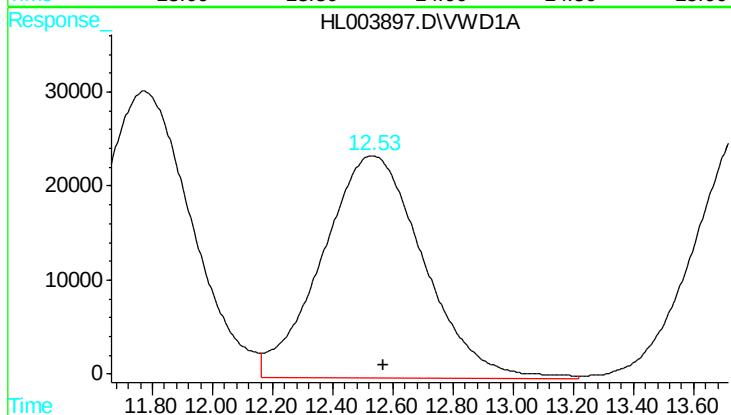


#15 4-Nitrotoluene

R.T.: 12.532 min
Delta R.T.: -0.038 min
Response: 5548743
Conc: 1011.25 ug/L

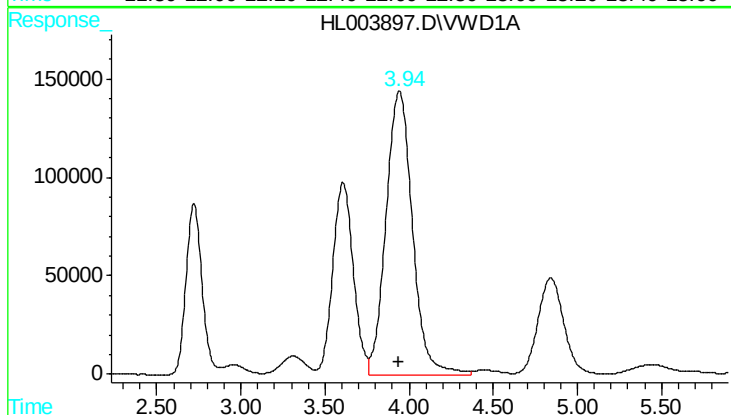


#16 3,5-Dinitroaniline

R.T.: 3.942 min
Delta R.T.: 0.000 min
Response: 15842321
Conc: 994.55 ug/L

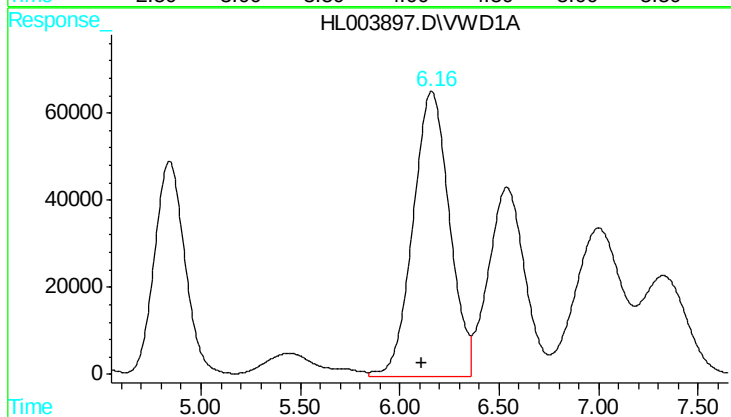

#17 Nitroglycerin

R.T.: 6.160 min
Delta R.T.: 0.047 min
Response: 8334564
Conc: 148592.10 ug/L

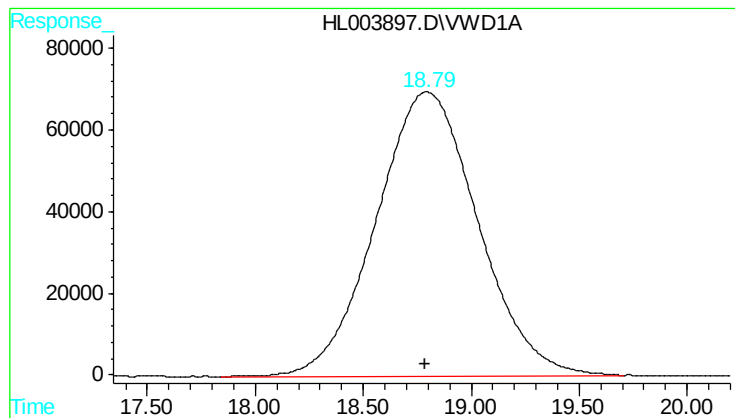

#18 PETN

R.T.: 18.794 min
Delta R.T.: 0.005 min
Response: 22904152
Conc: 2496.27 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV