

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003905.D Vial: 47
 Acq On : 01-Jan-2013, 14:42 Operator: HLM
 Sample : PB67574BS2 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Jan 2 11:27 2013 Quant Results File: HL123112.RES

Instrument :
 HPLC_L
 ClientSampleId :
 PB67574BS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Wed Jan 02 11:22:54 2013
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S 4-Nitroaniline	1.35	1025687	263.840 ug/L
Spiked Amount 300.000	Range 37 - 149	Recovery	= 87.95%

Target Compounds


5) T Tetrvl	6.12f	251134	28.161 ug/L
17) T Nitroglycerin	6.12	251134	4477.327 ug/L


Data File : H:\VOL1\HPLC\HPLC L\121231\HL003905.D Vial: 47
Acq On : 01-Jan-2013, 14:42 Operator: HLM
Sample : PB67574BS2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Jan 2 11:27 2013 Quant Results File: HL123112.RES

Instrument :
HPLC_L
ClientSampleId :
PB67574BS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Wed Jan 02 11:22:54 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

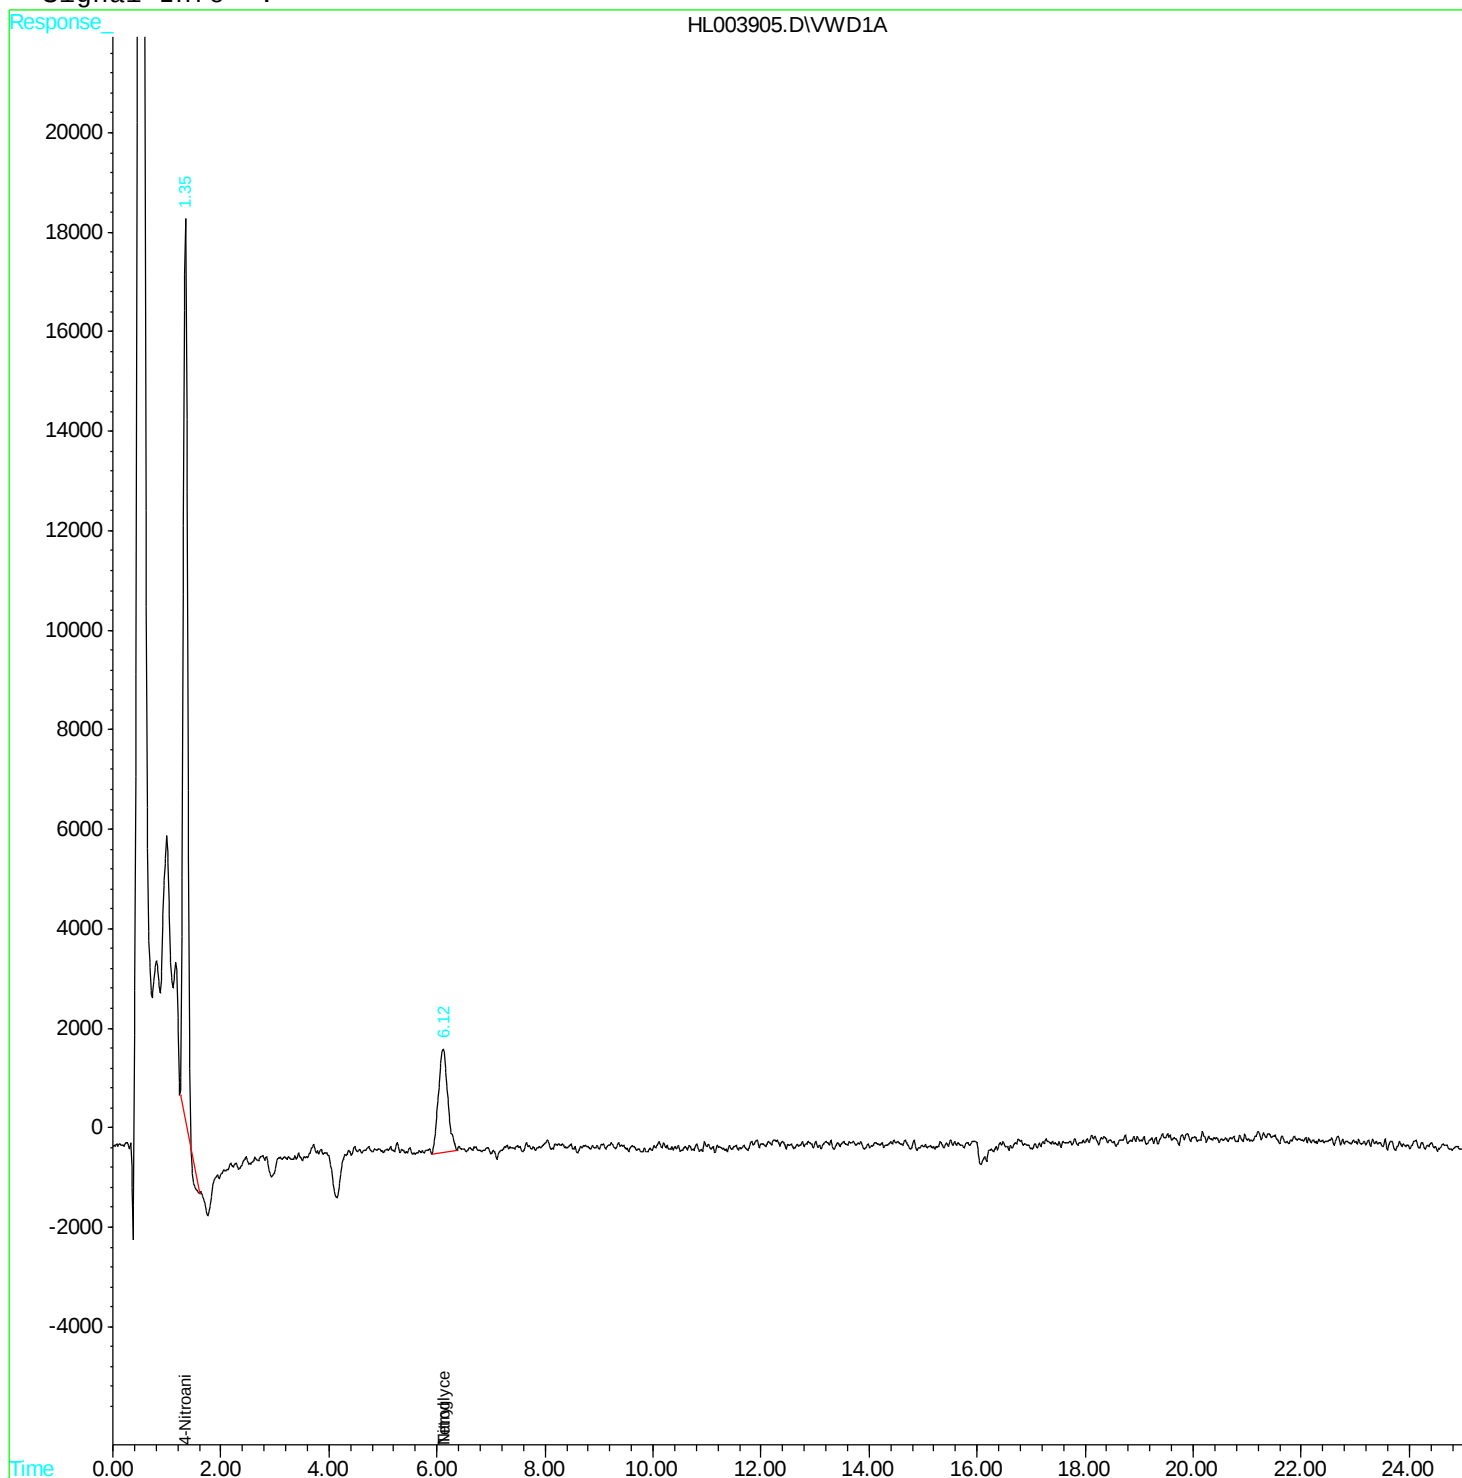


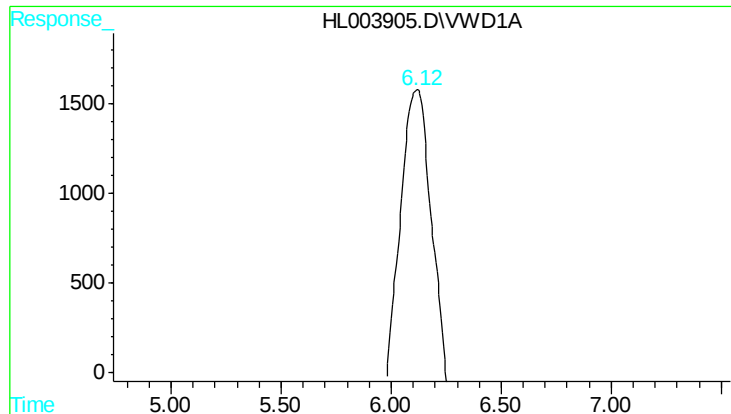

#5 Tetryl

R.T.: 6.120 min
Delta R.T.: -0.042 min
Response: 251134
Conc: 28.16 ug/L

Instrument :
HPLC_L
ClientSampleId :
PB67574BS2

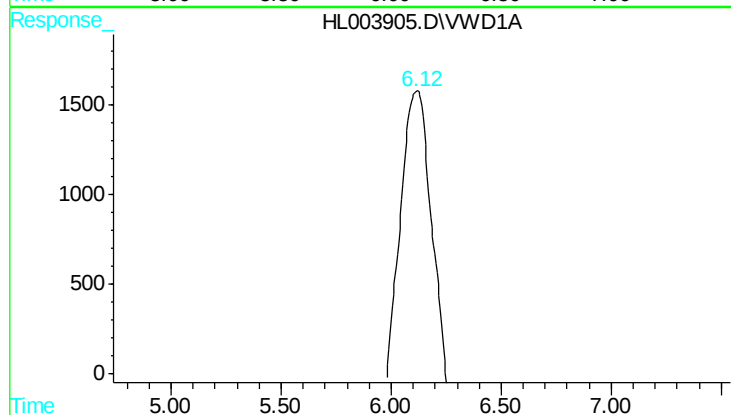

#17 Nitroglycerin

R.T.: 6.120 min
Delta R.T.: 0.006 min
Response: 251134
Conc: 4477.33 ug/L