

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003907.D Vial: 49
Acq On : 01-Jan-2013, 15:36 Operator: HLM
Sample : PB67574BSD2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Jan 2 11:27 2013 Quant Results File: HL123112.RES

Instrument :
HPLC_L
ClientSampleId :
PB67574BSD2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Wed Jan 02 11:22:54 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.35	965377	248.327 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 82.78%

Target Compounds

5) T	Tetrvl	6.11f	254026	28.486 ug/L
17) T	Nitroglycerin	6.11	254026	4528.885 ug/L


Quantitation Report


Data File : H:\VOL1\HPLC\HPLC L\121231\HL003907.D Vial: 49
 Acq On : 01-Jan-2013, 15:36 Operator: HLM
 Sample : PB67574BSD2 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Jan 2 11:27 2013 Quant Results File: HL123112.RES

Instrument :
 HPLC_L
 ClientSampleId :
 PB67574BSD2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Wed Jan 02 11:22:54 2013
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

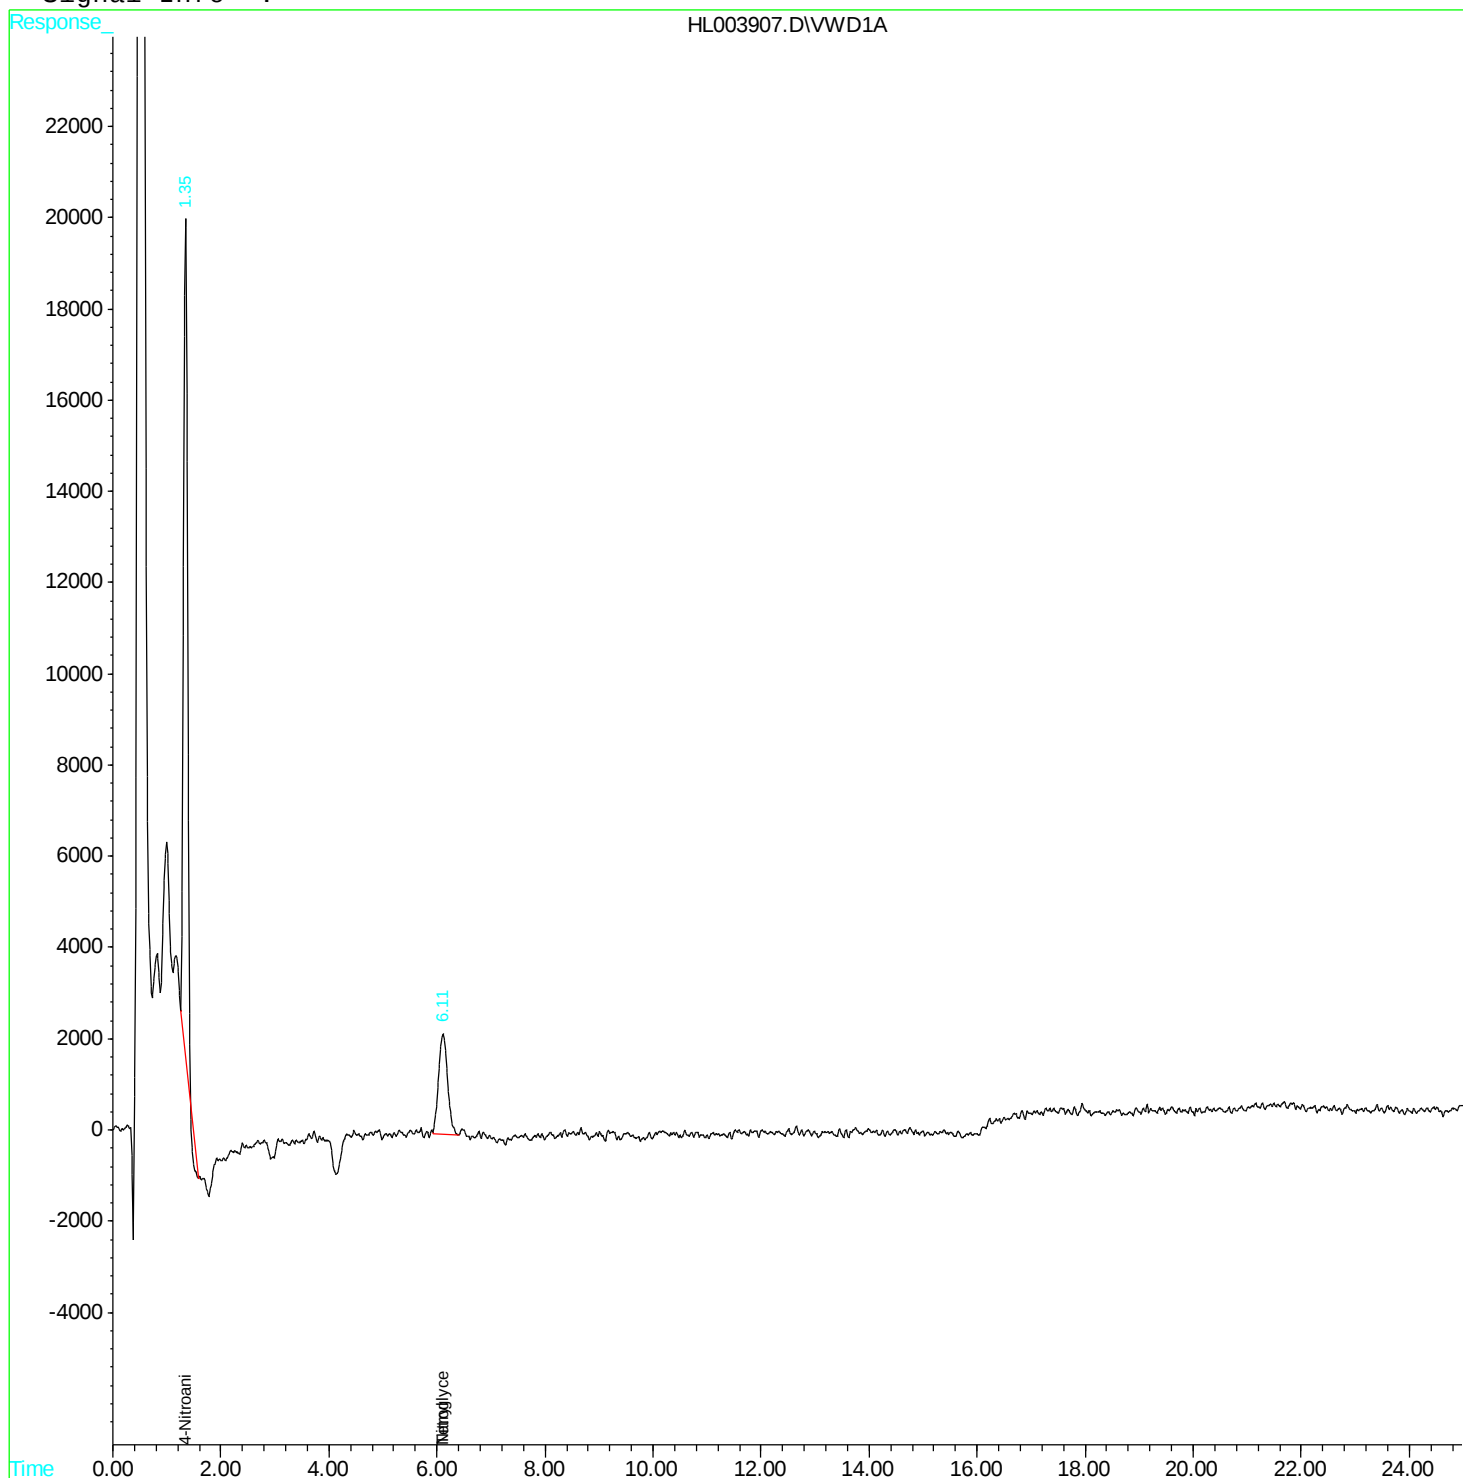


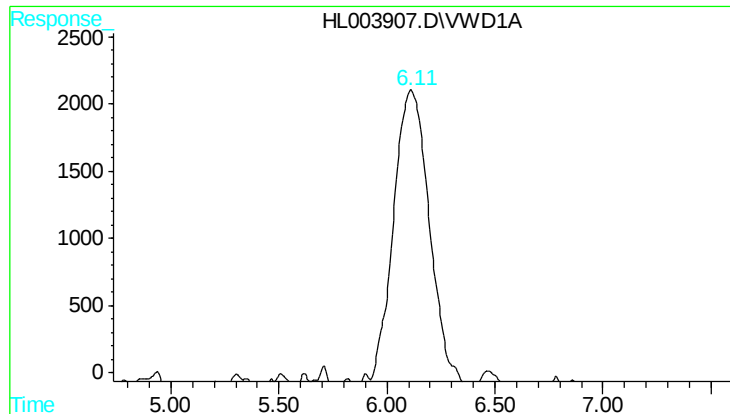

#5 Tetryl

R.T.: 6.111 min
Delta R.T.: -0.051 min
Response: 254026
Conc: 28.49 ug/L

Instrument :
HPLC_L
ClientSampleId :
PB67574BSD2

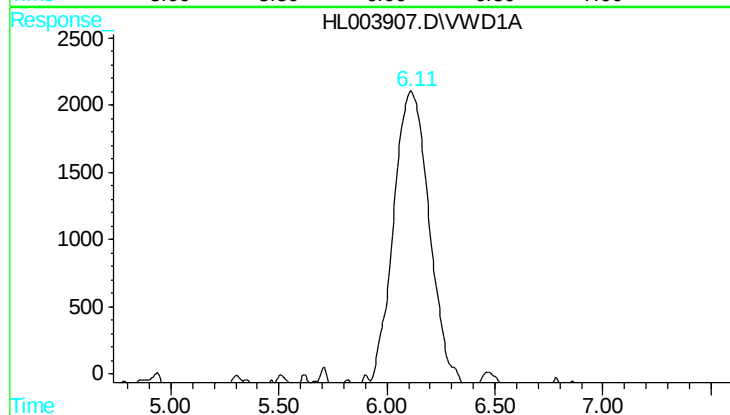

#17 Nitroglycerin

R.T.: 6.111 min
Delta R.T.: -0.002 min
Response: 254026
Conc: 4528.89 ug/L