

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003910.D Vial: 2
 Acq On : 01-Jan-2013, 16:57 Operator: HLM
 Sample : 8330-CCV Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Jan 2 11:27 2013 Quant Results File: HL123112.RES

Instrument :
 HPLC_L
 LabSampleId :
 8330-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Wed Jan 02 11:22:54 2013
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.35	3682866	947.354 ug/L
Spiked Amount 300.000 Range 37 - 149		Recovery	=	315.78%#

Target Compounds

2) T	HMX	0.91	4499200	1045.542 ug/L
3) T	RDX	1.74	5635664	1039.111 ug/L
4) T	1,3,5-Trinitrobenzene	2.72	5766691	486.709 ug/L
5) T	Tetryl	6.15	8236662	923.629 ug/L
6) T	2,4,6-Trinitrotoluene	6.53	5536206	472.459 ug/L
7) T	2-Amino-4,6-dinitrotoluene	6.99	5488346	486.596 ug/L
8) T	4-Amino-2,6-dinitrotoluene	7.32	3681964	502.976 ug/L
9) T	2,4-Dinitrotoluene	8.15	7735563	496.426 ug/L
10) T	2,6-Dinitrotoluene	8.53	4213548	486.704 ug/L
11) T	1,3-Dinitrobenzene	3.60	8348821	493.113 ug/L
12) T	Nitrobenzene	4.83	5319791	495.382 ug/L
13) T	2-Nitrotoluene	11.75f	6633583	1001.605 ug/L
14) T	3-Nitrotoluene	13.76	7176499	1009.075 ug/L
15) T	4-Nitrotoluene	12.50f	5606498	1021.772 ug/L
16) T	3,5-Dinitroaniline	3.94	15839246	994.354 ug/L
17) T	Nitroglycerin	6.15f	8236662	146846.655 ug/L
18) T	PETN	18.77	22802620	2485.202 ug/L

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003910.D

Vial: 2

Acq On : 01-Jan-2013, 16:57

Operator: HLM

Sample : 8330-CCV

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Jan 2 11:27 2013 Quant Results File: HL123112.RES

Instrument :

HPLC_L

LabSampleId :

8330-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)

Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)

Last Update : Wed Jan 02 11:22:54 2013


Response via : Multiple Level Calibration


DataAcq Meth : 8330AGIP.M

Volume Inj. :

Signal Phase :

Signal Info :

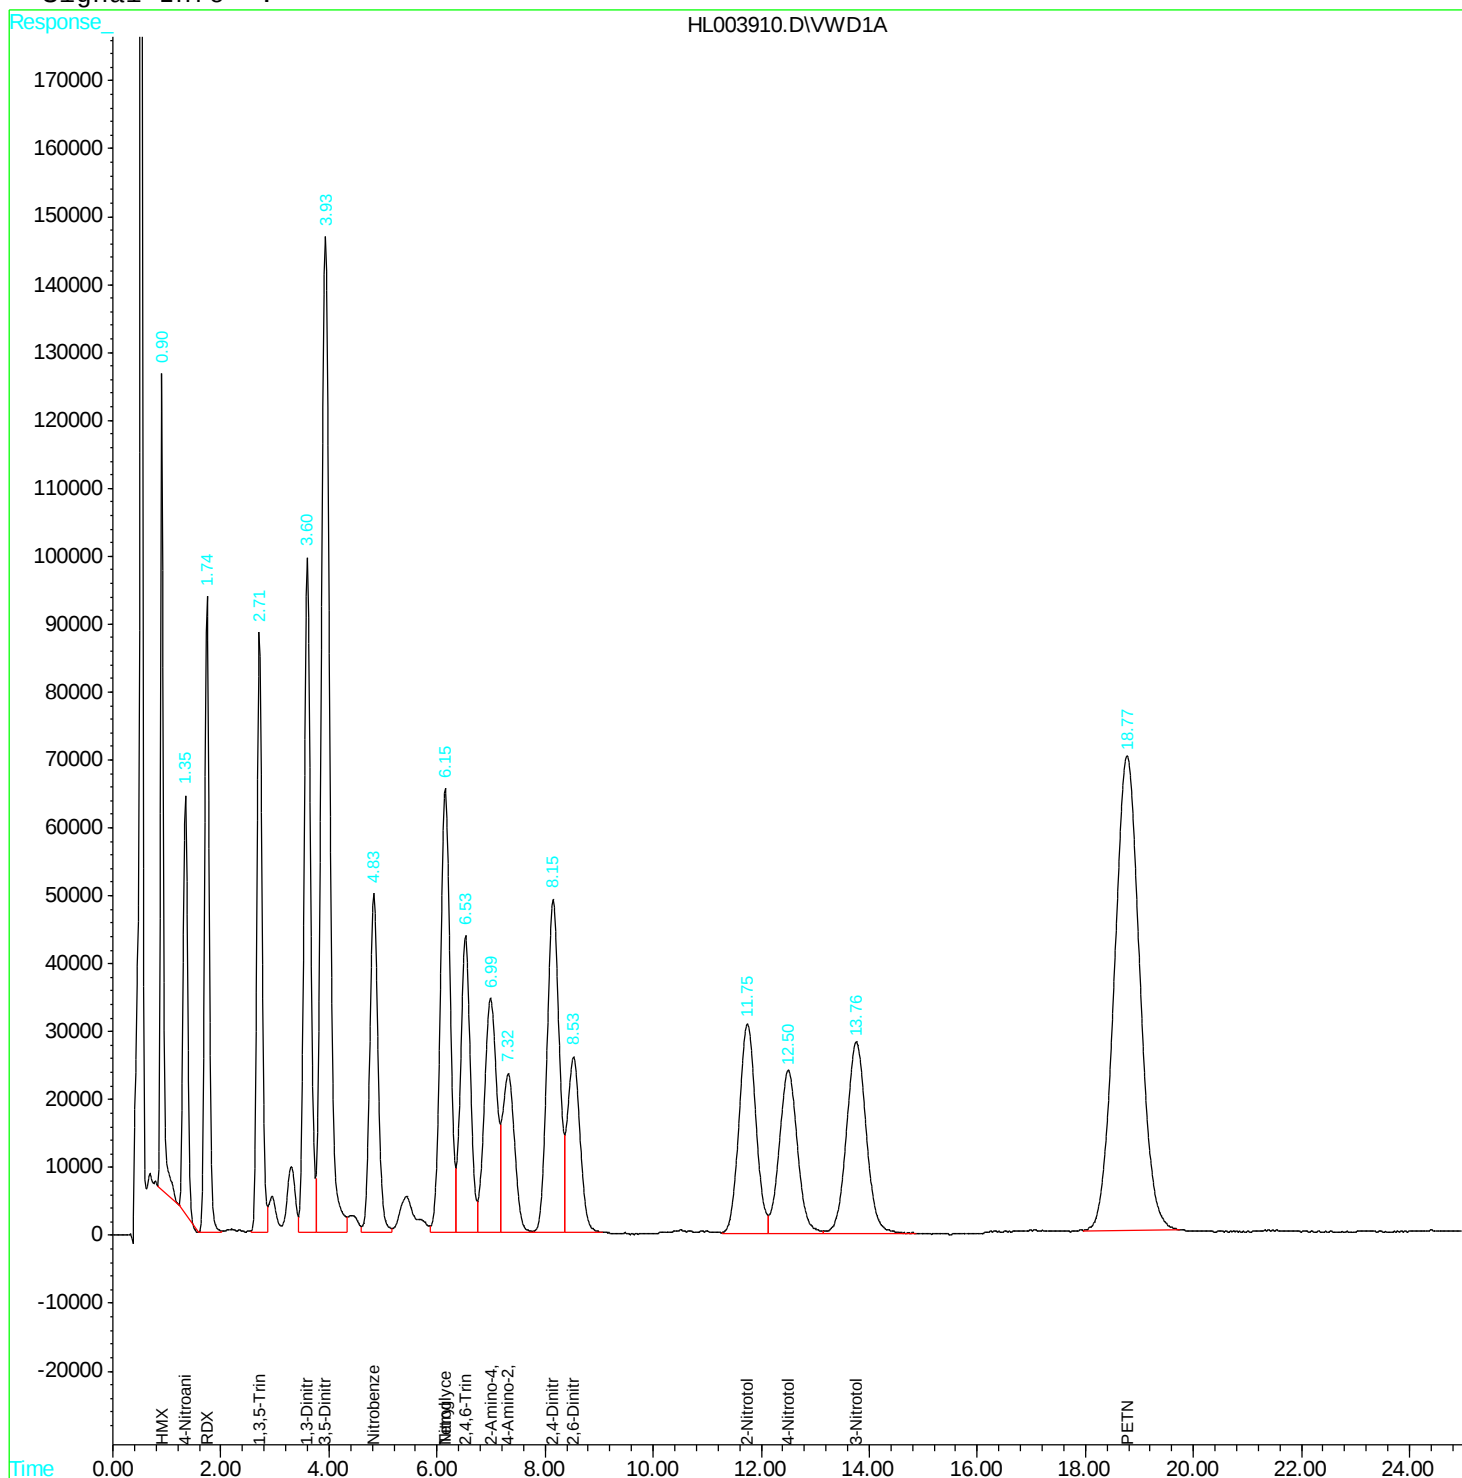


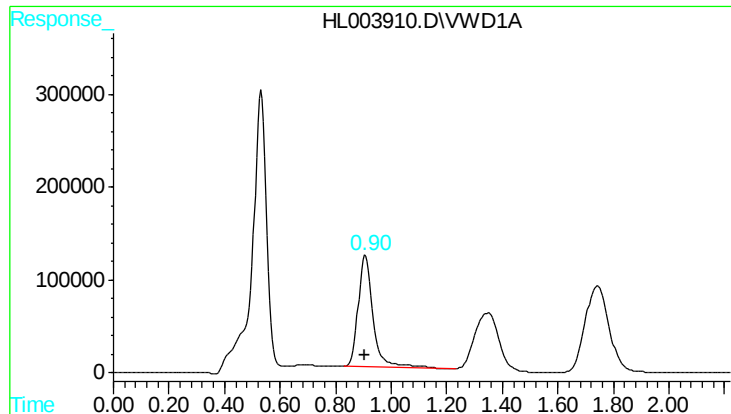

#2 HMX


R.T.: 0.906 min
Delta R.T.: 0.000 min
Response: 4499200
Conc: 1045.54 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

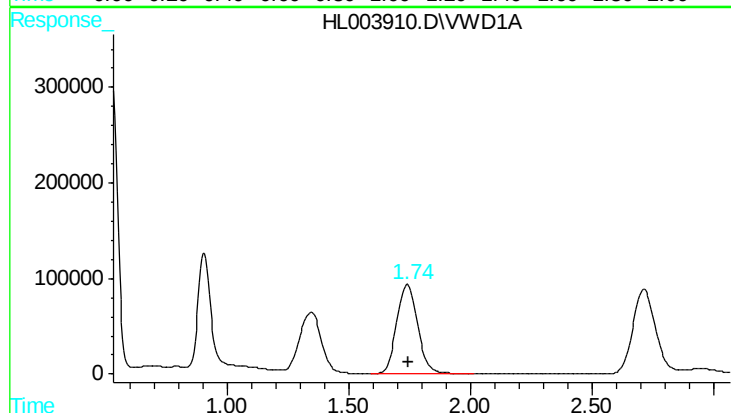


#3 RDX

R.T.: 1.742 min
Delta R.T.: -0.004 min
Response: 5635664
Conc: 1039.11 ug/L

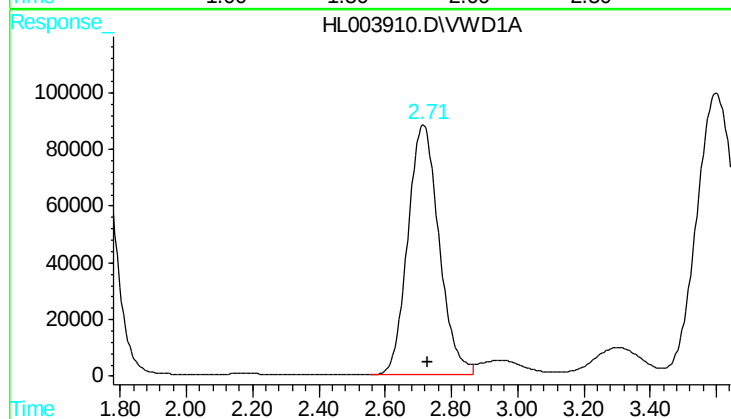


#4 1,3,5-Trinitrobenzene

R.T.: 2.715 min
Delta R.T.: -0.012 min
Response: 5766691
Conc: 486.71 ug/L

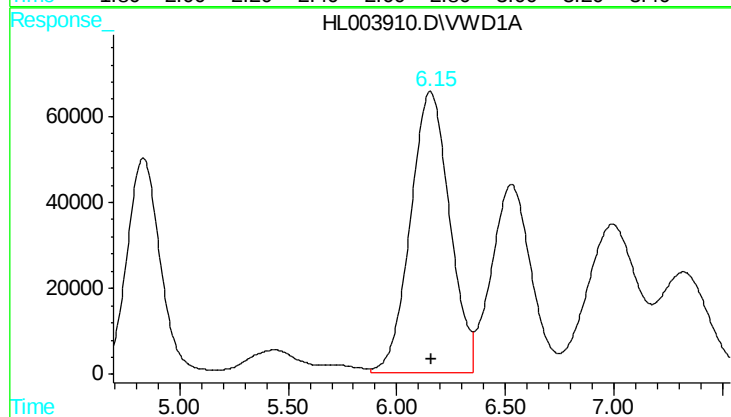

#5 Tetryl


R.T.: 6.155 min
Delta R.T.: -0.007 min
Response: 8236662
Conc: 923.63 ug/L

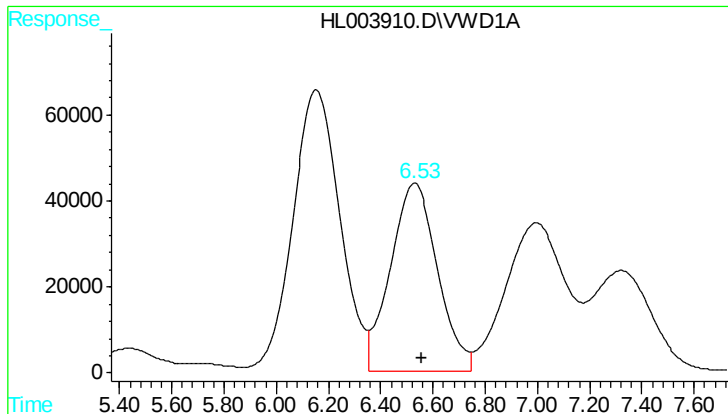

#6 2,4,6-Trinitrotoluene


R.T.: 6.529 min
Delta R.T.: -0.026 min
Response: 5536206
Conc: 472.46 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

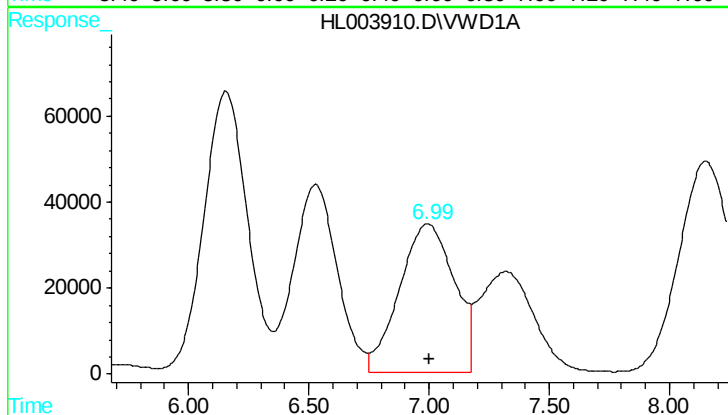


#7 2-Amino-4,6-dinitrotoluene

R.T.: 6.994 min
Delta R.T.: -0.008 min
Response: 5488346
Conc: 486.60 ug/L

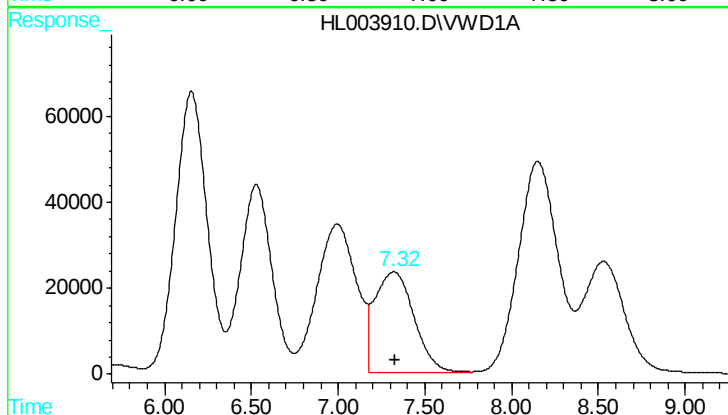


#8 4-Amino-2,6-dinitrotoluene

R.T.: 7.320 min
Delta R.T.: -0.007 min
Response: 3681964
Conc: 502.98 ug/L

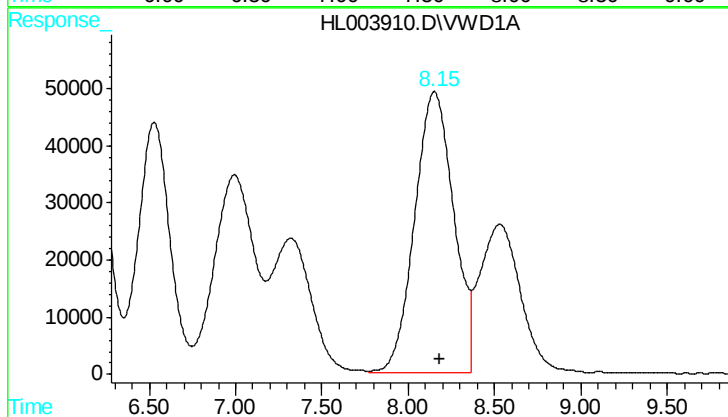

#9 2,4-Dinitrotoluene


R.T.: 8.151 min
Delta R.T.: -0.032 min
Response: 7735563
Conc: 496.43 ug/L

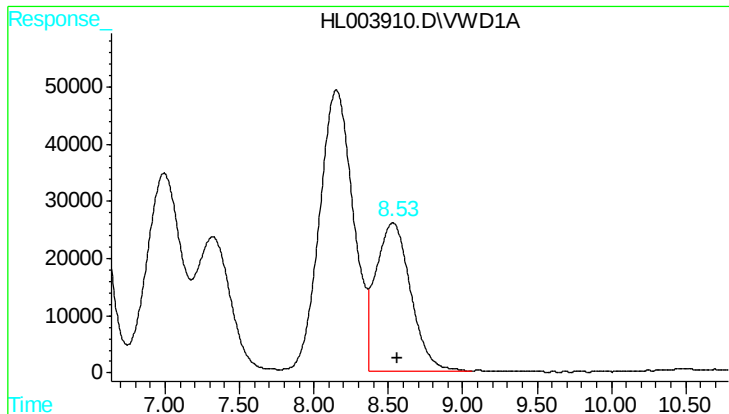

#10 2,6-Dinitrotoluene


R.T.: 8.530 min
Delta R.T.: -0.031 min
Response: 4213548
Conc: 486.70 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

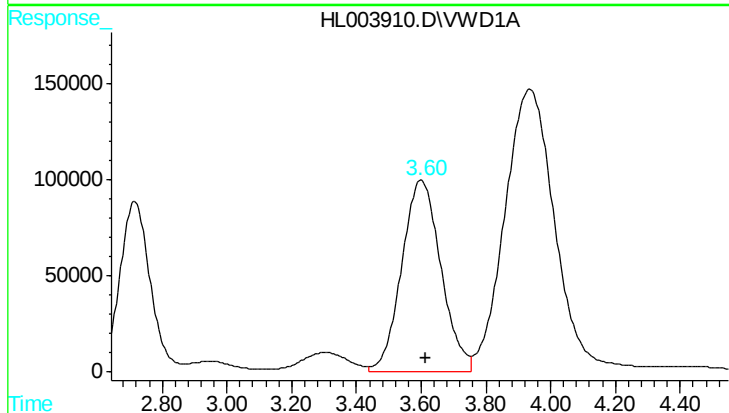


#11 1,3-Dinitrobenzene

R.T.: 3.601 min
Delta R.T.: -0.014 min
Response: 8348821
Conc: 493.11 ug/L

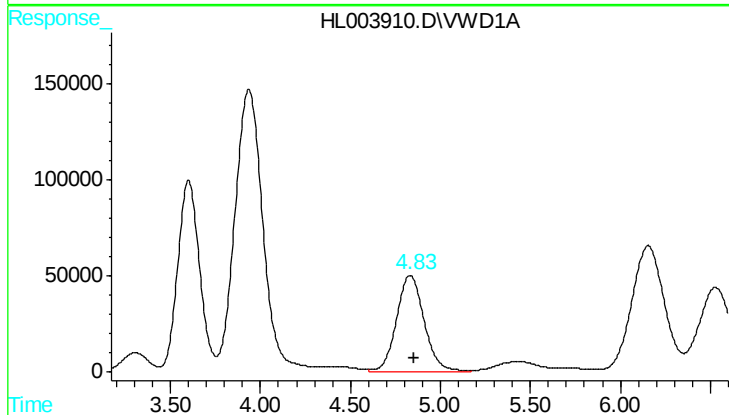


#12 Nitrobenzene

R.T.: 4.832 min
Delta R.T.: -0.023 min
Response: 5319791
Conc: 495.38 ug/L

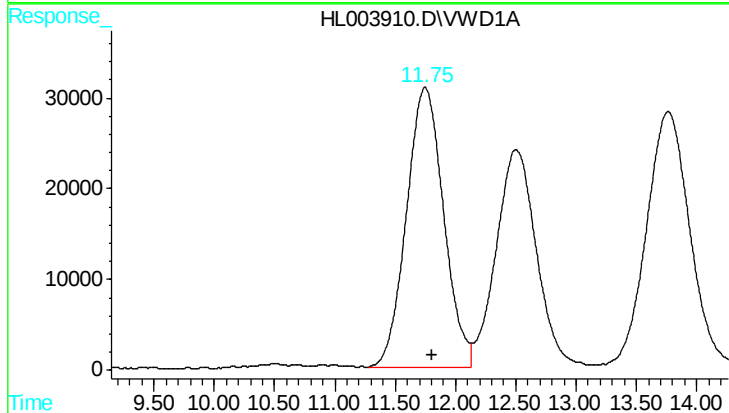

#13 2-Nitrotoluene


R.T.: 11.748 min
Delta R.T.: -0.058 min
Response: 6633583
Conc: 1001.61 ug/L

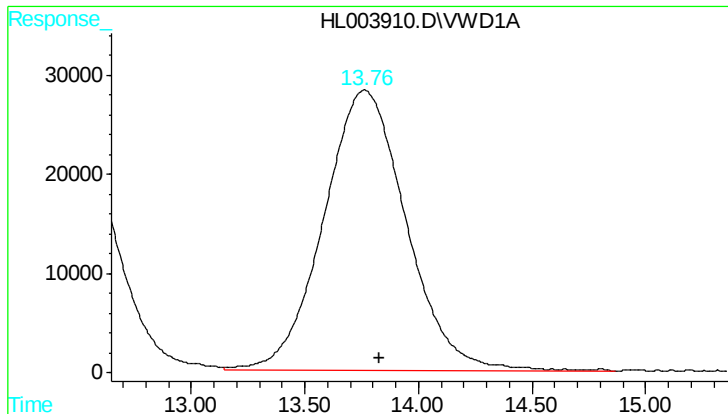

#14 3-Nitrotoluene


R.T.: 13.763 min
Delta R.T.: -0.069 min
Response: 7176499
Conc: 1009.07 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

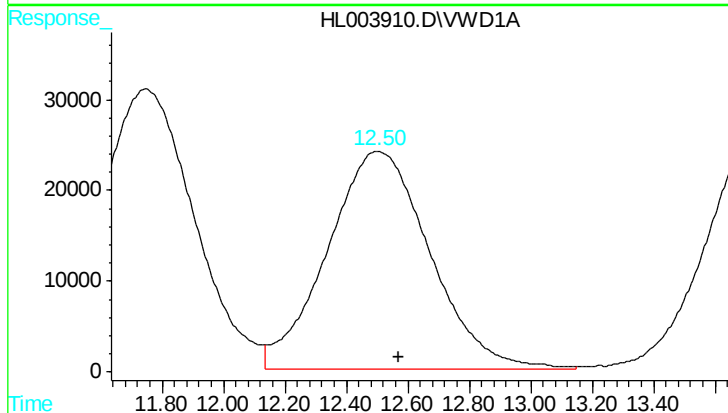


#15 4-Nitrotoluene

R.T.: 12.502 min
Delta R.T.: -0.068 min
Response: 5606498
Conc: 1021.77 ug/L

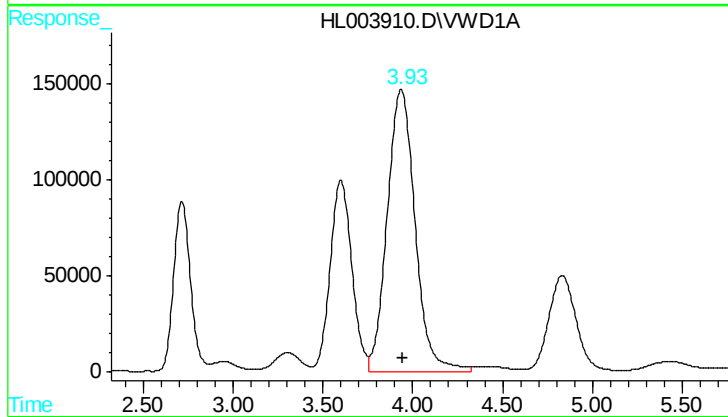


#16 3,5-Dinitroaniline

R.T.: 3.936 min
Delta R.T.: -0.006 min
Response: 15839246
Conc: 994.35 ug/L

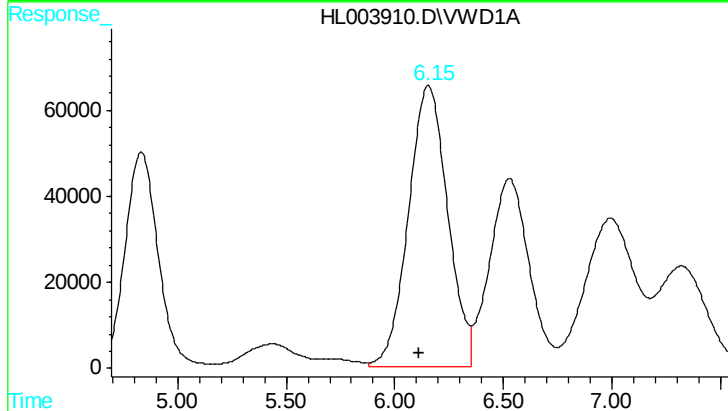

#17 Nitroglycerin

R.T.: 6.155 min
Delta R.T.: 0.042 min
Response: 8236662
Conc: 146846.65 ug/L

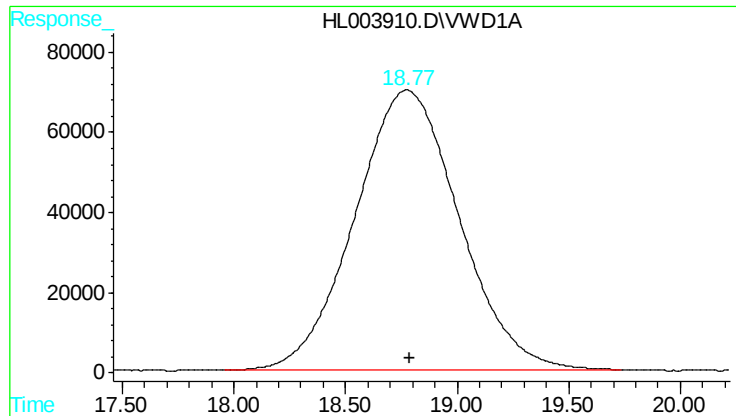

#18 PETN

R.T.: 18.774 min
Delta R.T.: -0.014 min
Response: 22802620
Conc: 2485.20 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV