

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003916.D Vial: 55
Acq On : 01-Jan-2013, 19:39 Operator: HLM
Sample : PB67745BS2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Jan 2 11:28 2013 Quant Results File: HL123112.RES

Instrument :
HPLC_L
ClientSampleId :
PB67745BS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Wed Jan 02 11:22:54 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.35	610885	157.140 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 52.38%

Target Compounds

5) T	Tetryl	6.11f	137327	15.399 ug/L
17) T	Nitroglycerin	6.11	137327	2448.330 ug/L

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003916.D

Vial: 55

Acq On : 01-Jan-2013, 19:39

Operator: HLM

Sample : PB67745BS2

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Jan 2 11:28 2013 Quant Results File: HL123112.RES

Instrument :

HPLC_L

ClientSampleId :

PB67745BS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)

Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)

Last Update : Wed Jan 02 11:22:54 2013


Response via : Multiple Level Calibration


DataAcq Meth : 8330AGIP.M

Volume Inj. :

Signal Phase :

Signal Info :

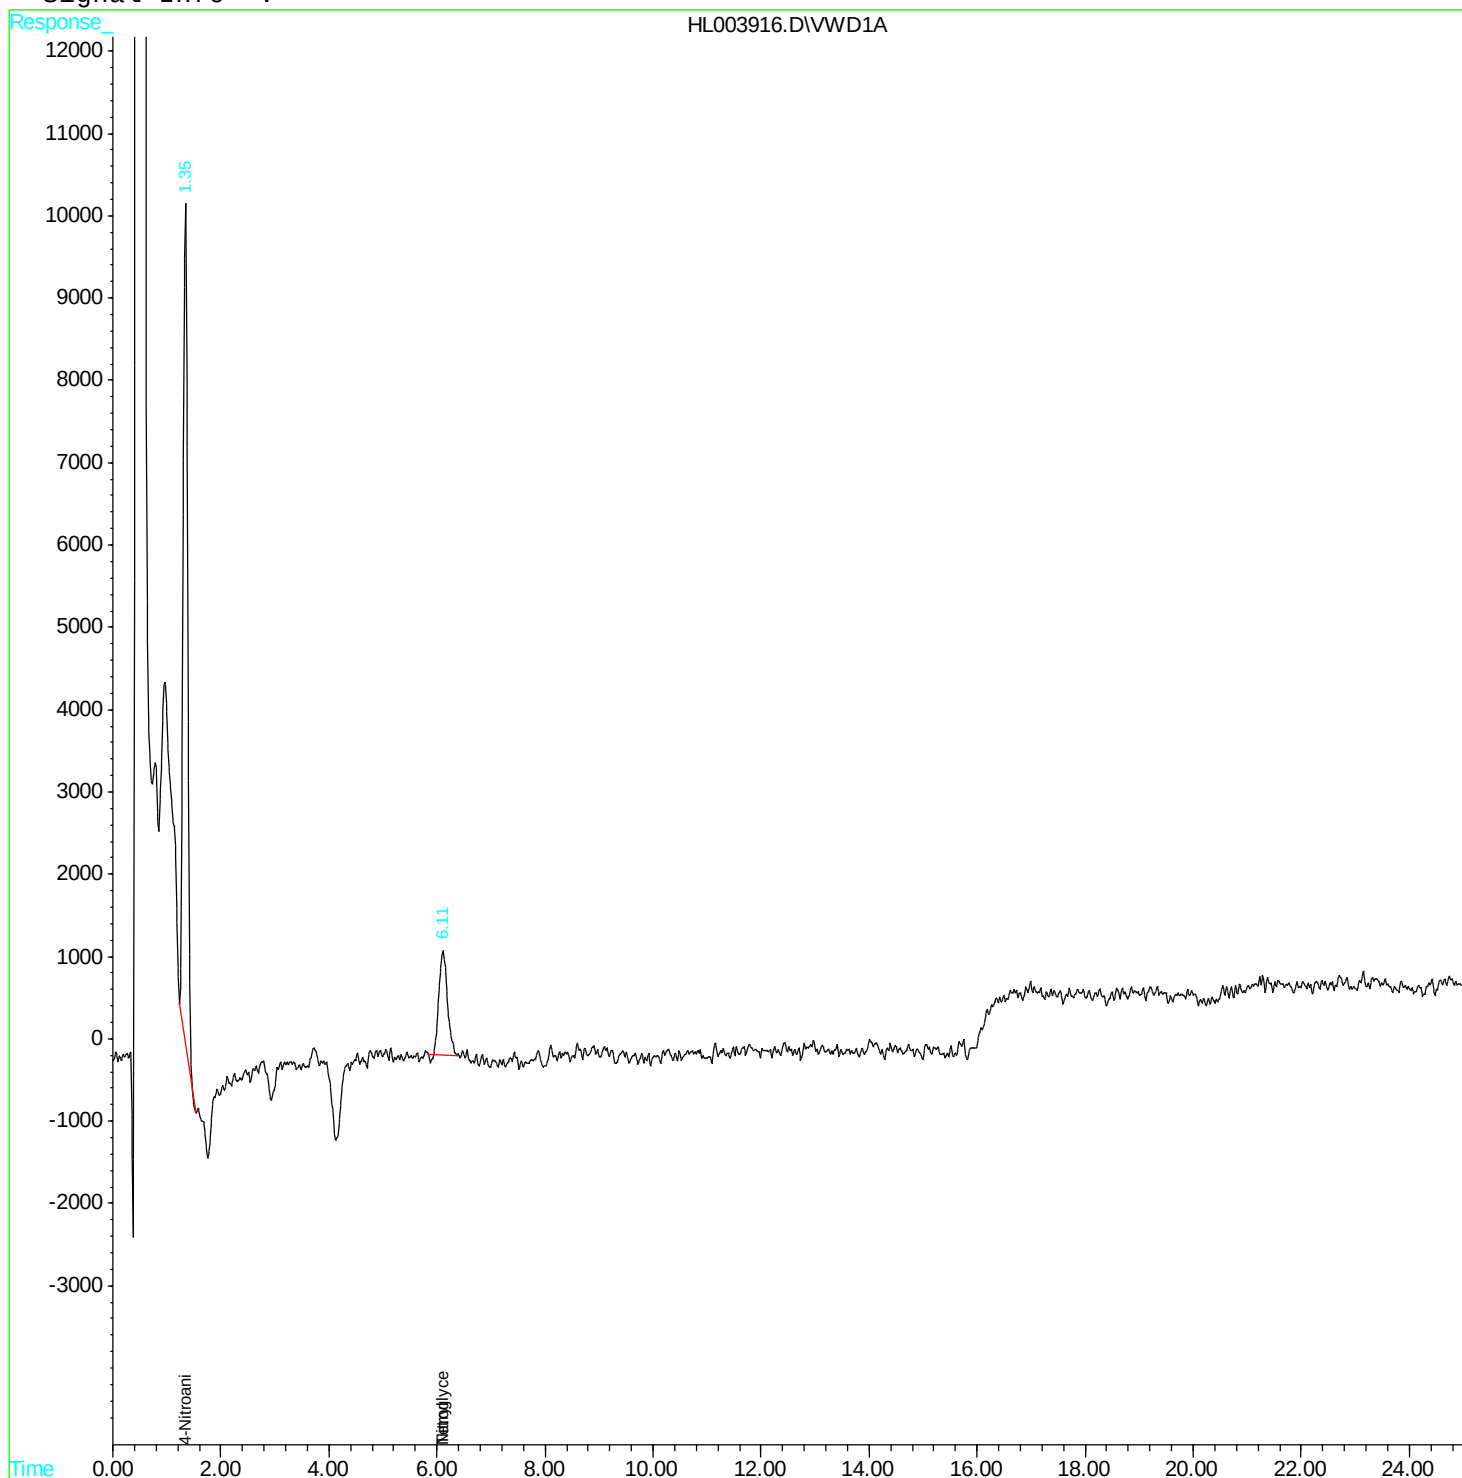


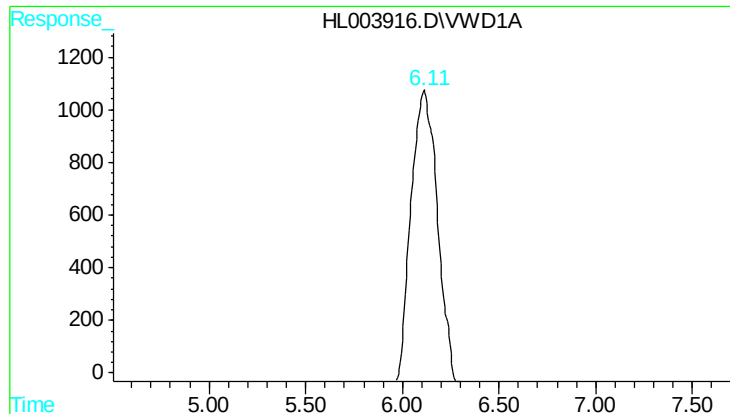

#5 Tetryl

R.T.: 6.113 min
Delta R.T.: -0.049 min
Response: 137327
Conc: 15.40 ug/L

Instrument :
HPLC_L
ClientSampleId :
PB67745BS2

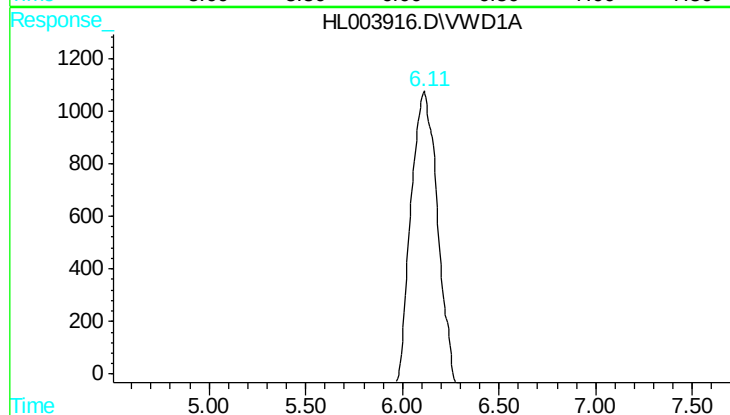

#17 Nitroglycerin

R.T.: 6.113 min
Delta R.T.: 0.000 min
Response: 137327
Conc: 2448.33 ug/L