

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003917.D Vial: 56
 Acq On : 01-Jan-2013, 20:06 Operator: HLM
 Sample : D5190-01 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Jan 2 11:28 2013 Quant Results File: HL123112.RES

Instrument :
 HPLC_L
 ClientSampleId :
 BACKGROUND-ISM-1

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Wed Jan 02 11:22:54 2013
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S 4-Nitroaniline	1.35	441548	113.581 ug/L
Spiked Amount 300.000	Range 37 - 149	Recovery	= 37.86%

Target Compounds

12) T Nitrobenzene	4.90f	4554	0.424 ug/L
--------------------	-------	------	------------


Quantitation Report


Data File : H:\VOL1\HPLC\HPLC L\121231\HL003917.D Vial: 56
 Acq On : 01-Jan-2013, 20:06 Operator: HLM
 Sample : D5190-01 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Jan 2 11:28 2013 Quant Results File: HL123112.RES

Instrument :
 HPLC_L
 ClientSampleId :
 BACKGROUND-ISM-1

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Wed Jan 02 11:22:54 2013
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

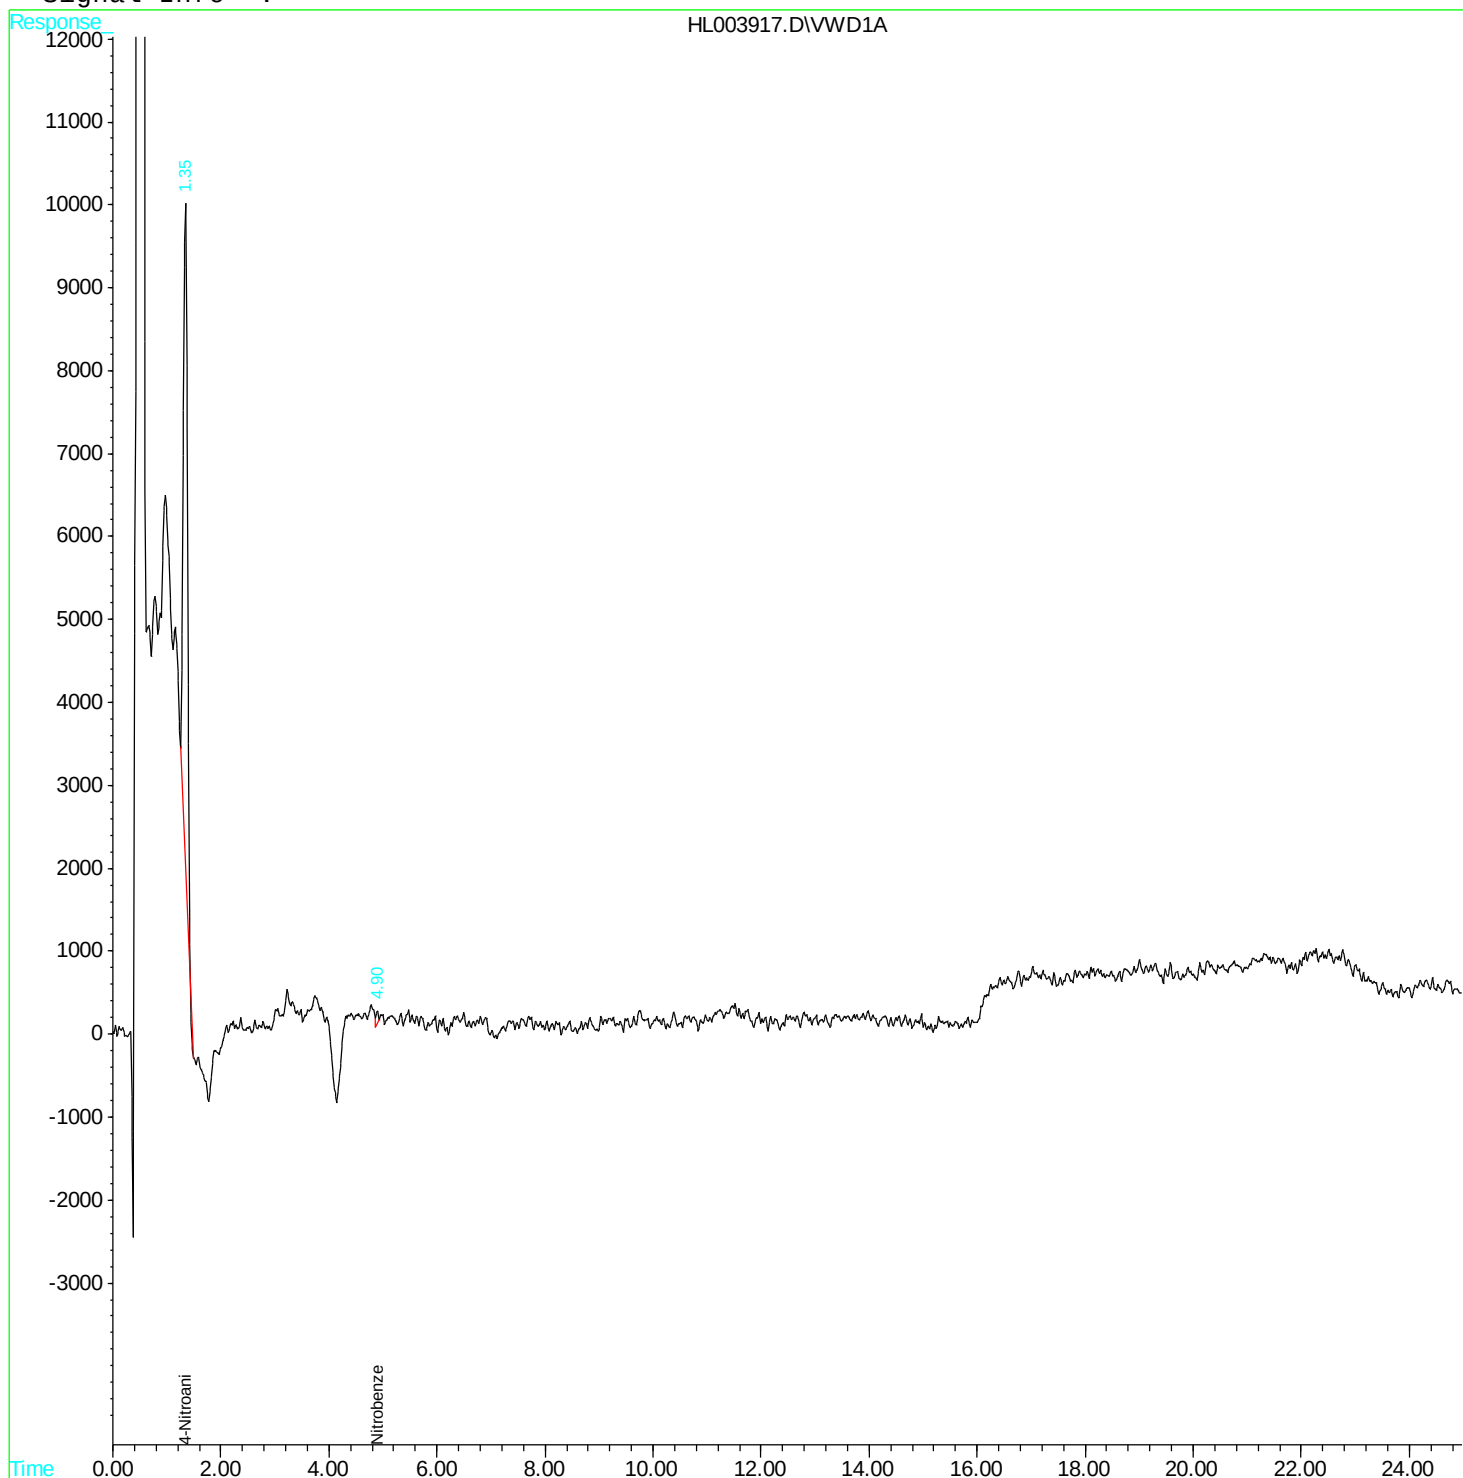

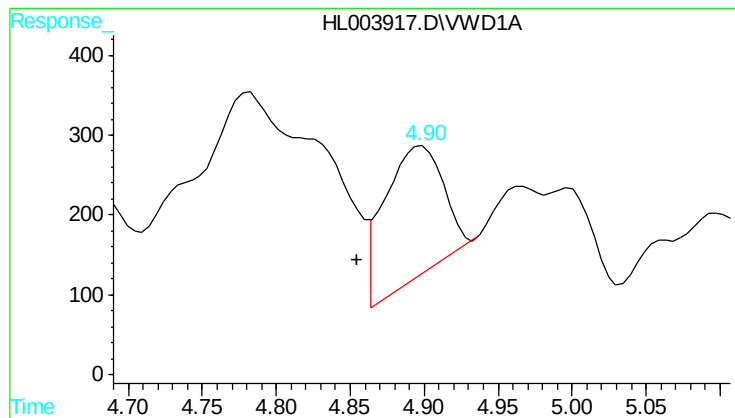

#12 Nitrobenzene

R.T.: 4.898 min
Delta R.T.: 0.043 min
Response: 4554
Conc: 0.42 ug/L

Instrument :
HPLC_L
ClientSampleId :
BACKGROUND-ISM-1