

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003920.D Vial: 59
 Acq On : 01-Jan-2013, 21:26 Operator: HLM
 Sample : D5190-02MS2 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Jan 2 11:28 2013 Quant Results File: HL123112.RES

Instrument :
 HPLC_L
 ClientSampleId :
 BACKGROUND-ISM-2MS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Wed Jan 02 11:22:54 2013
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S 4-Nitroaniline	1.35	361654	93.029 ug/L
Spiked Amount 300.000	Range 37 - 149	Recovery =	31.01%#

Target Compounds

5) T Tetrvl	6.13f	120321	13.492 ug/L
17) T Nitroglycerin	6.13	120321	2145.138 ug/L


Quantitation Report


Data File : H:\VOL1\HPLC\HPLC L\121231\HL003920.D Vial: 59
 Acq On : 01-Jan-2013, 21:26 Operator: HLM
 Sample : D5190-02MS2 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Jan 2 11:28 2013 Quant Results File: HL123112.RES

Instrument :
 HPLC_L
 ClientSampleId :
 BACKGROUND-ISM-2MS2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Wed Jan 02 11:22:54 2013
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

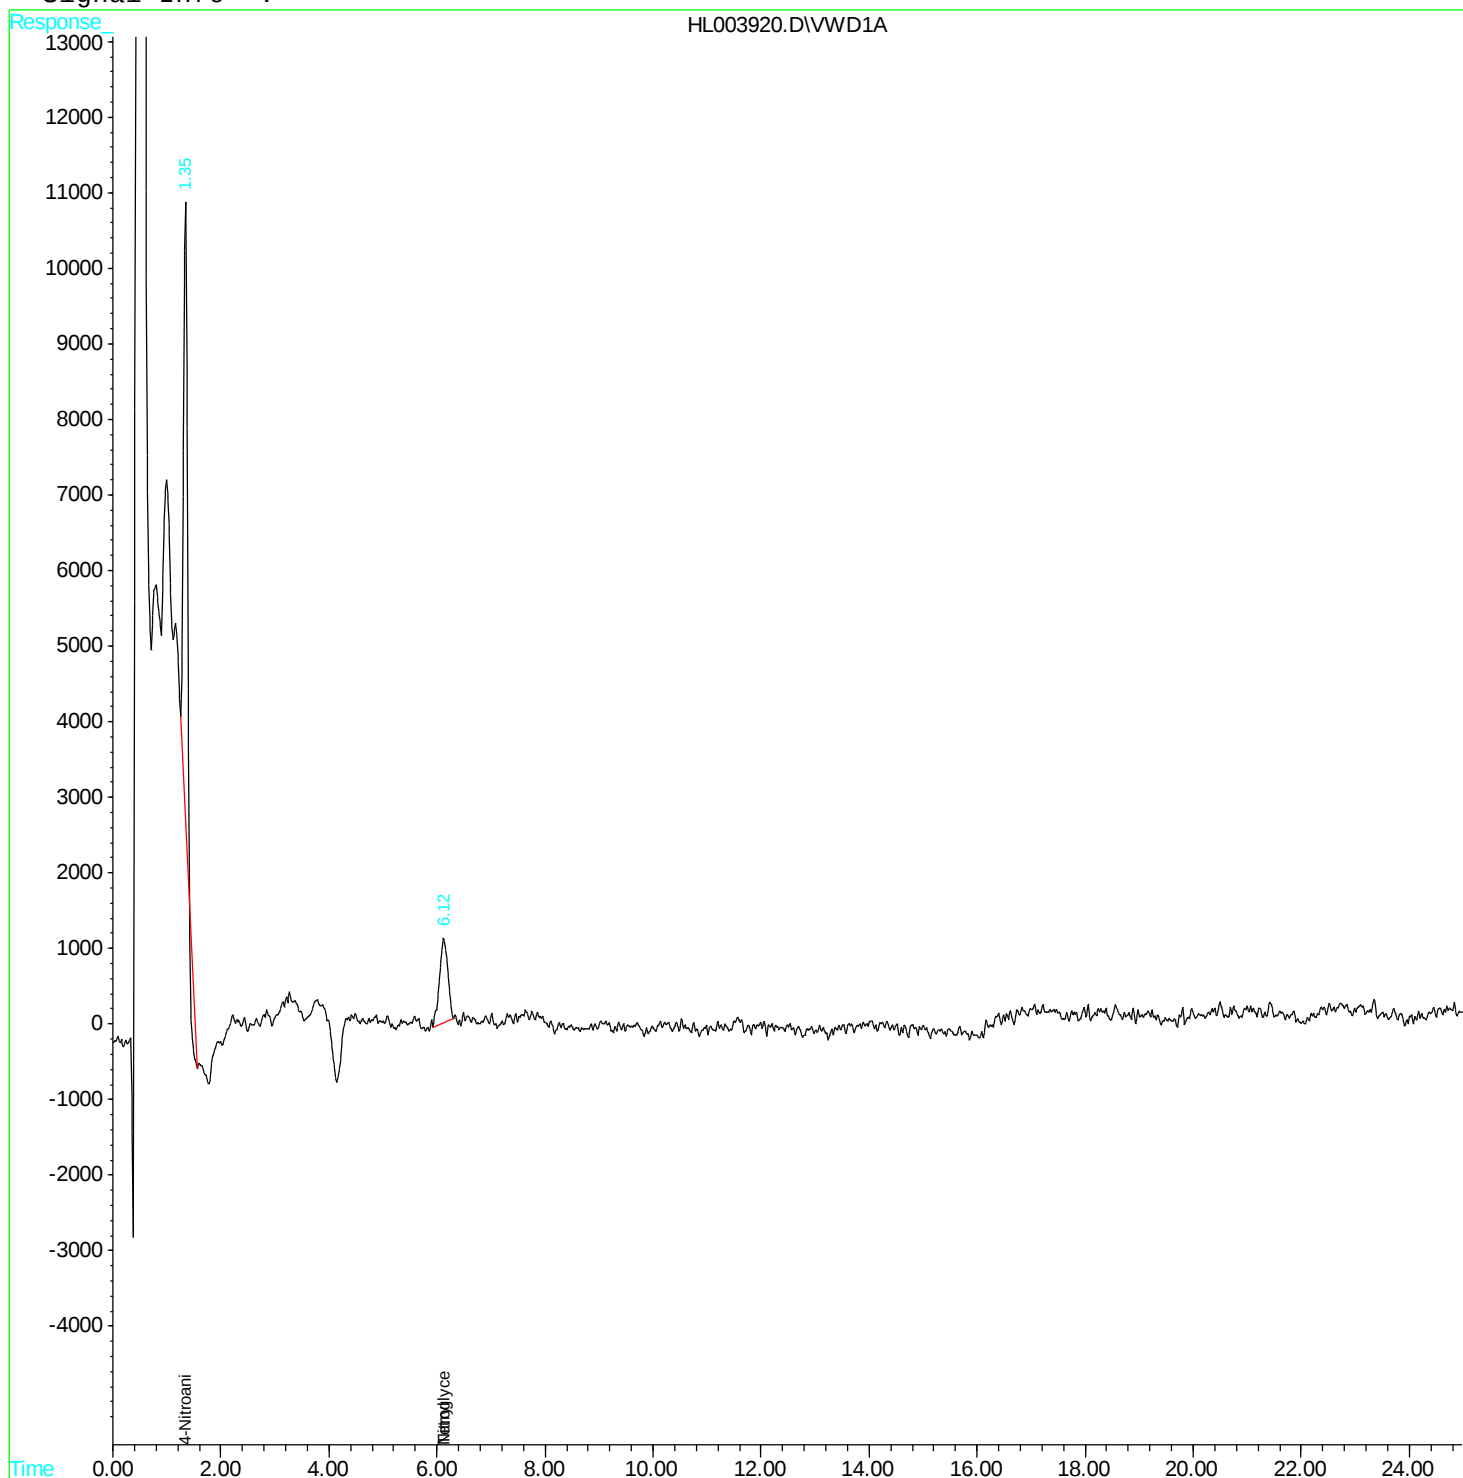


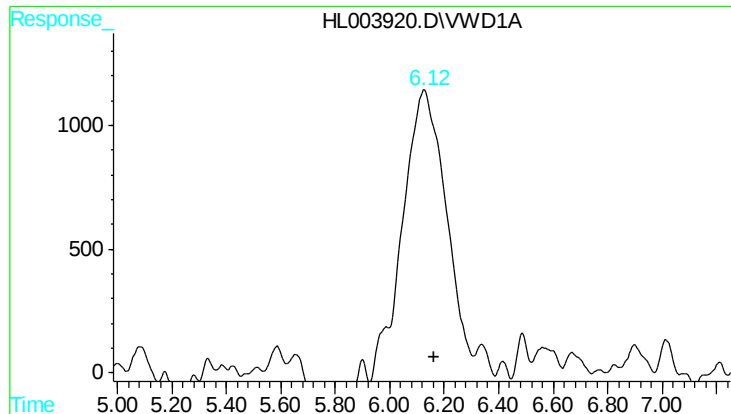

#5 Tetryl

R.T.: 6.126 min
Delta R.T.: -0.036 min
Response: 120321
Conc: 13.49 ug/L

Instrument :
HPLC_L
ClientSampleId :
BACKGROUND-ISM-2MS2

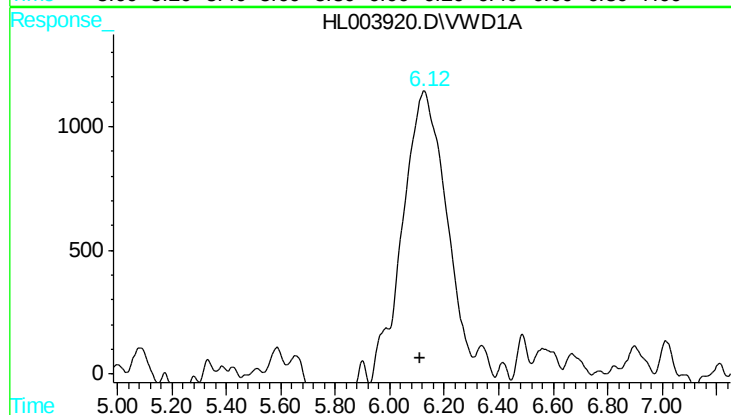

#17 Nitroglycerin

R.T.: 6.126 min
Delta R.T.: 0.013 min
Response: 120321
Conc: 2145.14 ug/L