

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003923.D Vial: 2
 Acq On : 01-Jan-2013, 22:47 Operator: HLM
 Sample : 8330-CCV Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Jan 2 11:28 2013 Quant Results File: HL123112.RES

Instrument :
 HPLC_L
 LabSampleId :
 8330-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Wed Jan 02 11:22:54 2013
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.35	3587534	922.831 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 307.61%#

Target Compounds

2) T	HMX	0.91	4560533	1061.077 ug/L
3) T	RDX	1.75	5617700	1035.799 ug/L
4) T	1,3,5-Trinitrobenzene	2.72	5779581	487.797 ug/L
5) T	Tetryl	6.17	8260931	926.351 ug/L
6) T	2,4,6-Trinitrotoluene	6.54	5524253	471.439 ug/L
7) T	2-Amino-4,6-dinitrotoluene	7.01	5540723	491.240 ug/L
8) T	4-Amino-2,6-dinitrotoluene	7.34	3664848	500.638 ug/L
9) T	2,4-Dinitrotoluene	8.16	7811115	501.275 ug/L
10) T	2,6-Dinitrotoluene	8.55	4243192	490.128 ug/L
11) T	1,3-Dinitrobenzene	3.61	8400032	496.138 ug/L
12) T	Nitrobenzene	4.84	5357534	498.897 ug/L
13) T	2-Nitrotoluene	11.77	6754052	1019.795 ug/L
14) T	3-Nitrotoluene	13.78	7298072	1026.169 ug/L
15) T	4-Nitrotoluene	12.52	5735826	1045.342 ug/L
16) T	3,5-Dinitroaniline	3.95	15930201	1000.064 ug/L
18) T	PETN	18.82	23796875	2593.564 ug/L

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003923.D

Vial: 2

Acq On : 01-Jan-2013, 22:47

Operator: HLM

Sample : 8330-CCV

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Jan 2 11:28 2013 Quant Results File: HL123112.RES

Instrument :

HPLC_L

LabSampleId :

8330-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)

Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)

Last Update : Wed Jan 02 11:22:54 2013


Response via : Multiple Level Calibration


DataAcq Meth : 8330AGIP.M

Volume Inj. :

Signal Phase :

Signal Info :

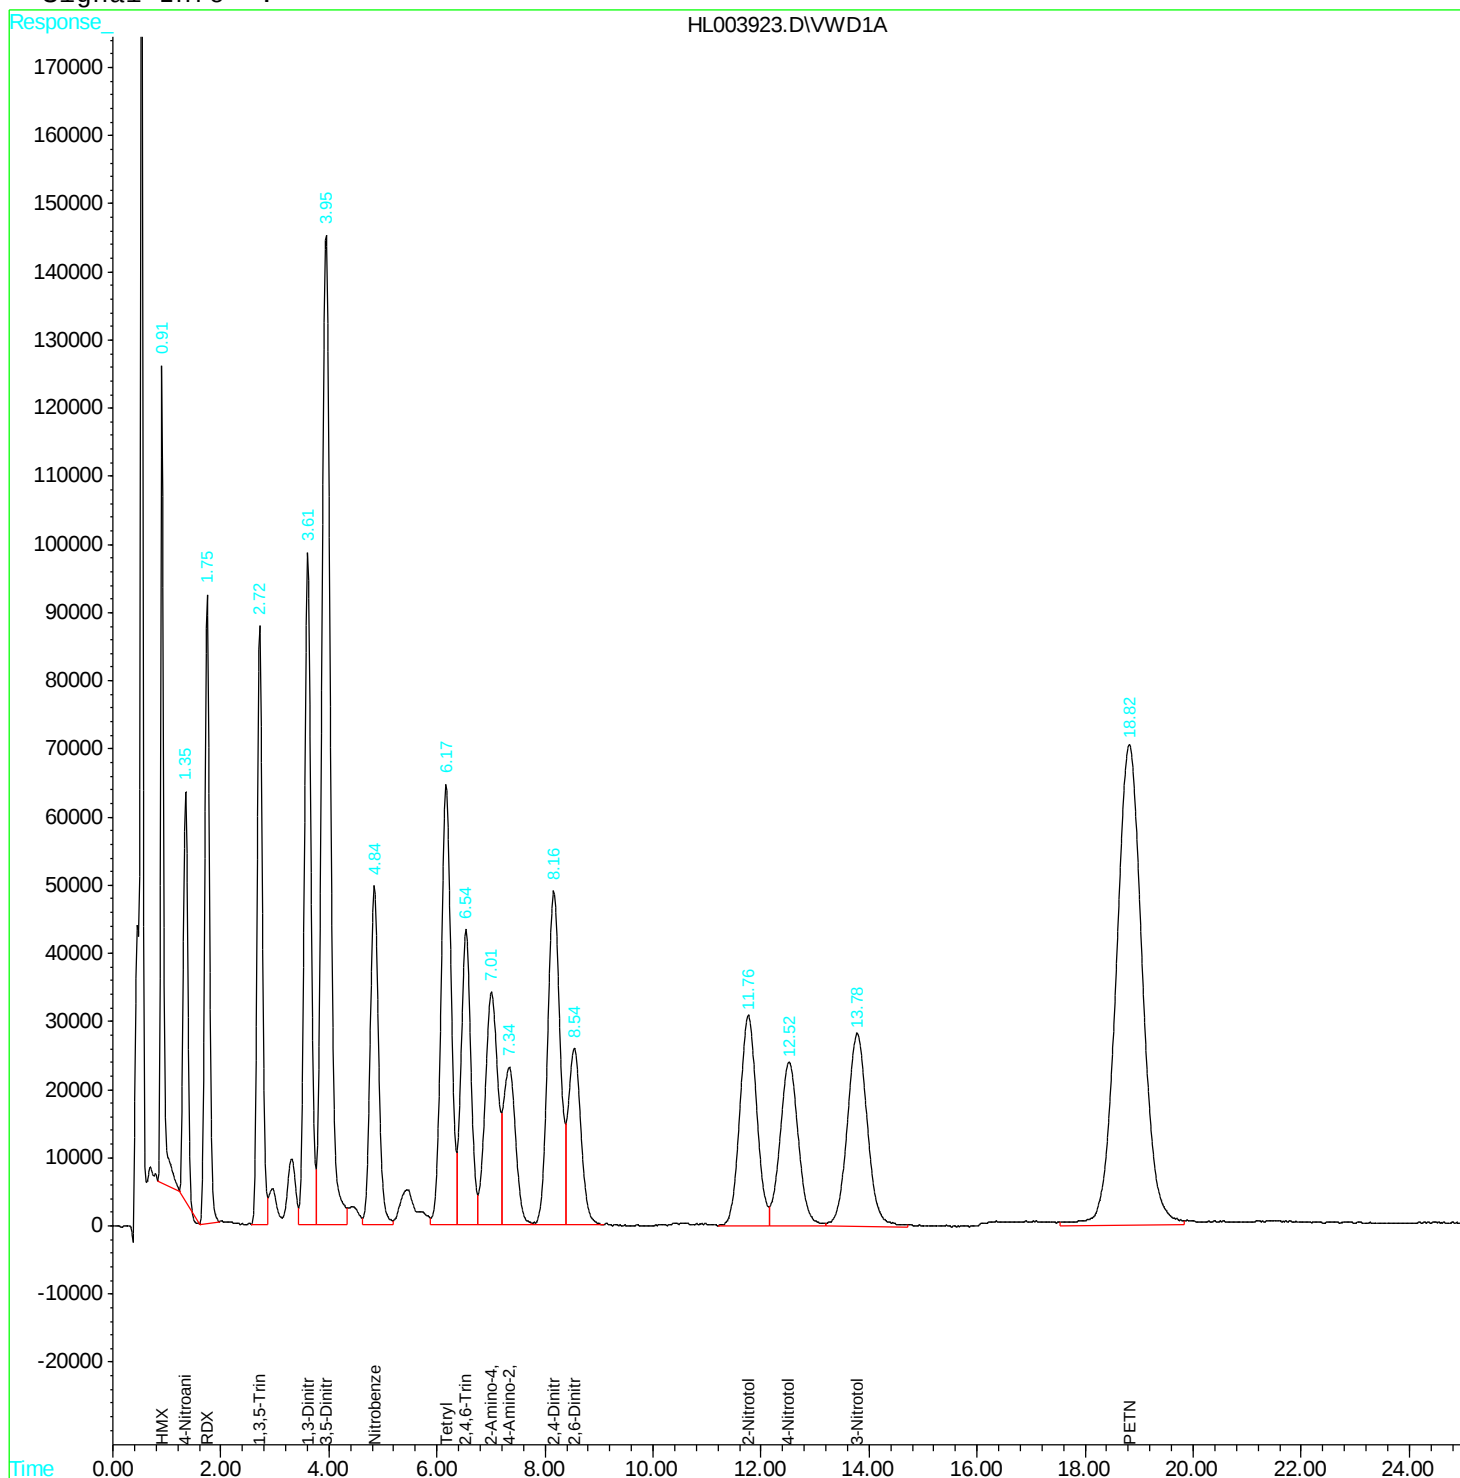


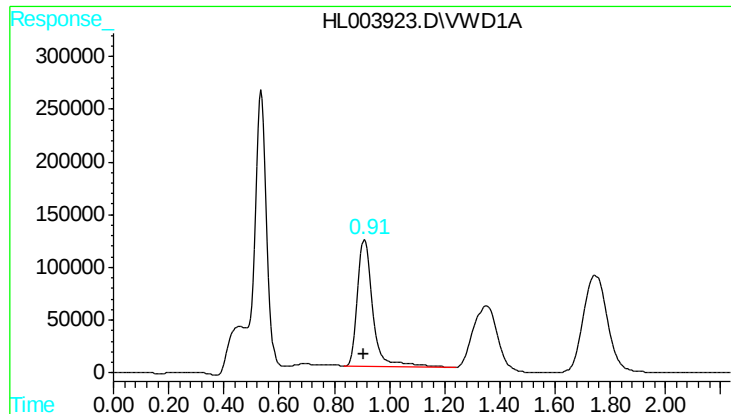

#2 HMX


R.T.: 0.910 min
Delta R.T.: 0.003 min
Response: 4560533
Conc: 1061.08 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

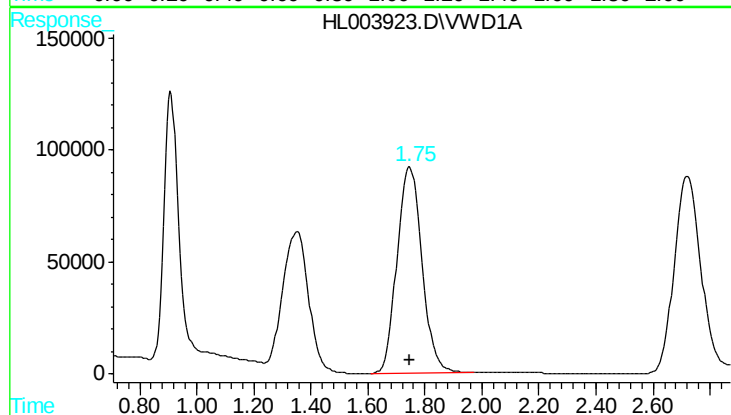


#3 RDX

R.T.: 1.747 min
Delta R.T.: 0.000 min
Response: 5617700
Conc: 1035.80 ug/L

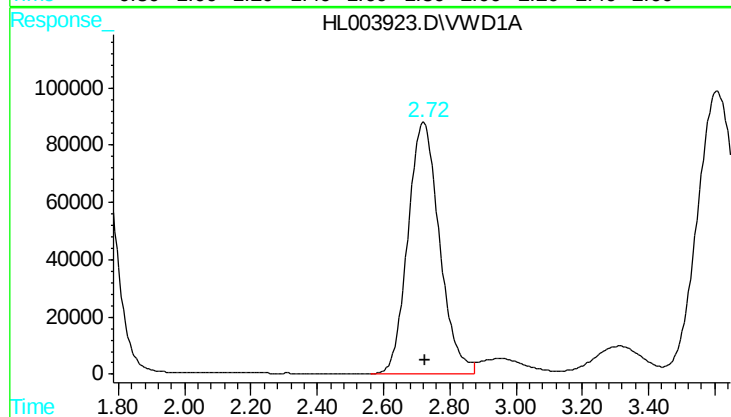


#4 1,3,5-Trinitrobenzene

R.T.: 2.721 min
Delta R.T.: -0.007 min
Response: 5779581
Conc: 487.80 ug/L

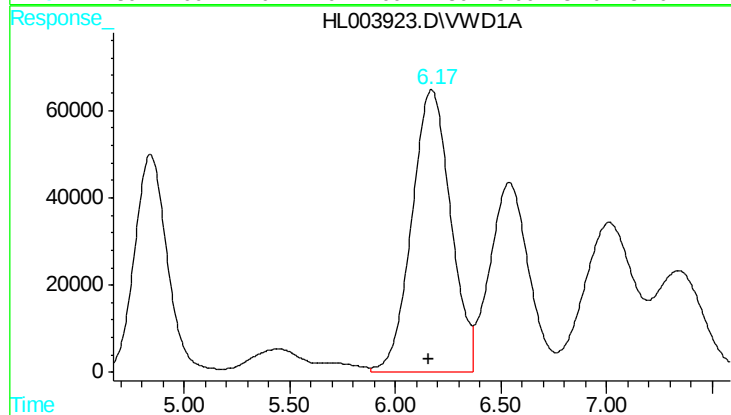

#5 Tetryl


R.T.: 6.171 min
Delta R.T.: 0.010 min
Response: 8260931
Conc: 926.35 ug/L

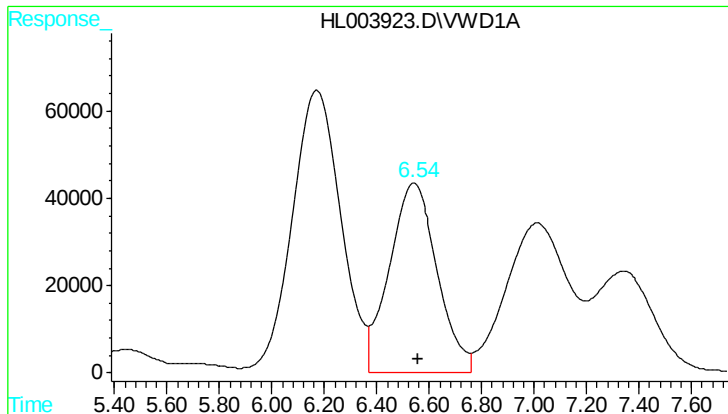

#6 2,4,6-Trinitrotoluene


R.T.: 6.540 min
Delta R.T.: -0.016 min
Response: 5524253
Conc: 471.44 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

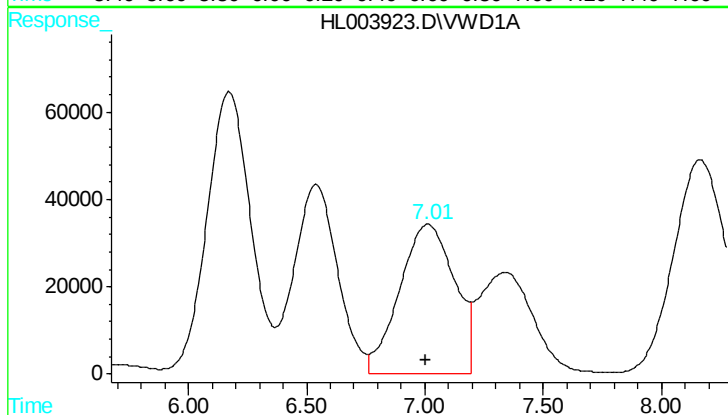


#7 2-Amino-4,6-dinitrotoluene

R.T.: 7.012 min
Delta R.T.: 0.011 min
Response: 5540723
Conc: 491.24 ug/L

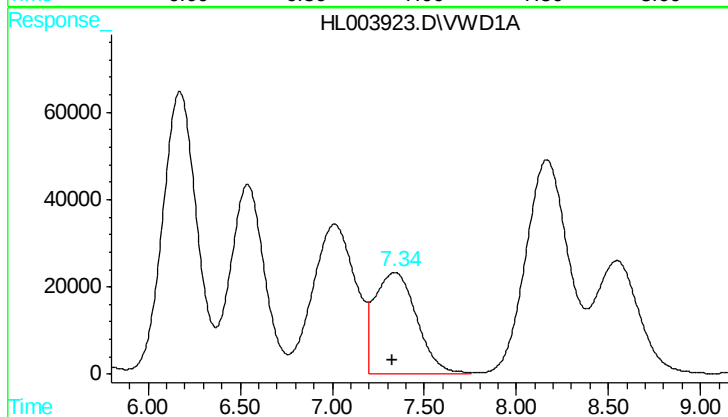


#8 4-Amino-2,6-dinitrotoluene

R.T.: 7.339 min
Delta R.T.: 0.012 min
Response: 3664848
Conc: 500.64 ug/L

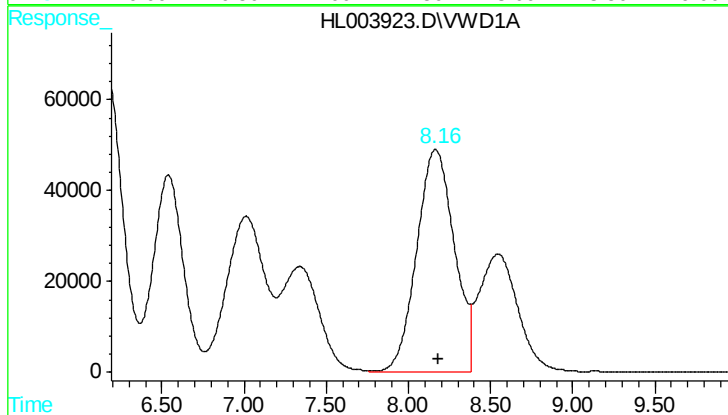

#9 2,4-Dinitrotoluene


R.T.: 8.165 min
Delta R.T.: -0.018 min
Response: 7811115
Conc: 501.27 ug/L

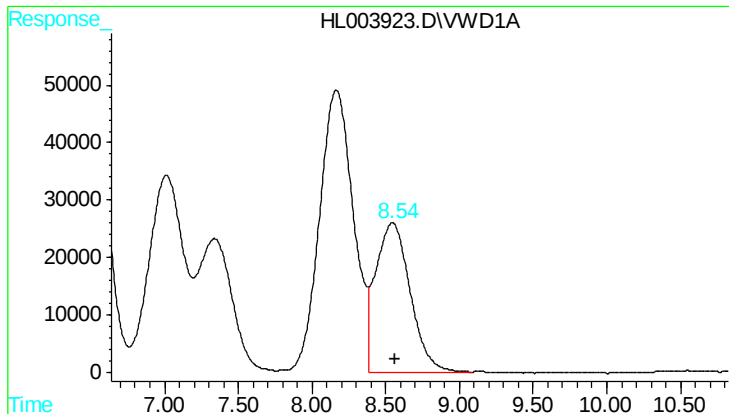

#10 2,6-Dinitrotoluene


R.T.: 8.546 min
Delta R.T.: -0.015 min
Response: 4243192
Conc: 490.13 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

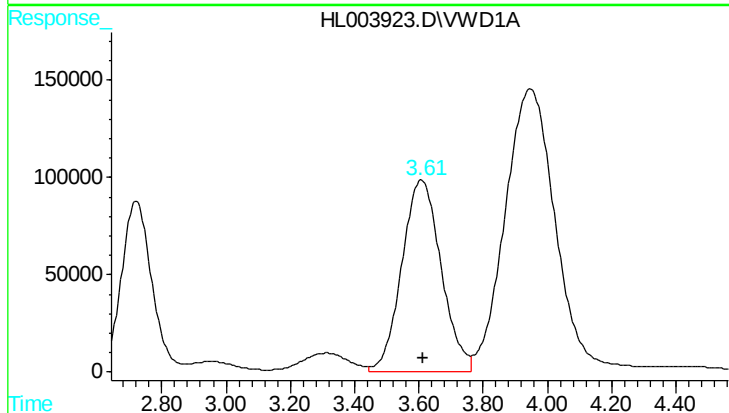


#11 1,3-Dinitrobenzene

R.T.: 3.608 min
Delta R.T.: -0.006 min
Response: 8400032
Conc: 496.14 ug/L

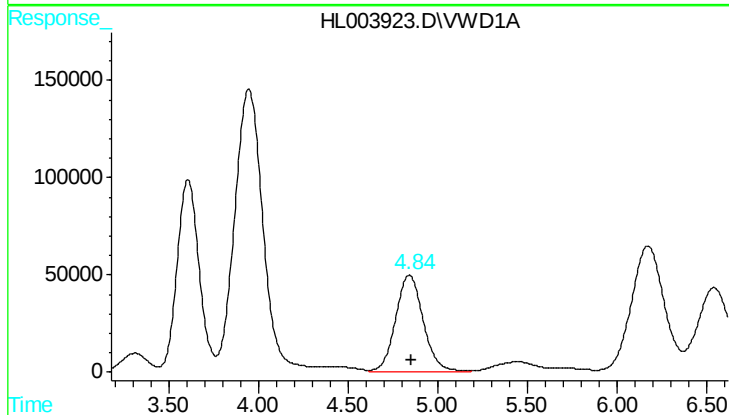


#12 Nitrobenzene

R.T.: 4.841 min
Delta R.T.: -0.014 min
Response: 5357534
Conc: 498.90 ug/L

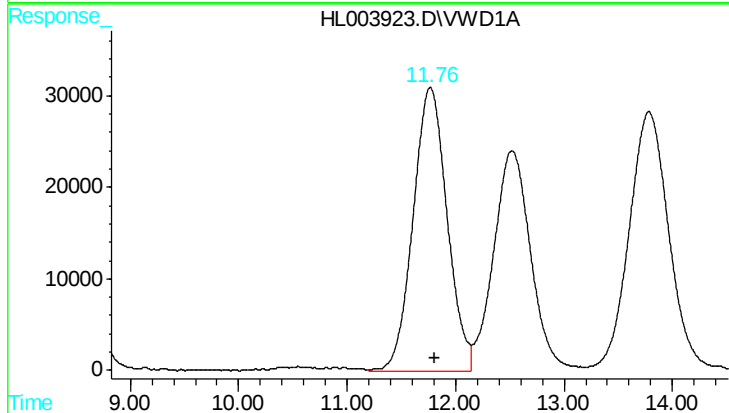

#13 2-Nitrotoluene


R.T.: 11.766 min
Delta R.T.: -0.040 min
Response: 6754052
Conc: 1019.79 ug/L

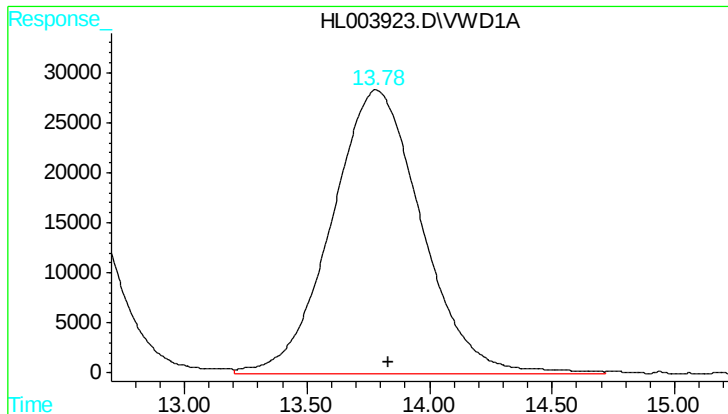

#14 3-Nitrotoluene


R.T.: 13.782 min
Delta R.T.: -0.049 min
Response: 7298072
Conc: 1026.17 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

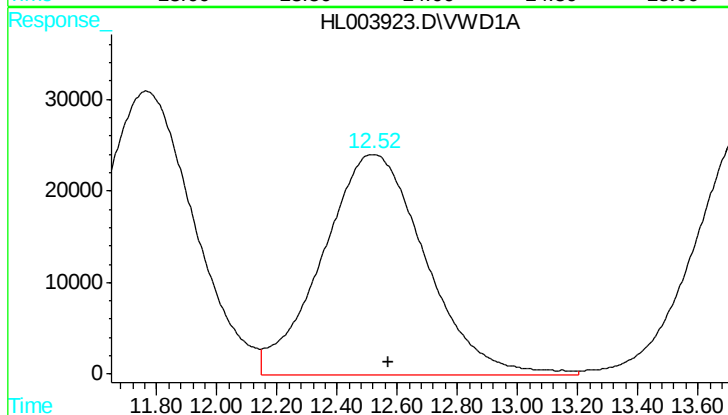


#15 4-Nitrotoluene

R.T.: 12.519 min
Delta R.T.: -0.051 min
Response: 5735826
Conc: 1045.34 ug/L

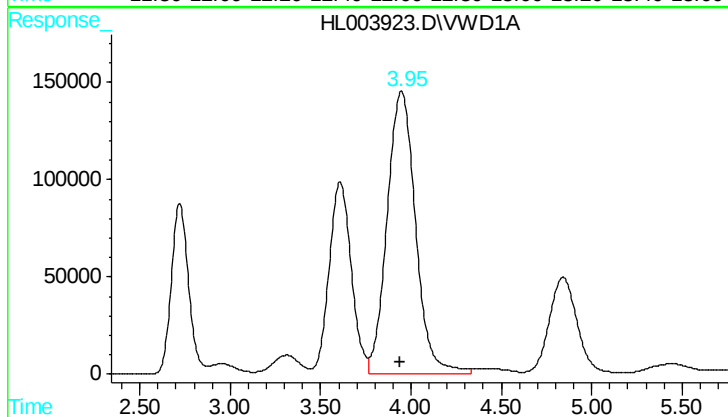

#16 3,5-Dinitroaniline

R.T.: 3.948 min
Delta R.T.: 0.006 min
Response: 15930201
Conc: 1000.06 ug/L

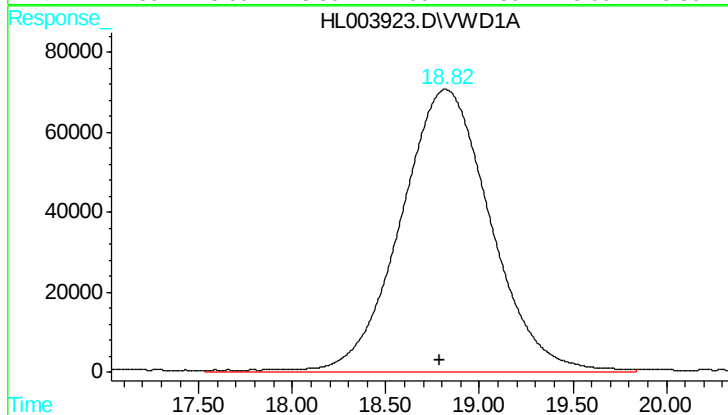

#18 PETN

R.T.: 18.819 min
Delta R.T.: 0.030 min
Response: 23796875
Conc: 2593.56 ug/L