

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003925.D Vial: 61
Acq On : 01-Jan-2013, 23:41 Operator: HLM
Sample : D5190-02MSD2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Jan 2 11:29 2013 Quant Results File: HL123112.RES

Instrument :
HPLC_L
ClientSampleId :
BACKGROUND-ISM-2MSD2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Wed Jan 02 11:22:54 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.35	345826	88.958 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 29.65%#

Target Compounds


5) T	Tetryl	6.13	135711	15.218 ug/L
17) T	Nitroglycerin	6.13	135711	2419.507 ug/L


Data File : H:\VOL1\HPLC\HPLC L\121231\HL003925.D Vial: 61
Acq On : 01-Jan-2013, 23:41 Operator: HLM
Sample : D5190-02MSD2 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Jan 2 11:29 2013 Quant Results File: HL123112.RES

Instrument :
HPLC_L
ClientSampleId :
BACKGROUND-ISM-2MSD2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Wed Jan 02 11:22:54 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

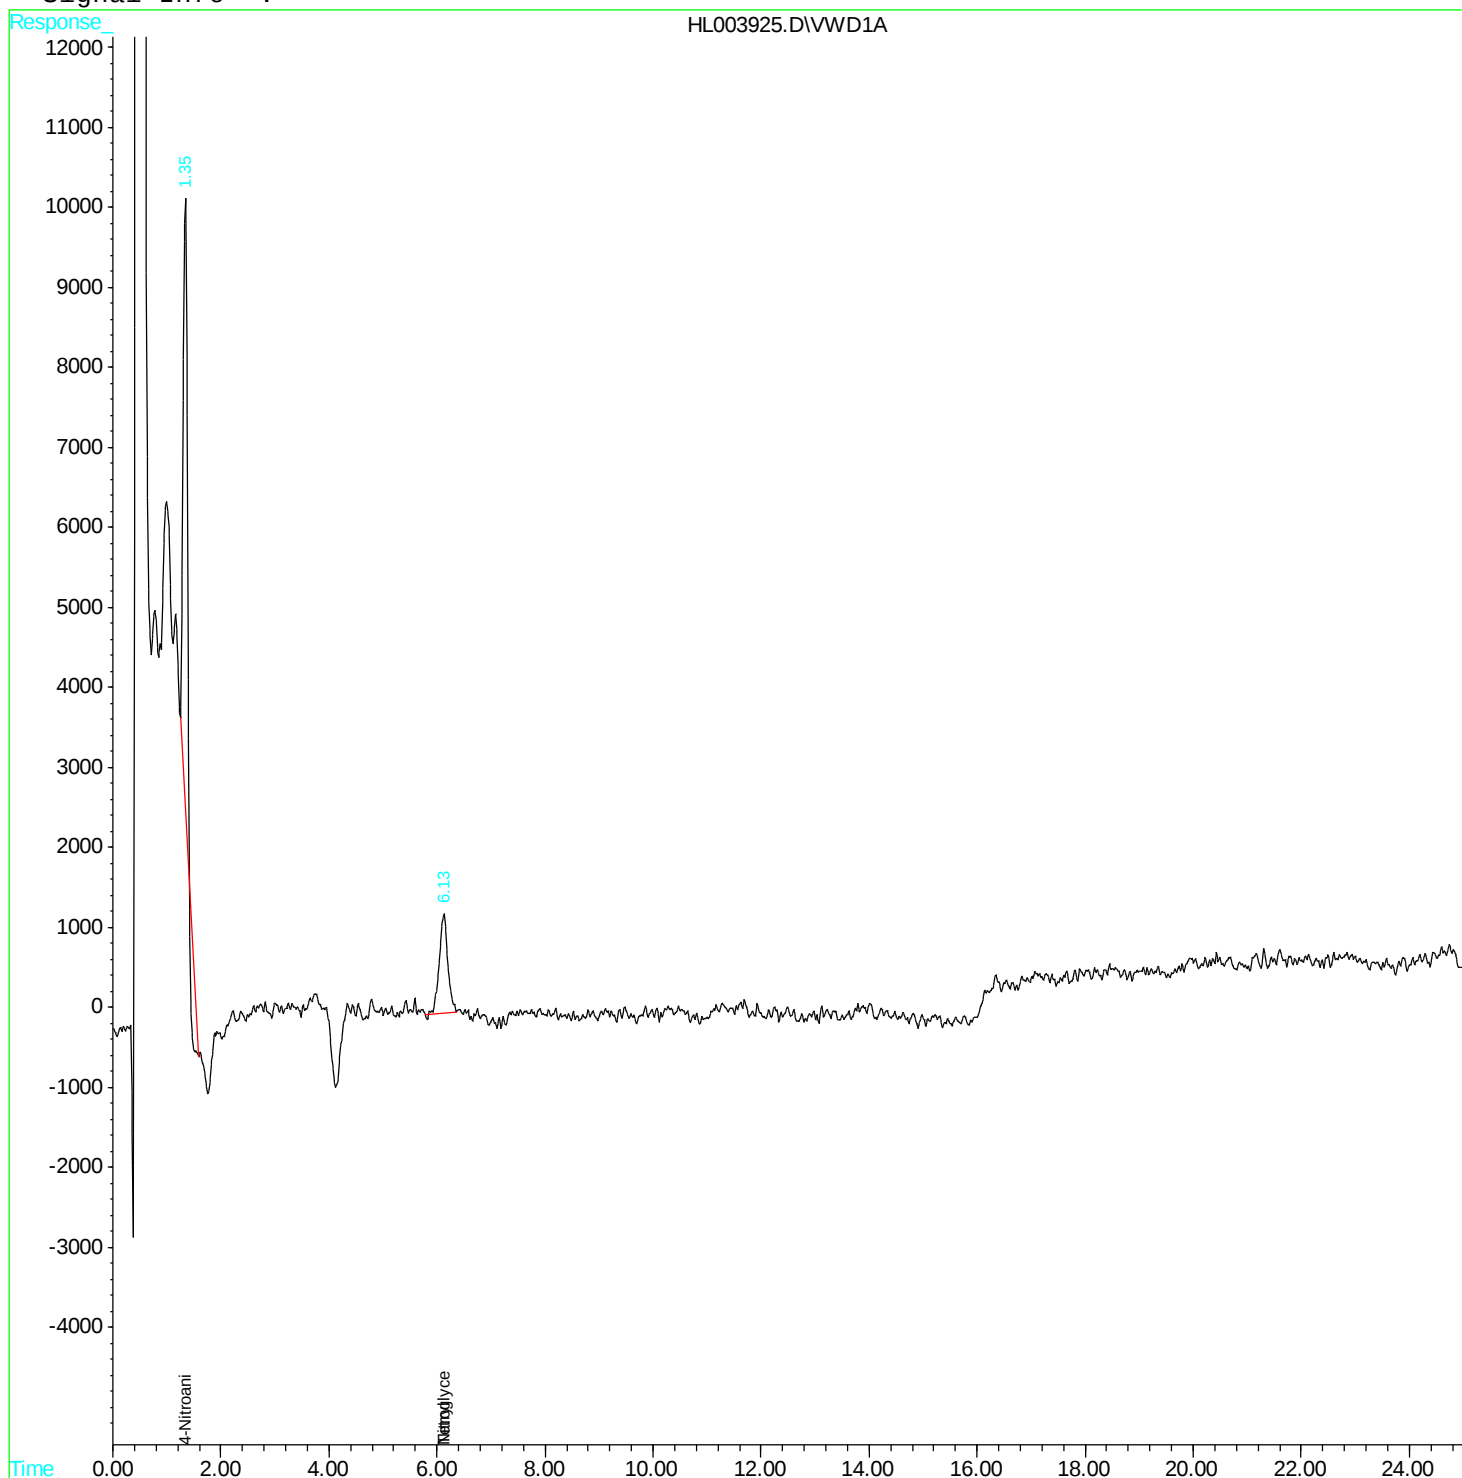


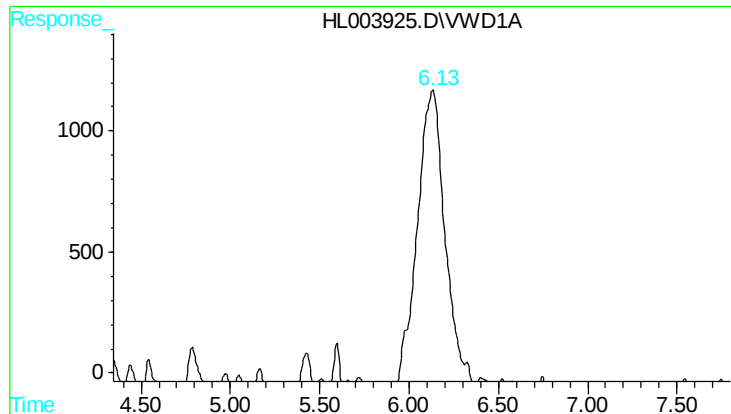

#5 Tetryl

R.T.: 6.135 min
Delta R.T.: -0.027 min
Response: 135711
Conc: 15.22 ug/L

Instrument :
HPLC_L
ClientSampleId :
BACKGROUND-ISM-2MSD2

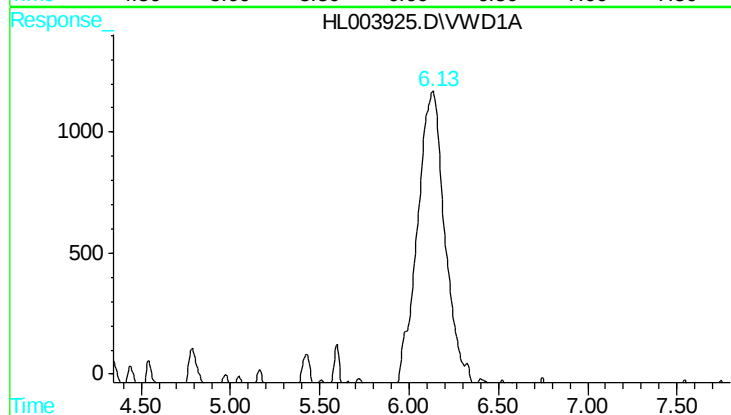

#17 Nitroglycerin

R.T.: 6.135 min
Delta R.T.: 0.022 min
Response: 135711
Conc: 2419.51 ug/L