

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003934.D Vial: 70
Acq On : 02-Jan-2013, 03:44 Operator: HLM
Sample : D5190-12 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Jan 2 11:29 2013 Quant Results File: HL123112.RES

Instrument :
HPLC_L
ClientSampleId :
SAOI4-ISM-2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Wed Jan 02 11:22:54 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.34	516116	132.762 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 44.25%

Target Compounds


6) T	2,4,6-Trinitrotoluene	6.56	74783	6.382 ug/L
------	-----------------------	------	-------	------------


Data File : H:\VOL1\HPLC\HPLC L\121231\HL003934.D Vial: 70
Acq On : 02-Jan-2013, 03:44 Operator: HLM
Sample : D5190-12 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : events.e
Quant Time: Jan 2 11:29 2013 Quant Results File: HL123112.RES

Instrument :
HPLC_L
ClientSampleId :
SAOI4-ISM-2

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Wed Jan 02 11:22:54 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

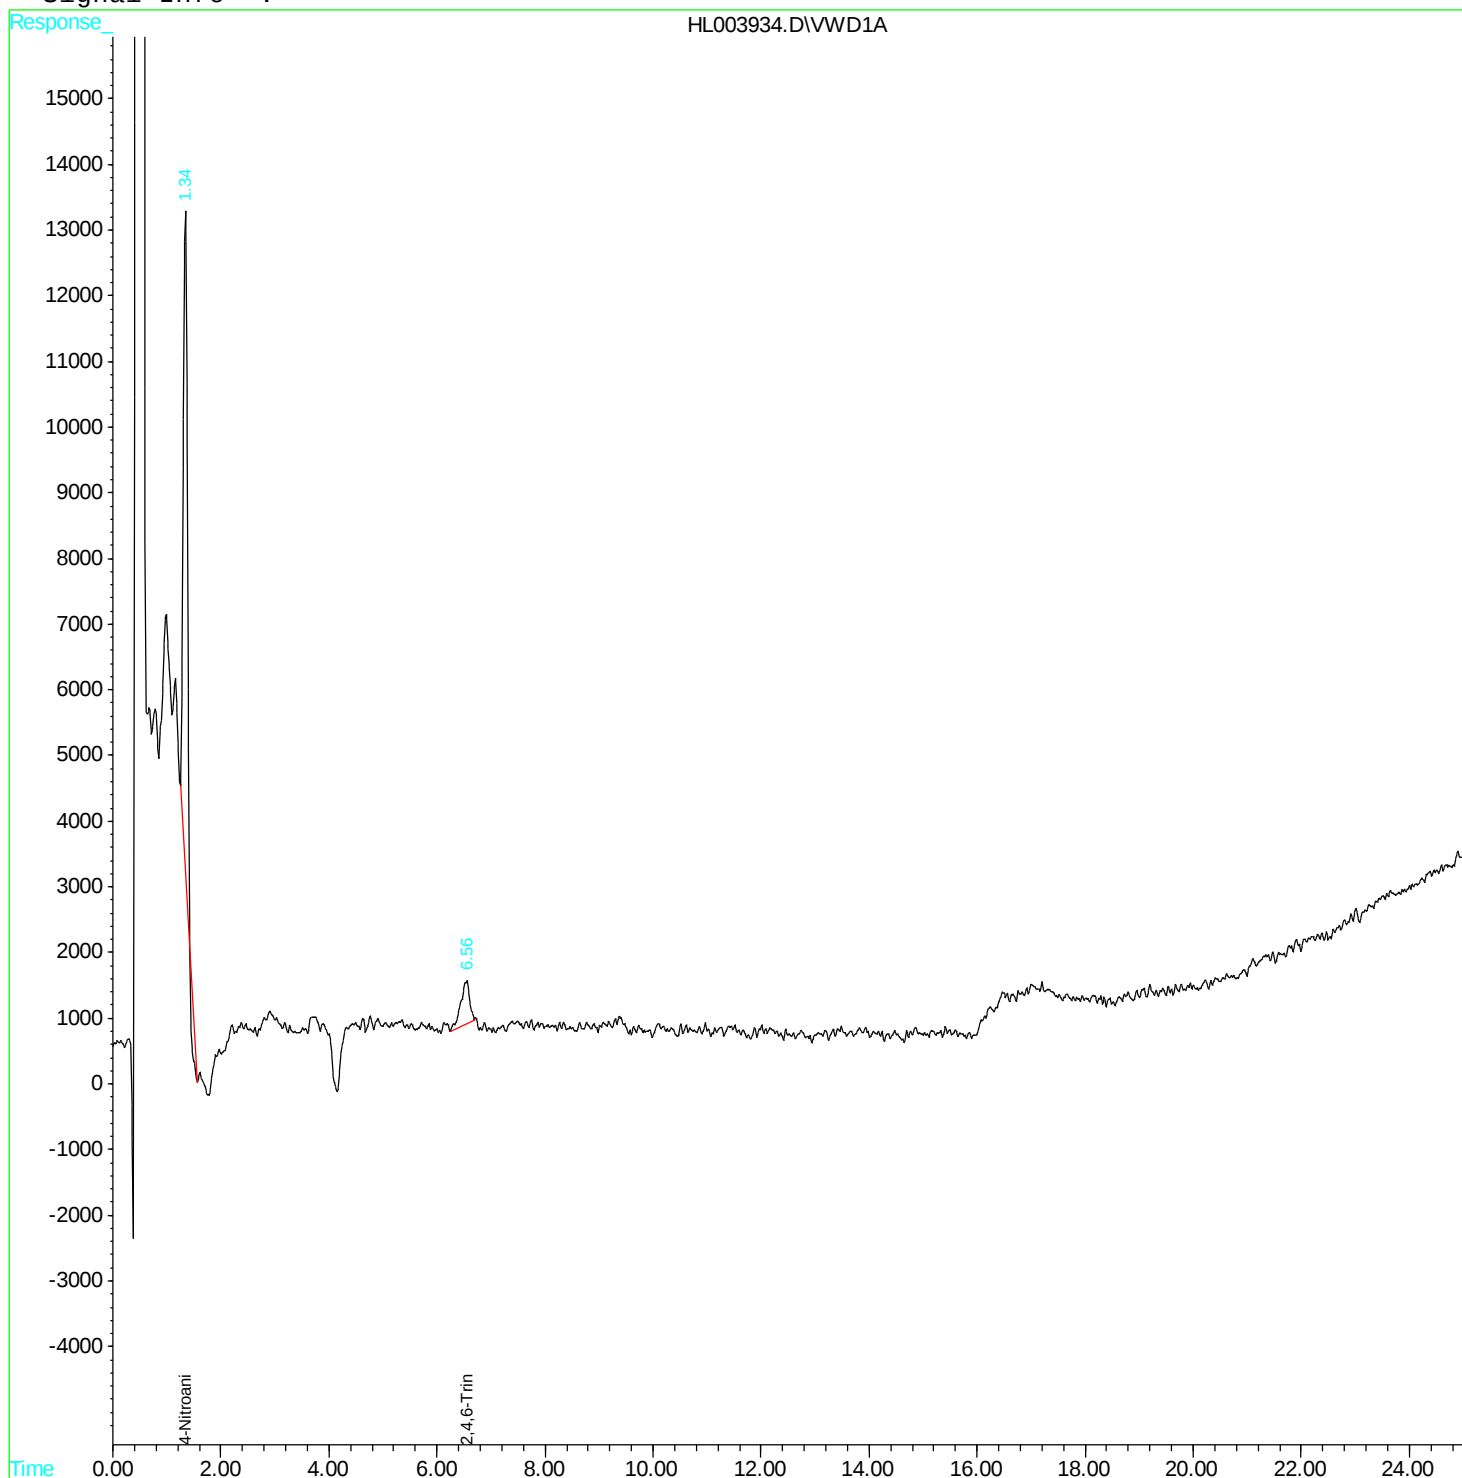

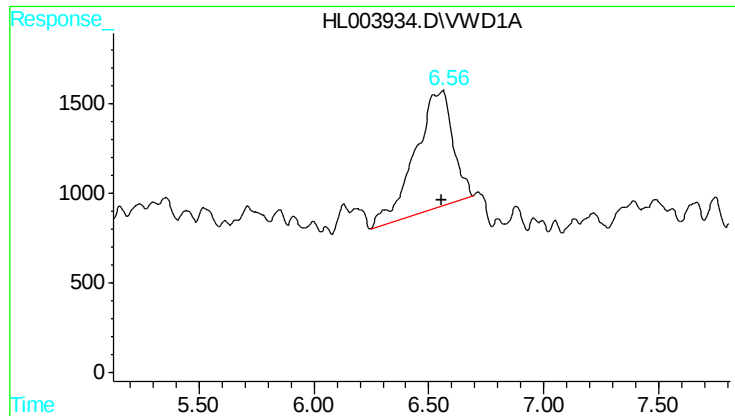

#6 2,4,6-Trinitrotoluene

R.T.: 6.562 min
Delta R.T.: 0.007 min
Response: 74783
Conc: 6.38 ug/L

Instrument :
HPLC_L
ClientSampleId :
SAOI4-ISM-2