

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003936.D Vial: 2
 Acq On : 02-Jan-2013, 04:37 Operator: HLM
 Sample : 8330-CCV Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Jan 2 11:29 2013 Quant Results File: HL123112.RES

Instrument :
 HPLC_L
 LabSampleId :
 8330-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Wed Jan 02 11:22:54 2013
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.35	3577920	920.358 ug/L
Spiked Amount 300.000		Range 37 - 149	Recovery	= 306.79%#

Target Compounds

2) T	HMX	0.91	4535648	1054.774 ug/L
3) T	RDX	1.75	5763305	1062.646 ug/L
4) T	1,3,5-Trinitrobenzene	2.72	5866000	495.091 ug/L
5) T	Tetryl	6.17	8353271	936.705 ug/L
6) T	2,4,6-Trinitrotoluene	6.54	5626798	480.190 ug/L
7) T	2-Amino-4,6-dinitrotoluene	7.01	5607834	497.190 ug/L
8) T	4-Amino-2,6-dinitrotoluene	7.34	3744358	511.499 ug/L
9) T	2,4-Dinitrotoluene	8.16	7910224	507.635 ug/L
10) T	2,6-Dinitrotoluene	8.54	4370161	504.795 ug/L
11) T	1,3-Dinitrobenzene	3.61	8488966	501.391 ug/L
12) T	Nitrobenzene	4.84	5424073	505.093 ug/L
13) T	2-Nitrotoluene	11.76	6733910	1016.753 ug/L
14) T	3-Nitrotoluene	13.77	7525102	1058.092 ug/L
15) T	4-Nitrotoluene	12.51	5731562	1044.565 ug/L
16) T	3,5-Dinitroaniline	3.95	16147386	1013.698 ug/L
18) T	PETN	18.83	22863261	2491.811 ug/L

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003936.D

Vial: 2

Acq On : 02-Jan-2013, 04:37

Operator: HLM

Sample : 8330-CCV

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Jan 2 11:29 2013 Quant Results File: HL123112.RES

Instrument :

HPLC_L

LabSampleId :

8330-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)

Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)

Last Update : Wed Jan 02 11:22:54 2013


Response via : Multiple Level Calibration


DataAcq Meth : 8330AGIP.M

Volume Inj. :

Signal Phase :

Signal Info :

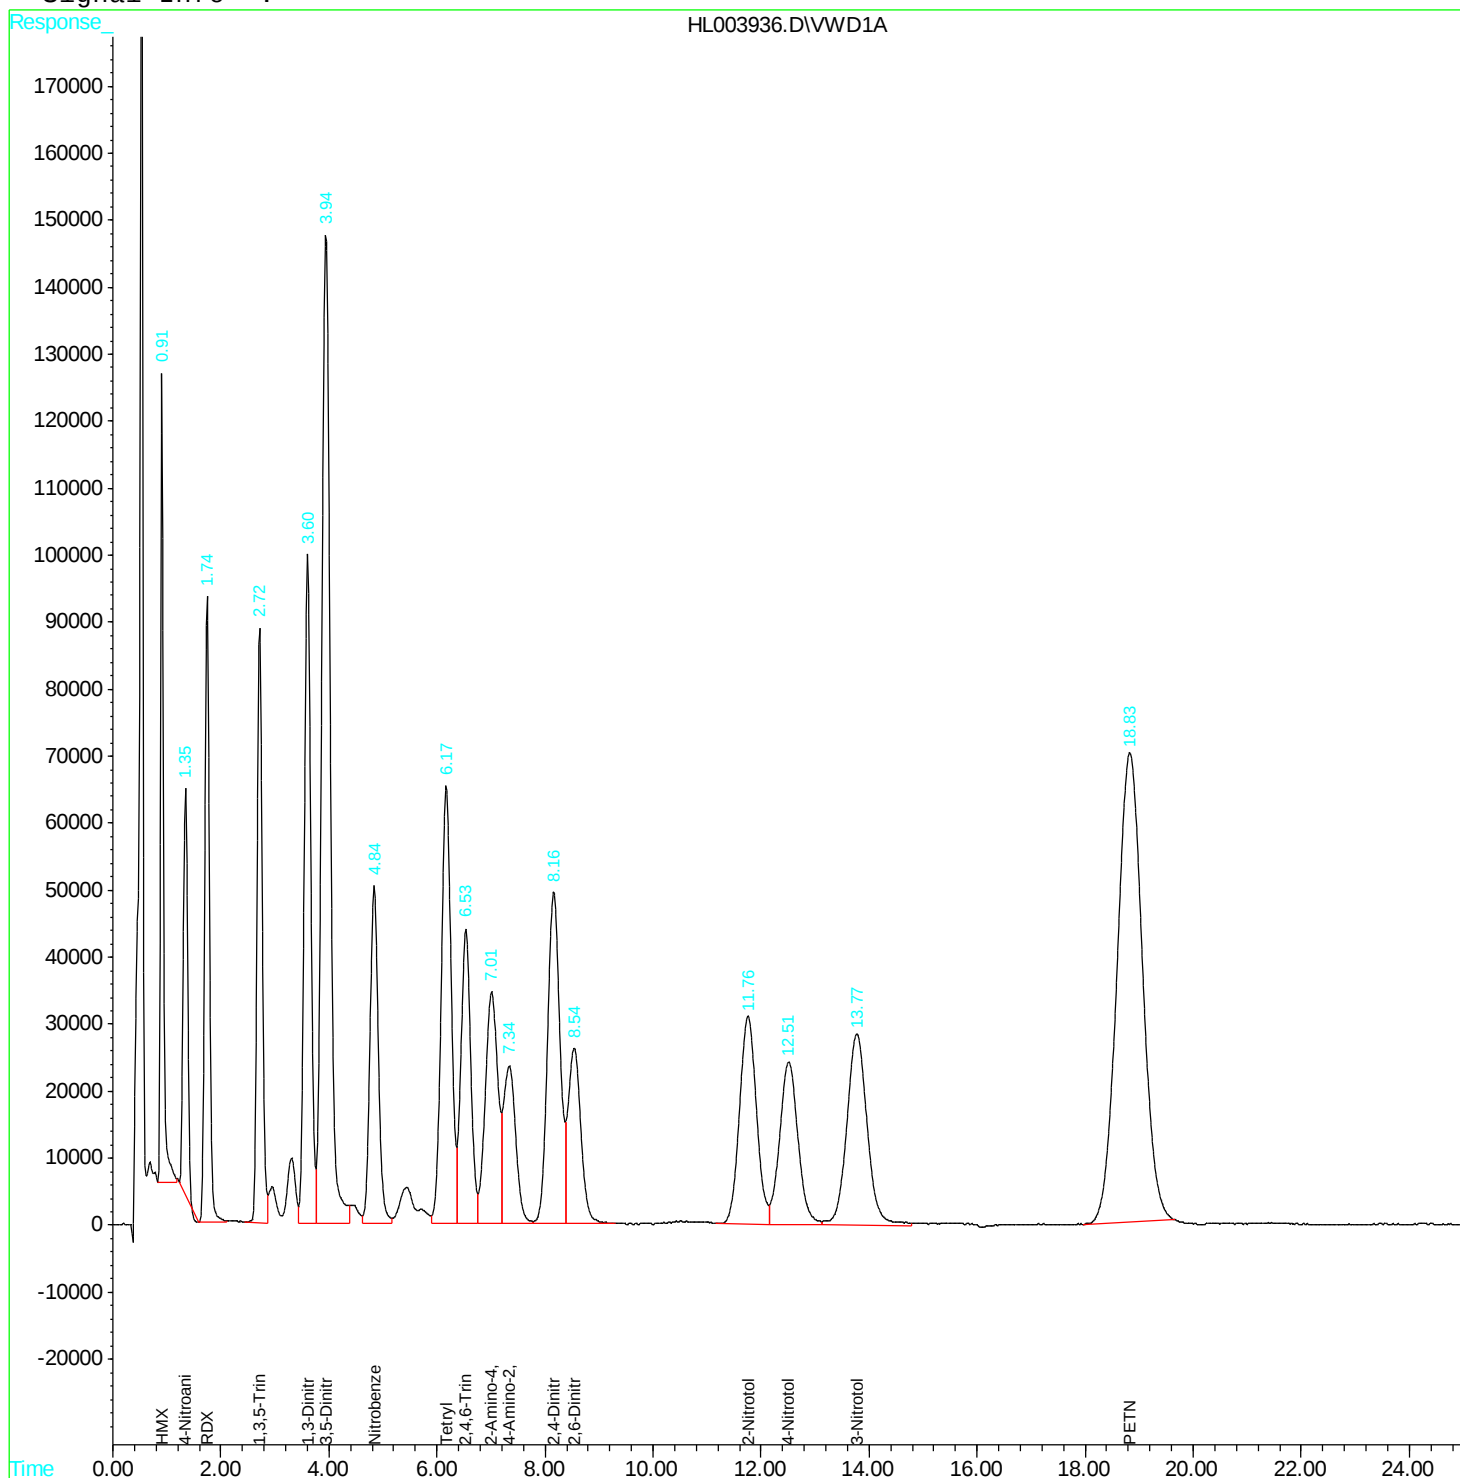


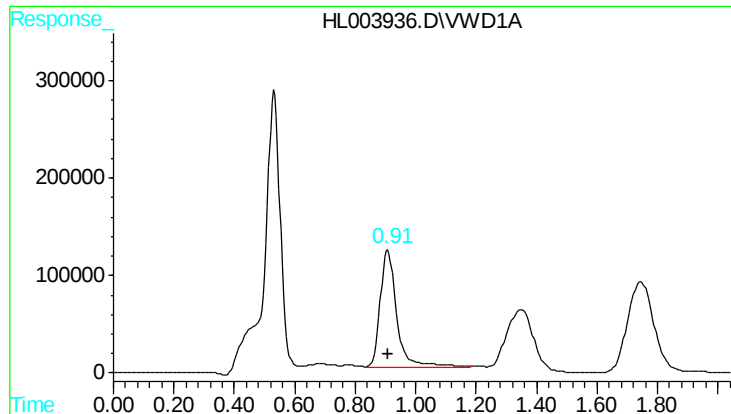

#2 HMX


R.T.: 0.908 min
Delta R.T.: 0.000 min
Response: 4535648
Conc: 1054.77 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

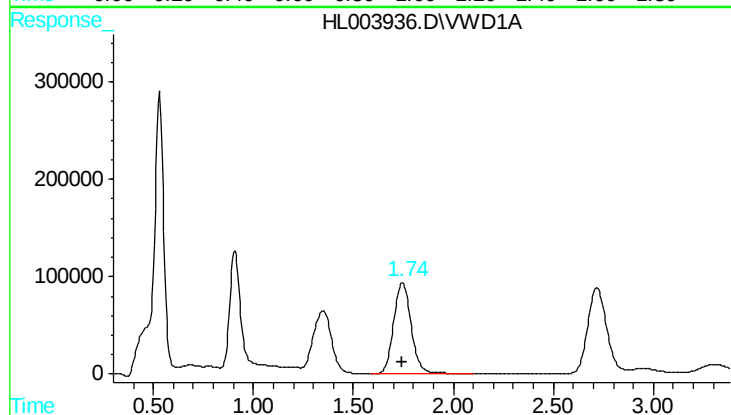


#3 RDX

R.T.: 1.746 min
Delta R.T.: 0.000 min
Response: 5763305
Conc: 1062.65 ug/L

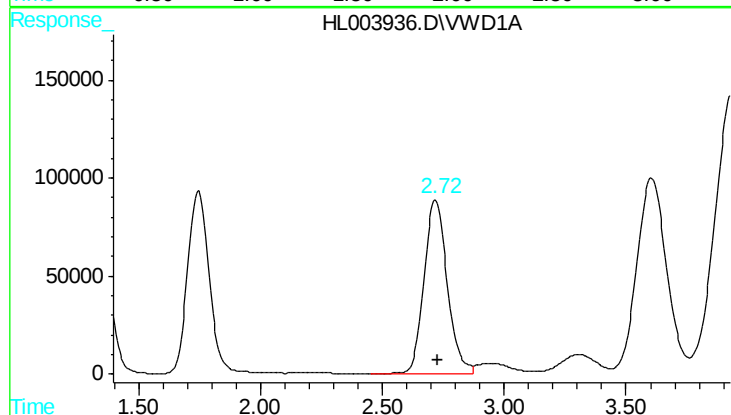


#4 1,3,5-Trinitrobenzene

R.T.: 2.718 min
Delta R.T.: -0.009 min
Response: 5866000
Conc: 495.09 ug/L

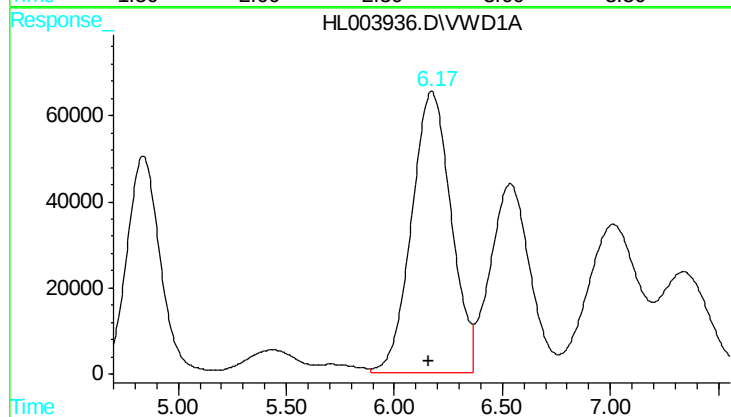

#5 Tetryl


R.T.: 6.174 min
Delta R.T.: 0.012 min
Response: 8353271
Conc: 936.71 ug/L

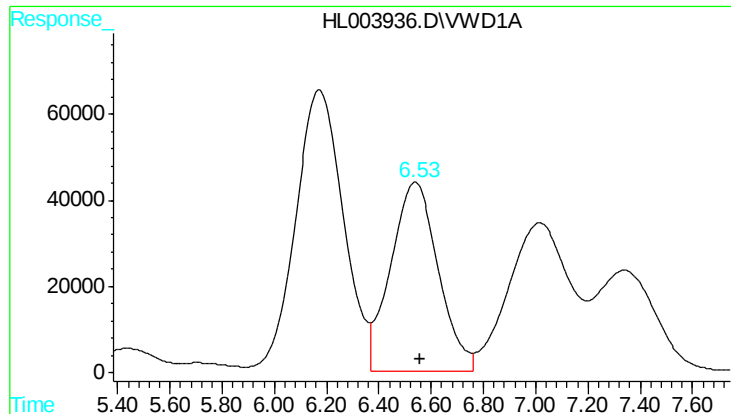

#6 2,4,6-Trinitrotoluene


R.T.: 6.537 min
Delta R.T.: -0.018 min
Response: 5626798
Conc: 480.19 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

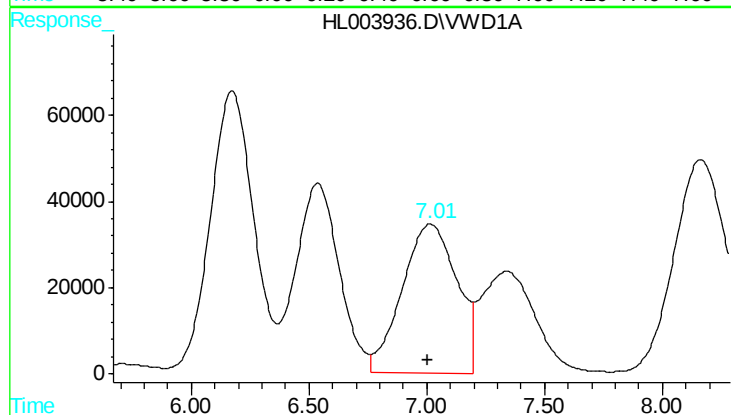


#7 2-Amino-4,6-dinitrotoluene

R.T.: 7.015 min
Delta R.T.: 0.014 min
Response: 5607834
Conc: 497.19 ug/L

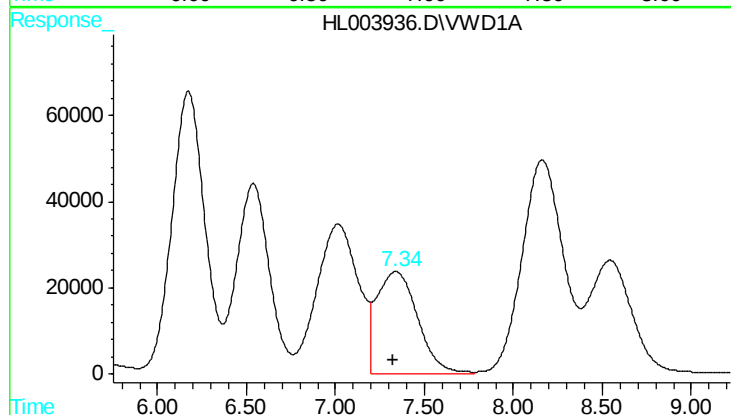


#8 4-Amino-2,6-dinitrotoluene

R.T.: 7.339 min
Delta R.T.: 0.012 min
Response: 3744358
Conc: 511.50 ug/L

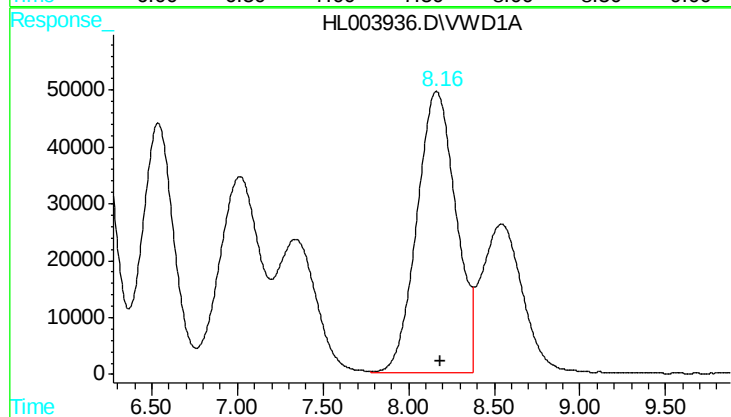

#9 2,4-Dinitrotoluene


R.T.: 8.163 min
Delta R.T.: -0.020 min
Response: 7910224
Conc: 507.64 ug/L

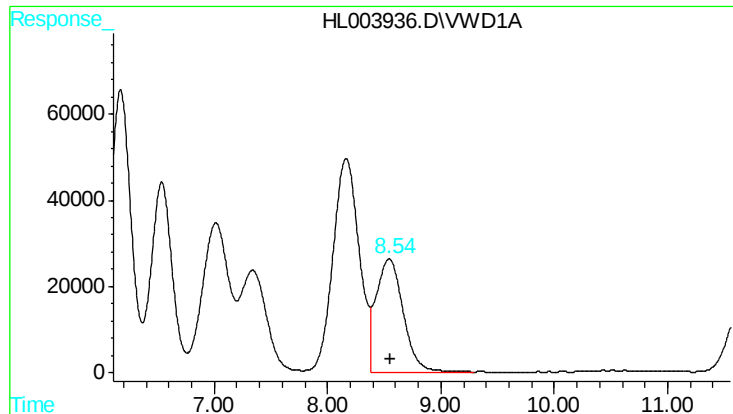

#10 2,6-Dinitrotoluene


R.T.: 8.543 min
Delta R.T.: -0.018 min
Response: 4370161
Conc: 504.79 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

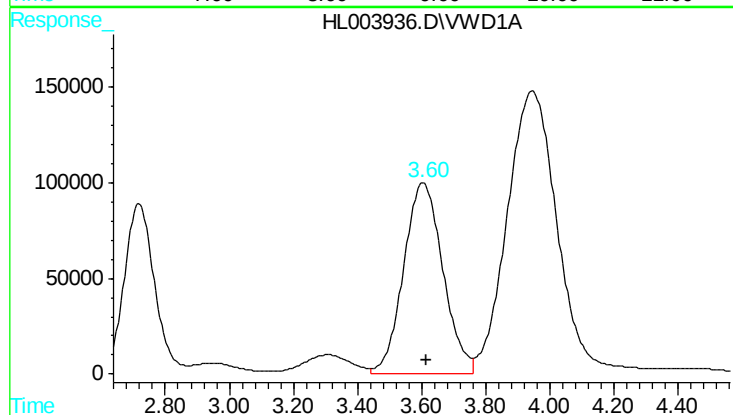


#11 1,3-Dinitrobenzene

R.T.: 3.605 min
Delta R.T.: -0.009 min
Response: 8488966
Conc: 501.39 ug/L

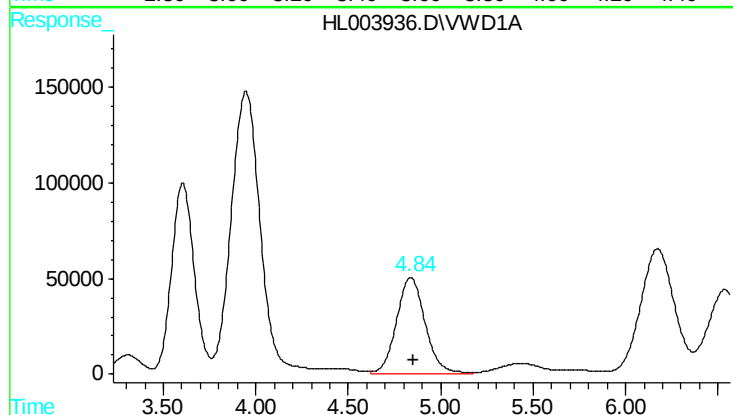


#12 Nitrobenzene

R.T.: 4.838 min
Delta R.T.: -0.017 min
Response: 5424073
Conc: 505.09 ug/L

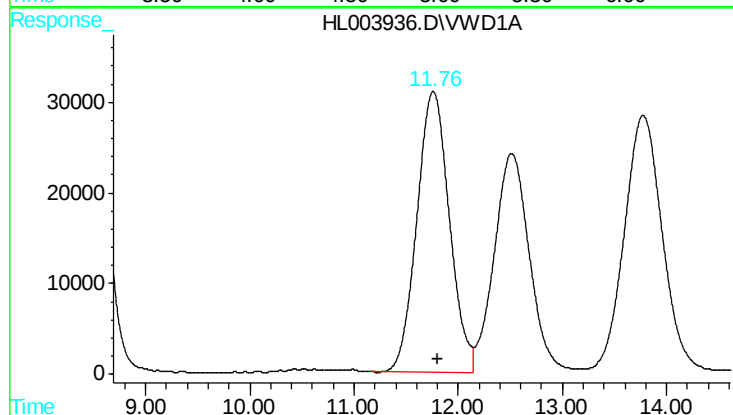

#13 2-Nitrotoluene


R.T.: 11.760 min
Delta R.T.: -0.046 min
Response: 6733910
Conc: 1016.75 ug/L

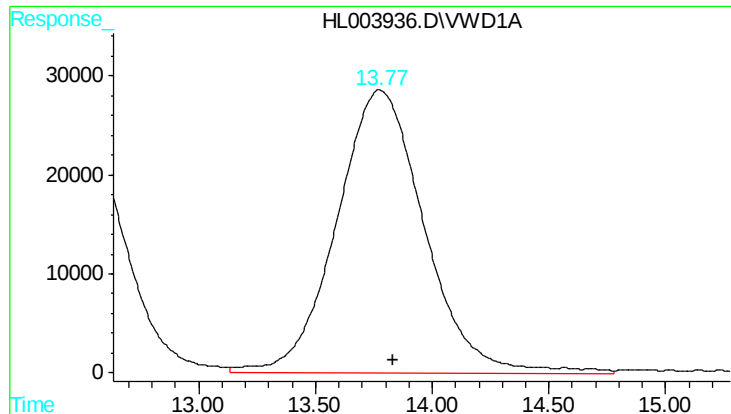

#14 3-Nitrotoluene


R.T.: 13.775 min
Delta R.T.: -0.057 min
Response: 7525102
Conc: 1058.09 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

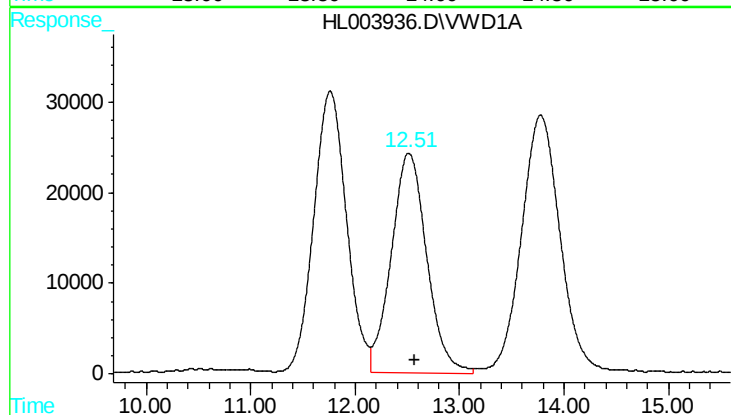


#15 4-Nitrotoluene

R.T.: 12.512 min
Delta R.T.: -0.058 min
Response: 5731562
Conc: 1044.56 ug/L

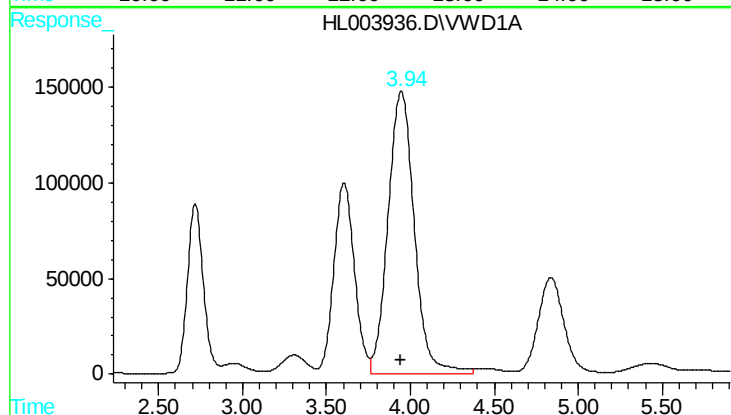

#16 3,5-Dinitroaniline

R.T.: 3.947 min
Delta R.T.: 0.004 min
Response: 16147386
Conc: 1013.70 ug/L

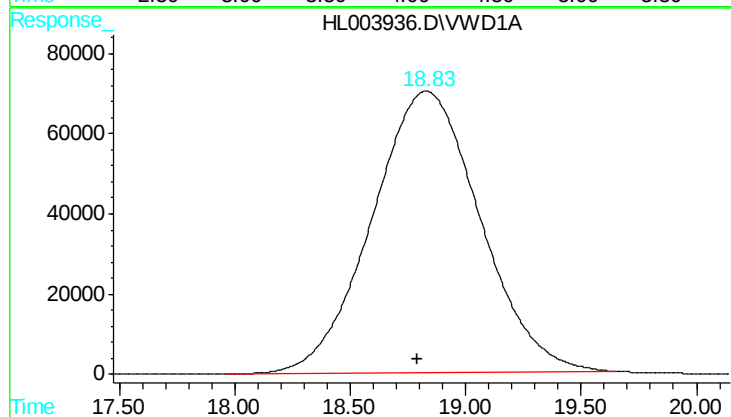

#18 PETN

R.T.: 18.830 min
Delta R.T.: 0.041 min
Response: 22863261
Conc: 2491.81 ug/L