

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003941.D Vial: 74
 Acq On : 02-Jan-2013, 06:52 Operator: HLM
 Sample : D5190-16 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Jan 2 11:30 2013 Quant Results File: HL123112.RES

Instrument :
 HPLC_L
 ClientSampleId :
 MRSEAST-M4-ISM-3

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Wed Jan 02 11:22:54 2013
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.36	263756	67.847 ug/L
Spiked Amount	300.000	Range	37 - 149	Recovery = 22.62%#

Target Compounds

4) T	1,3,5-Trinitrobenzene	2.73	9743	0.822 ug/L
------	-----------------------	------	------	------------


Quantitation Report


Data File : H:\VOL1\HPLC\HPLC L\121231\HL003941.D Vial: 74
 Acq On : 02-Jan-2013, 06:52 Operator: HLM
 Sample : D5190-16 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Jan 2 11:30 2013 Quant Results File: HL123112.RES

Instrument :
 HPLC_L
 ClientSampleId :
 MRSEAST-M4-ISM-3

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Wed Jan 02 11:22:54 2013
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

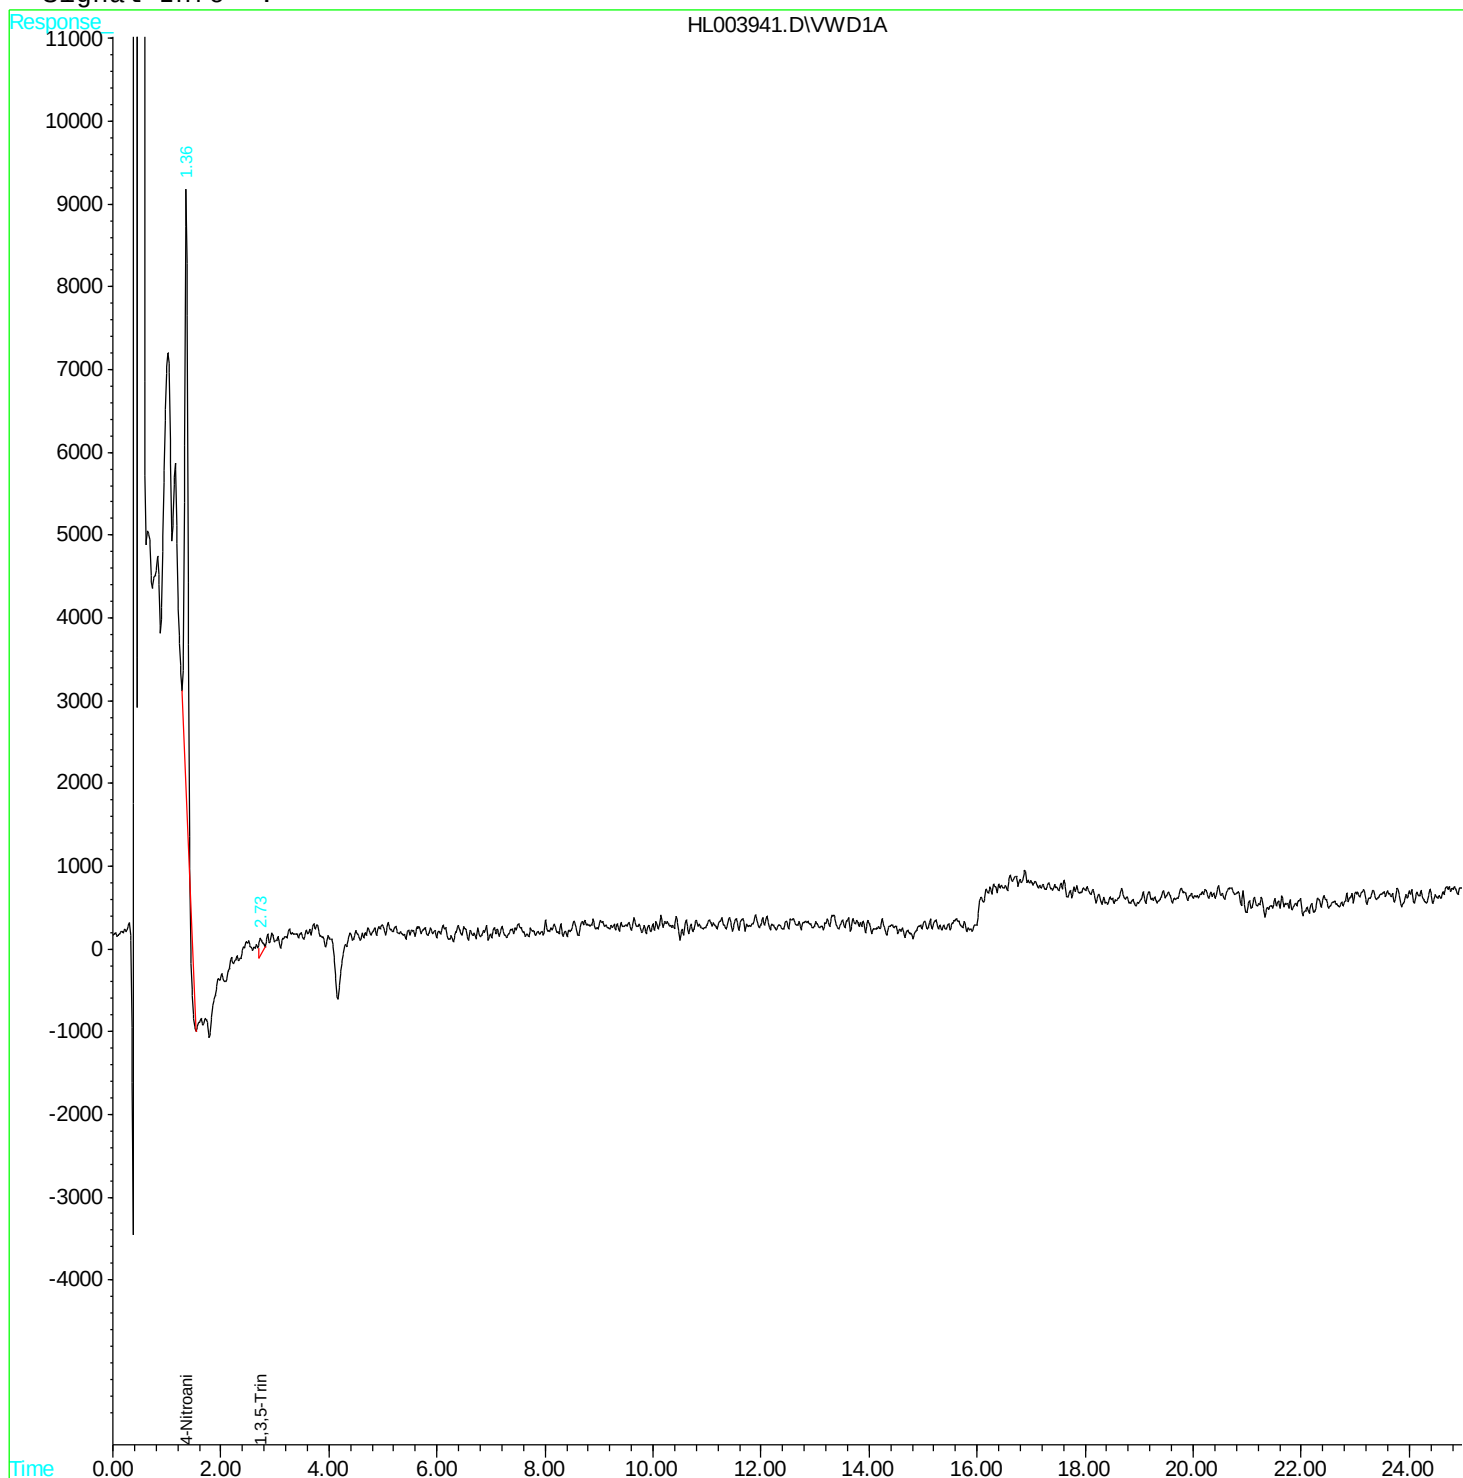

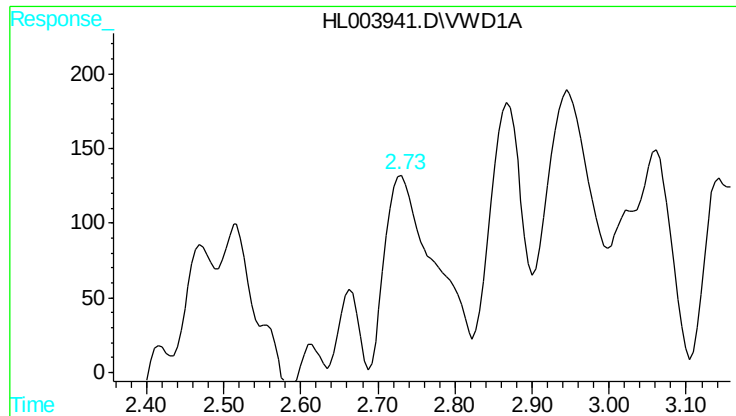

#4 1,3,5-Trinitrobenzene

R.T.: 2.731 min
Delta R.T.: 0.004 min
Response: 9743
Conc: 0.82 ug/L

Instrument :
HPLC_L
ClientSampleId :
MRSEAST-M4-ISM-3