

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003946.D Vial: 2
 Acq On : 02-Jan-2013, 09:07 Operator: HLM
 Sample : 8330-CCV Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Jan 2 11:30 2013 Quant Results File: HL123112.RES

Instrument :
 HPLC_L
 LabSampleId :
 8330-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)
 Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 Last Update : Wed Jan 02 11:22:54 2013
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) S	4-Nitroaniline	1.35	3635996	935.297 ug/L
Spiked Amount 300.000 Range 37 - 149		Recovery	= 311.77%#	

Target Compounds

2) T	HMX	0.91	4585722	1067.458 ug/L
3) T	RDX	1.75	5757709	1061.614 ug/L
4) T	1,3,5-Trinitrobenzene	2.72	5863923	494.915 ug/L
5) T	Tetryl	6.18	8332932	934.424 ug/L
6) T	2,4,6-Trinitrotoluene	6.54	5629005	480.378 ug/L
7) T	2-Amino-4,6-dinitrotoluene	7.02	5596648	496.198 ug/L
8) T	4-Amino-2,6-dinitrotoluene	7.35	3776137	515.840 ug/L
9) T	2,4-Dinitrotoluene	8.17	7942745	509.722 ug/L
10) T	2,6-Dinitrotoluene	8.55	4362631	503.925 ug/L
11) T	1,3-Dinitrobenzene	3.61	8522875	503.394 ug/L
12) T	Nitrobenzene	4.84	5423543	505.043 ug/L
13) T	2-Nitrotoluene	11.76	6759618	1020.635 ug/L
14) T	3-Nitrotoluene	13.78	7164273	1007.356 ug/L
15) T	4-Nitrotoluene	12.52	5658204	1031.196 ug/L
16) T	3,5-Dinitroaniline	3.95	16076717	1009.262 ug/L
18) T	PETN	18.85	23266939	2535.807 ug/L

Data File : H:\VOL1\HPLC\HPLC L\121231\HL003946.D

Vial: 2

Acq On : 02-Jan-2013, 09:07

Operator: HLM

Sample : 8330-CCV

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Jan 2 11:30 2013 Quant Results File: HL123112.RES

Instrument :

HPLC_L

LabSampleId :

8330-CCV

Quant Method : H:\VOL1\HPLC\HPLC L\METHODS\HL123112.M (Chemstation Integrator)

Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)

Last Update : Wed Jan 02 11:22:54 2013


Response via : Multiple Level Calibration


DataAcq Meth : 8330AGIP.M

Volume Inj. :

Signal Phase :

Signal Info :

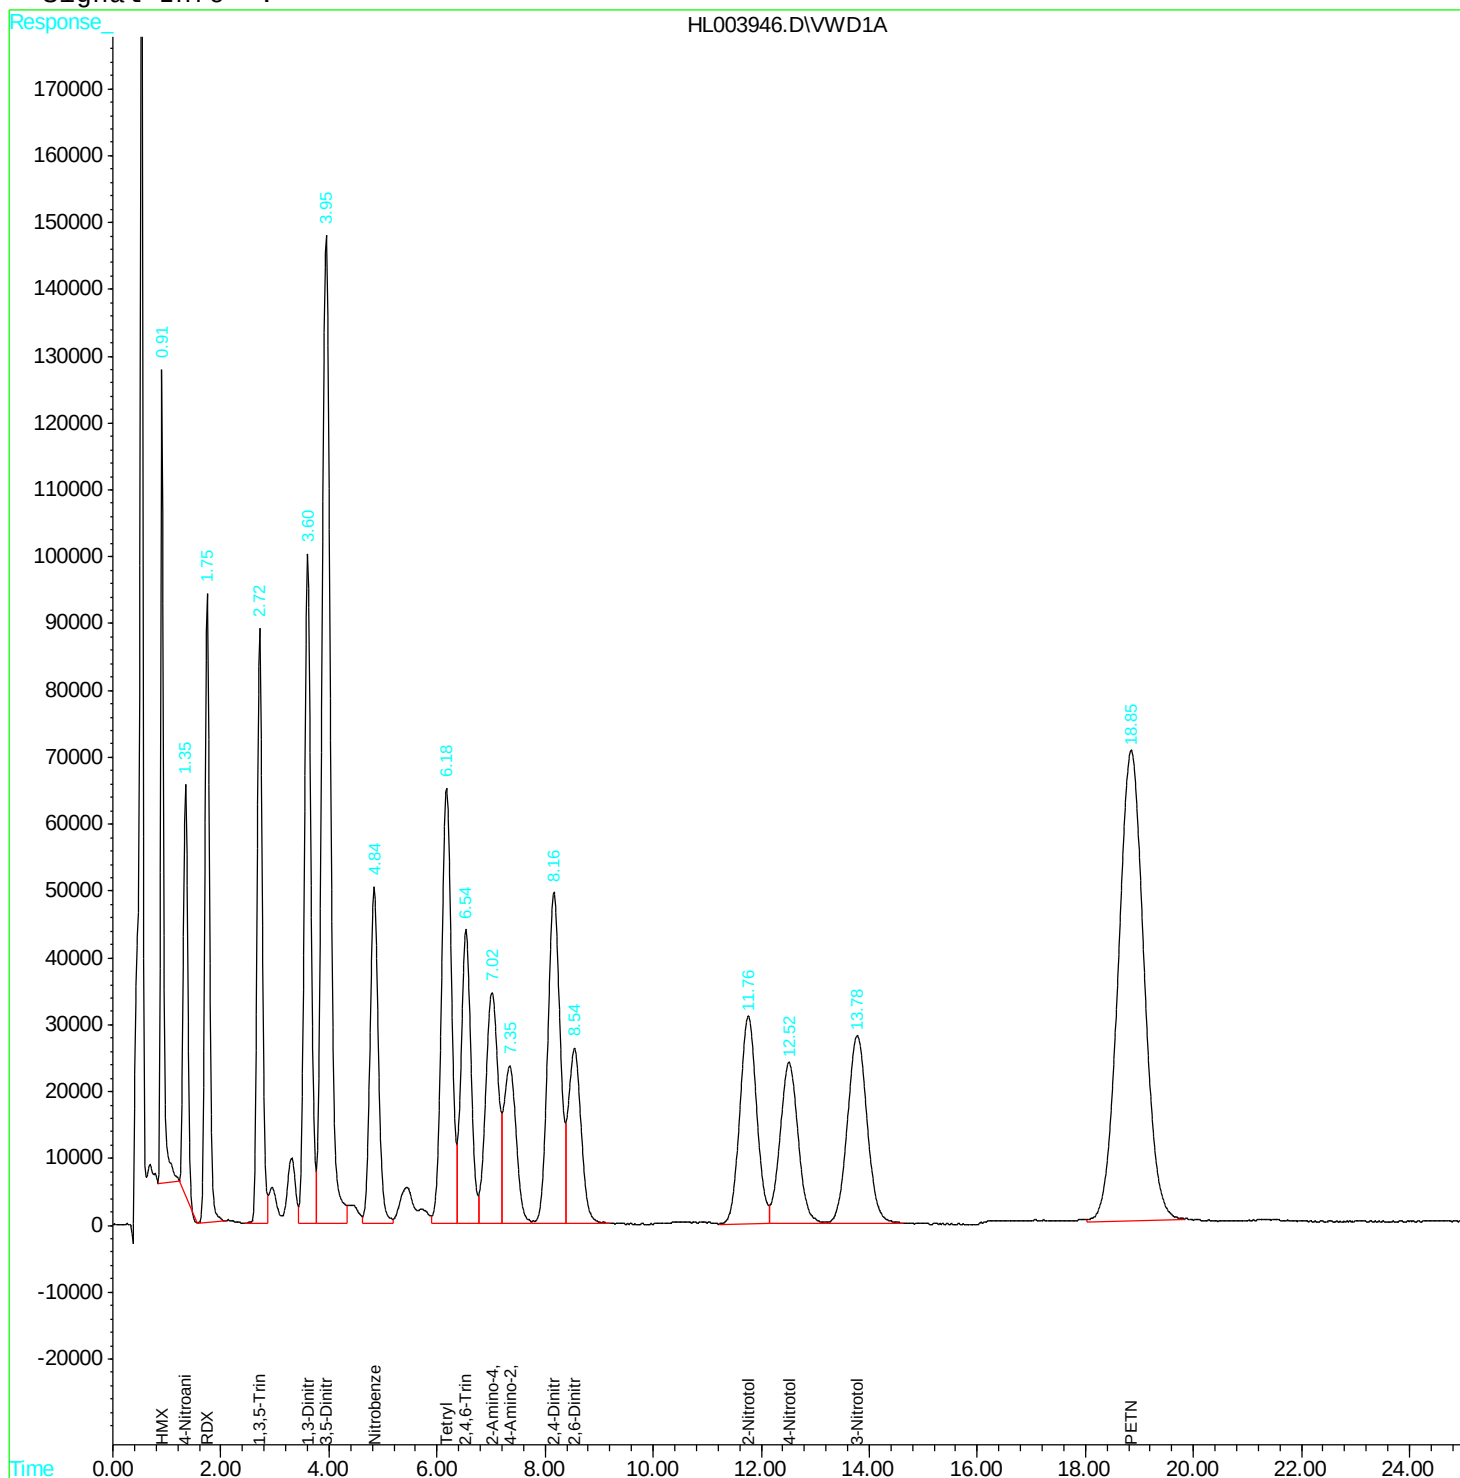


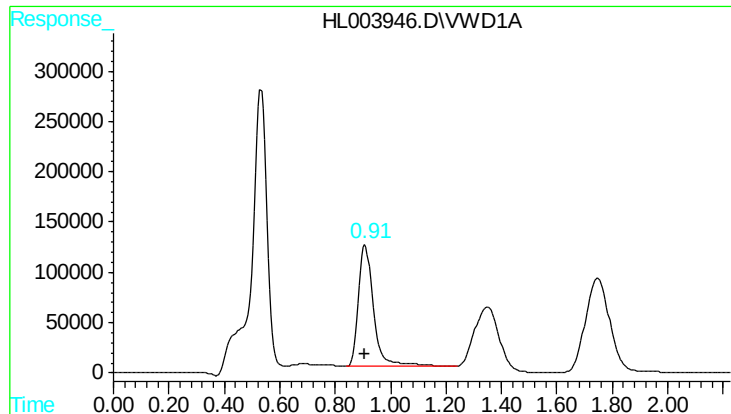

#2 HMX


R.T.: 0.909 min
Delta R.T.: 0.002 min
Response: 4585722
Conc: 1067.46 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

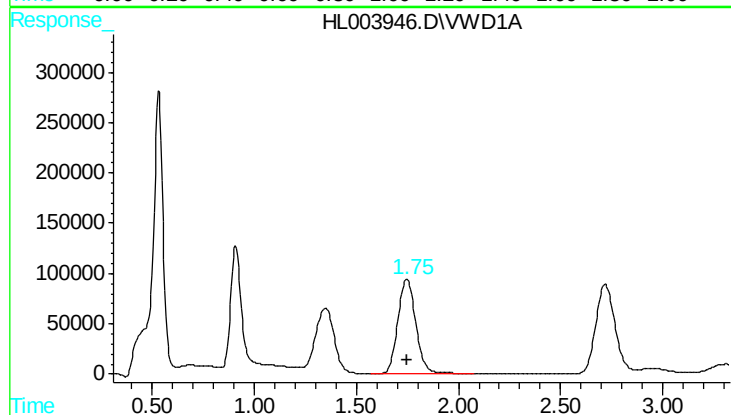


#3 RDX

R.T.: 1.748 min
Delta R.T.: 0.001 min
Response: 5757709
Conc: 1061.61 ug/L

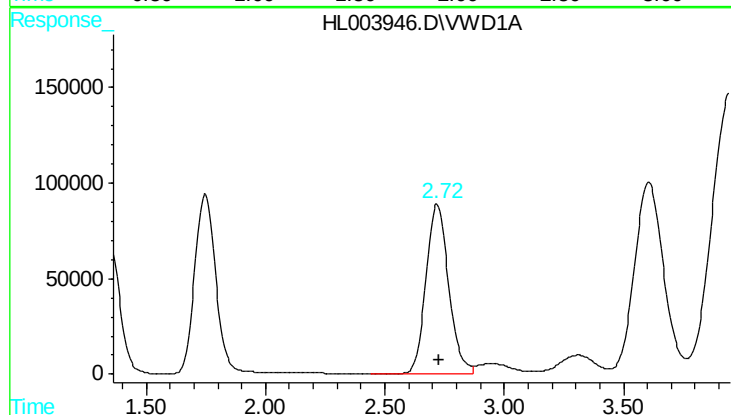


#4 1,3,5-Trinitrobenzene

R.T.: 2.719 min
Delta R.T.: -0.008 min
Response: 5863923
Conc: 494.92 ug/L

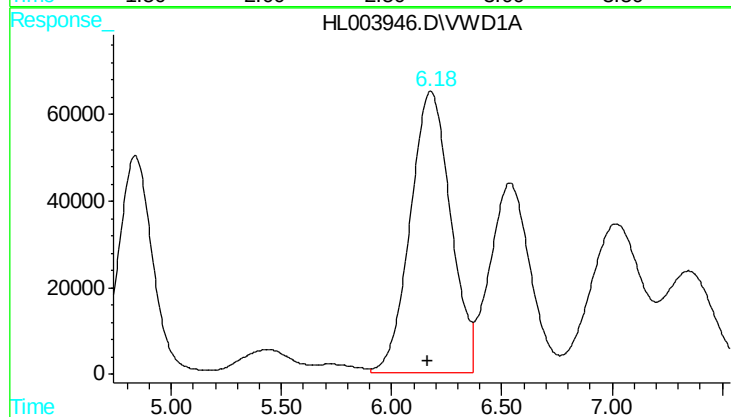

#5 Tetryl


R.T.: 6.178 min
Delta R.T.: 0.016 min
Response: 8332932
Conc: 934.42 ug/L

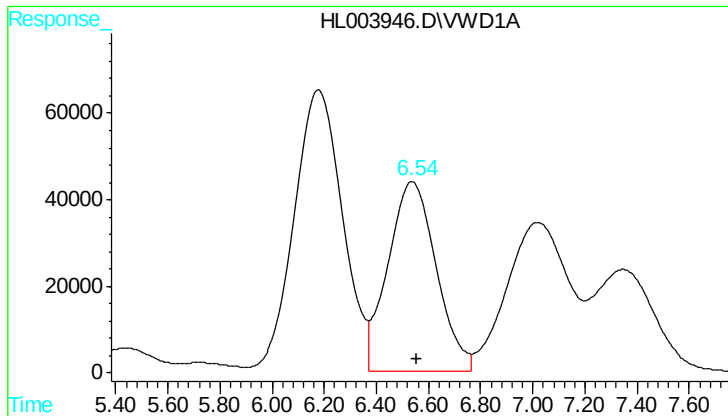

#6 2,4,6-Trinitrotoluene


R.T.: 6.538 min
Delta R.T.: -0.017 min
Response: 5629005
Conc: 480.38 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

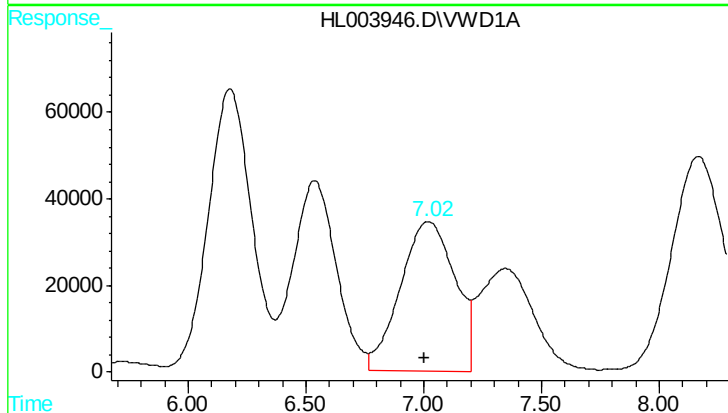


#7 2-Amino-4,6-dinitrotoluene

R.T.: 7.019 min
Delta R.T.: 0.018 min
Response: 5596648
Conc: 496.20 ug/L

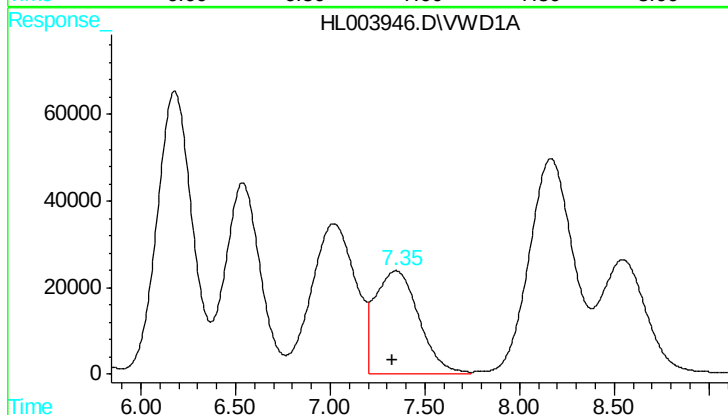


#8 4-Amino-2,6-dinitrotoluene

R.T.: 7.347 min
Delta R.T.: 0.020 min
Response: 3776137
Conc: 515.84 ug/L

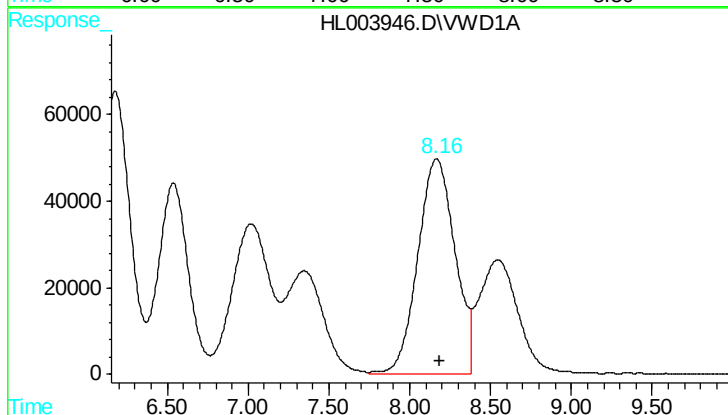

#9 2,4-Dinitrotoluene


R.T.: 8.166 min
Delta R.T.: -0.018 min
Response: 7942745
Conc: 509.72 ug/L

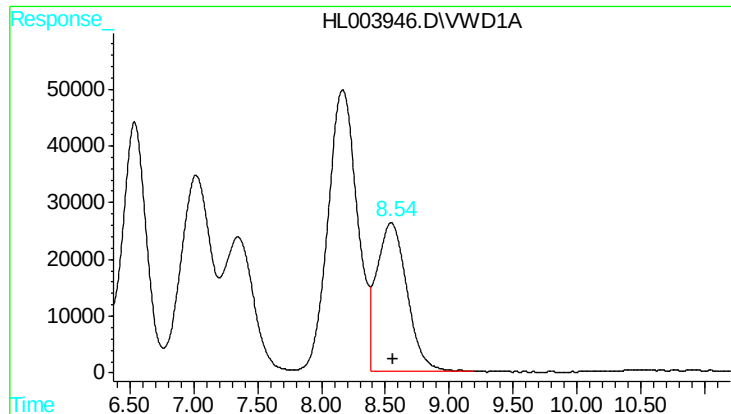

#10 2,6-Dinitrotoluene


R.T.: 8.546 min
Delta R.T.: -0.015 min
Response: 4362631
Conc: 503.92 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

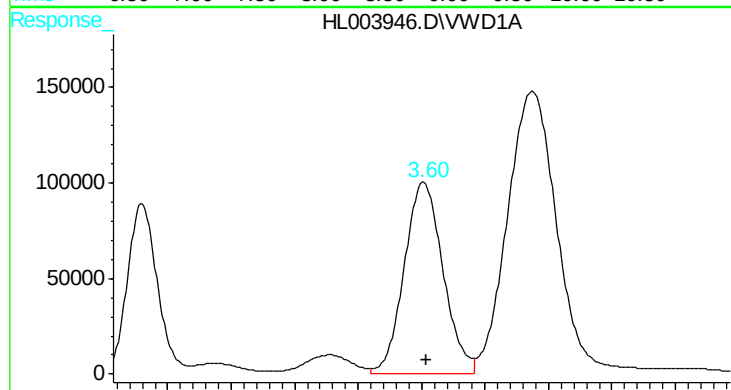


#11 1,3-Dinitrobenzene

R.T.: 3.607 min
Delta R.T.: -0.008 min
Response: 8522875
Conc: 503.39 ug/L

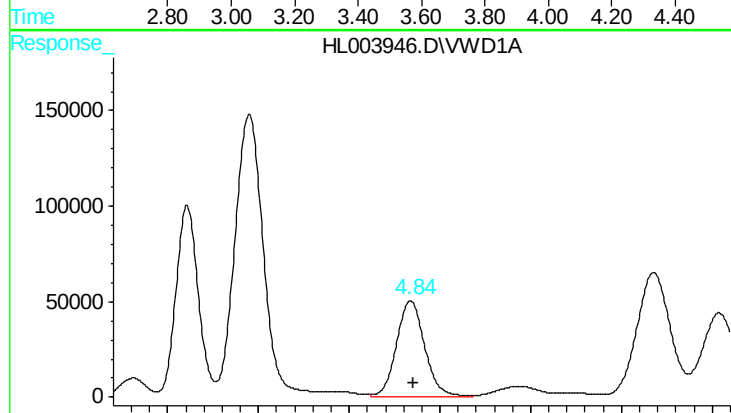


#12 Nitrobenzene

R.T.: 4.838 min
Delta R.T.: -0.018 min
Response: 5423543
Conc: 505.04 ug/L

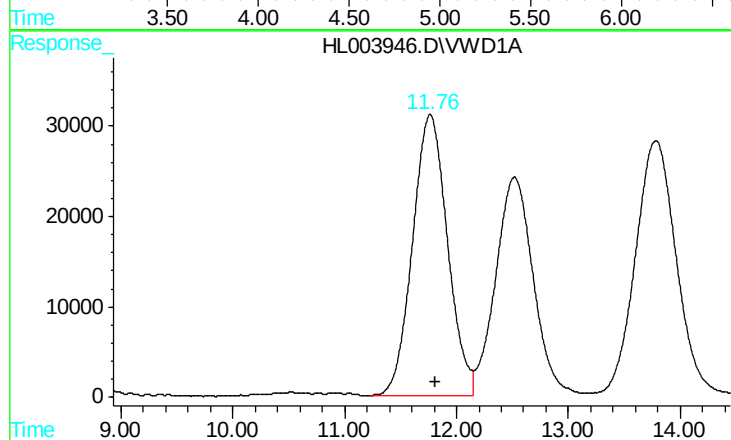

#13 2-Nitrotoluene


R.T.: 11.764 min
Delta R.T.: -0.042 min
Response: 6759618
Conc: 1020.64 ug/L

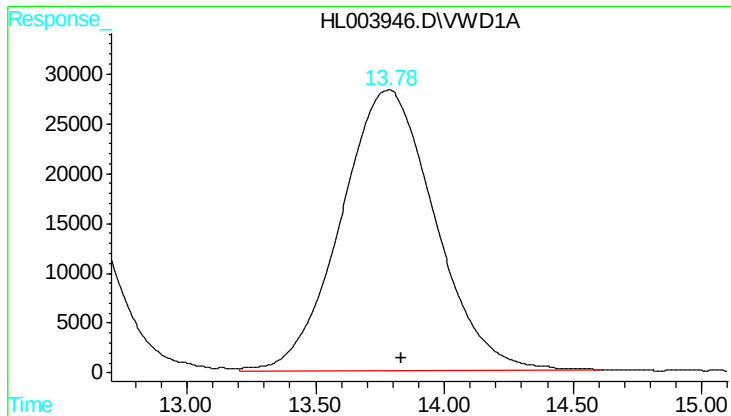

#14 3-Nitrotoluene


R.T.: 13.781 min
Delta R.T.: -0.050 min
Response: 7164273
Conc: 1007.36 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

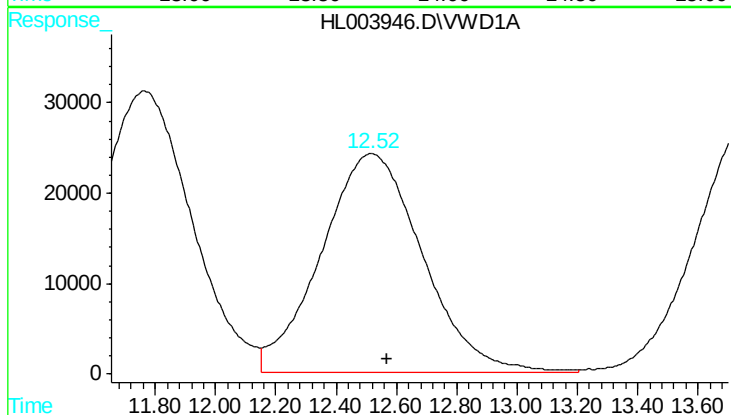


#15 4-Nitrotoluene

R.T.: 12.518 min
Delta R.T.: -0.052 min
Response: 5658204
Conc: 1031.20 ug/L

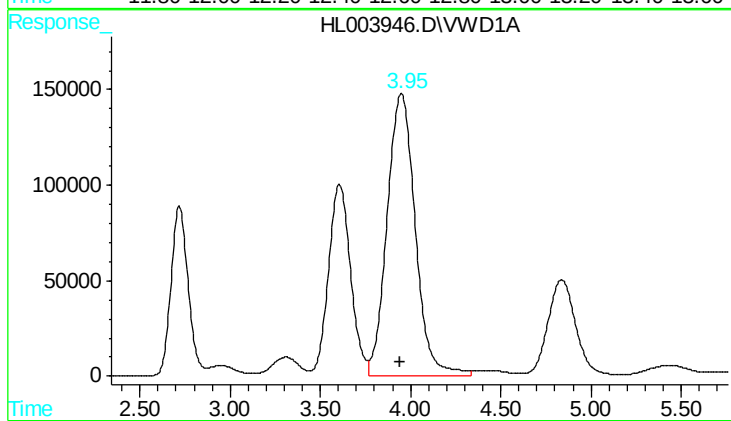

#16 3,5-Dinitroaniline

R.T.: 3.949 min
Delta R.T.: 0.007 min
Response: 16076717
Conc: 1009.26 ug/L

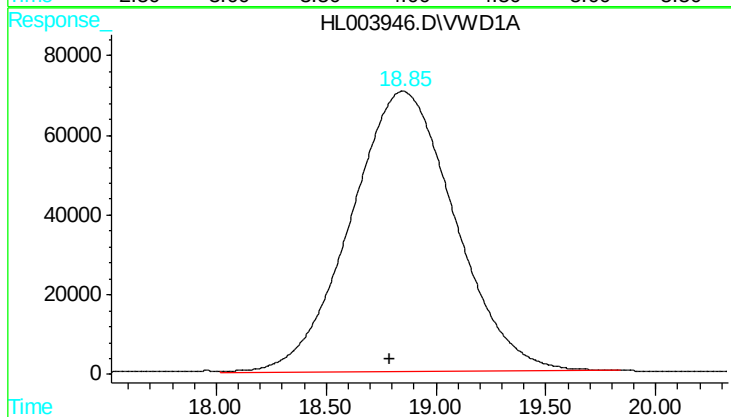

#18 PETN

R.T.: 18.850 min
Delta R.T.: 0.061 min
Response: 23266939
Conc: 2535.81 ug/L