

Data Path : S:\HPCHEM1\HPLC_L\Data\HL123112\
 Data File : HL003936.D
 Signal(s) : VWD1A.CH
 Acq On : 02-Jan-2013, 04:37
 Operator : HLM
 Sample : 8330-CCV
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 HPLC_L
 LabSampleId :
 8330-CCV

Integration File: events.e
 Quant Time: Jan 03 04:13:00 2013
 Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL123112.M
 Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
 QLast Update : Wed Jan 02 11:22:54 2013
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.350	3577920	920.358 ug/L
Spiked Amount 300.000	Range 37 - 149	Recovery	= 306.79%#
Target Compounds			
2) T HMX	0.908	4535648	1054.774 ug/L
3) T RDX	1.746	5763305	1062.646 ug/L
4) T 1,3,5-Trinitrobenzene	2.718	5866000	495.091 ug/L
5) T Tetryl	6.173	8353271	936.705 ug/L
6) T 2,4,6-Trinitrotoluene	6.537	5626798	480.190 ug/L
7) T 2-Amino-4,6-dinitroto...	7.015	5607834	497.190 ug/L
8) T 4-Amino-2,6-dinitroto...	7.339	3744358	511.499 ug/L
9) T 2,4-Dinitrotoluene	8.163	7910224	507.635 ug/L
10) T 2,6-Dinitrotoluene	8.543	4370161	504.795 ug/L
11) T 1,3-Dinitrobenzene	3.605	8488966	501.391 ug/L
12) T Nitrobenzene	4.838	5424073	505.093 ug/L
13) T 2-Nitrotoluene	11.760	6733910	1016.753 ug/L
14) T 3-Nitrotoluene	13.775	7525102	1058.092 ug/L
15) T 4-Nitrotoluene	12.512	5731562	1044.565 ug/L
16) T 3,5-Dinitroaniline	3.947	16147386	1013.698 ug/L
18) T PETN	18.830	22863261	2491.811 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_L\Data\HL123112\
Data File : HL003936.D
Signal(s) : VWD1A.CH
Acq On : 02-Jan-2013, 04:37
Operator : HLM
Sample : 8330-CCV
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
HPLC_L
LabSampleId :
8330-CCV

Integration File: events.e
Quant Time: Jan 03 04:13:00 2013
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL123112.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Wed Jan 02 11:22:54 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

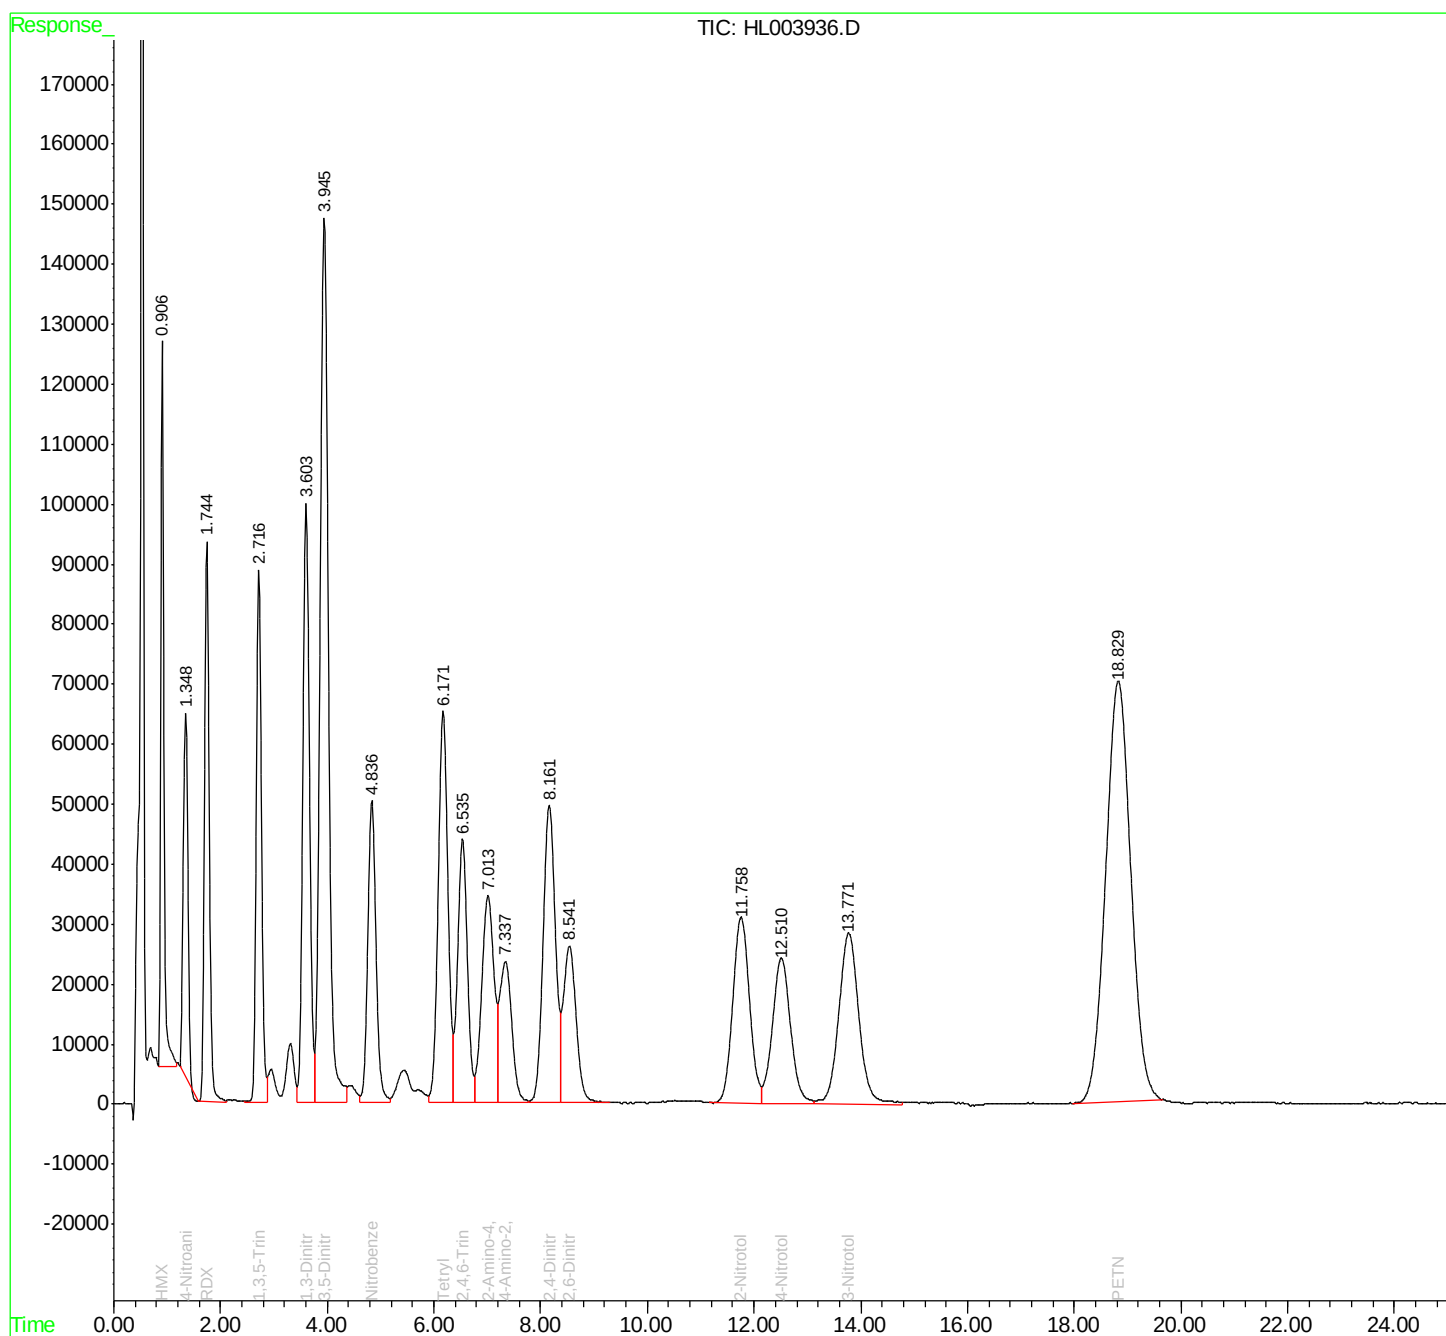


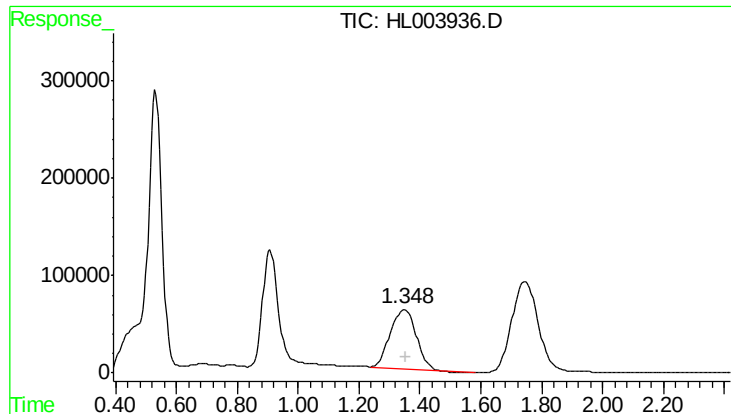

#1 4-Nitroaniline


R.T.: 1.350 min
Delta R.T.: -0.003 min
Response: 3577920
Conc: 920.36 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

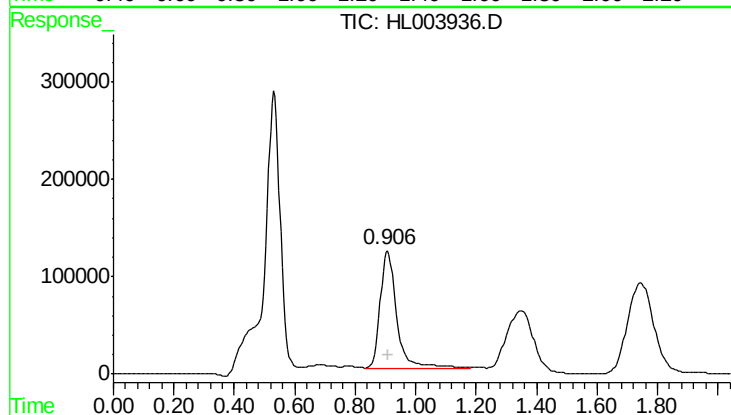


#2 HMX

R.T.: 0.908 min
Delta R.T.: 0.000 min
Response: 4535648
Conc: 1054.77 ug/L

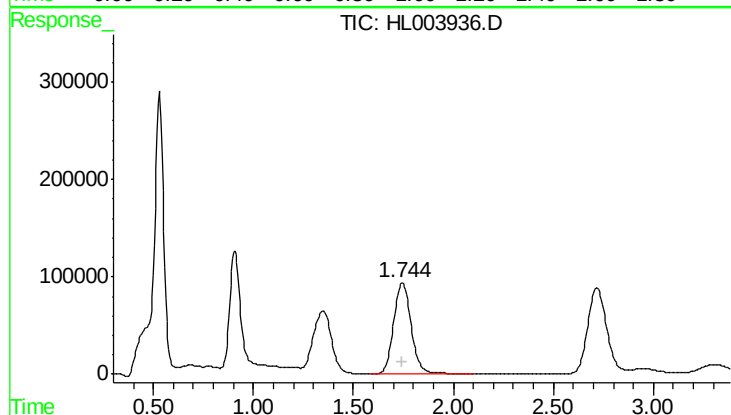


#3 RDX

R.T.: 1.746 min
Delta R.T.: 0.000 min
Response: 5763305
Conc: 1062.65 ug/L

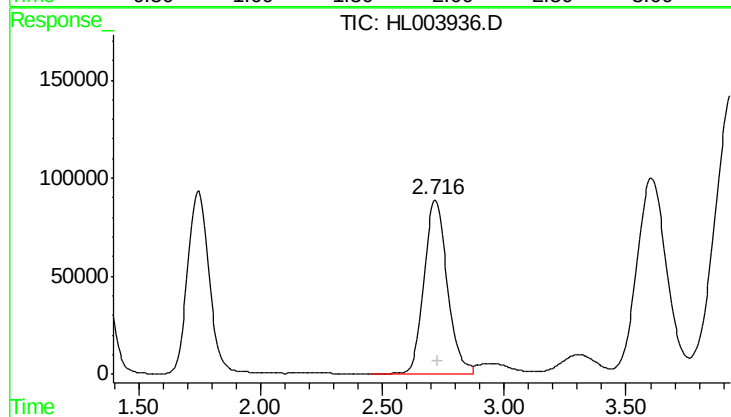

#4 1,3,5-Trinitrobenzene


R.T.: 2.718 min
Delta R.T.: -0.009 min
Response: 5866000
Conc: 495.09 ug/L

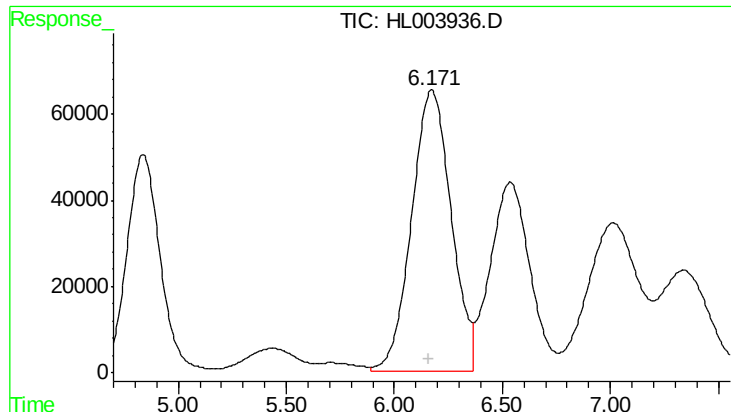

#5 Tetryl


R.T.: 6.173 min
Delta R.T.: 0.012 min
Response: 8353271
Conc: 936.71 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

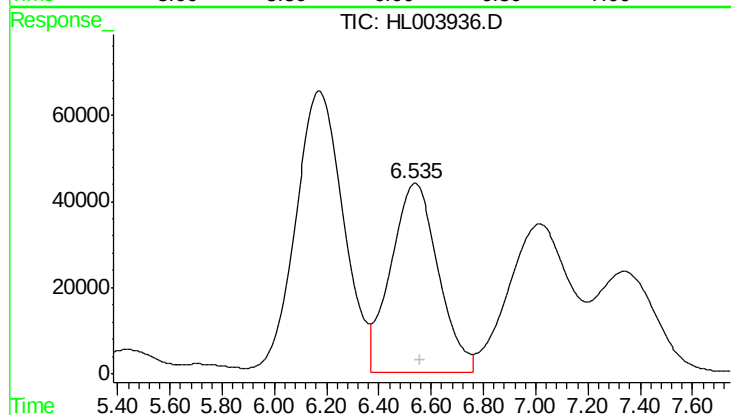


#6 2,4,6-Trinitrotoluene

R.T.: 6.537 min
Delta R.T.: -0.018 min
Response: 5626798
Conc: 480.19 ug/L

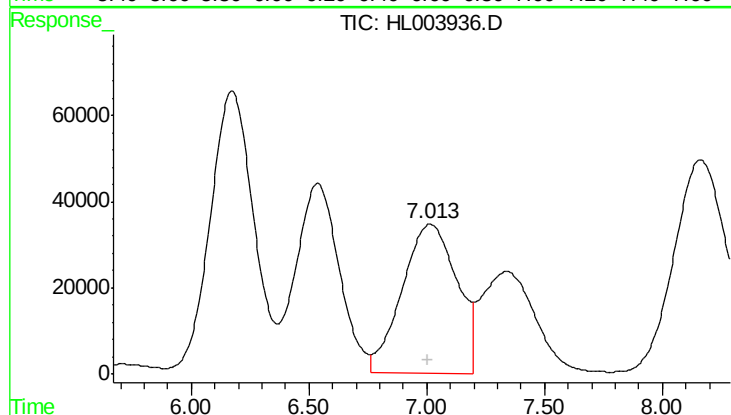


#7 2-Amino-4,6-dinitrotoluene

R.T.: 7.015 min
Delta R.T.: 0.014 min
Response: 5607834
Conc: 497.19 ug/L

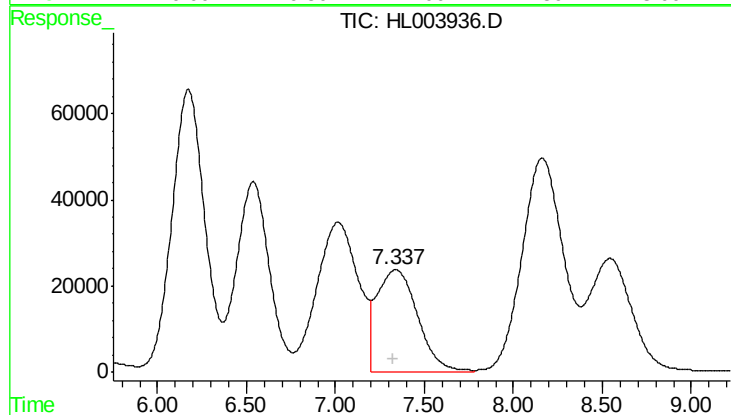

#8 4-Amino-2,6-dinitrotoluene


R.T.: 7.339 min
Delta R.T.: 0.012 min
Response: 3744358
Conc: 511.50 ug/L

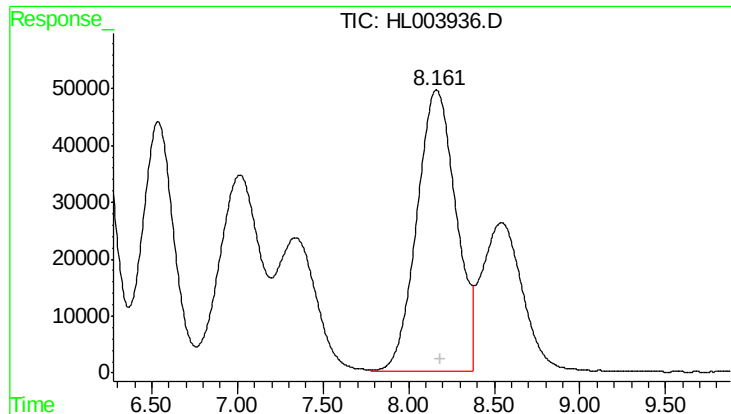

#9 2,4-Dinitrotoluene


R.T.: 8.163 min
Delta R.T.: -0.020 min
Response: 7910224
Conc: 507.64 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

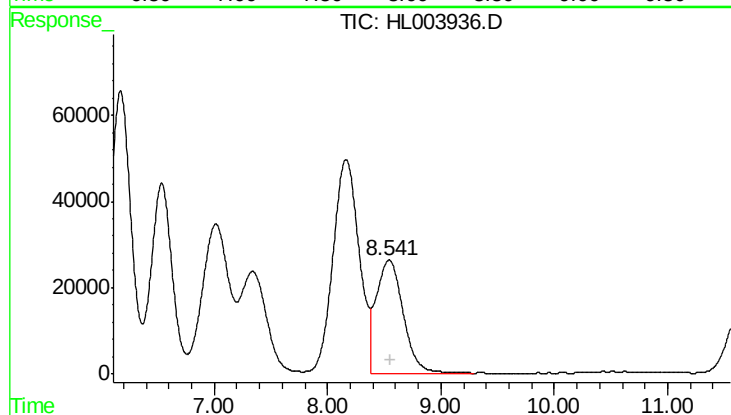


#10 2,6-Dinitrotoluene

R.T.: 8.543 min
Delta R.T.: -0.018 min
Response: 4370161
Conc: 504.79 ug/L

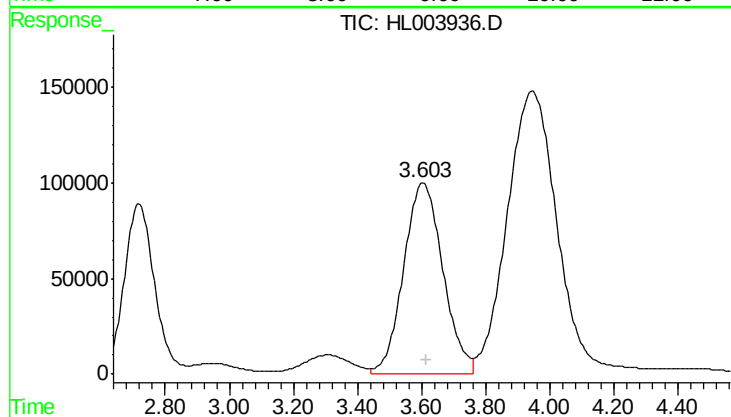


#11 1,3-Dinitrobenzene

R.T.: 3.605 min
Delta R.T.: -0.009 min
Response: 8488966
Conc: 501.39 ug/L

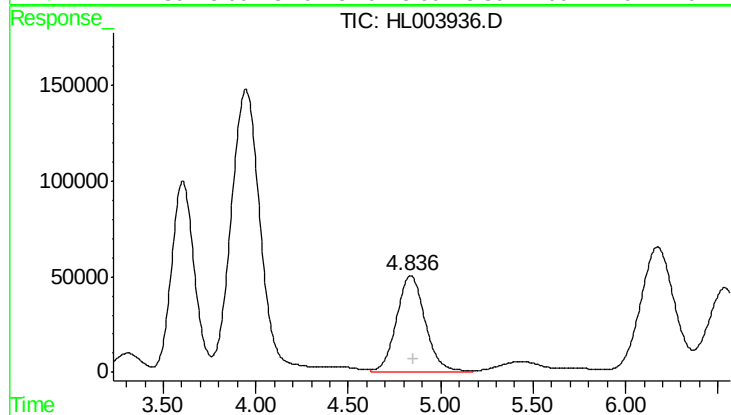

#12 Nitrobenzene


R.T.: 4.838 min
Delta R.T.: -0.017 min
Response: 5424073
Conc: 505.09 ug/L

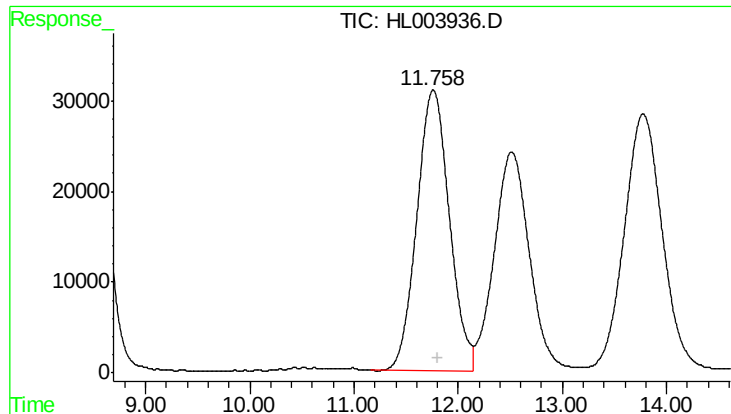

#13 2-Nitrotoluene


R.T.: 11.760 min
Delta R.T.: -0.046 min
Response: 6733910
Conc: 1016.75 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV

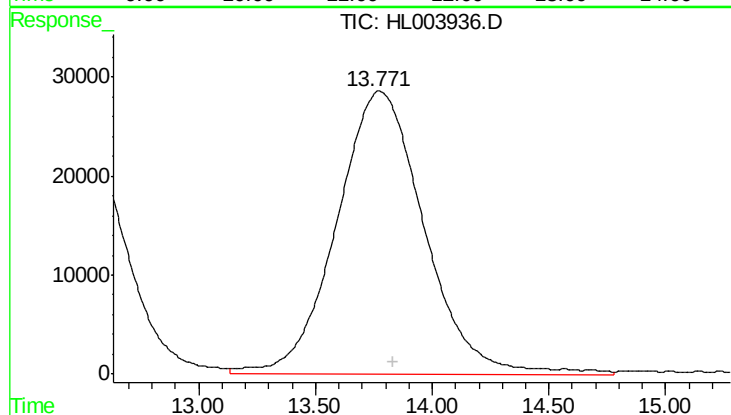


#14 3-Nitrotoluene

R.T.: 13.775 min
Delta R.T.: -0.057 min
Response: 7525102
Conc: 1058.09 ug/L

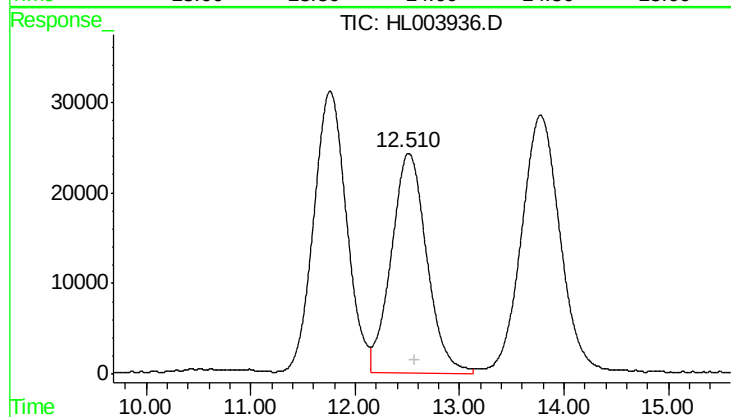


#15 4-Nitrotoluene

R.T.: 12.512 min
Delta R.T.: -0.058 min
Response: 5731562
Conc: 1044.56 ug/L

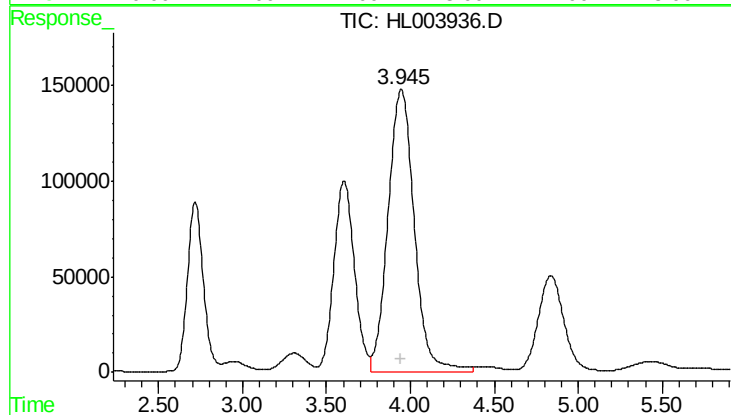

#16 3,5-Dinitroaniline

R.T.: 3.947 min
Delta R.T.: 0.004 min
Response: 16147386
Conc: 1013.70 ug/L

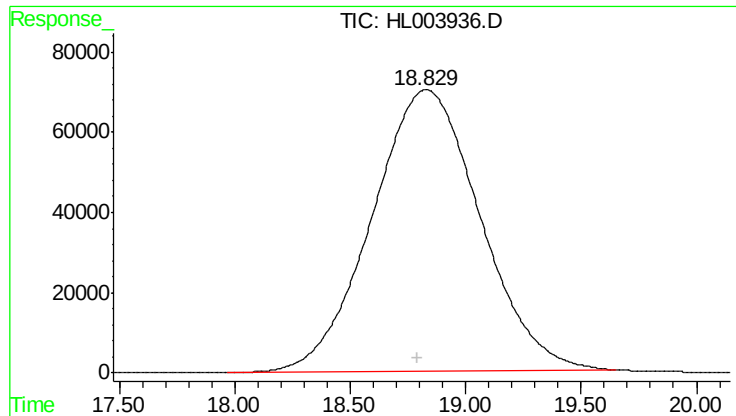

#18 PETN

R.T.: 18.830 min
Delta R.T.: 0.041 min
Response: 22863261
Conc: 2491.81 ug/L

Instrument :
HPLC_L
LabSampleId :
8330-CCV