

Data Path : S:\HPCHEM1\HPLC_L\Data\HL123112\
Data File : HL003939.D
Signal(s) : VWD1A.CH
Acq On : 02-Jan-2013, 05:58
Operator : HLM
Sample : D5190-14
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
HPLC_L
ClientSampleId :
MRSEAST-M4-ISM-1

Manual Integrations
APPROVED

AHPatel
1/5/2013 12:47:10 AM

Integration File: events.e
Quant Time: Jan 03 04:13:16 2013
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL123112.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Wed Jan 02 11:22:54 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.368f	109904	28.271 ug/L m
Spiked Amount 300.000	Range 37 - 149	Recovery =	9.42%#
Target Compounds			

(f)=RT Delta > 1/2 Window (m)=manual int.

Data Path : S:\HPCHEM1\HPLC_L\Data\HL123112\
Data File : HL003939.D
Signal(s) : VWD1A.CH
Acq On : 02-Jan-2013, 05:58
Operator : HLM
Sample : D5190-14
Misc :
ALS Vial : 72 Sample Multiplier: 1


Instrument :
HPLC_L
ClientSampleId :
MRSEAST-M4-ISM-1


Manual Integrations
APPROVED

AHPatel
1/5/2013 12:47:10 AM

Integration File: events.e
Quant Time: Jan 03 04:13:16 2013
Quant Method : H:\VOL1\HPLC\HPLC_L\METHODS\HL123112.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Wed Jan 02 11:22:54 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

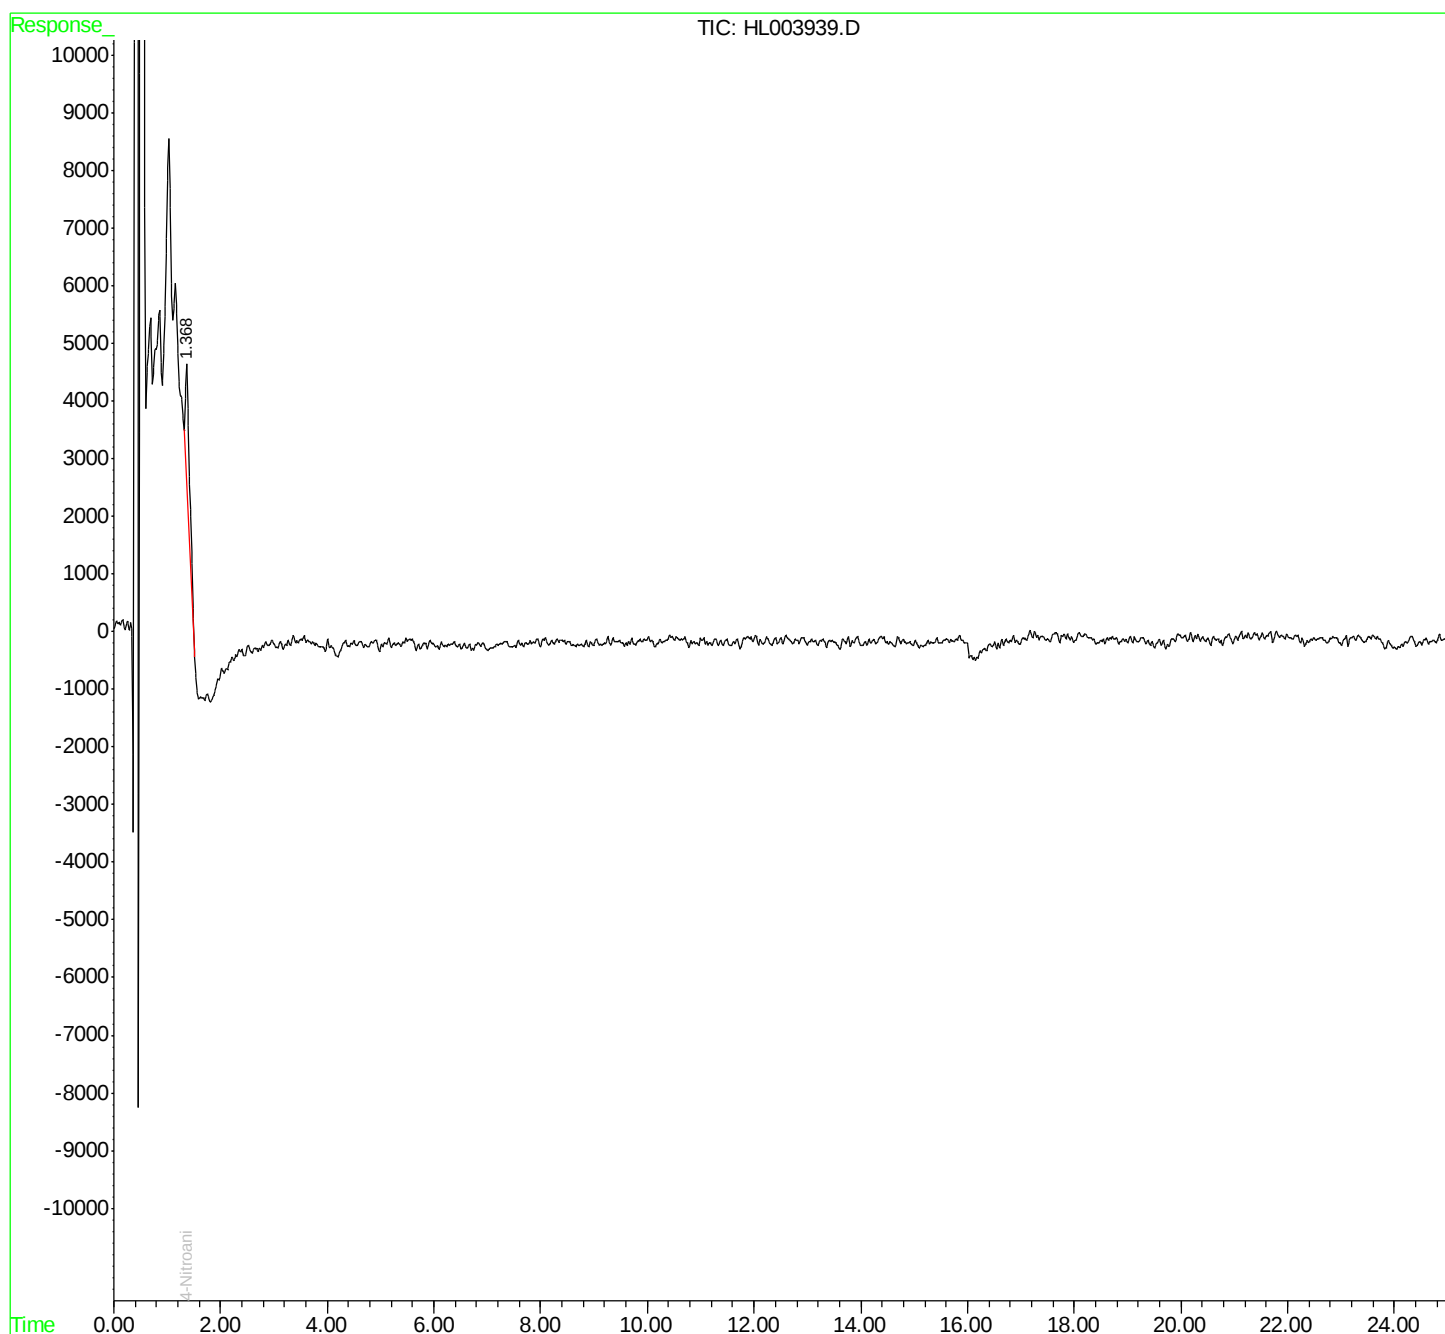

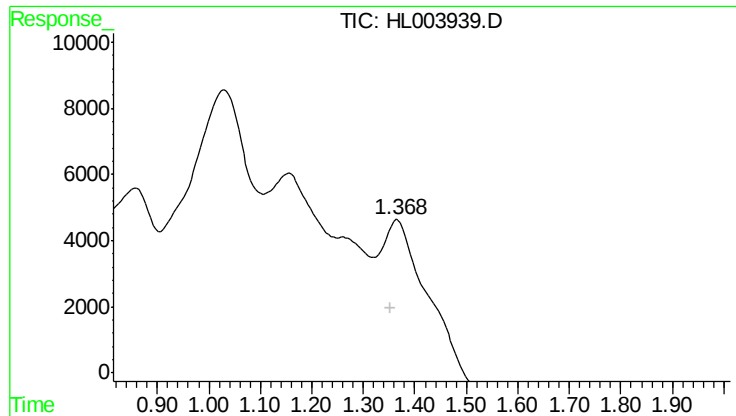

#1 4-Nitroaniline

R.T.: 1.368 min
Delta R.T.: 0.014 min
Response: 109904
Conc: 28.27 ug/L m

Instrument :
HPLC_L
ClientSampleId :
MRSEAST-M4-ISM-1

Manual Integrations
APPROVED

AHPatel
1/5/2013 12:47:10 AM