

Data File : S:\HPCHEM1\HPLC_L\DATA\HL012414\HL005641.D Vial: 4
Acq On : 24-Jan-2014, 20:43 Operator: QM
Sample : HSTDCCC005 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Jan 24 23:43 2014 Quant Results File: HL0124NG.RES

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL0124NG.M
Title :
Last Update : Mon Oct 07 18:04:20 2013
Response via : Initial Calibration
DataAcq Meth : 8330BNG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.51	22270908	5.068 ng/ul

Target Compounds

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.


HL005641.D HL0124NG.M Fri Jan 24 23:43:56 2014 RPT1


Quantitation Report

Data File : S:\HPCHEM1\HPLC_L\DATA\HL012414\HL005641.D Vial: 4
Acq On : 24-Jan-2014, 20:43 Operator: QM
Sample : HSTDCCC005 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Jan 24 23:43 2014 Quant Results File: HL0124NG.RES

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL0124NG.M
Title :
Last Update : Mon Oct 07 18:04:20 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330BNG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

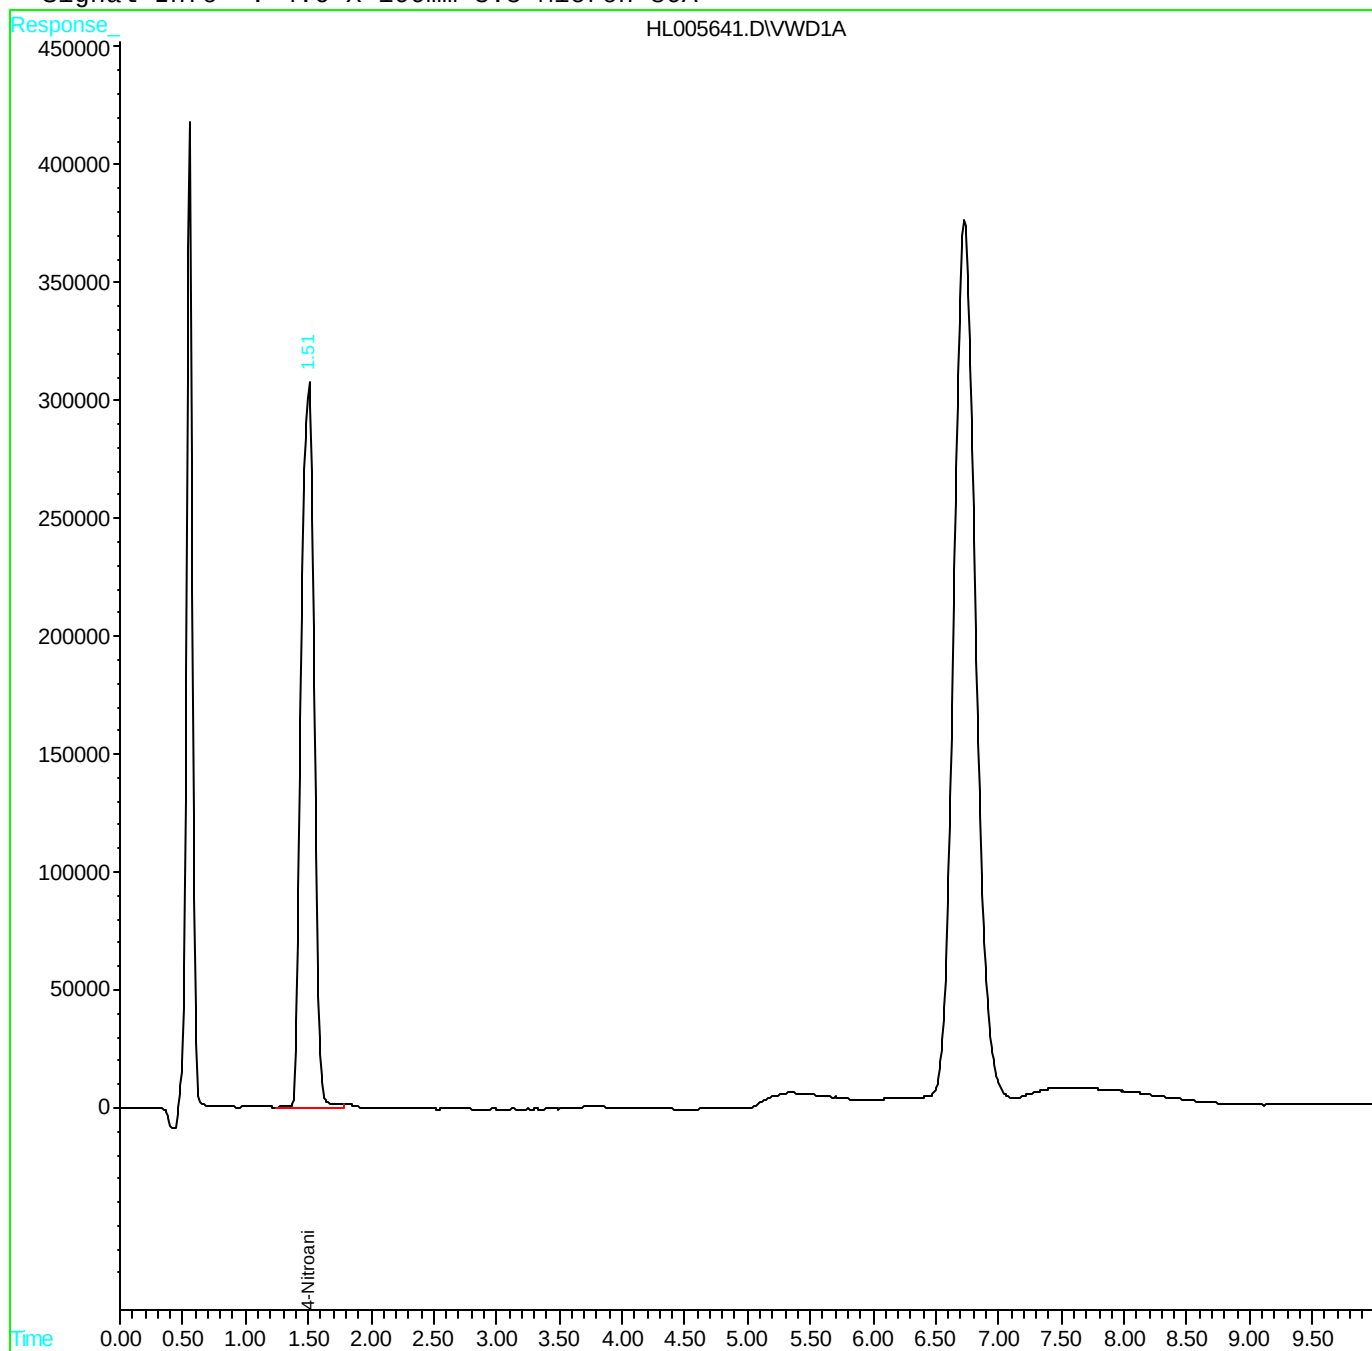

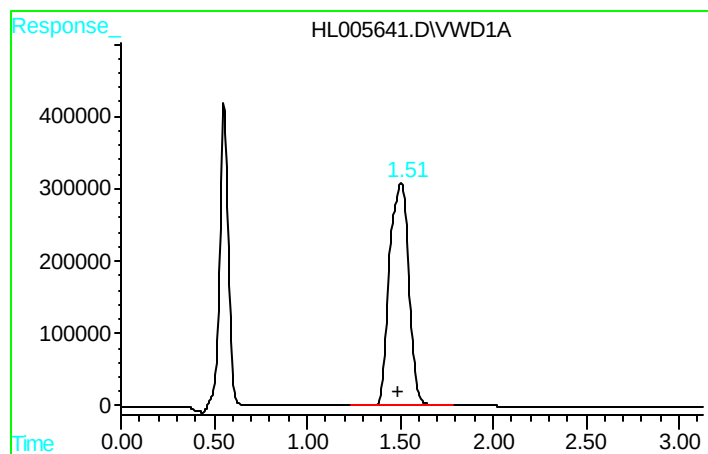

#1 4-Nitroaniline

R.T.: 1.508 min
Delta R.T.: 0.020 min
Response: 22270908
Conc: 5.07 ng/ul