

Data File : S:\HPCHEM1\HPLC_L\DATA\HL012414\HL005652.D Vial: 33
 Acq On : 25-Jan-2014, 01:24 Operator: QM
 Sample : F1002-05 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : AUTOINT1.E
 Quant Time: Jan 27 3:11 2014 Quant Results File: HL012414.RES

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL012414.M
 Title :
 Last Update : Mon Jan 27 02:24:42 2014
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

 Analyst Signature: _____ Analyst Name: _____ Date: _____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #: _____

___Peak integrated by software incorrectly.Compound #: _____

___OTHER: _____ Compound #: _____


(f)=RT Delta > 1/2 Window (m)=manual int.


Quantitation Report

Data File : S:\HPCHEM1\HPLC_L\DATA\HL012414\HL005652.D Vial: 33
Acq On : 25-Jan-2014, 01:24 Operator: QM
Sample : F1002-05 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Jan 27 3:11 2014 Quant Results File: HL012414.RES

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL012414.M
Title :
Last Update : Mon Jan 27 02:24:42 2014
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

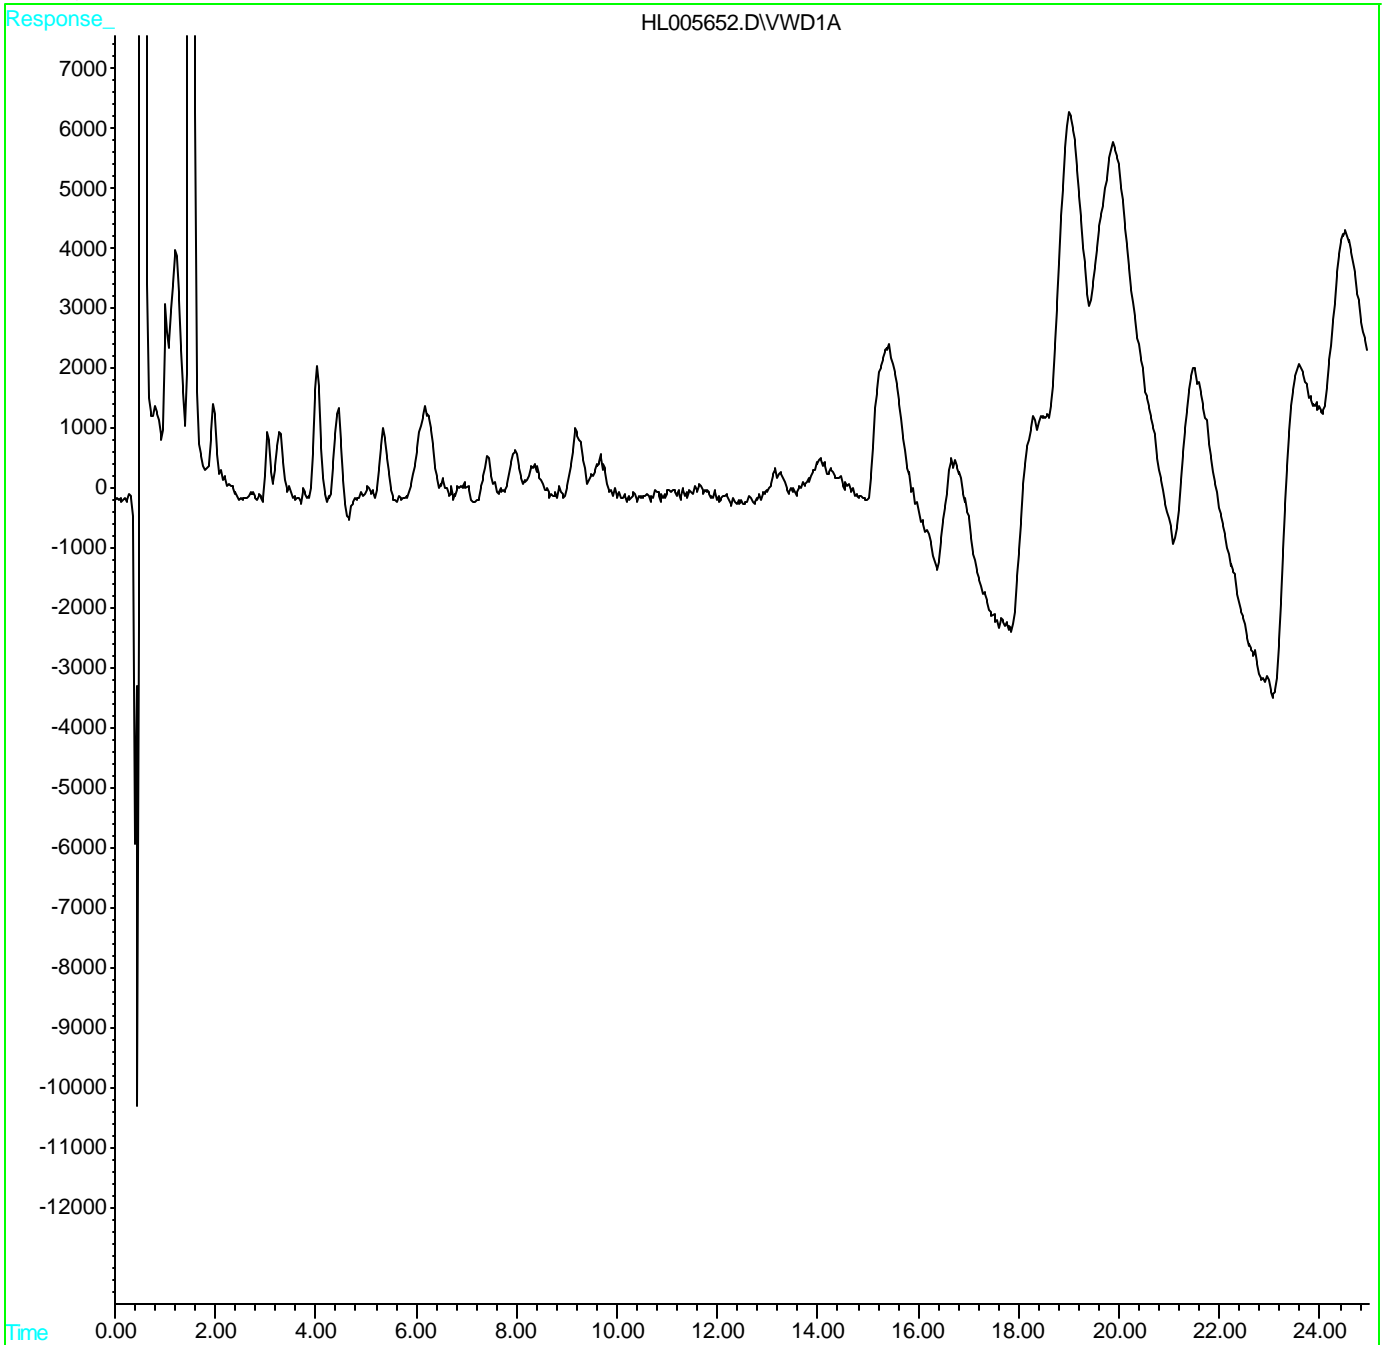

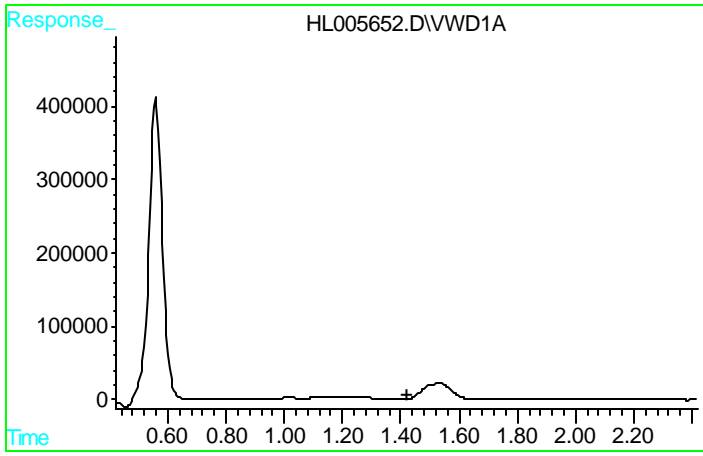

#1 4-Nitroaniline

R.T.: 0.000 min
Exp R.T. : 1.421 min
Response: 0
Conc: N.D.