

Data File : S:\HPCHEM1\HPLC_L\DATA\HL012414\HL005656.D Vial: 24
Acq On : 25-Jan-2014, 03:12 Operator: QM
Sample : HSTDCCC0500 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Jan 27 3:18 2014 Quant Results File: HL012414.RES

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL012414.M
Title :
Last Update : Mon Jan 27 02:24:42 2014
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.48	1931681	482.087 ug/L
Target Compounds			
2) T HMX	0.97	2167051	481.412 ug/L

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.


HL005656.D HL012414.M Mon Jan 27 03:18:22 2014 RPT1


Quantitation Report

Data File : S:\HPCHEM1\HPLC_L\DATA\HL012414\HL005656.D Vial: 24
Acq On : 25-Jan-2014, 03:12 Operator: QM
Sample : HSTDCCC0500 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Jan 27 3:18 2014 Quant Results File: HL012414.RES

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL012414.M
Title :
Last Update : Mon Jan 27 02:24:42 2014
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M


Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

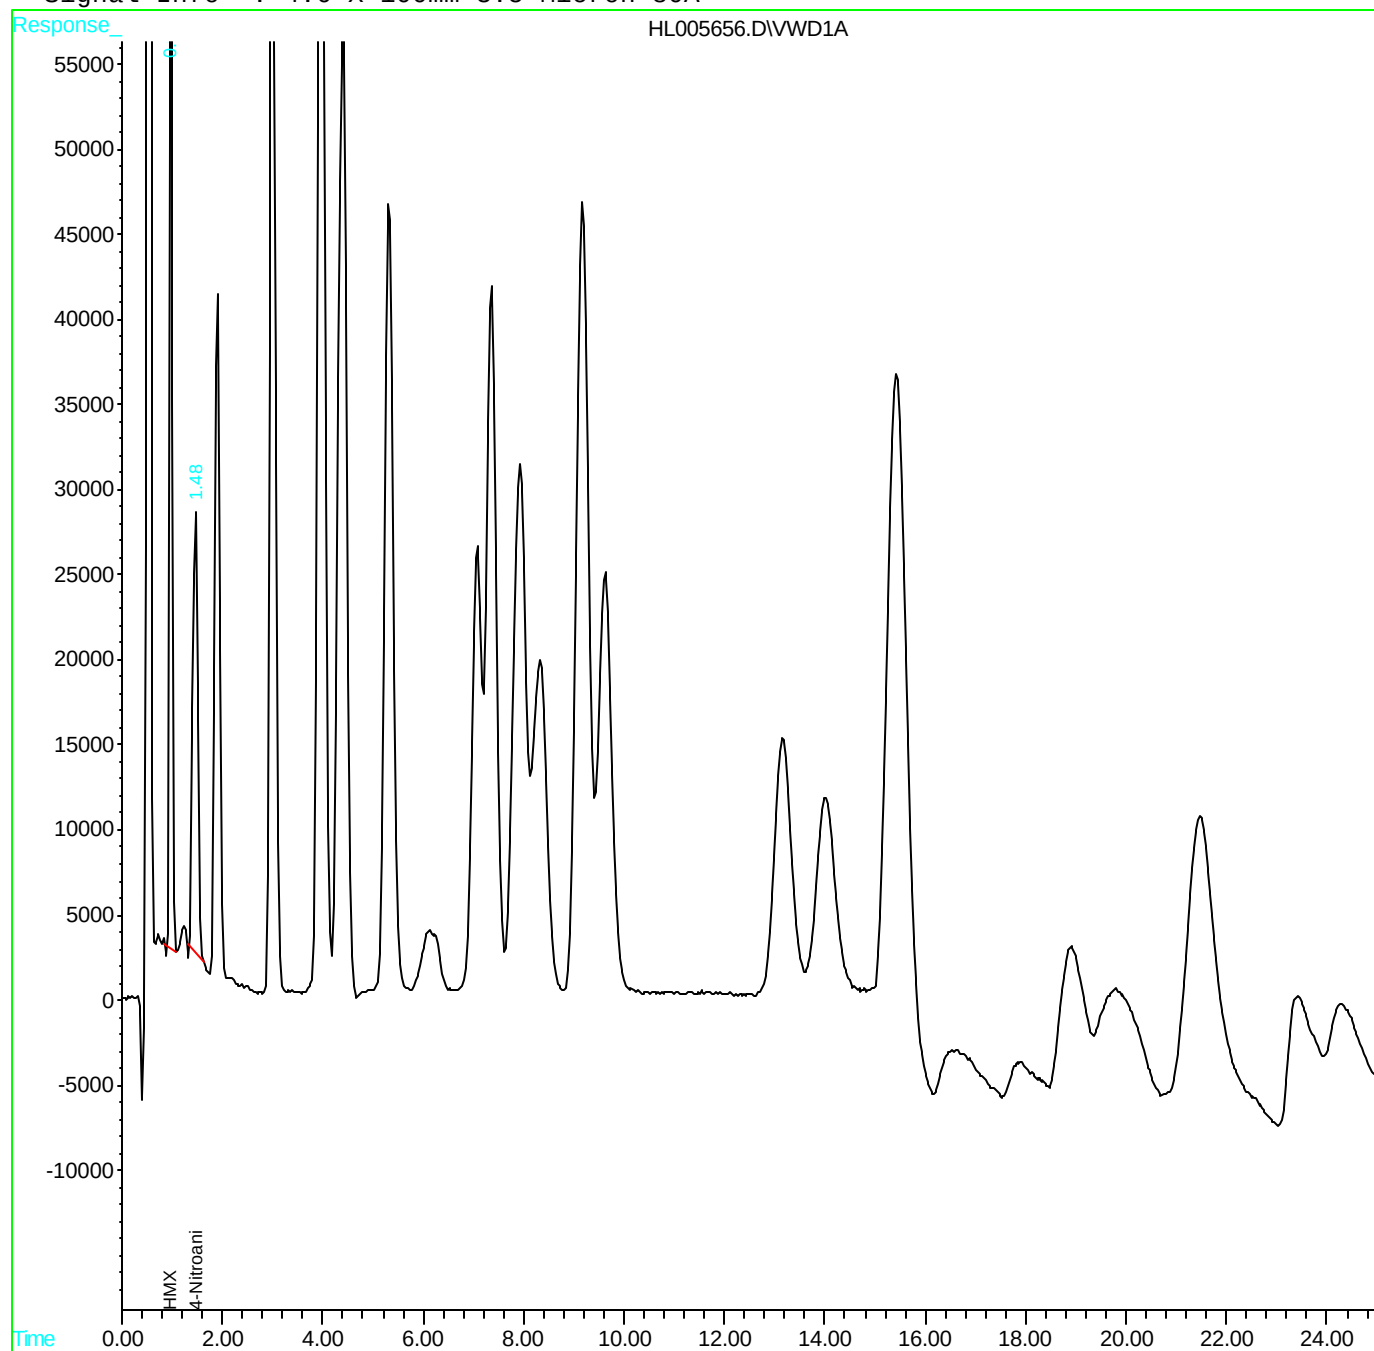

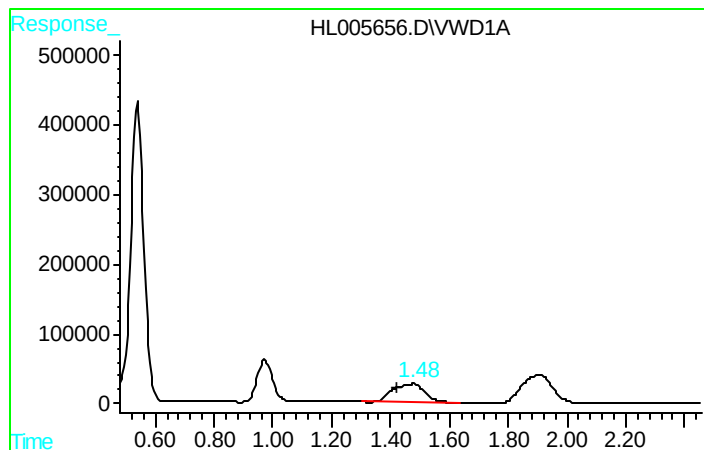

#1 4-Nitroaniline

R.T.: 1.477 min
 Delta R.T.: 0.055 min
 Response: 1931681
 Conc: 482.09 ug/L

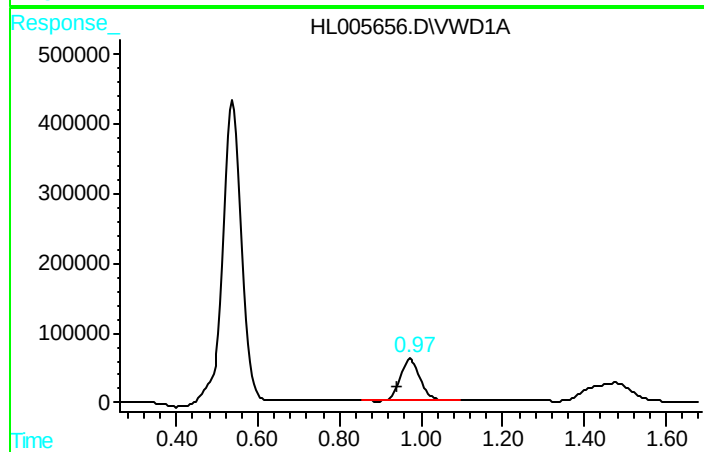

#2 HMX

R.T.: 0.974 min
 Delta R.T.: 0.036 min
 Response: 2167051
 Conc: 481.41 ug/L