

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL022713\HL005085.D Vial: 53
Acq On : 27-Feb-2013, 18:09 Operator: QM
Sample : HSTDICC1000 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Feb 28 14:38 2013 Quant Results File: HL022713.RES

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL022713.M
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Thu Feb 28 14:20:05 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units


System Monitoring Compounds			
1) S 4-Nitroaniline	1.48	4350452	1006.884 ug/L
Spiked Amount 300.000	Range 37 - 149	Recovery	= 335.63%#
Target Compounds			
2) L1 3,5-Dinitroaniline	4.42	14327867	1015.679 ug/L
3) L2 PETN	21.77	8213162	867.516 ug/L


Quantitation Report

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL022713\HL005085.D Vial: 53
Acq On : 27-Feb-2013, 18:09 Operator: QM
Sample : HSTDICC1000 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Feb 28 14:38 2013 Quant Results File: HL022713.RES

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL022713.M
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Thu Feb 28 14:20:05 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M


Volume Inj. :
Signal Phase :
Signal Info :

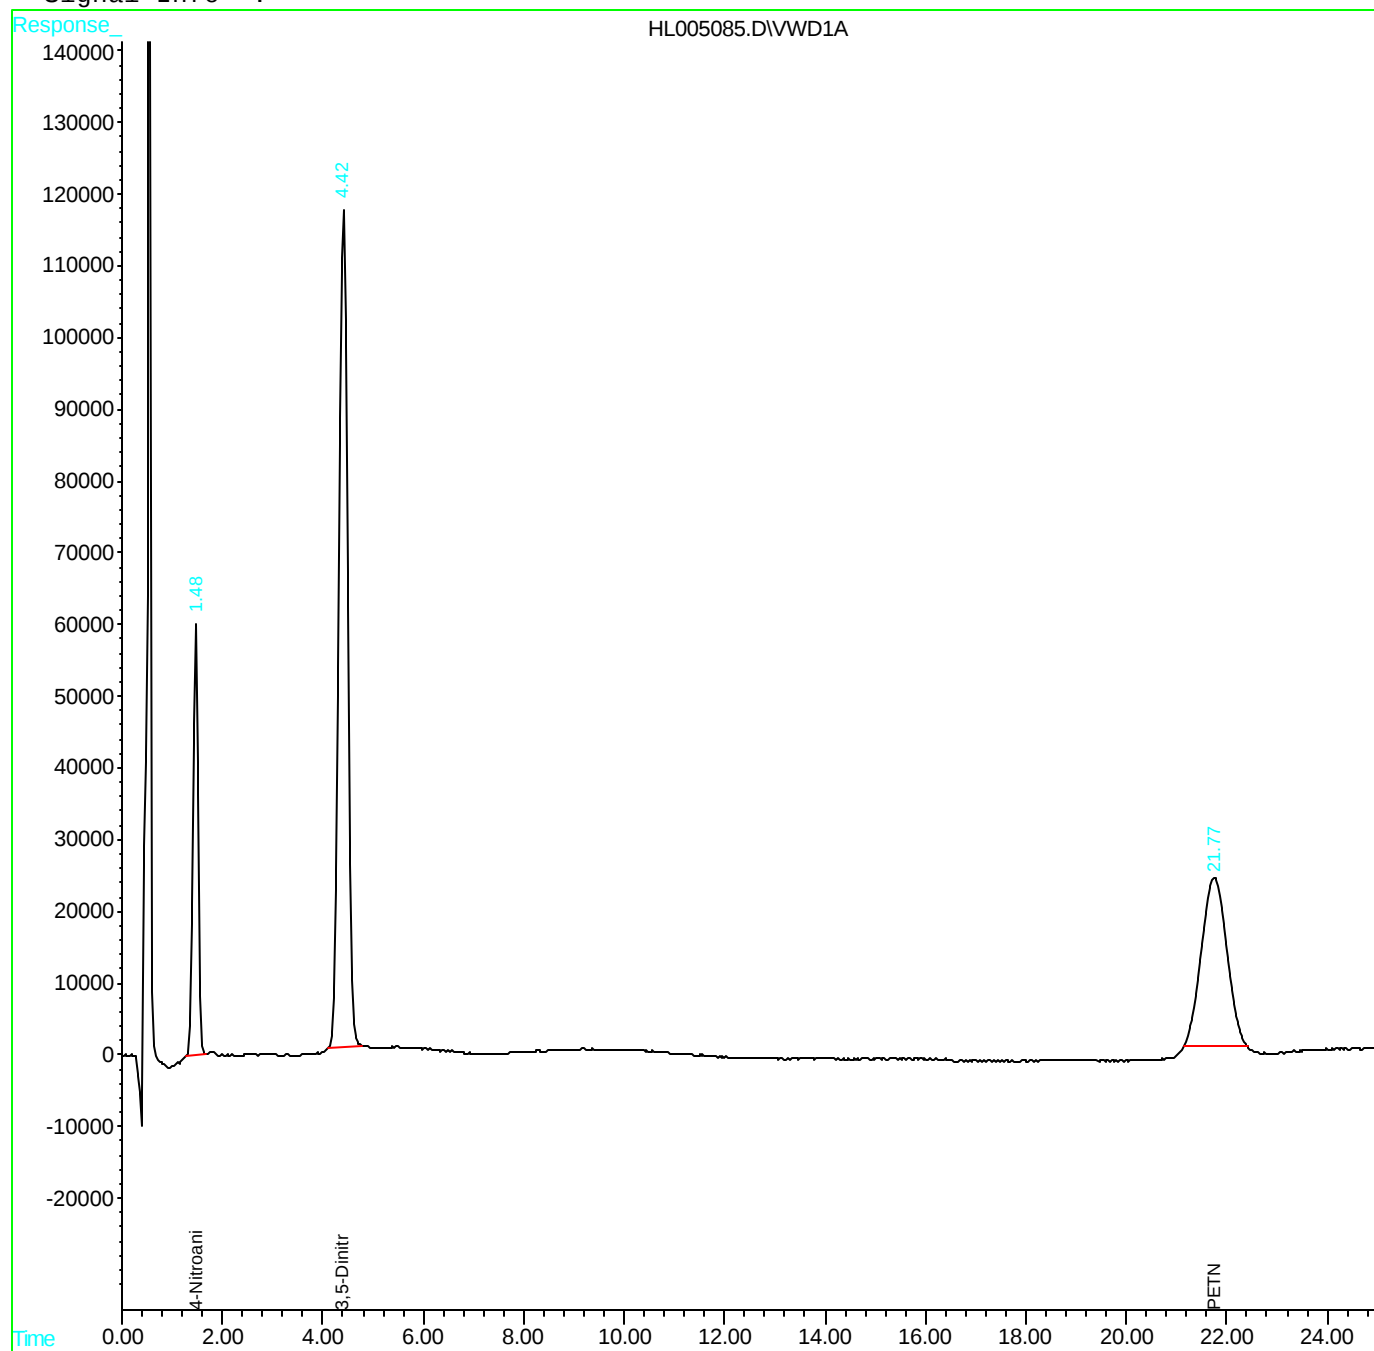

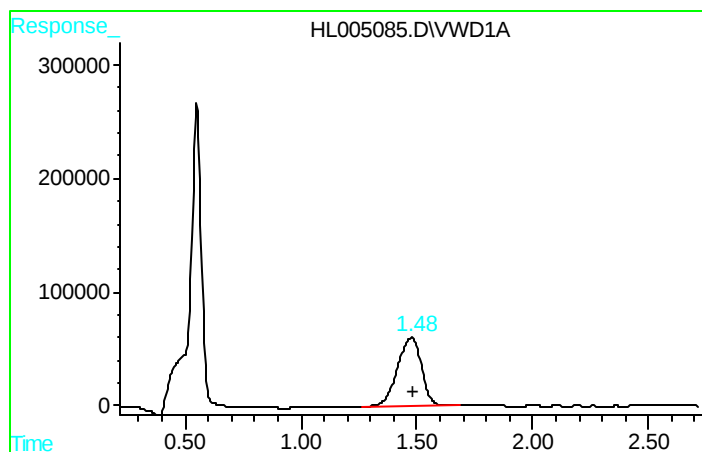


#1 4-Nitroaniline

R.T.: 1.478 min
 Delta R.T.: -0.002 min
 Response: 4350452
 Conc: 1006.88 ug/L

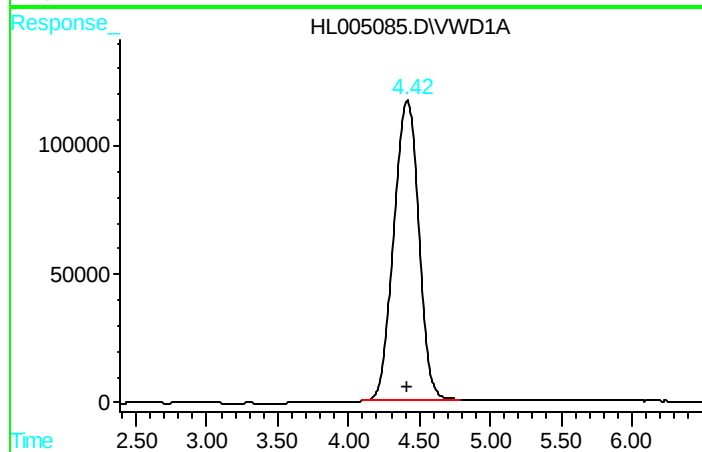

#2 3,5-Dinitroaniline

R.T.: 4.417 min
 Delta R.T.: 0.007 min
 Response: 14327867
 Conc: 1015.68 ug/L

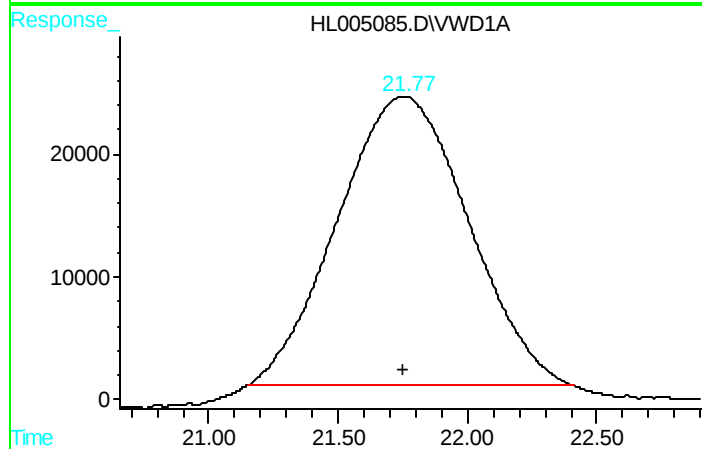

#3 PETN

R.T.: 21.765 min
 Delta R.T.: 0.015 min
 Response: 8213162
 Conc: 867.52 ug/L