

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL022713\HL005087.D Vial: 55
Acq On : 27-Feb-2013, 19:03 Operator: QM
Sample : HSTDICC0100 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Feb 28 14:41 2013 Quant Results File: HL022713.RES

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL022713.M
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Thu Feb 28 14:20:05 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds


Target Compounds


Quantitation Report

Data File : Z:\HPCHEM1\HPLC_L\DATA\HL022713\HL005087.D Vial: 55
Acq On : 27-Feb-2013, 19:03 Operator: QM
Sample : HSTDICC0100 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Feb 28 14:41 2013 Quant Results File: HL022713.RES

Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL022713.M
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Thu Feb 28 14:20:05 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

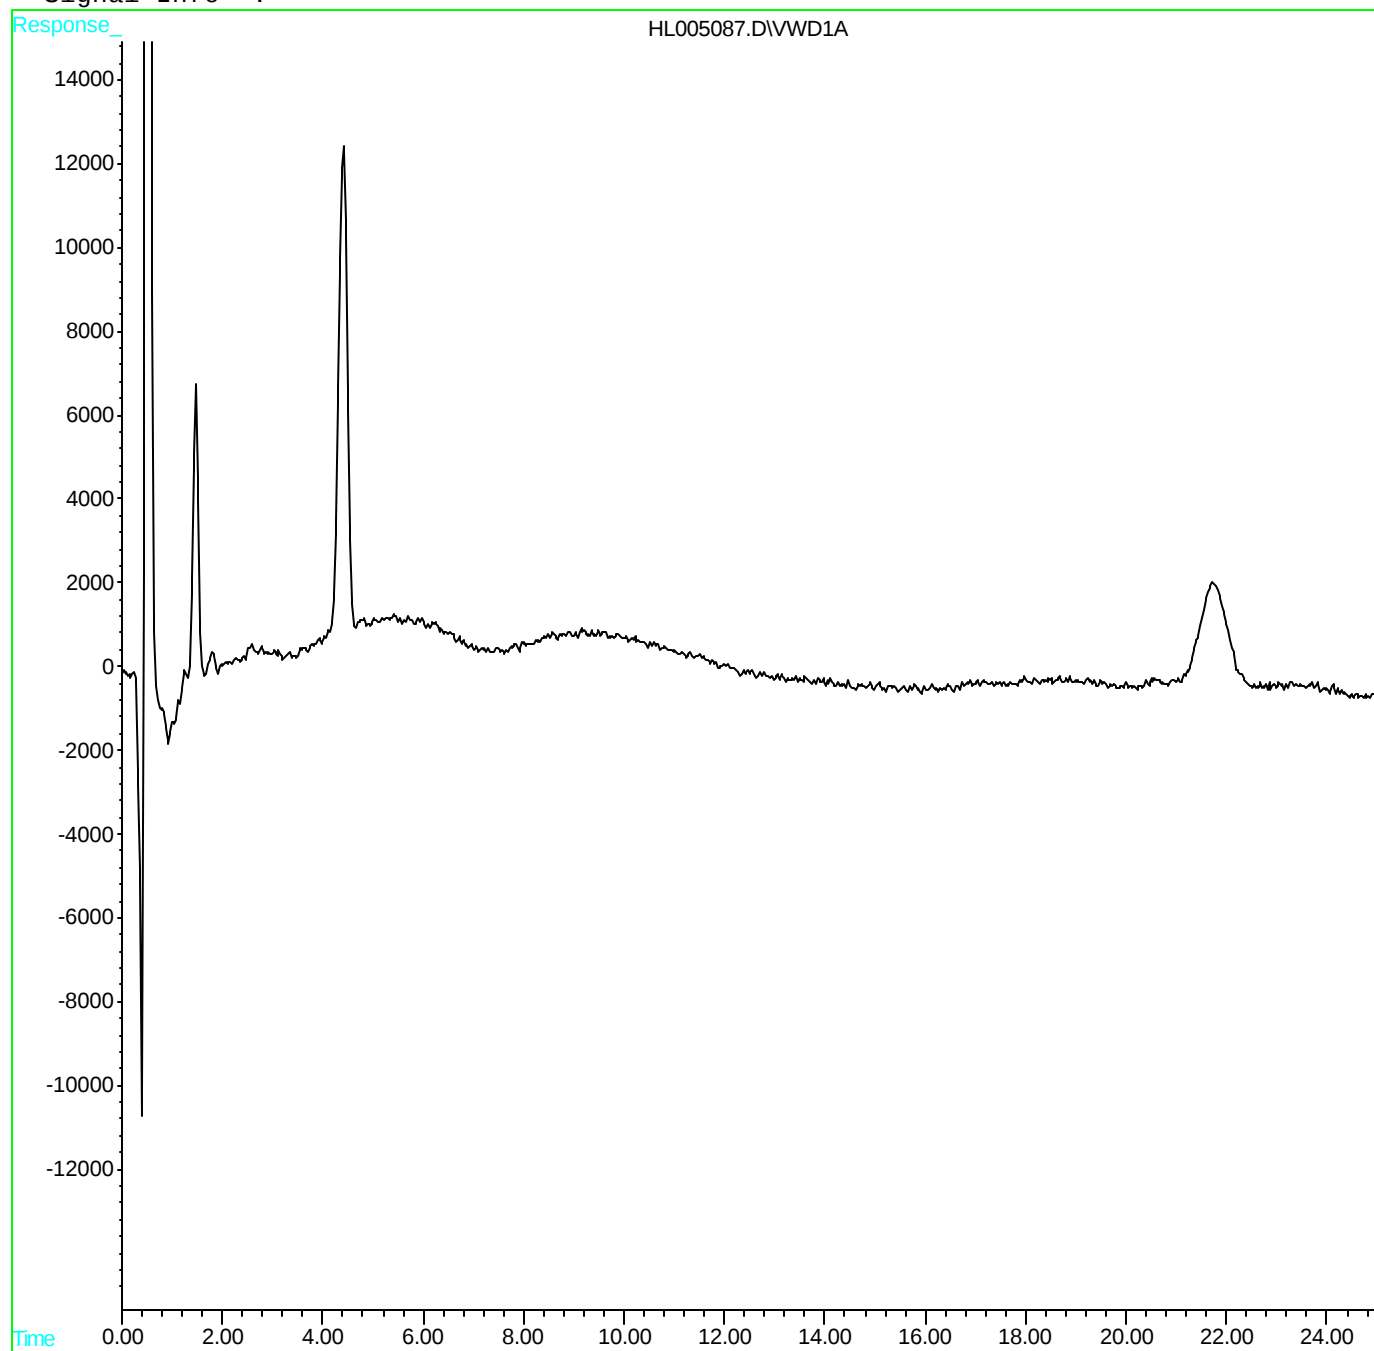

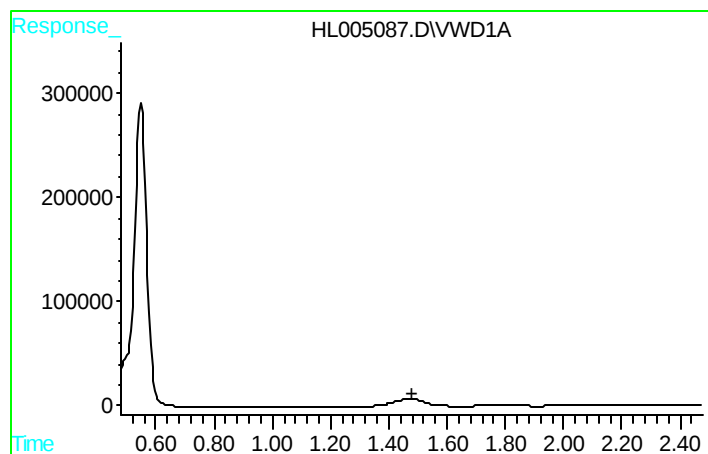

#1 4-Nitroaniline

R.T.: 0.000 min
Exp R.T. : 1.480 min
Response: 0
Conc: N.D.