

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN022813\HN005100.D Vial: 54
Acq On : 28-Feb-2013, 15:31 Operator: QM
Sample : HSTDCCC0500 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Feb 28 15:55 2013 Quant Results File: HN022813.RES

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN022813.M
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Thu Feb 28 14:12:42 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units


System Monitoring Compounds			
1) S 4-Nitroaniline	1.27	2495489	568.557 ug/L
Spiked Amount 300.000	Range 37 - 149	Recovery	= 189.52%#
Target Compounds			
2) T 3,5-Dinitroaniline	3.70	7173490	508.587 ug/L
3) T PETN	17.56	4908935	514.659 ug/L


Quantitation Report

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN022813\HN005100.D Vial: 54
Acq On : 28-Feb-2013, 15:31 Operator: QM
Sample : HSTDCCC0500 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Feb 28 15:55 2013 Quant Results File: HN022813.RES

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN022813.M
Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
Last Update : Thu Feb 28 14:12:42 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M


Volume Inj. :
Signal Phase :
Signal Info :

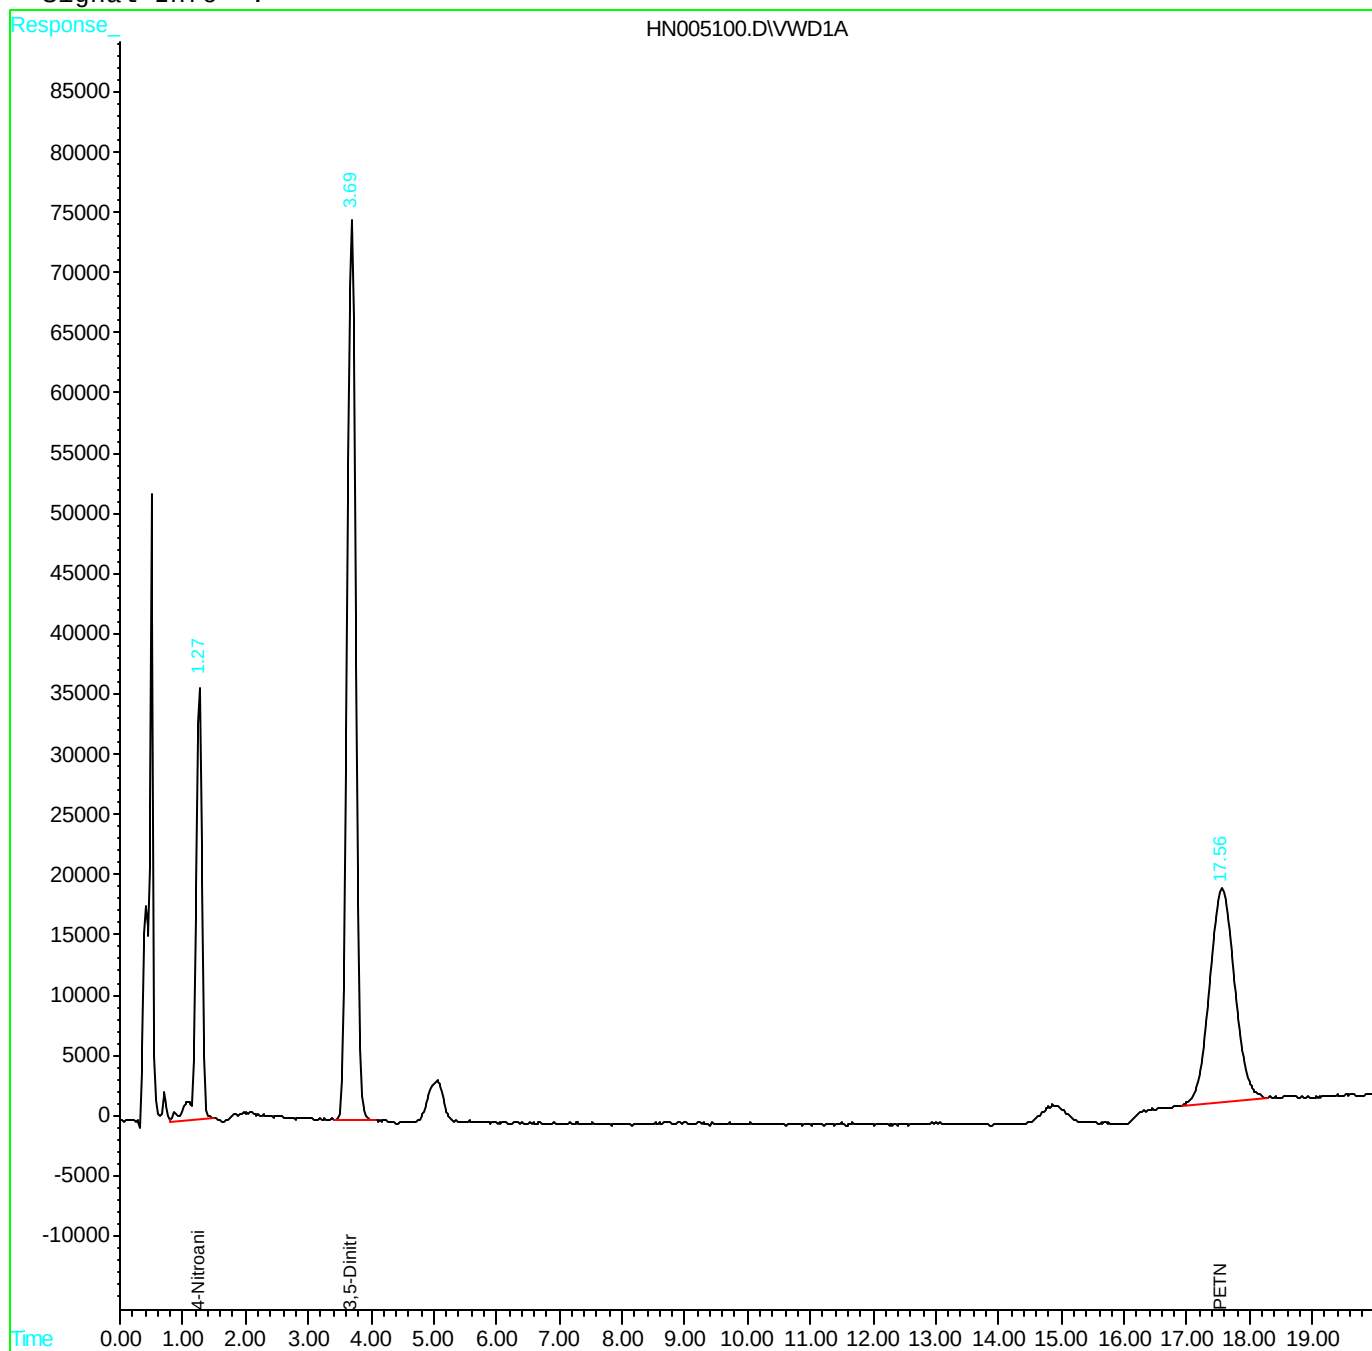

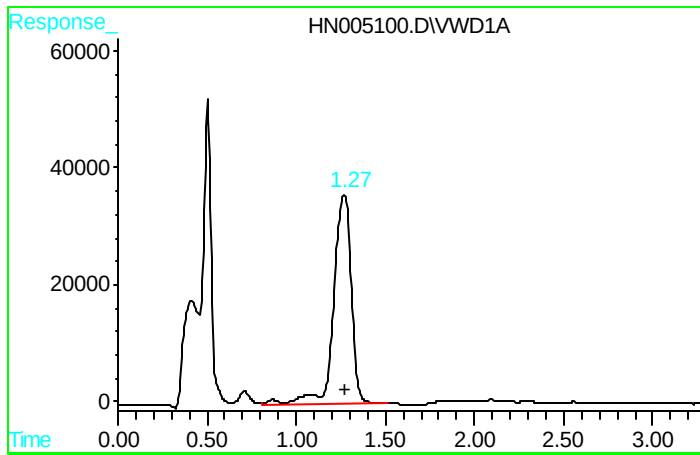


#1 4-Nitroaniline

R.T.: 1.268 min
 Delta R.T.: -0.002 min
 Response: 2495489
 Conc: 568.56 ug/L

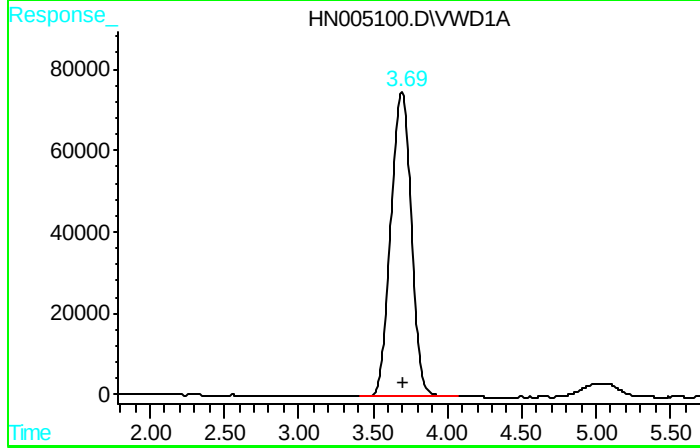

#2 3,5-Dinitroaniline

R.T.: 3.695 min
 Delta R.T.: -0.005 min
 Response: 7173490
 Conc: 508.59 ug/L

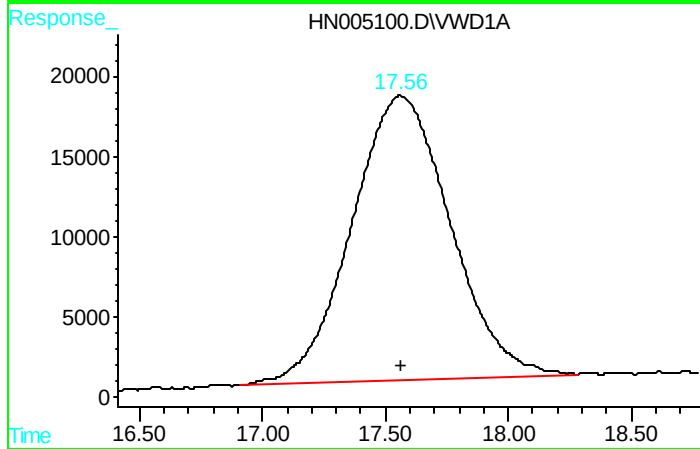

#3 PETN

R.T.: 17.561 min
 Delta R.T.: 0.001 min
 Response: 4908935
 Conc: 514.66 ug/L