

Data Path : S:\HPCHEM1\HPLC_L\Data\HL022713\
Data File : HL005083.D
Signal(s) : VWD1A.CH
Acq On : 27-Feb-2013, 17:16
Operator : QM
Sample : HSTDICC5000
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 01 00:25:17 2013
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL022713.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Feb 28 14:20:05 2013
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.479	22024429	5097.413 ug/L
Spiked Amount 300.000	Range 37 - 149	Recovery	= 1699.14%#
Target Compounds			
2) L1 3,5-Dinitroaniline	4.420	71792786	5089.271 ug/L
3) L2 PETN	21.771	47281497	4994.110 ug/L


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : S:\HPCHEM1\HPLC_L\Data\HL022713\
Data File : HL005083.D
Signal(s) : VWD1A.CH
Acq On : 27-Feb-2013, 17:16
Operator : QM
Sample : HSTDICC5000
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 01 00:25:17 2013
Quant Method : Z:\HPCHEM1\HPLC_L\METHODS\HL022713.M
Quant Title : SW8330A/B Primary (Extend C18 3.5u 4.6x10mm)
QLast Update : Thu Feb 28 14:20:05 2013
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. :
Signal Phase :
Signal Info :

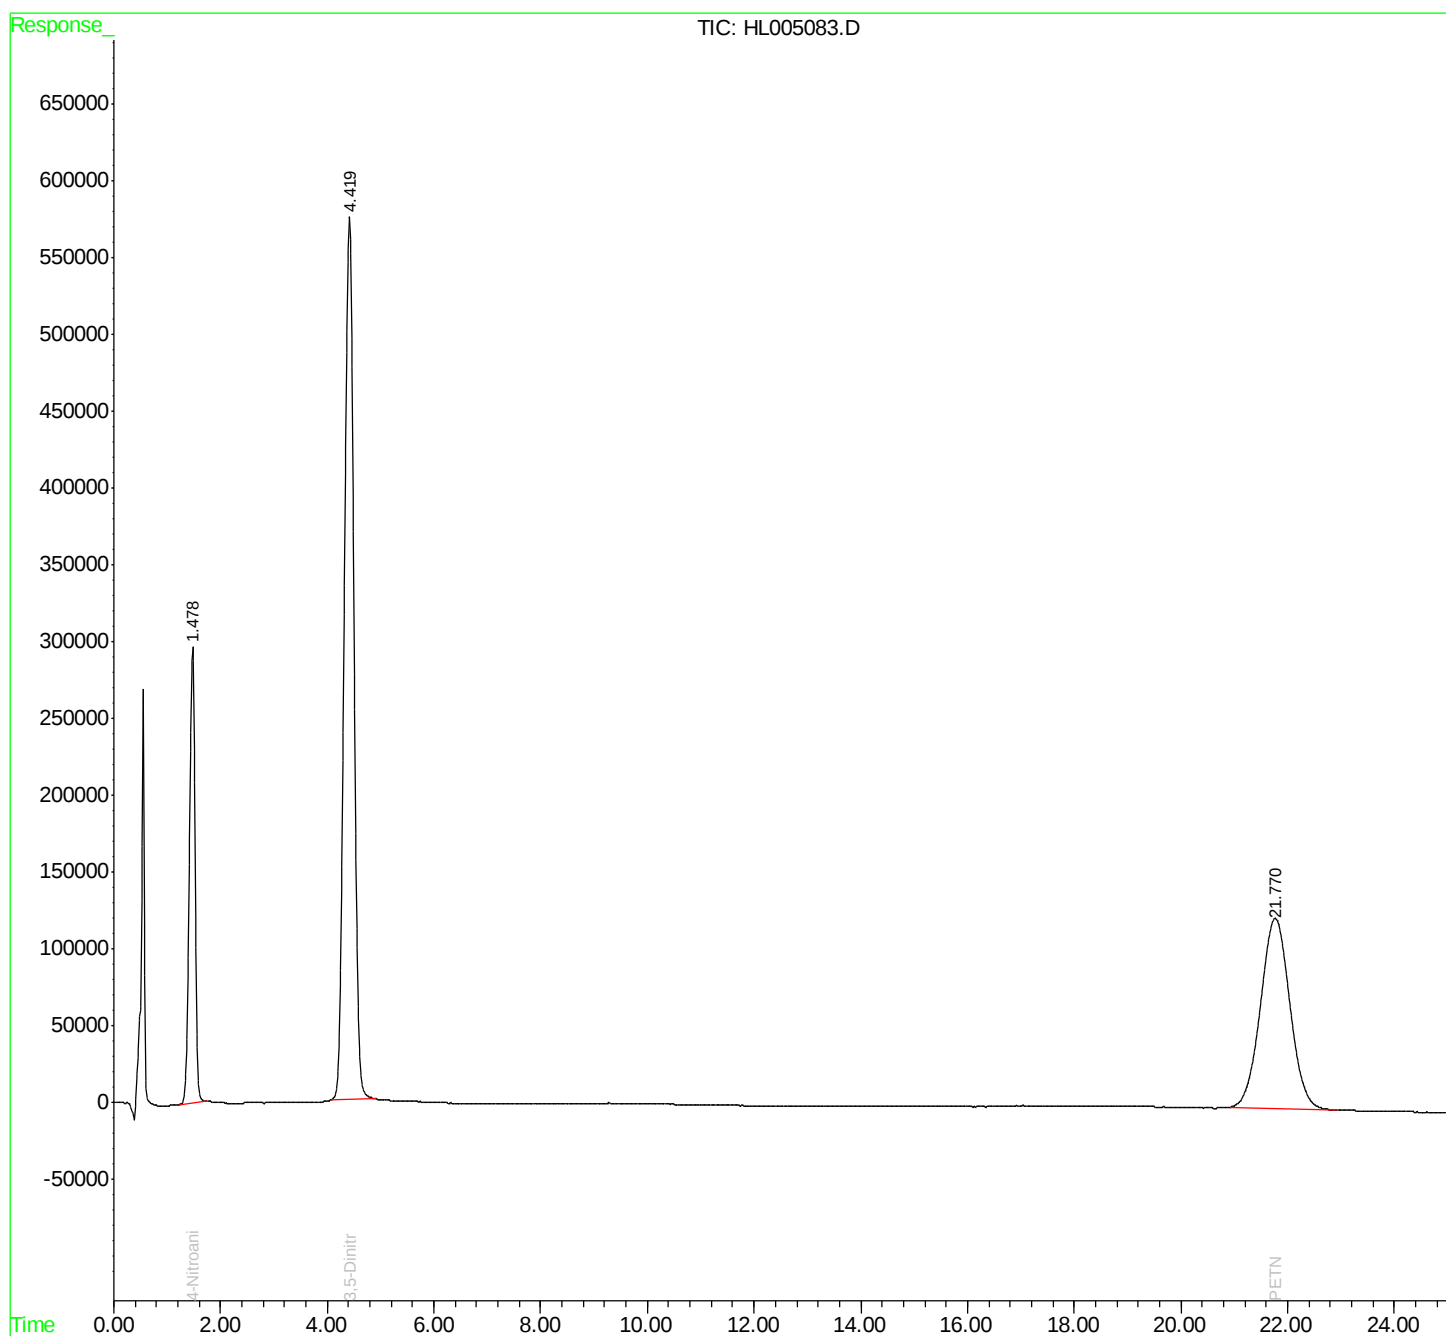

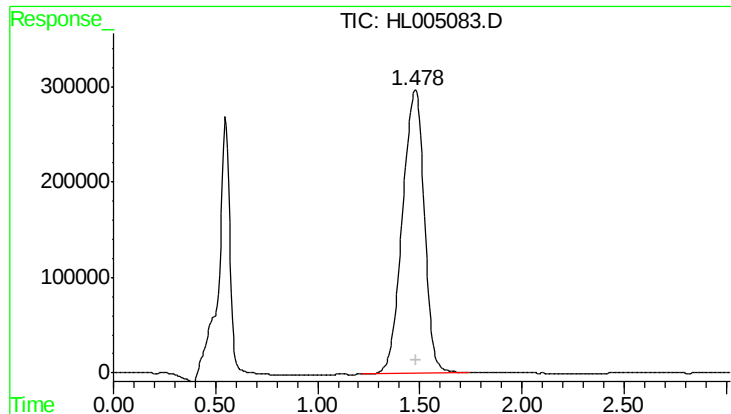


#1 4-Nitroaniline

R.T.: 1.479 min
Delta R.T.: 0.000 min
Response: 22024429
Conc: 5097.41 ug/L

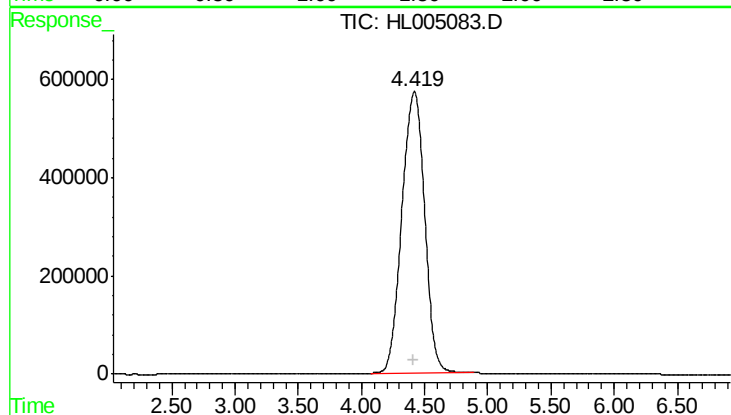

#2 3,5-Dinitroaniline

R.T.: 4.420 min
Delta R.T.: 0.010 min
Response: 71792786
Conc: 5089.27 ug/L

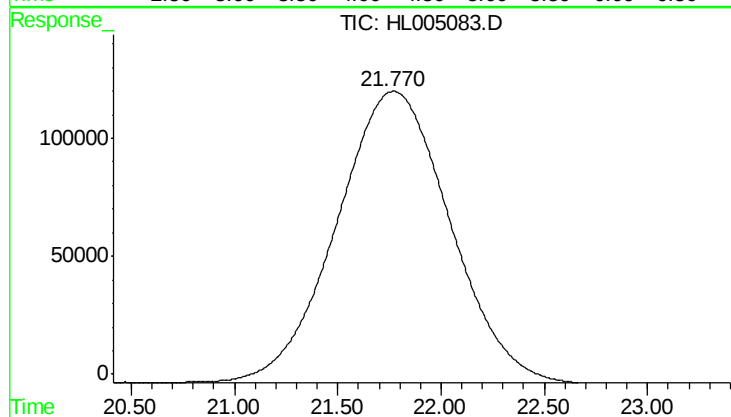

#3 PETN

R.T.: 21.771 min
Delta R.T.: 0.021 min
Response: 47281497
Conc: 4994.11 ug/L